

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052724\
 Data File : PD083114.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2024 00:25
 Operator : AR\AJ
 Sample : P2549-09MS
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH625MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/28/2024
 Supervised By : Ankita Jodhani 05/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 01:31:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.564	2.775	17933127	60571069	11.989	15.576 #
27)	SA Decachlor...	9.111	7.901	42583512	100.5E6	21.245m	25.393
Target Compounds							
2)	A alpha-BHC	4.022	3.274	156.1E6	384.5E6	61.195	61.854
3)	MA gamma-BHC...	4.354	3.603	129.1E6	363.4E6	52.332m	62.796
4)	MA Heptachlor	4.946	3.941	146.6E6	331.1E6	58.221m	59.467
5)	MB Aldrin	5.292	4.221	137.0E6	335.2E6	56.599	60.637
6)	B beta-BHC	4.552	3.899	48627132	135.8E6	44.822m	54.128
7)	B delta-BHC	4.801	4.128	139.4E6	359.4E6	56.939	60.756
8)	B Heptachlo...	5.718	4.722	124.5E6	307.3E6	55.740m	60.149
9)	A Endosulfan I	6.107	5.093	112.8E6	178.3E6	54.185	39.529 #
10)	B trans-Chl...	5.975	4.971	181.7E6	423.9E6	83.923m	85.113
11)	B cis-Chlor...	6.057	5.035	247.7E6	490.7E6	110.927	96.617
12)	B 4,4'-DDE	6.227	5.224	363.2E6	1026.9E6	166.529	215.343 #
13)	MA Dieldrin	6.383	5.354	256.9E6	719.5E6	116.873	143.986m
14)	MA Endrin	6.614	5.631	184.2E6	643.6E6	103.298	147.148 #
15)	B Endosulfa...	6.831	5.922	200.7E6	504.9E6	104.199m	119.814m
16)	A 4,4'-DDD	6.744	5.777	206.3E6	426.5E6	133.045m	113.336
17)	MA 4,4'-DDT	7.061	6.027	363.5E6	795.1E6	225.991	207.081
18)	B Endrin al...	6.961	6.101	148.6E6	326.6E6	107.010m	103.559m
19)	B Endosulfa...	7.198	6.325	191.2E6	464.3E6	108.344	115.482
20)	A Methoxychlor	7.538	6.602	470.5E6	1043.4E6	543.897	531.761
21)	B Endrin ke...	7.685	6.830	185.0E6	424.9E6	98.114	94.478

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052724\
Data File : PD083114.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2024 00:25
Operator : AR\AJ
Sample : P2549-09MS
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 01:31:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

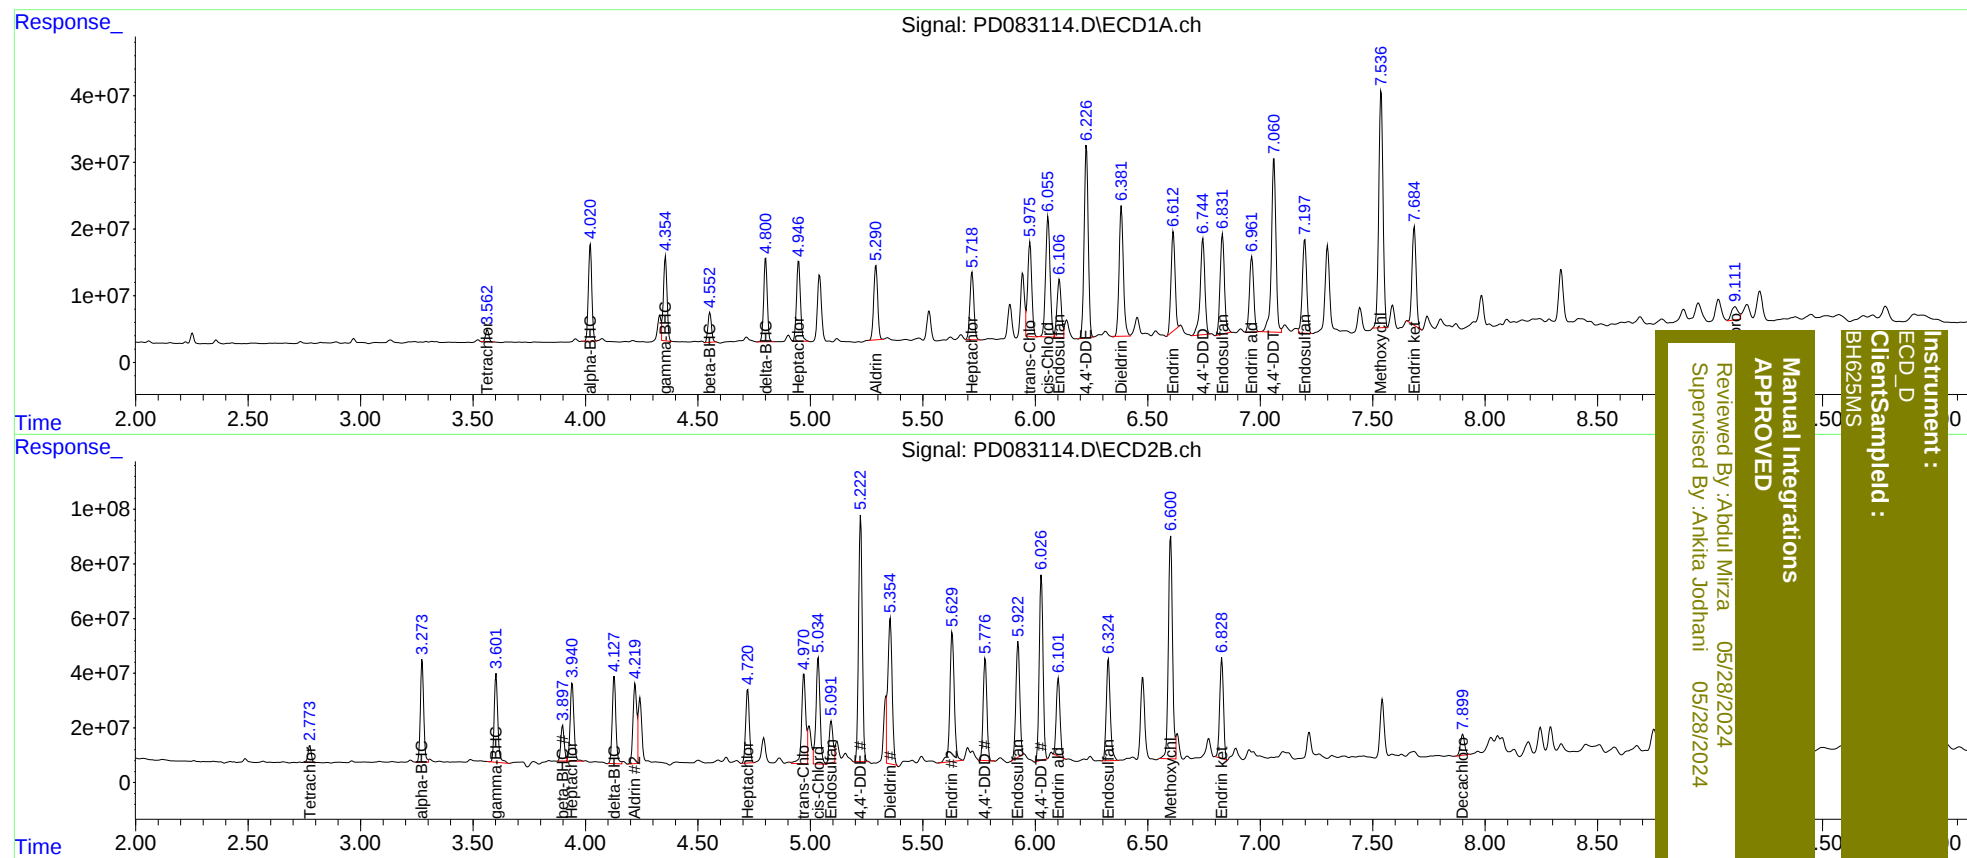

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/28/2024
Supervised By: Ankita Jodhani 05/28/2024

Instrument :
ECD_D
Client Sampled :
BH625MS