

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD052724\  
 Data File : PD083158.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 May 2024 19:03  
 Operator : AR\AJ  
 Sample : P2569-19  
 Misc :  
 ALS Vial : 56 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 BH6A5

Manual Integrations  
 APPROVED

Reviewed By : Abdul Mirza 06/04/2024  
 Supervised By : Ankita Jodhani 06/04/2024

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 27 22:01:41 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD051924CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Fri May 17 05:17:58 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm


|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml     |
|-----------------------------|-----------------|-------|-------|----------|----------|---------|-----------|
| -----                       |                 |       |       |          |          |         |           |
| System Monitoring Compounds |                 |       |       |          |          |         |           |
| 1)                          | SA Tetrachlo... | 3.563 | 2.775 | 16460243 | 69326762 | 11.005m | 17.828 #  |
| 27)                         | SA Decachlor... | 9.113 | 7.901 | 153.8E6  | 241.0E6  | 76.720m | 60.916    |
| Target Compounds            |                 |       |       |          |          |         |           |
| 9)                          | A Endosulfan I  | 6.139 | 5.117 | 175.1E6  | 258.8E6  | 84.160m | 57.395m#  |
| 12)                         | B 4,4'-DDE      | 6.228 | 5.223 | 360.6E6  | 1039.0E6 | 165.363 | 217.881 # |
| 13)                         | MA Dieldrin     | 6.401 | 5.361 | 174.0E6  | 328.5E6  | 79.182m | 65.731m   |
| 14)                         | MA Endrin       | 6.642 | 5.637 | 91793126 | 106.6E6  | 51.476m | 24.380m#  |
| 16)                         | A 4,4'-DDD      | 6.731 | 5.775 | 127.1E6  | 279.9E6  | 81.982m | 74.382m   |
| 17)                         | MA 4,4'-DDT     | 7.063 | 6.027 | 317.5E6  | 637.4E6  | 197.394 | 166.003   |
| -----                       |                 |       |       |          |          |         |           |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD052724\  
Data File : PD083158.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 27 May 2024 19:03  
Operator : AR\AJ  
Sample : P2569-19  
Misc :  
ALS Vial : 56 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: May 27 22:01:41 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD051924CLP.M  
Quant Title : GC Extractables  
QLast Update : Fri May 17 05:17:58 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

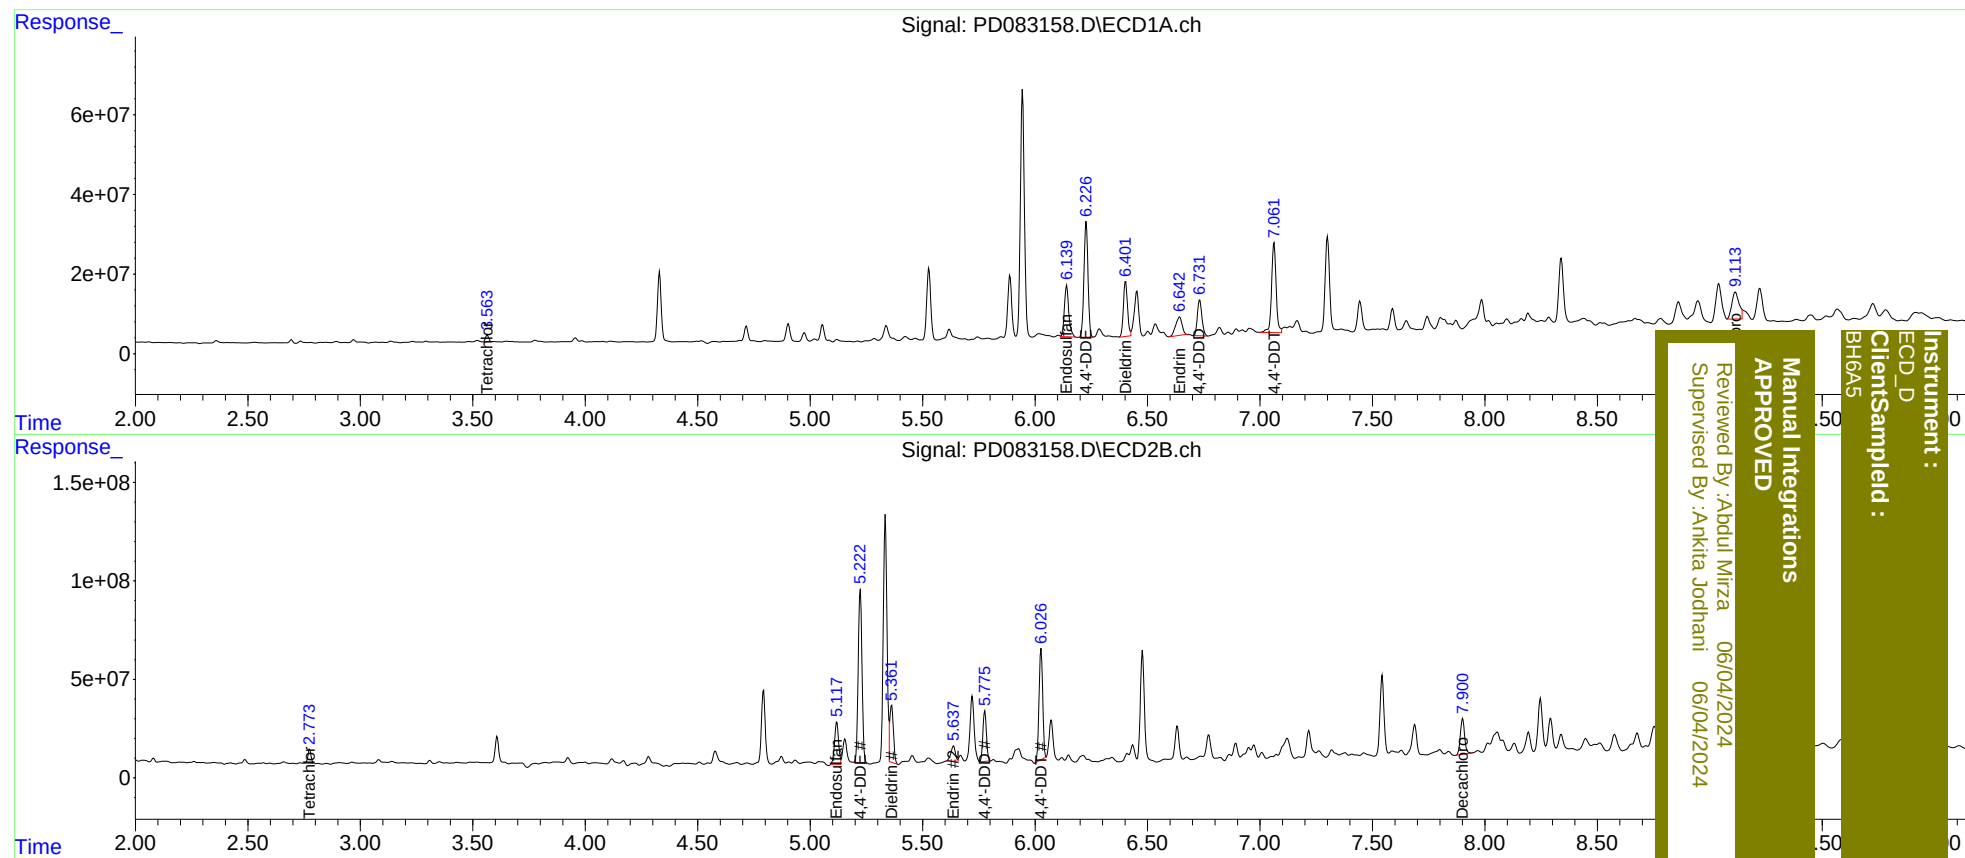

Reviewed By: Abdul Mirza 06/04/2024  
Supervised By: Ankita Jodhani 06/04/2024

Manual Integrations  
APPROVED

Instrument :  
ECD\_D  
ClientSampled :  
BH6A5