

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052820\
 Data File : PD058167.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2020 09:01
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 00:41:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:46:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.210	3.866	19810366	27780736	25.348	24.393
28)	SA Decachlor...	7.850	8.850	19509306	23936341	24.399	23.089
Target Compounds							
3)	MA gamma-BHC...	3.922f	0.000	1129329	0	0.963	N.D. #
5)	MB Aldrin	4.431	0.000	611205	0	0.582	N.D. #
8)	B Heptachlo...	4.872f	0.000	712359	0	0.730	N.D. #
10)	B gamma-Chl...	5.070	0.000	73463	0	0.074	N.D. #
13)	MA Dieldrin	5.405	0.000	342042	0	0.349	N.D. #
14)	MA Endrin	5.690f	0.000	228559	0	0.286	N.D. #
24)	Chlordane-2	4.501f	0.000	1145823	0	35.841	N.D. #
25)	Chlordane-3	5.070	0.000	73463	0	0.820	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052820\
Data File : PD058167.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2020 09:01
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 00:41:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:46:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

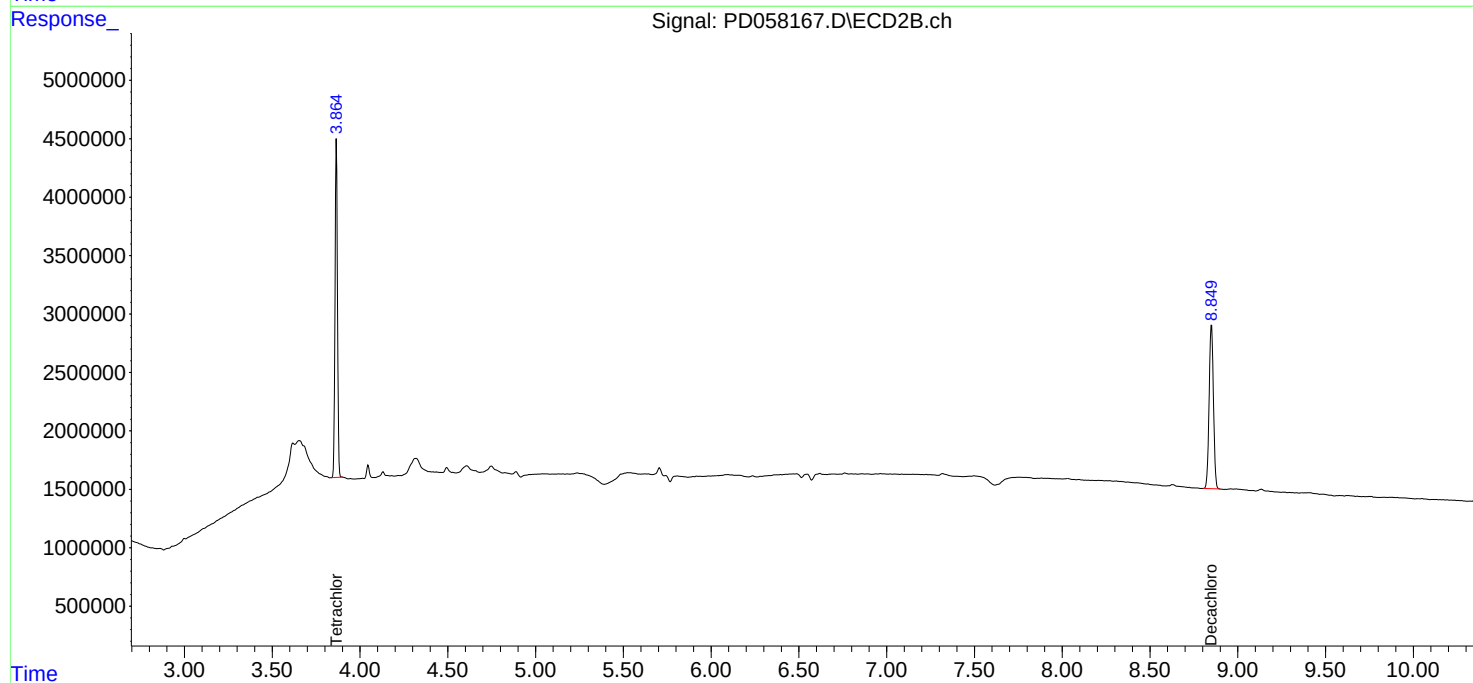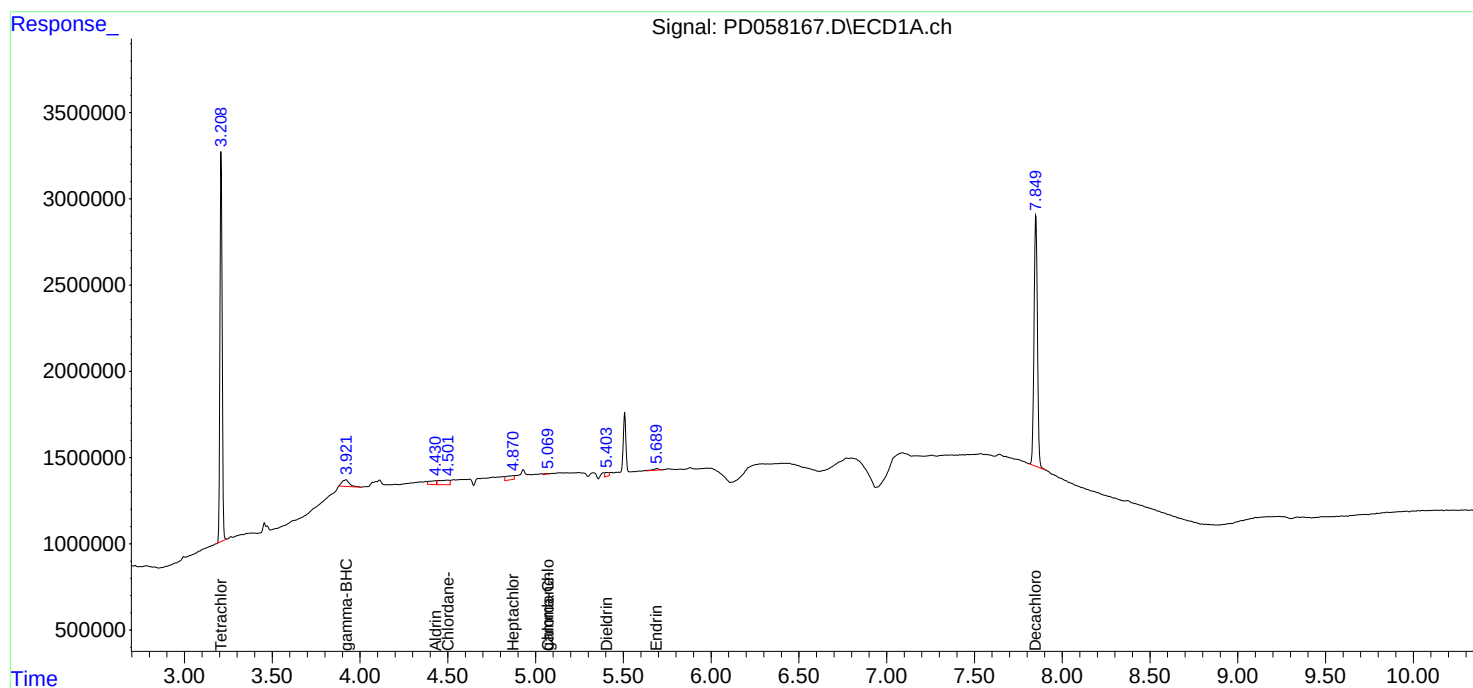


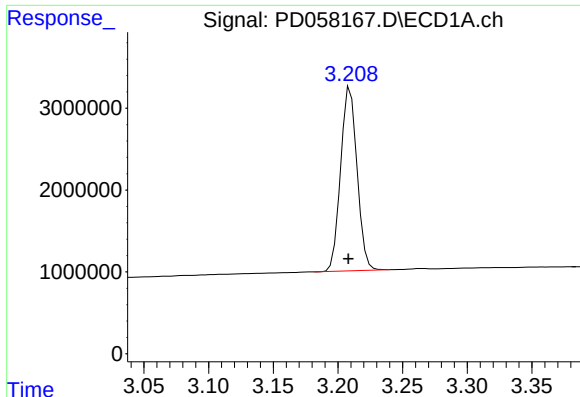

#1 Tetrachloro-m-xylene


R.T.: 3.210 min
Delta R.T.: 0.002 min
Response: 19810366
Conc: 25.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

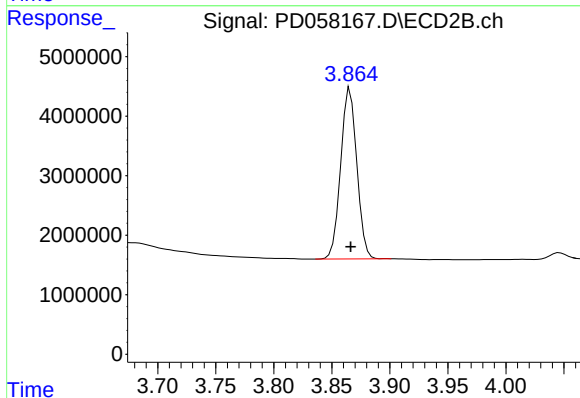


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 27780736
Conc: 24.39 ng/ml

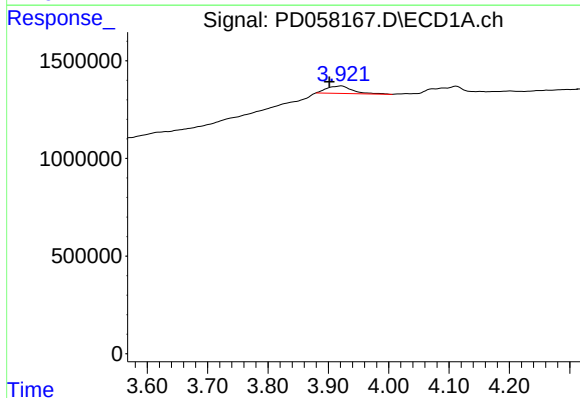


#3 gamma-BHC (Lindane)

R.T.: 3.922 min
Delta R.T.: 0.020 min
Response: 1129329
Conc: 0.96 ng/ml

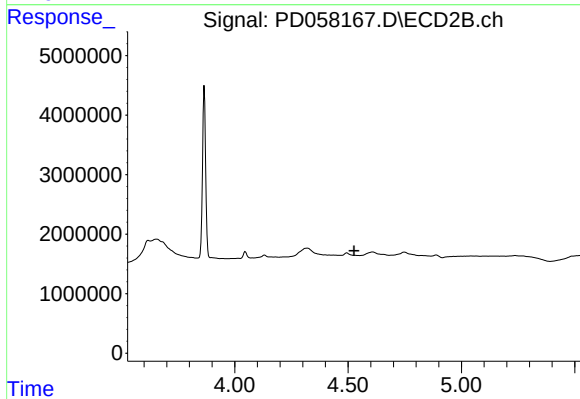

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.527 min
Response: 0
Conc: N.D.

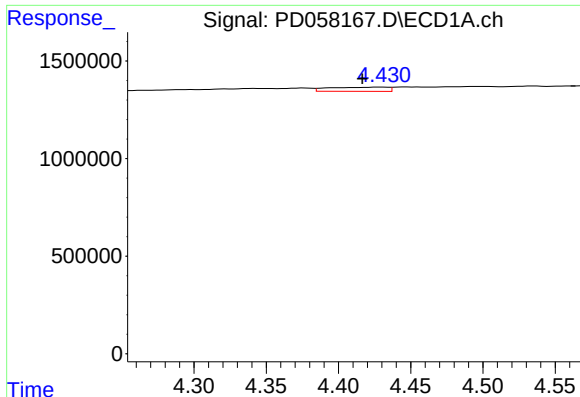

#5 Aldrin


R.T.: 4.431 min
Delta R.T.: 0.014 min
Response: 611205
Conc: 0.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

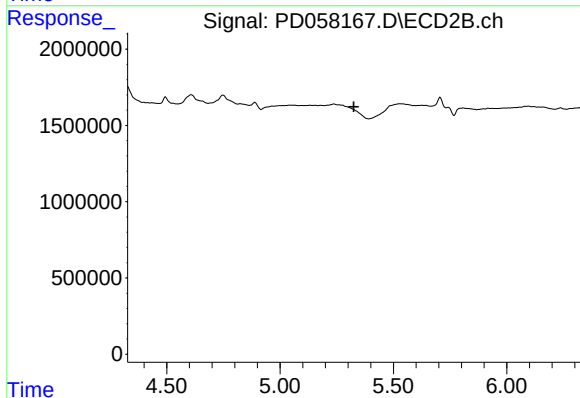


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.325 min
Response: 0
Conc: N.D.

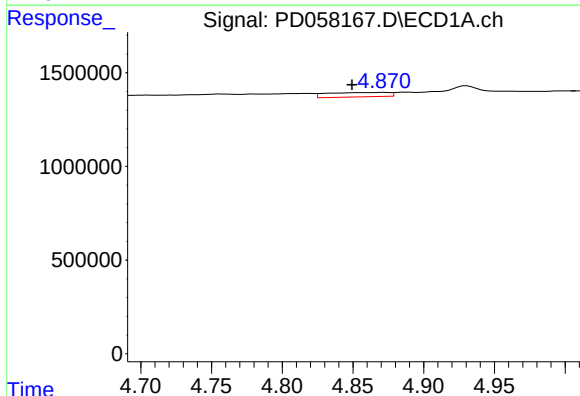


#8 Heptachlor epoxide

R.T.: 4.872 min
Delta R.T.: 0.022 min
Response: 712359
Conc: 0.73 ng/ml

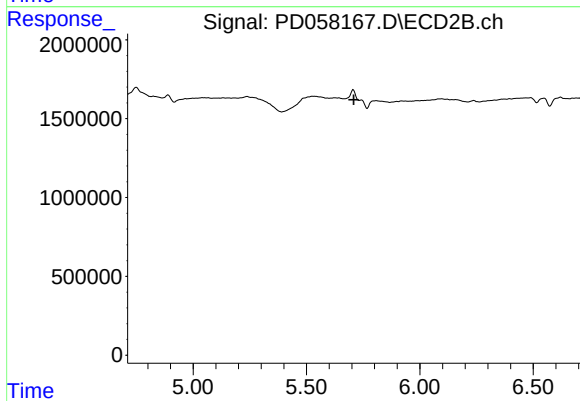

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.708 min
Response: 0
Conc: N.D.

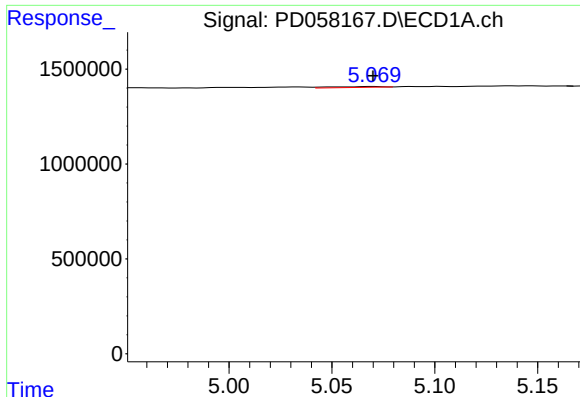

#10 gamma-Chlordane


R.T.: 5.070 min
Delta R.T.: 0.000 min
Response: 73463
Conc: 0.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

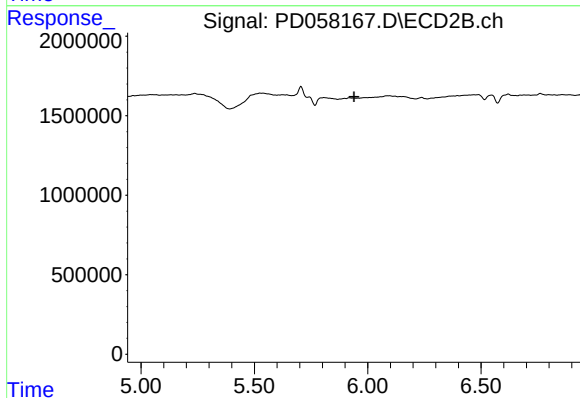


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.940 min
Response: 0
Conc: N.D.

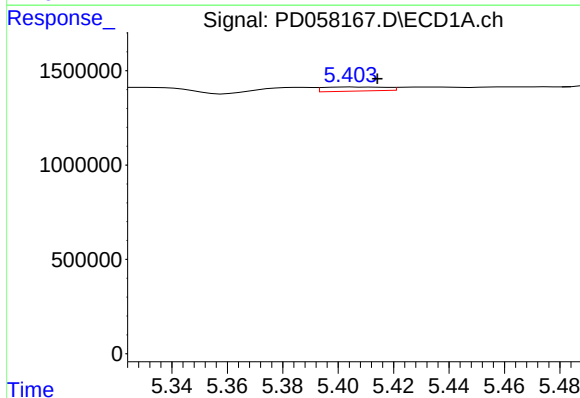


#13 Dieldrin

R.T.: 5.405 min
Delta R.T.: -0.009 min
Response: 342042
Conc: 0.35 ng/ml

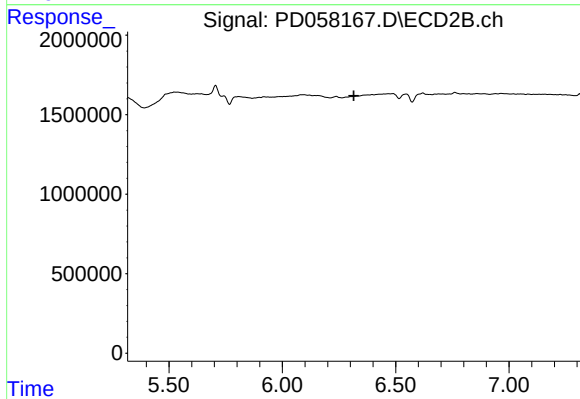

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.315 min
Response: 0
Conc: N.D.

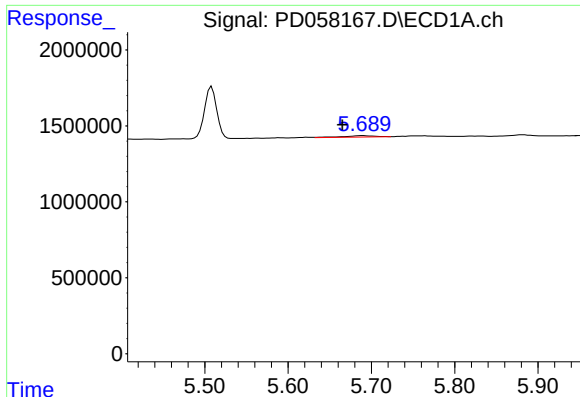

#14 Endrin


R.T.: 5.690 min
Delta R.T.: 0.025 min
Response: 228559
Conc: 0.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

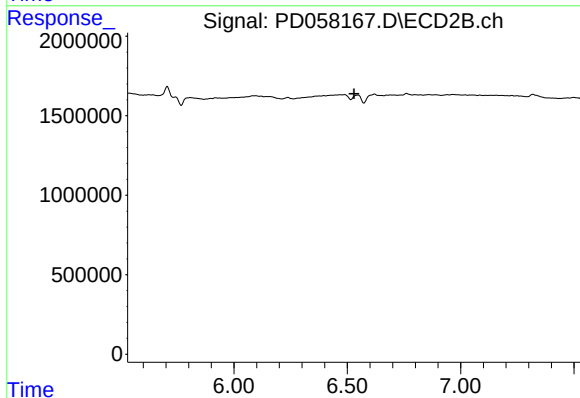


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.530 min
Response: 0
Conc: N.D.

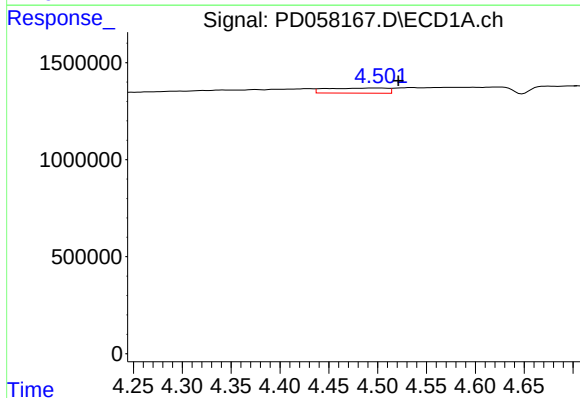


#24 Chlordane-2

R.T.: 4.501 min
Delta R.T.: -0.020 min
Response: 1145823
Conc: 35.84 ng/ml

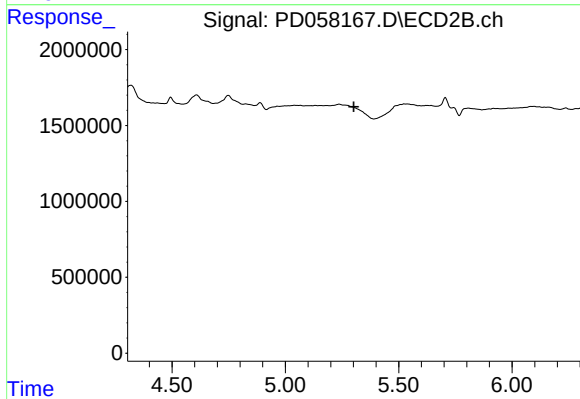

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.302 min
Response: 0
Conc: N.D.

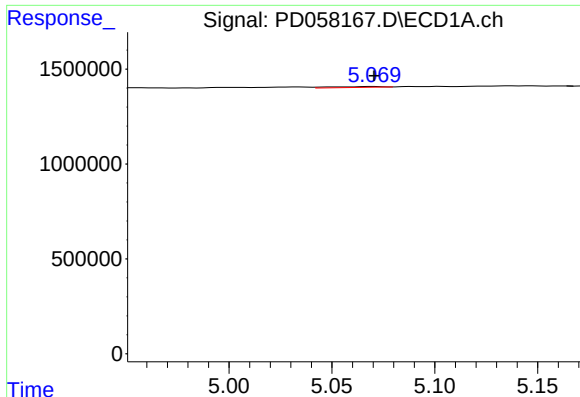

#25 Chlordane-3


R.T.: 5.070 min
Delta R.T.: 0.000 min
Response: 73463
Conc: 0.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

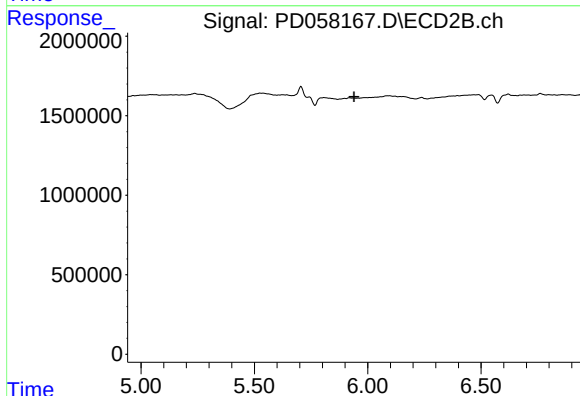


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.941 min
Response: 0
Conc: N.D.

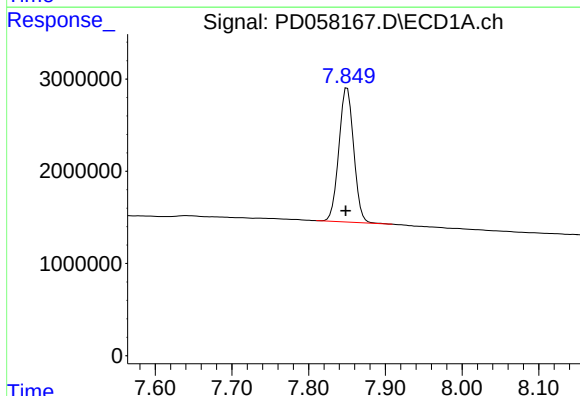

#28 Decachlorobiphenyl

R.T.: 7.850 min
Delta R.T.: 0.002 min
Response: 19509306
Conc: 24.40 ng/ml

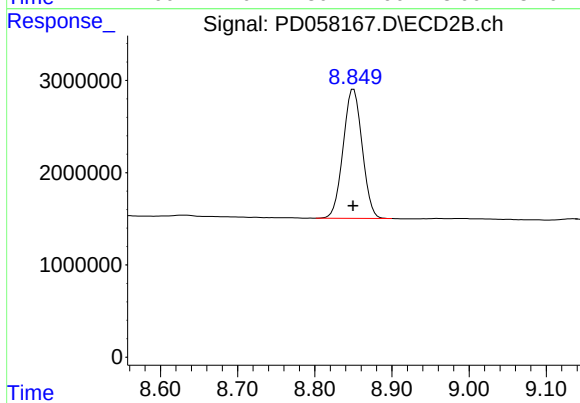

#28 Decachlorobiphenyl

R.T.: 8.850 min
Delta R.T.: 0.000 min
Response: 23936341
Conc: 23.09 ng/ml