

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052820\
 Data File : PD058202.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2020 18:43
 Operator : AJ\MA
 Sample : L2773-27
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 NM-EB-06

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 00:47:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:46:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.210	3.867	18300128	24967391	23.416	21.922
28)	SA Decachlor...	7.849	8.852	12250662	14702278	15.321	14.182
Target Compounds							
2)	A alpha-BHC	3.643	0.000	311073	0	0.257	N.D. #
3)	MA gamma-BHC...	3.913	0.000	2232254	0	1.903	N.D. #
5)	MB Aldrin	4.396f	0.000	524704	0	0.500	N.D. #
11)	B alpha-Chl...	5.110f	0.000	332686	0	0.336	N.D. #
15)	B Endosulfa...	0.000	6.766f	0	4997276	N.D.	4.156 #
16)	A 4,4'-DDD	5.824f	0.000	374857	0	0.465	N.D. #
25)	Chlordane-3	5.110f	0.000	332686	0	3.712	N.D. #
26)	Chlordane-4	5.110f	0.000	332686	0	3.894	N.D. #
27)	Chlordane-5	5.970f	0.000	2715235	0	100.523	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052820\
Data File : PD058202.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2020 18:43
Operator : AJ\MA
Sample : L2773-27
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleID :
NM-EB-06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 00:47:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:46:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

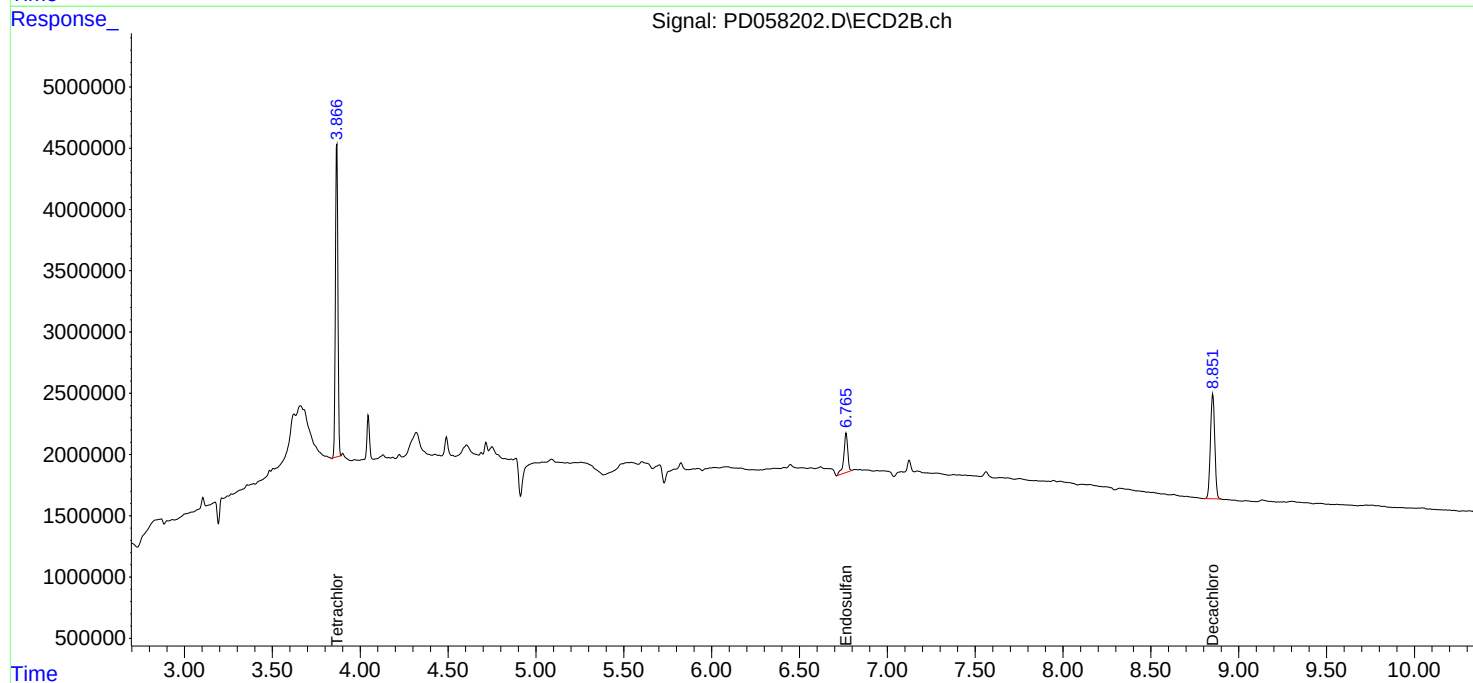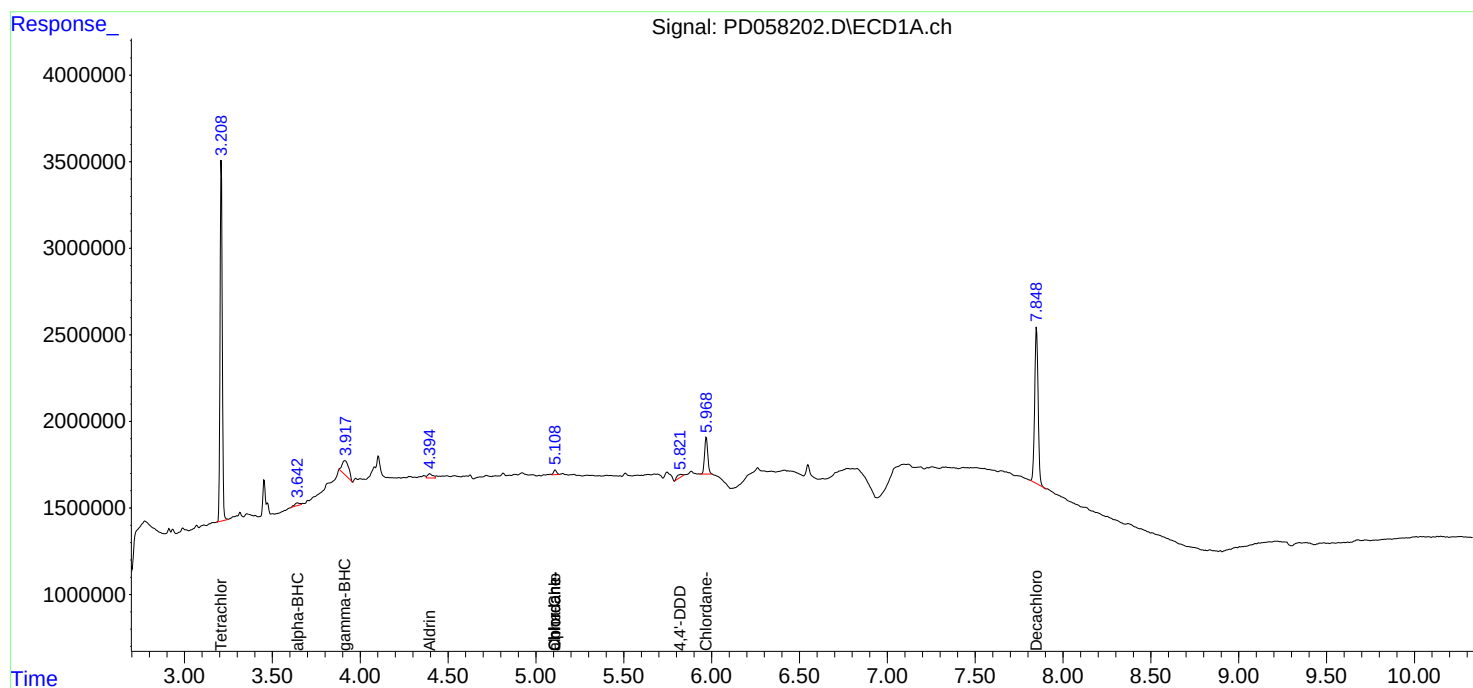


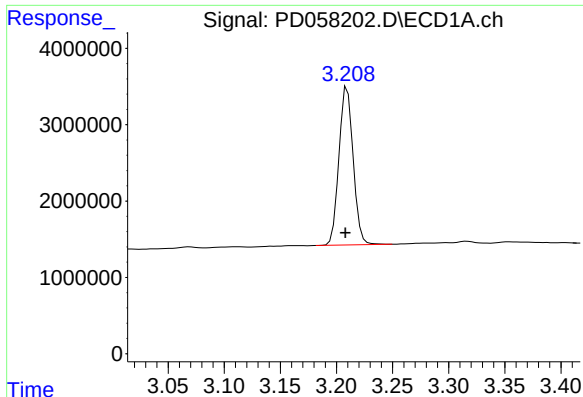

#1 Tetrachloro-m-xylene


R.T.: 3.210 min
Delta R.T.: 0.002 min
Response: 18300128
Conc: 23.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
NM-EB-06

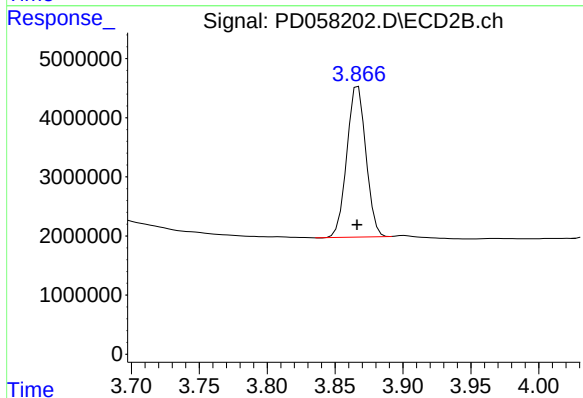


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 24967391
Conc: 21.92 ng/ml

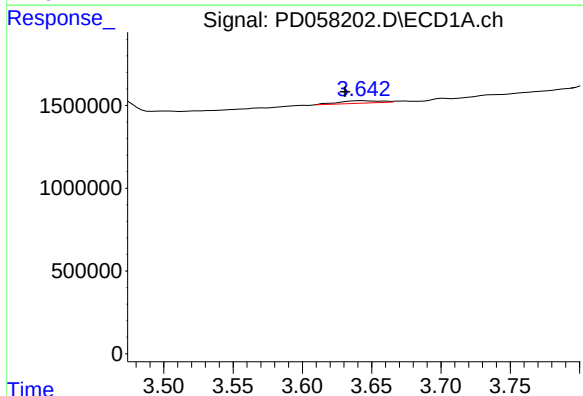


#2 alpha-BHC

R.T.: 3.643 min
Delta R.T.: 0.013 min
Response: 311073
Conc: 0.26 ng/ml

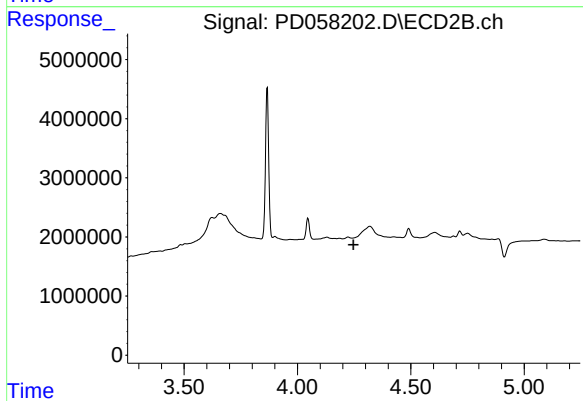

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.247 min
Response: 0
Conc: N.D.

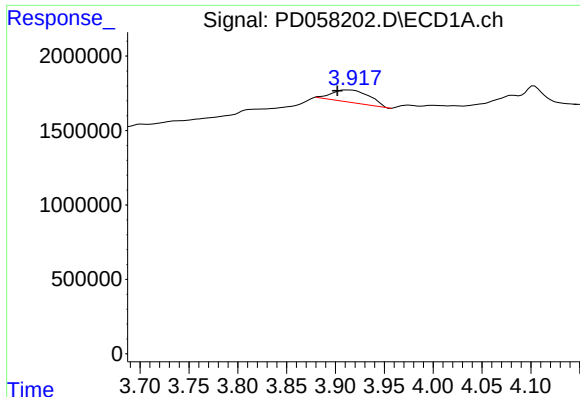

#3 gamma-BHC (Lindane)


R.T.: 3.913 min
Delta R.T.: 0.011 min
Response: 2232254
Conc: 1.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
NM-EB-06

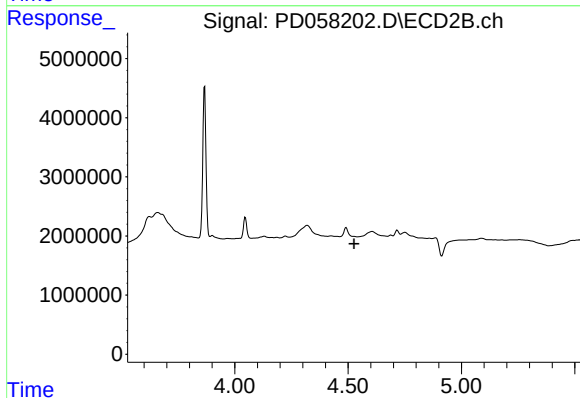


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.527 min
Response: 0
Conc: N.D.

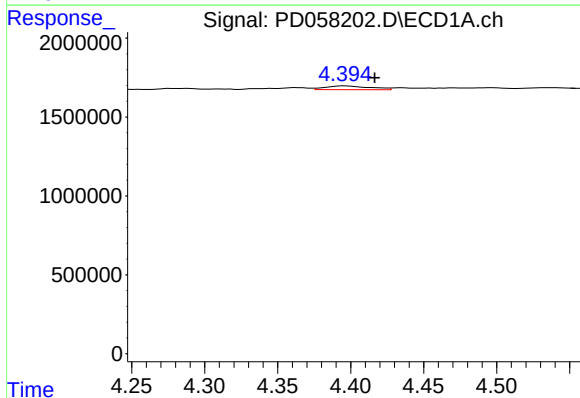


#5 Aldrin

R.T.: 4.396 min
Delta R.T.: -0.021 min
Response: 524704
Conc: 0.50 ng/ml

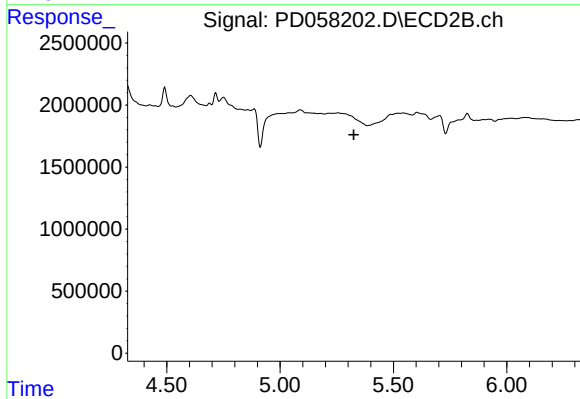

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.325 min
Response: 0
Conc: N.D.

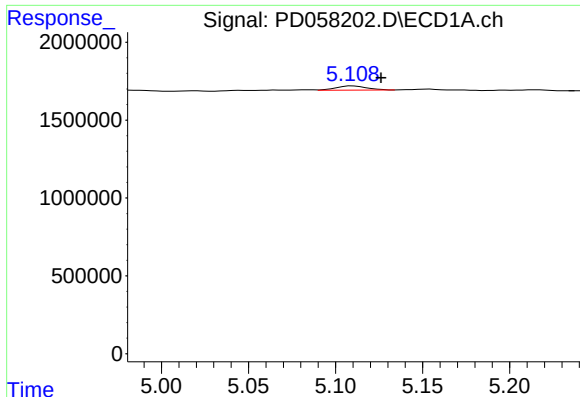

#11 alpha-Chlordane


R.T.: 5.110 min
Delta R.T.: -0.016 min
Response: 332686
Conc: 0.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
NM-EB-06

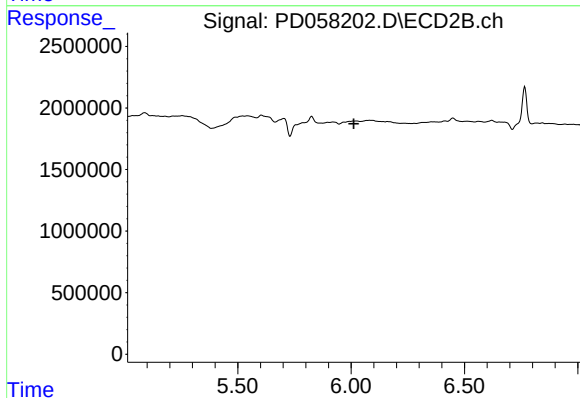


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.012 min
Response: 0
Conc: N.D.

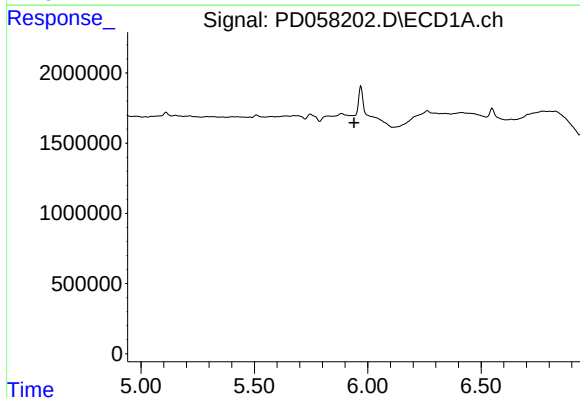


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.939 min
Response: 0
Conc: N.D.

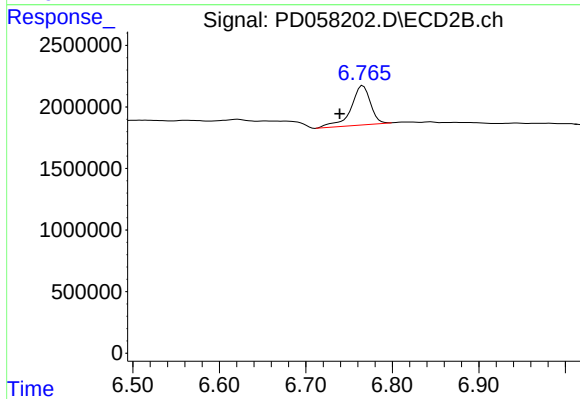

#15 Endosulfan II


R.T.: 6.766 min
Delta R.T.: 0.027 min
Response: 4997276
Conc: 4.16 ng/ml

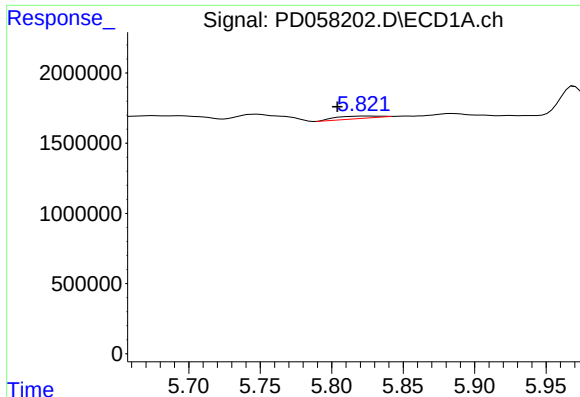

#16 4,4'-DDD


R.T.: 5.824 min
Delta R.T.: 0.020 min
Response: 374857
Conc: 0.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
NM-EB-06

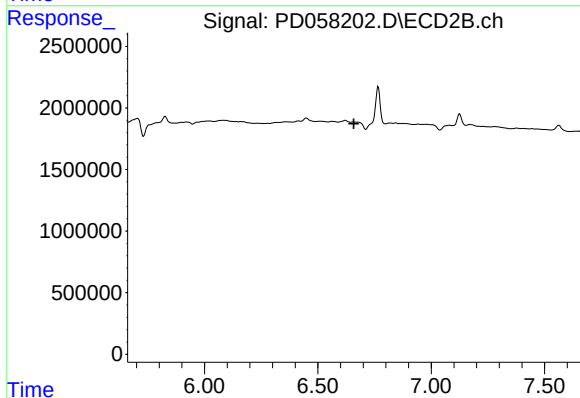


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.658 min
Response: 0
Conc: N.D.

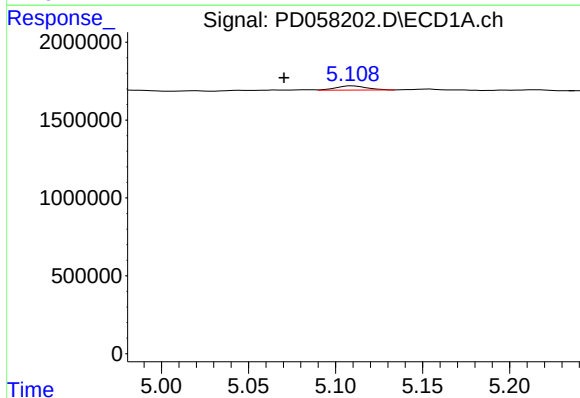


#25 Chlordane-3

R.T.: 5.110 min
Delta R.T.: 0.039 min
Response: 332686
Conc: 3.71 ng/ml

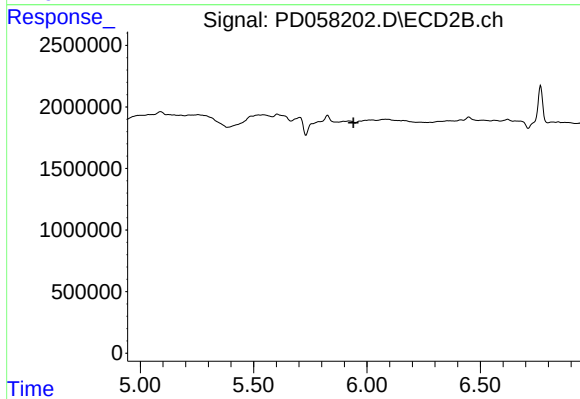

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.941 min
Response: 0
Conc: N.D.

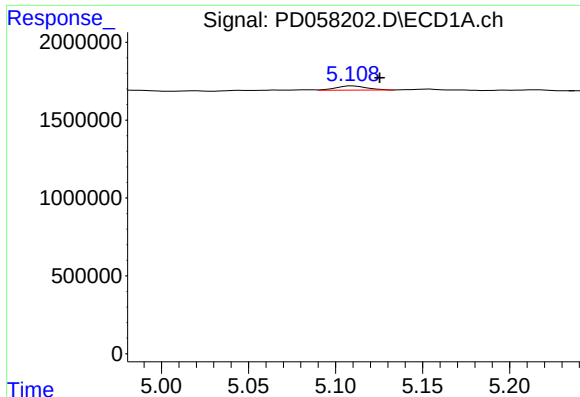

#26 Chlordane-4


R.T.: 5.110 min
Delta R.T.: -0.015 min
Response: 332686
Conc: 3.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
NM-EB-06

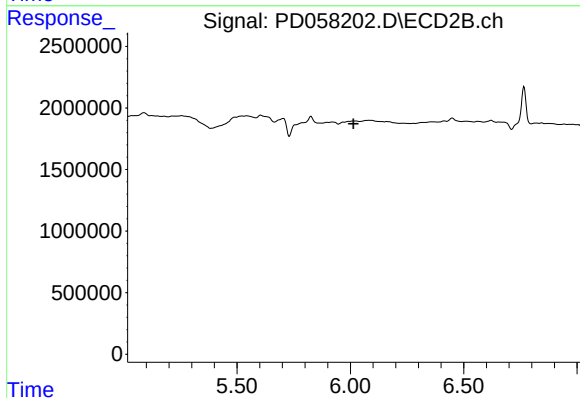


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.015 min
Response: 0
Conc: N.D.

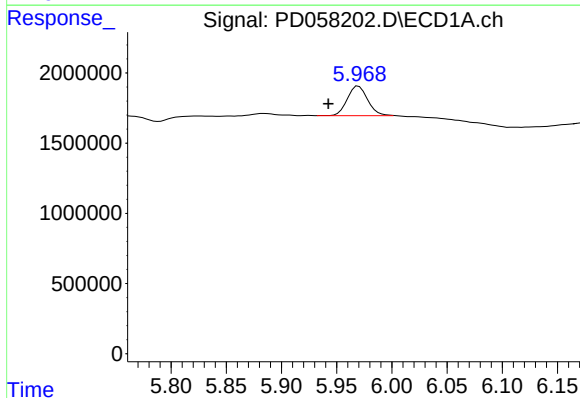


#27 Chlordane-5

R.T.: 5.970 min
Delta R.T.: 0.027 min
Response: 2715235
Conc: 100.52 ng/ml

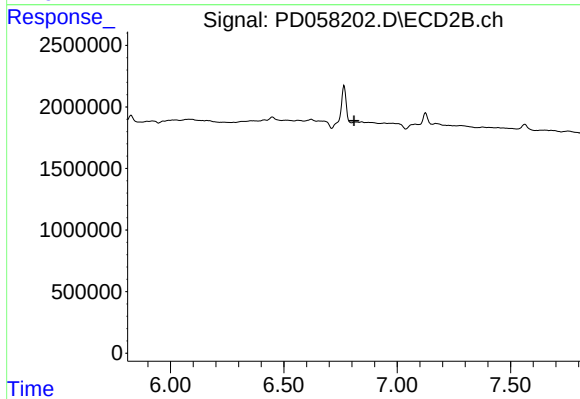

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.810 min
Response: 0
Conc: N.D.

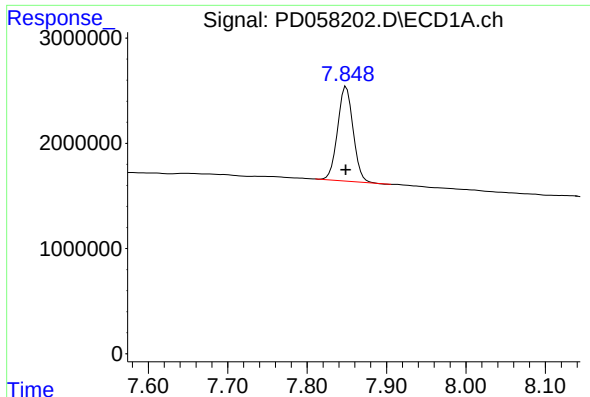

#28 Decachlorobiphenyl

R.T.: 7.849 min
Delta R.T.: 0.000 min
Response: 12250662
Conc: 15.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
NM-EB-06

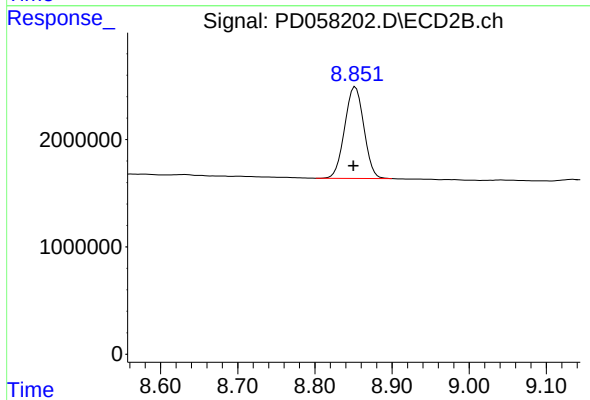

#28 Decachlorobiphenyl

R.T.: 8.852 min
Delta R.T.: 0.003 min
Response: 14702278
Conc: 14.18 ng/ml