

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052820\
 Data File : PD058205.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2020 19:25
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 00:48:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:46:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.867	17989004	24990248	23.018	21.942
28)	SA Decachlor...	7.850	8.852	18735069	22919127	23.431	22.107
Target Compounds							
2)	A alpha-BHC	3.643	0.000	188230	0	0.155	N.D. #
3)	MA gamma-BHC...	3.917f	0.000	1162234	0	0.991	N.D. #
8)	B Heptachlo...	4.873f	0.000	199680	0	0.205	N.D. #
10)	B gamma-Chl...	5.083	0.000	88347	0	0.089	N.D. #
11)	B alpha-Chl...	5.115	0.000	40510	0	0.041	N.D. #
14)	MA Endrin	5.688f	0.000	156603	0	0.196	N.D. #
25)	Chlordane-3	5.083	0.000	88347	0	0.986	N.D. #
26)	Chlordane-4	5.115	0.000	40510	0	0.474	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052820\
Data File : PD058205.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2020 19:25
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 00:48:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:46:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

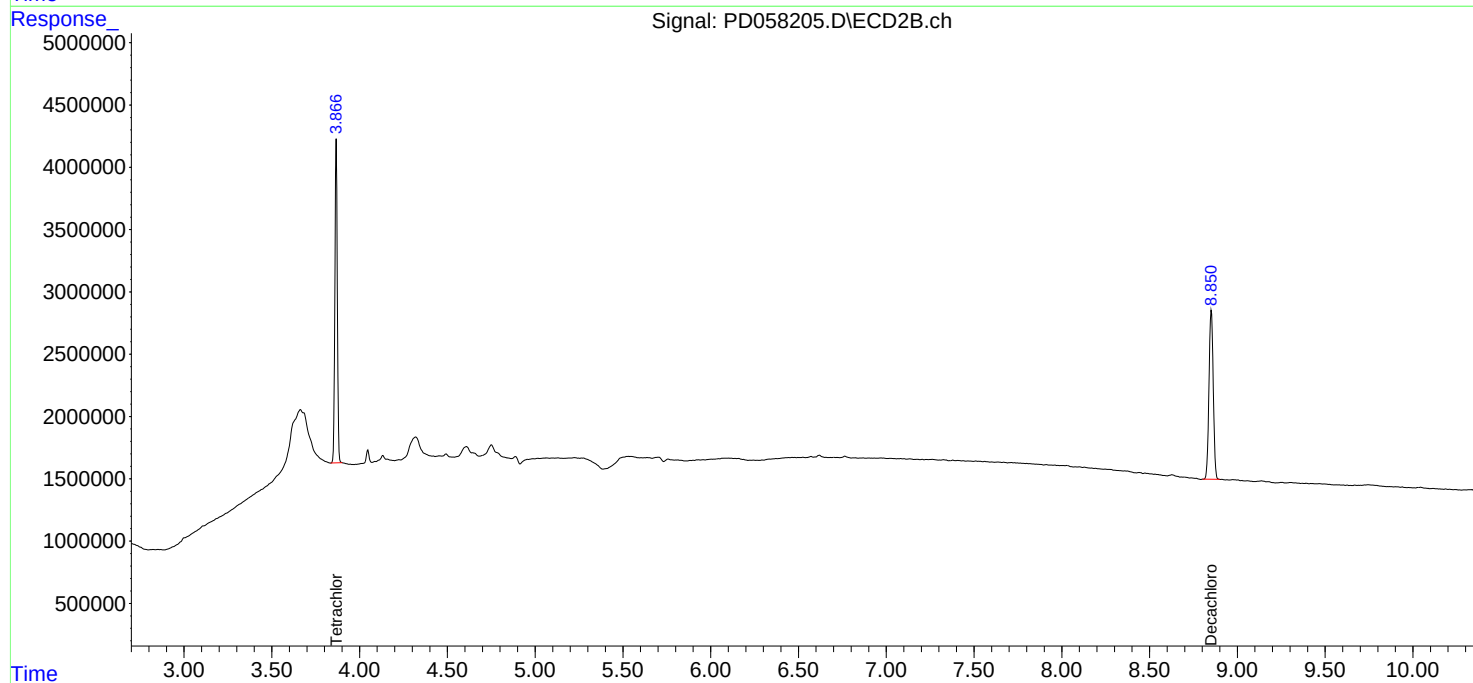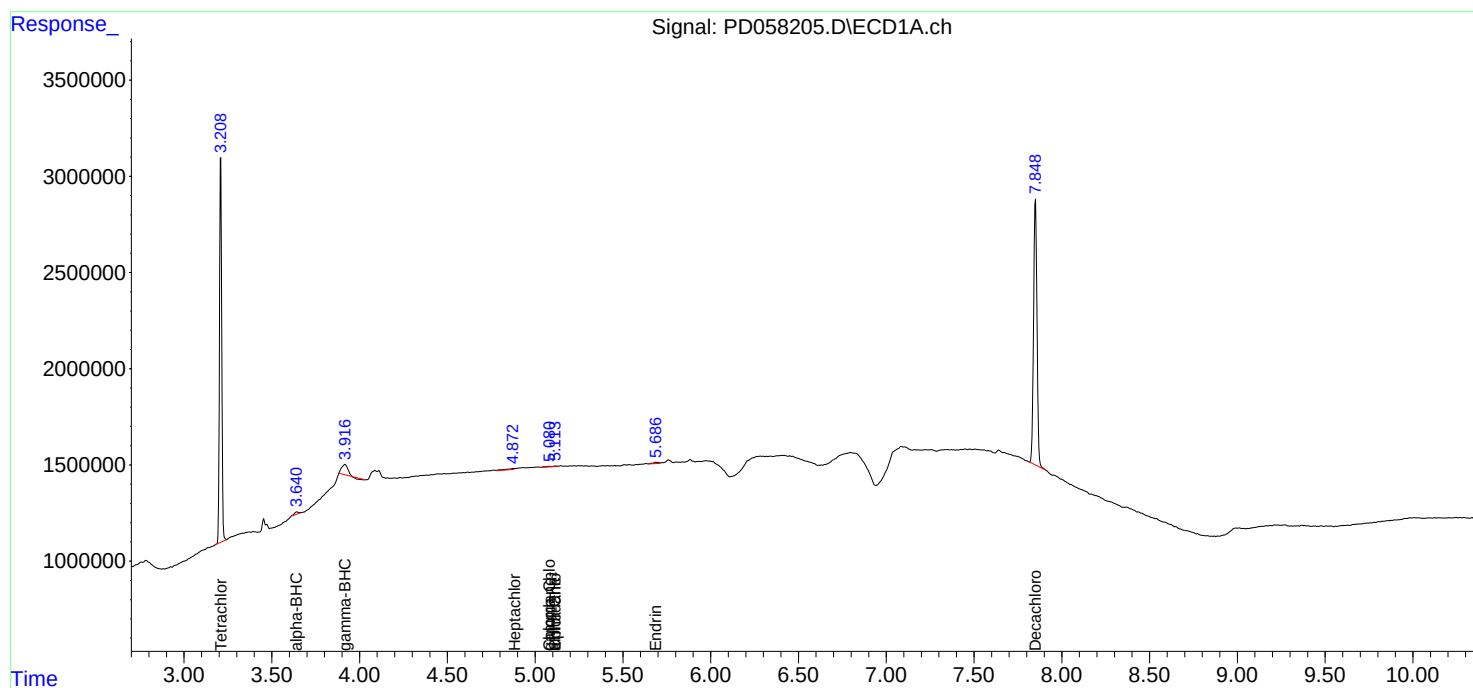


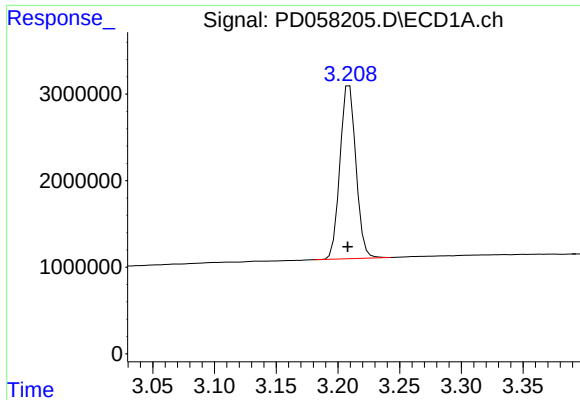

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: 0.001 min
Response: 17989004
Conc: 23.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

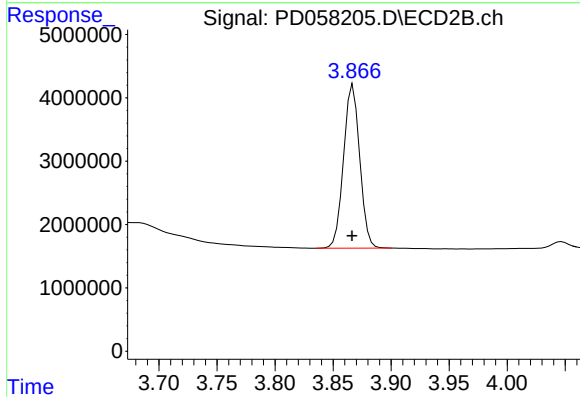


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.001 min
Response: 24990248
Conc: 21.94 ng/ml

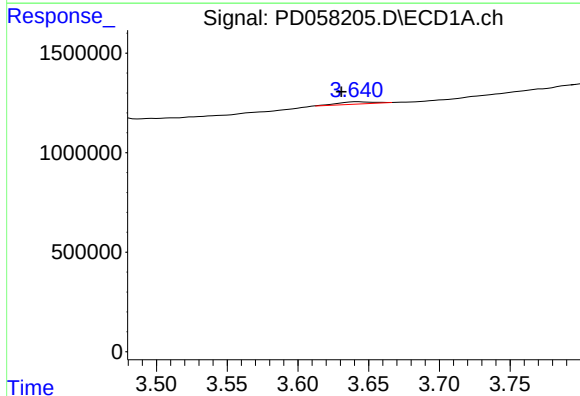


#2 alpha-BHC

R.T.: 3.643 min
Delta R.T.: 0.012 min
Response: 188230
Conc: 0.16 ng/ml

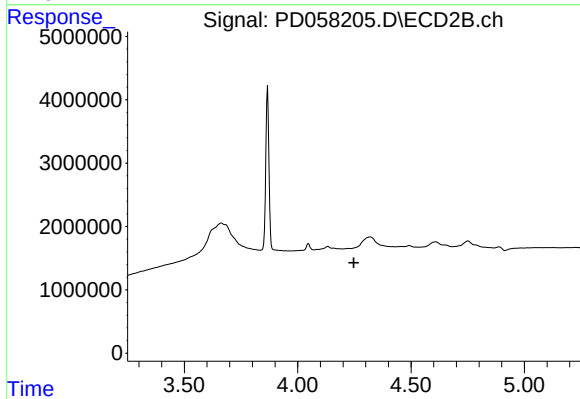

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.247 min
Response: 0
Conc: N.D.

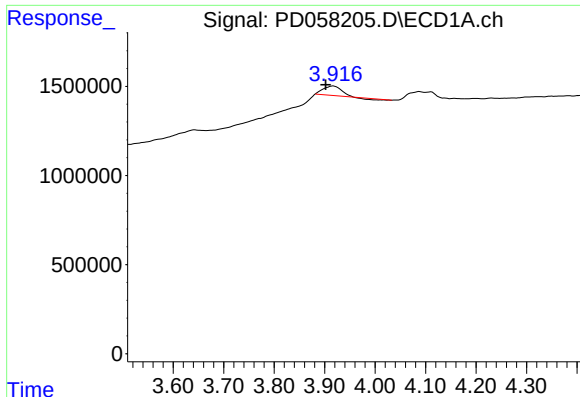

#3 gamma-BHC (Lindane)


R.T.: 3.917 min
Delta R.T.: 0.015 min
Response: 1162234
Conc: 0.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

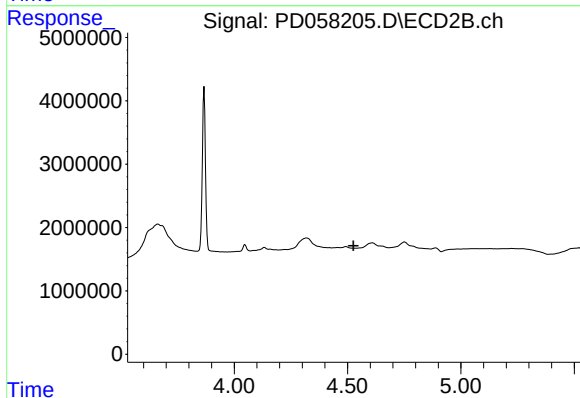


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.527 min
Response: 0
Conc: N.D.

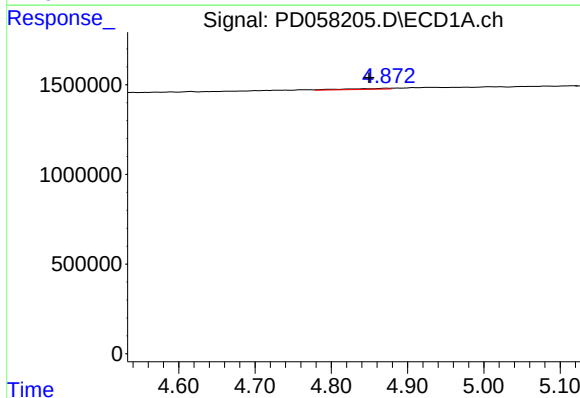


#8 Heptachlor epoxide

R.T.: 4.873 min
Delta R.T.: 0.024 min
Response: 199680
Conc: 0.20 ng/ml

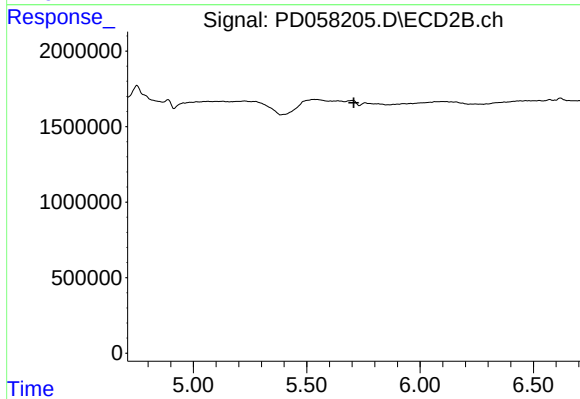

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.708 min
Response: 0
Conc: N.D.

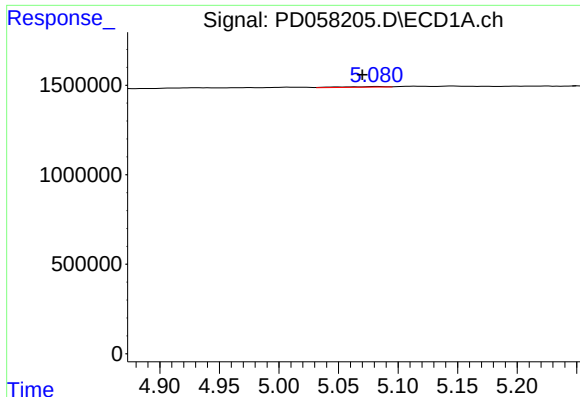

#10 gamma-Chlordane


R.T.: 5.083 min
Delta R.T.: 0.013 min
Response: 88347
Conc: 0.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

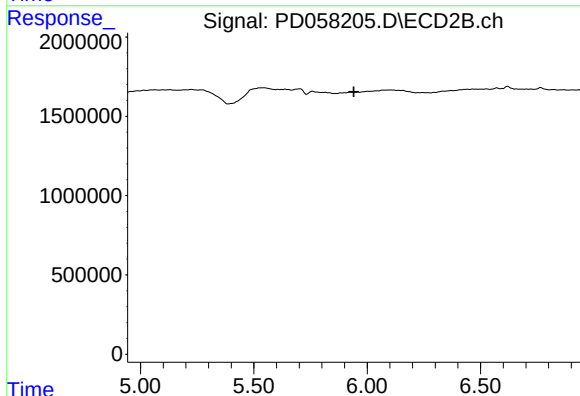


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.940 min
Response: 0
Conc: N.D.

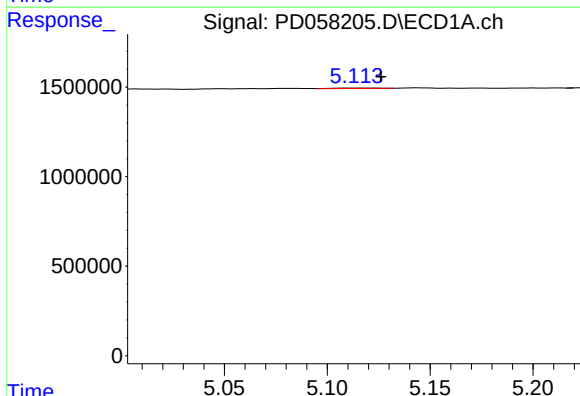


#11 alpha-Chlordane

R.T.: 5.115 min
Delta R.T.: -0.011 min
Response: 40510
Conc: 0.04 ng/ml

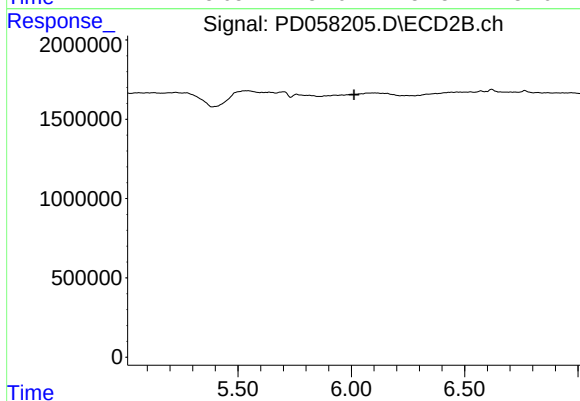

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.012 min
Response: 0
Conc: N.D.

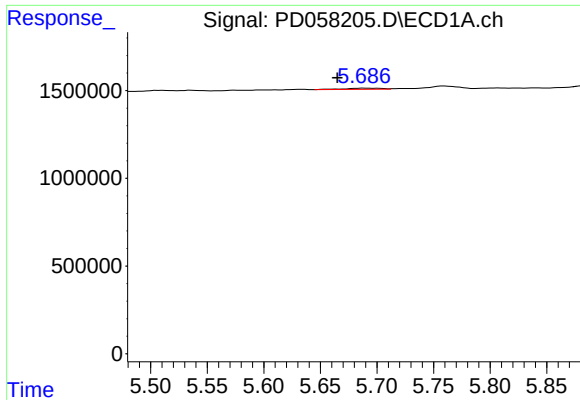

#14 Endrin


R.T.: 5.688 min
Delta R.T.: 0.023 min
Response: 156603
Conc: 0.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

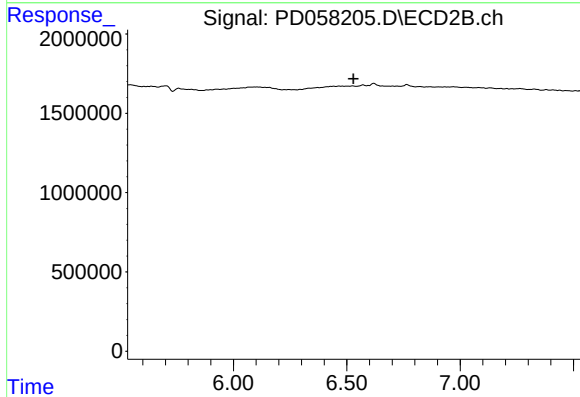


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.530 min
Response: 0
Conc: N.D.

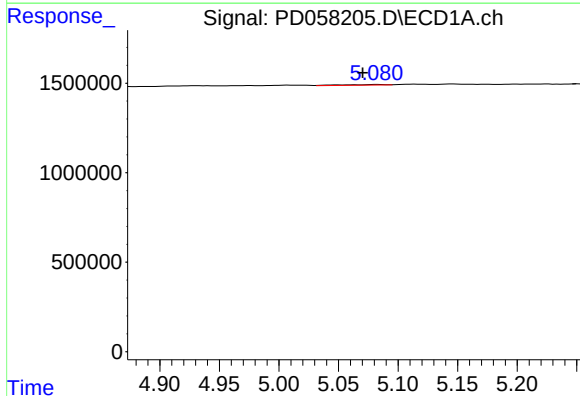


#25 Chlordane-3

R.T.: 5.083 min
Delta R.T.: 0.012 min
Response: 88347
Conc: 0.99 ng/ml

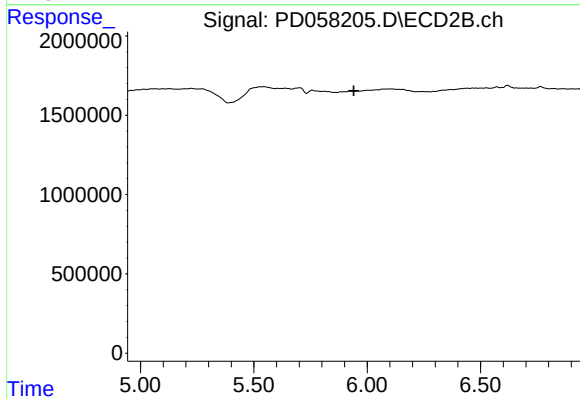

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.941 min
Response: 0
Conc: N.D.

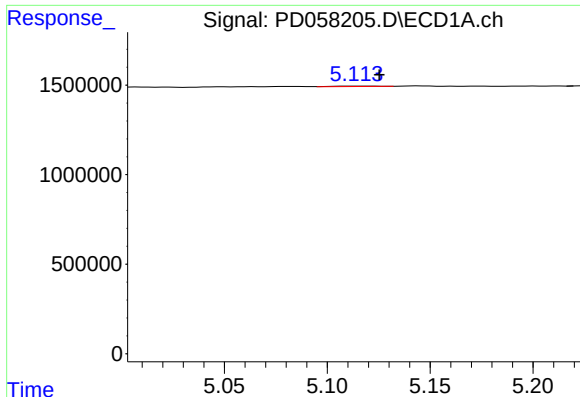

#26 Chlordane-4


R.T.: 5.115 min
Delta R.T.: -0.010 min
Response: 40510
Conc: 0.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

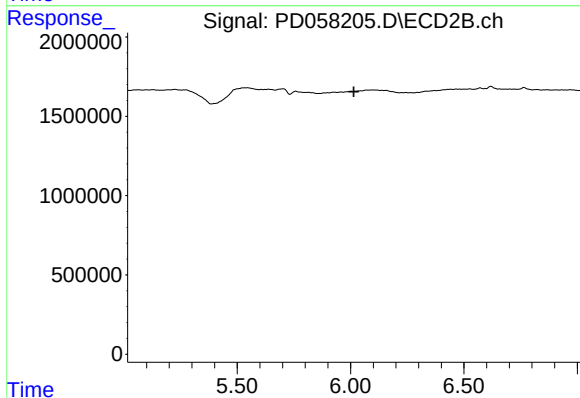


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.015 min
Response: 0
Conc: N.D.

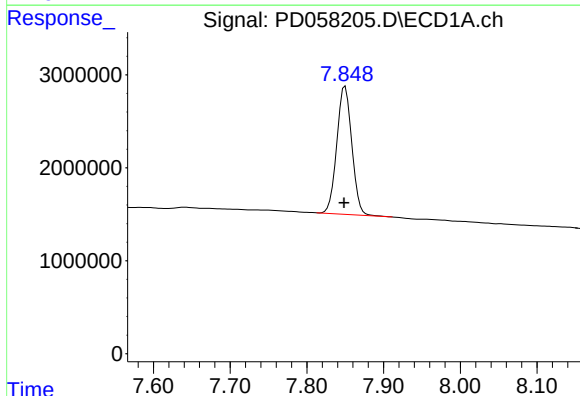

#28 Decachlorobiphenyl

R.T.: 7.850 min
Delta R.T.: 0.001 min
Response: 18735069
Conc: 23.43 ng/ml

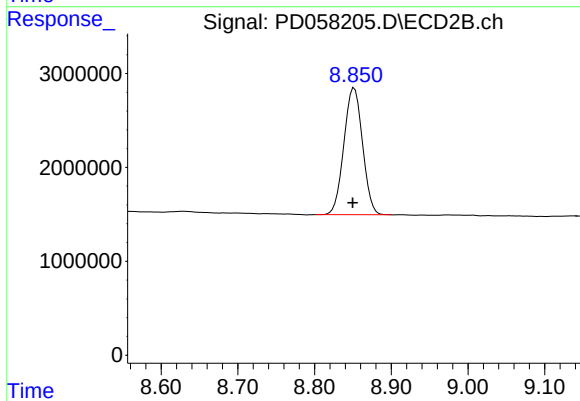

#28 Decachlorobiphenyl

R.T.: 8.852 min
Delta R.T.: 0.002 min
Response: 22919127
Conc: 22.11 ng/ml