

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052820\
 Data File : PD058176.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2020 11:14
 Operator : AJ\MA
 Sample : L2182-07
 Misc : TOX 50 PPB LOD
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 01:17:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 14:47:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.209	3.867	16395087	23026009	21.187	20.513
7) SA Decachlor...	7.850	8.852	17118804	21078936	21.259	20.858
Target Compounds						
2) Toxaphene-1	5.598	6.409	413631	545922	42.118	41.397
3) Toxaphene-2	5.972	6.700	674018	726654	43.362	48.456
4) Toxaphene-3	6.213	6.985	986903	1403963	61.069m	44.544 #
5) Toxaphene-4	6.351	7.071	264207	784669	36.679	40.544
6) Toxaphene-5	6.634	7.482	148483	661107	27.636	43.193 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052820\
Data File : PD058176.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2020 11:14
Operator : AJ\MA
Sample : L2182-07
Misc : TOX 50 PPB LOD
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 01:17:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 14:47:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

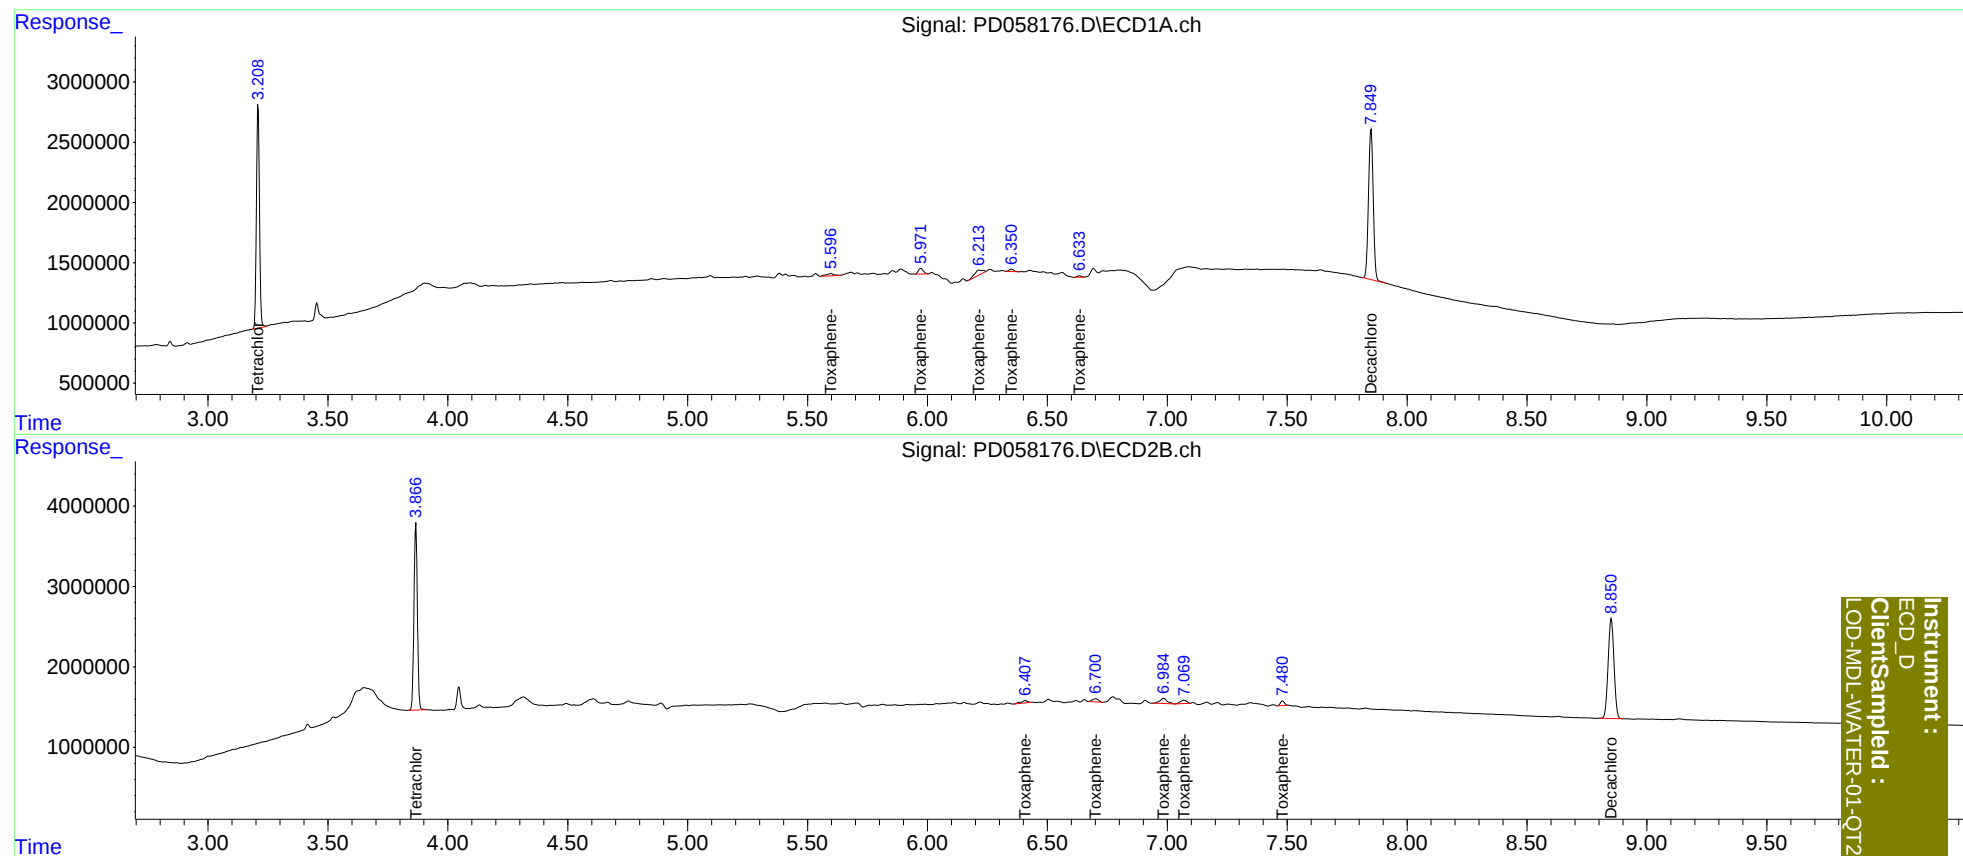

Instrument :
ECD_D
Client Sample :
LOD-MDL-WATER-01-QT2-2020