

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052820\
 Data File : PD058170.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2020 09:50
 Operator : AJ\MA
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 00:42:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:46:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.214	3.866	46114060	57049088	59.005	50.091
28)	SA Decachlor...	7.857	8.853	39432135	46968946	49.316	45.305
Target Compounds							
23)	Chlordane-1	4.043	4.842	14861492	20914384	571.716	528.947
24)	Chlordane-2	4.529	5.304	16448254	23143942	514.498	481.305
25)	Chlordane-3	5.078	5.943	48794547	87519566	544.402	508.975
26)	Chlordane-4	5.134	6.016	44870257	105.4E6	525.176	505.937
27)	Chlordane-5	5.951	6.813	15993032	18561370	592.093	503.476



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052820\
Data File : PD058170.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2020 09:50
Operator : AJ\MA
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 00:42:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:46:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

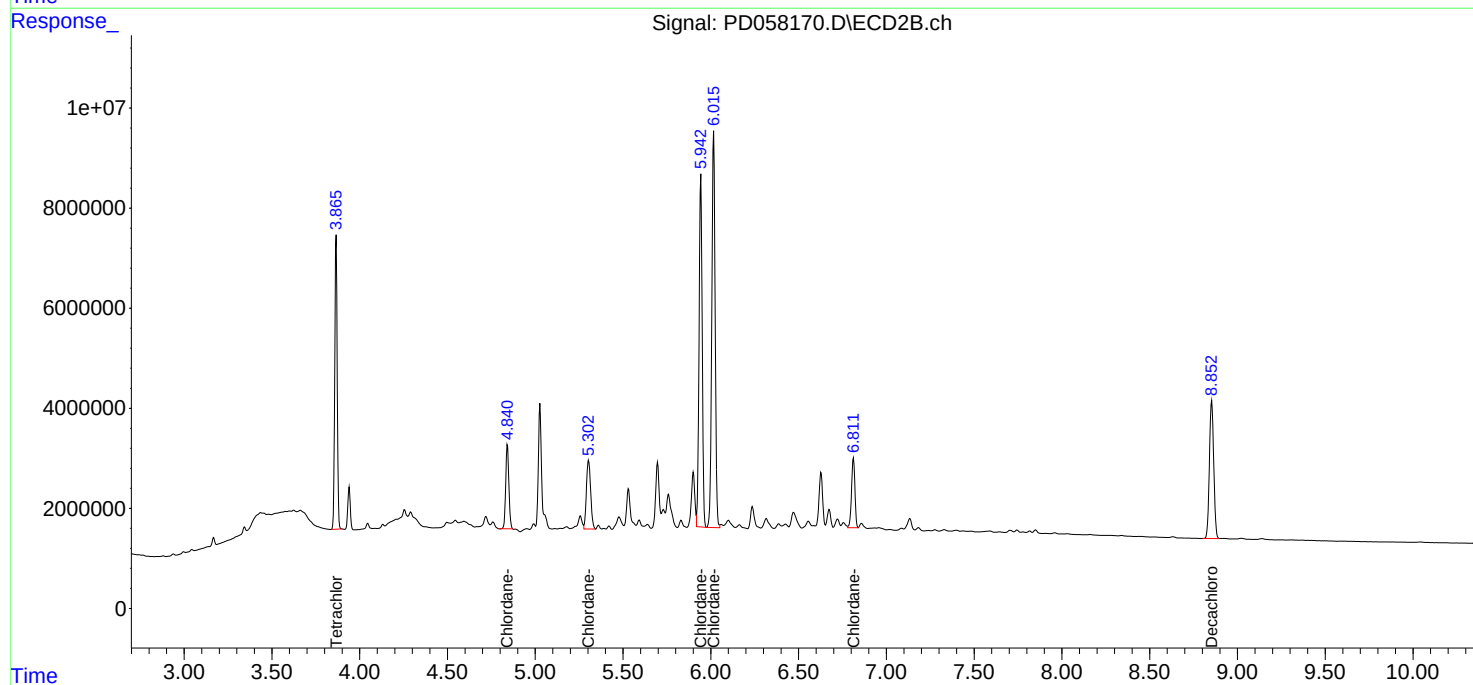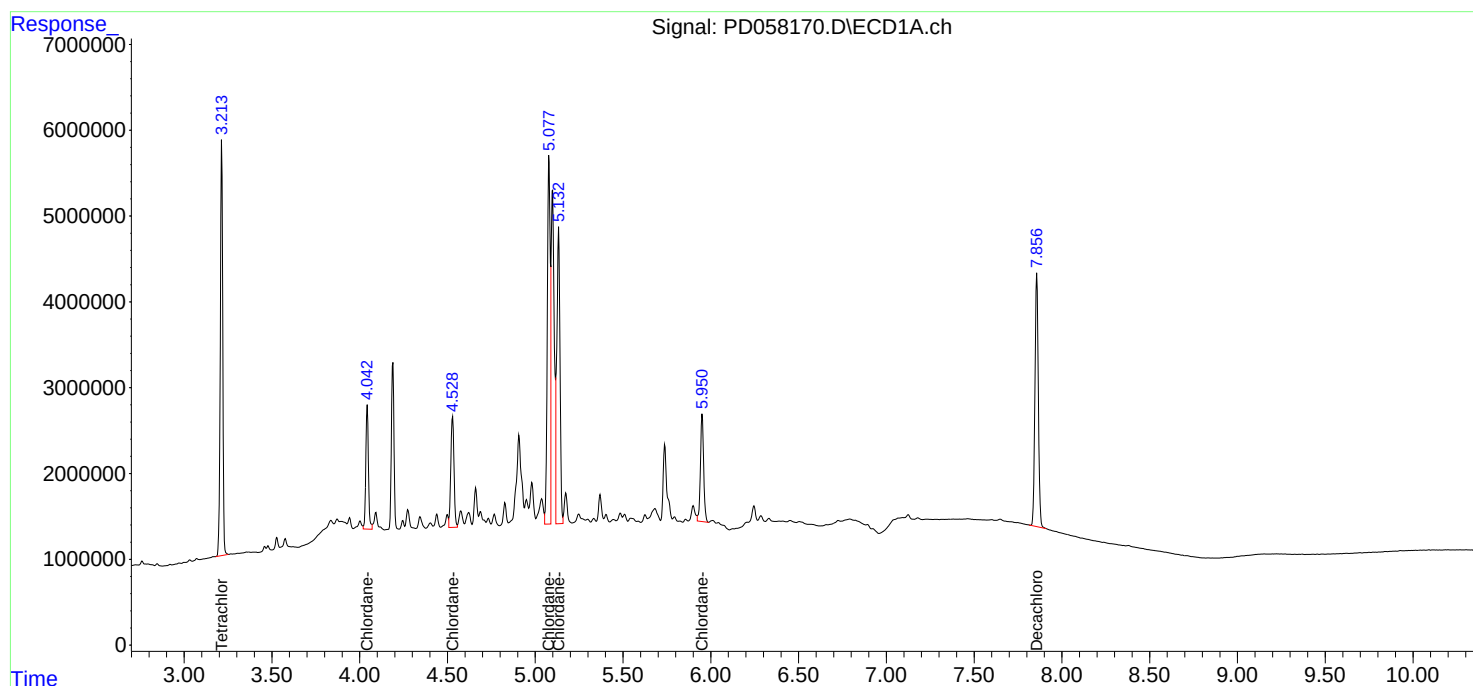


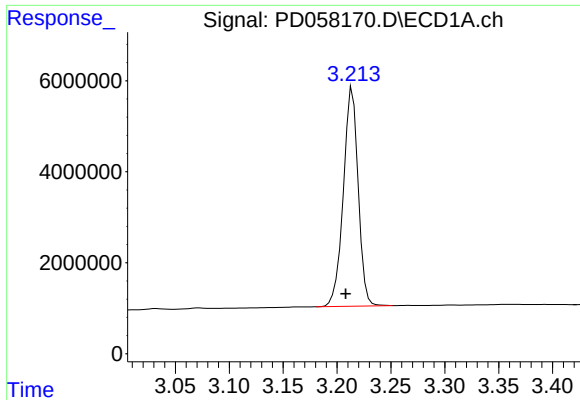

#1 Tetrachloro-m-xylene


R.T.: 3.214 min
Delta R.T.: 0.006 min
Response: 46114060
Conc: 59.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

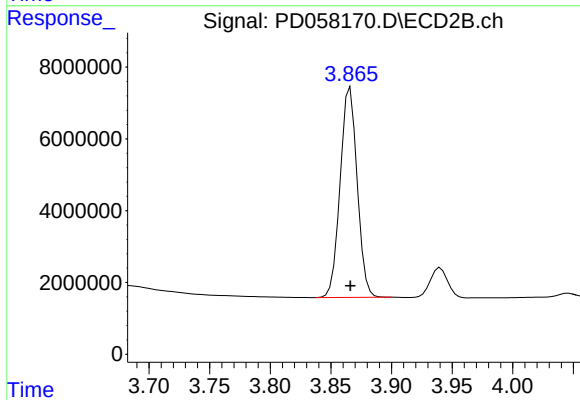


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 57049088
Conc: 50.09 ng/ml

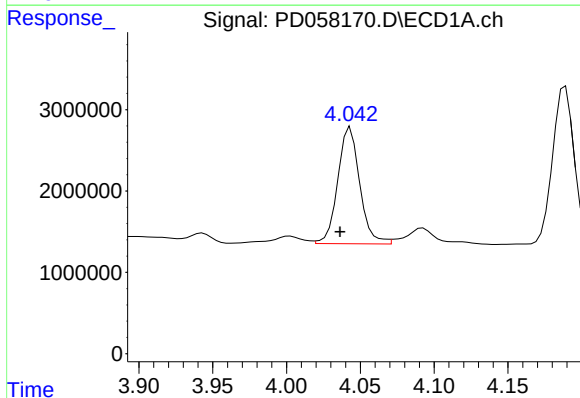


#23 Chlordane-1

R.T.: 4.043 min
Delta R.T.: 0.007 min
Response: 14861492
Conc: 571.72 ng/ml

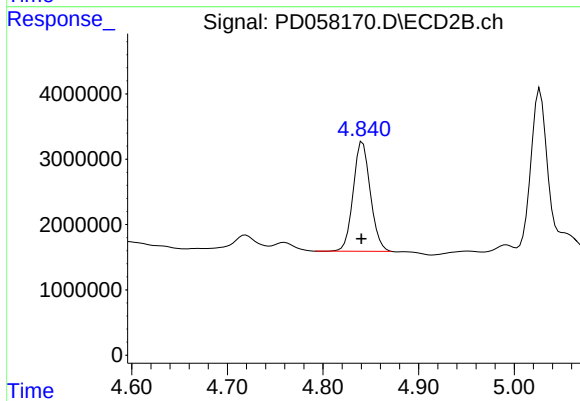

#23 Chlordane-1


R.T.: 4.842 min
Delta R.T.: 0.001 min
Response: 20914384
Conc: 528.95 ng/ml

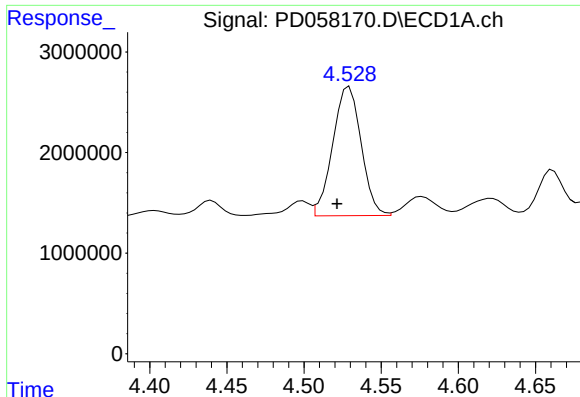

#24 Chlordane-2


R.T.: 4.529 min
Delta R.T.: 0.008 min
Response: 16448254
Conc: 514.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

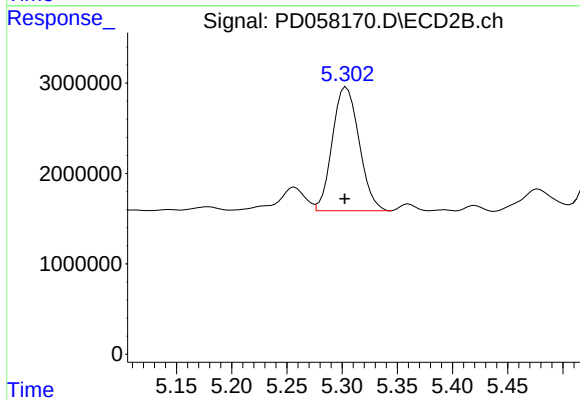


#24 Chlordane-2

R.T.: 5.304 min
Delta R.T.: 0.002 min
Response: 23143942
Conc: 481.31 ng/ml

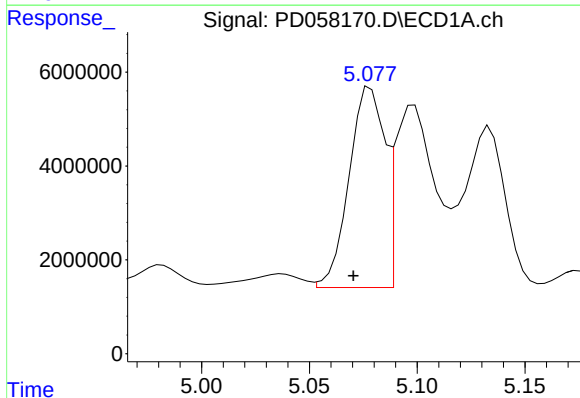


#25 Chlordane-3

R.T.: 5.078 min
Delta R.T.: 0.008 min
Response: 48794547
Conc: 544.40 ng/ml

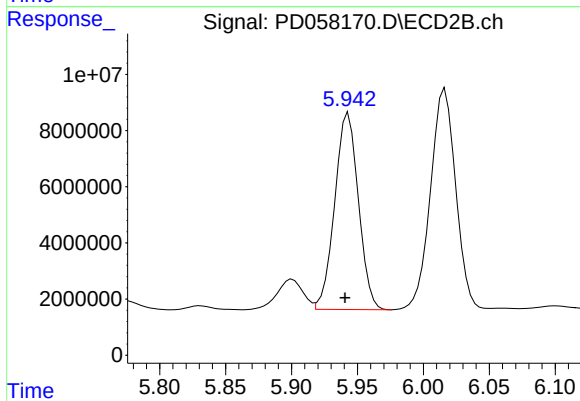

#25 Chlordane-3


R.T.: 5.943 min
Delta R.T.: 0.003 min
Response: 87519566
Conc: 508.97 ng/ml

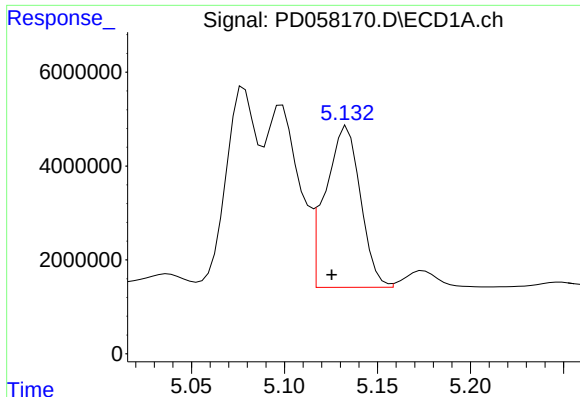

#26 Chlordane-4


R.T.: 5.134 min
Delta R.T.: 0.008 min
Response: 44870257
Conc: 525.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

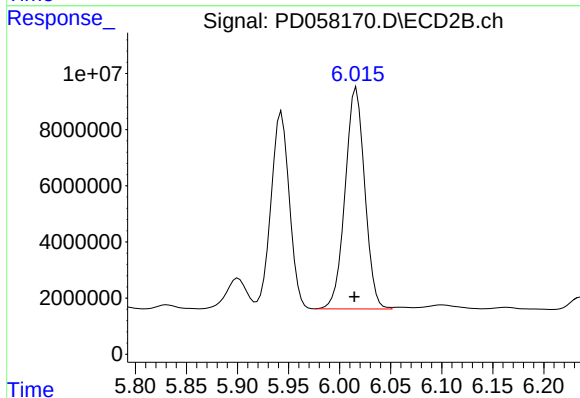


#26 Chlordane-4

R.T.: 6.016 min
Delta R.T.: 0.002 min
Response: 105430792
Conc: 505.94 ng/ml

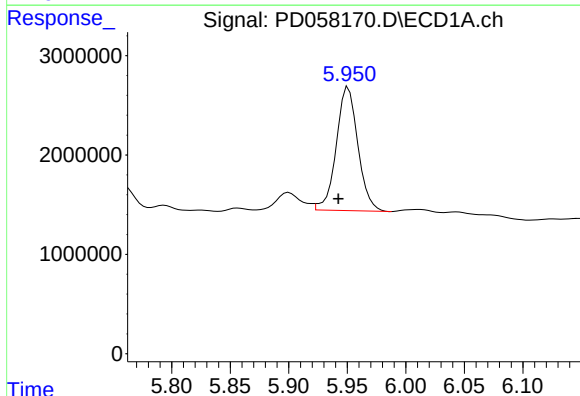


#27 Chlordane-5

R.T.: 5.951 min
Delta R.T.: 0.009 min
Response: 15993032
Conc: 592.09 ng/ml

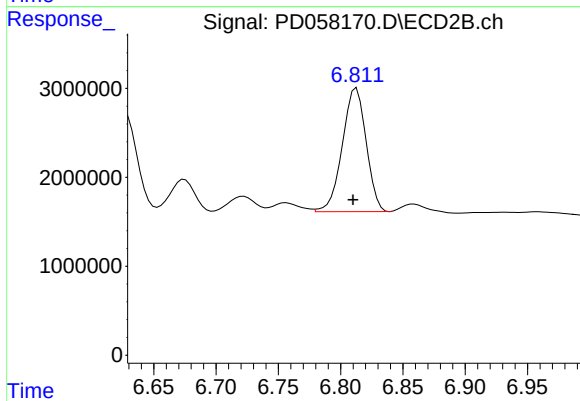

#27 Chlordane-5


R.T.: 6.813 min
Delta R.T.: 0.003 min
Response: 18561370
Conc: 503.48 ng/ml

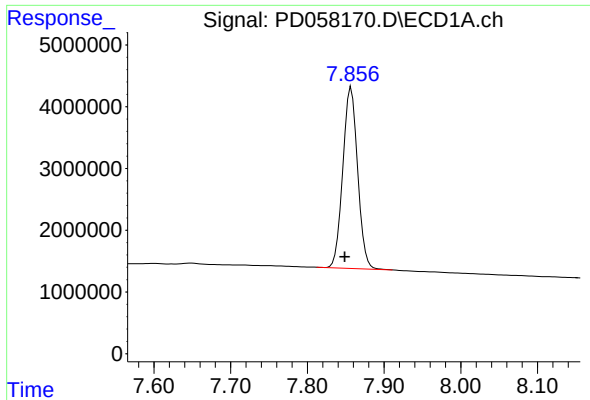

#28 Decachlorobiphenyl

R.T.: 7.857 min
Delta R.T.: 0.008 min
Response: 39432135
Conc: 49.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

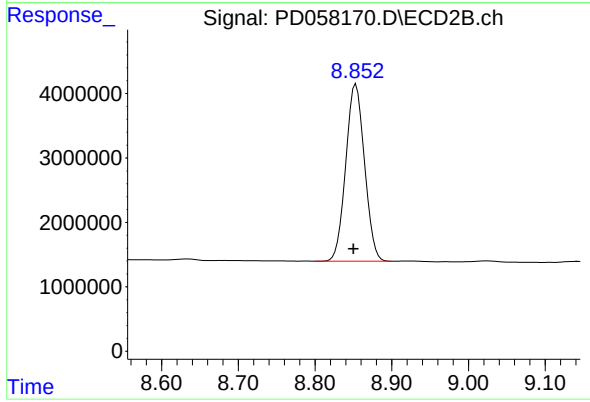

#28 Decachlorobiphenyl

R.T.: 8.853 min
Delta R.T.: 0.003 min
Response: 46968946
Conc: 45.31 ng/ml