

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052824\
 Data File : PD083173.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2024 16:10
 Operator : AR\AJ
 Sample : P2549-13DL 8X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH629DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/29/2024
 Supervised By : Ankita Jodhani 05/30/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 21:29:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.569	2.771	1917953	9257521	1.282m	2.381 #
2) SA Decachlor...	9.114	7.903	9179522	22118410	4.580m	5.590
Target Compounds						
12) B 4,4'-DDE	6.237	5.223	293.4E6	901.0E6	134.544	188.934 #
13) MA Dieldrin	6.410	5.361	5551188	43208645	2.526m	8.647m#
16) A 4,4'-DDD	6.743	5.777	10547373	15956585	6.801	4.241m#
17) MA 4,4'-DDT	7.069	6.027	233.2E6	606.7E6	145.000m	158.013

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052824\
Data File : PD083173.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2024 16:10
Operator : AR\AJ
Sample : P2549-13DL 8X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 21:29:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

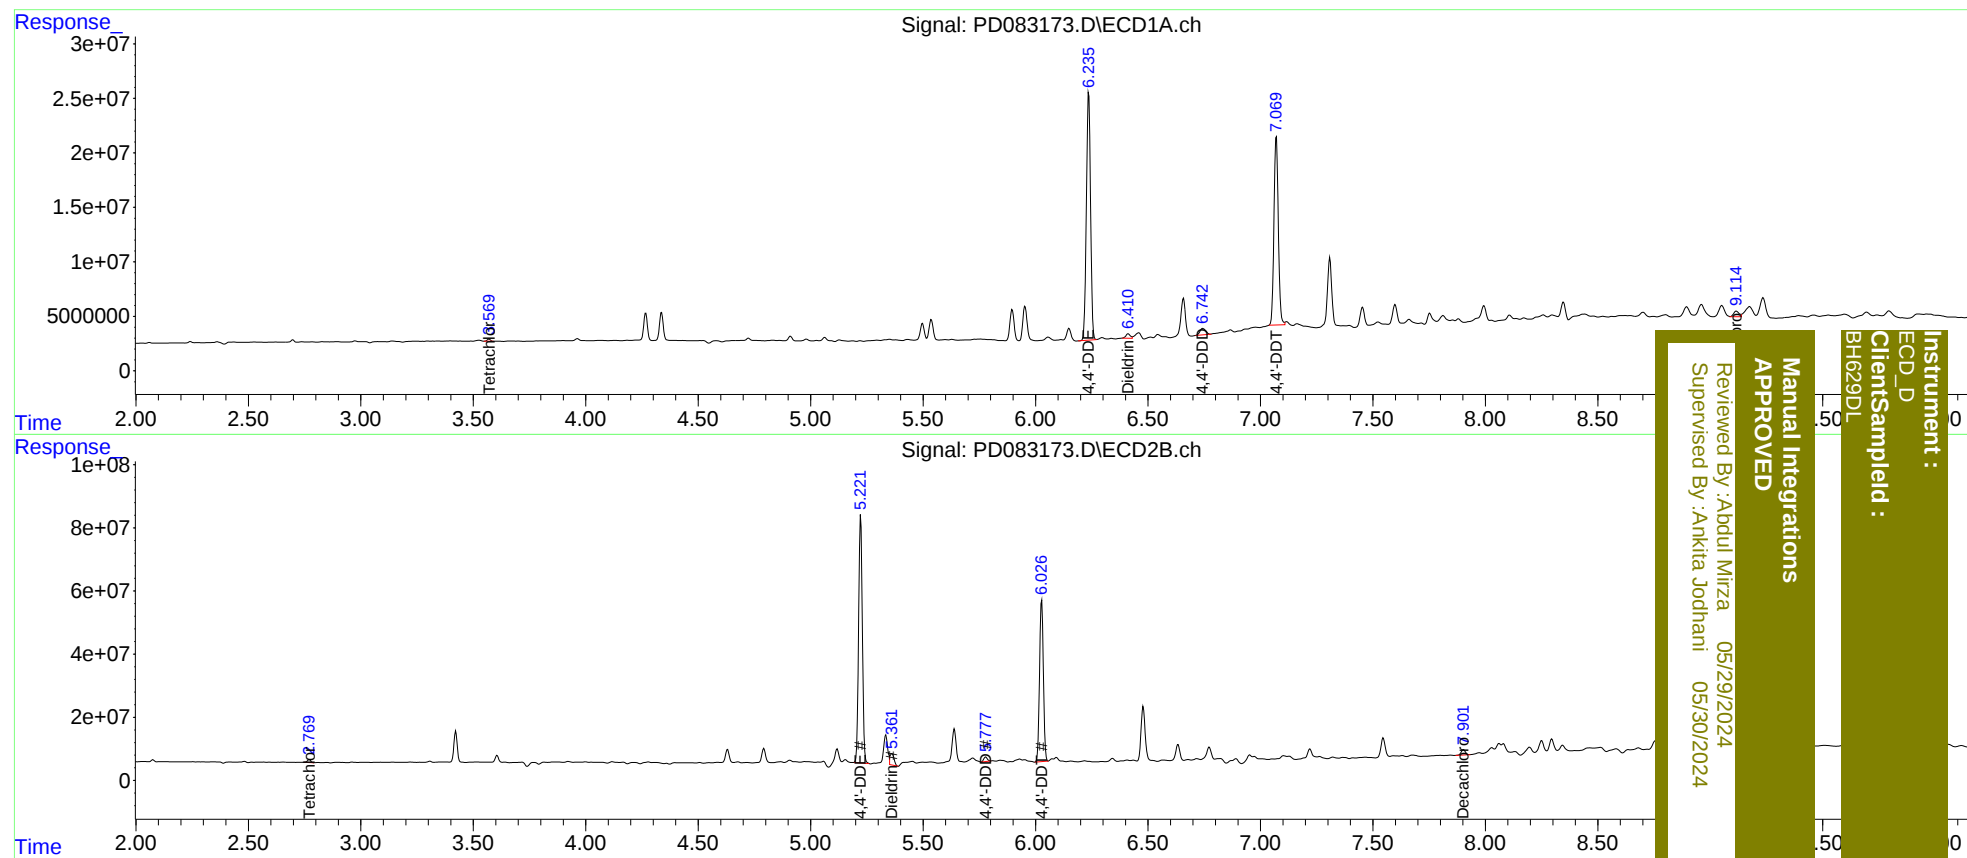

Reviewed By: Abdul Mirza 05/29/2024
Supervised By: Ankita Jodhani 05/30/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
BH629DL