

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052824\
 Data File : PD083192.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2024 00:53
 Operator : AR\AJ
 Sample : P2571-07
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH661

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/03/2024
 Supervised By :Ankita Jodhani 06/03/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 10:32:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.773	18972155	55967040	12.684	14.392
2)	SA Decachlor...	9.119	7.902	20236381	49450780	10.096	12.499
Target Compounds							
9)	A Endosulfan I	6.140	5.117	1066521	2047057	0.513m	0.454m
12)	B 4,4'-DDE	6.224	5.222	697243	2983353	0.320m	0.626 #
17)	MA 4,4'-DDT	7.061	6.026	801879	2802295	0.499m	0.730 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052824\
Data File : PD083192.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2024 00:53
Operator : AR\AJ
Sample : P2571-07
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 10:32:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

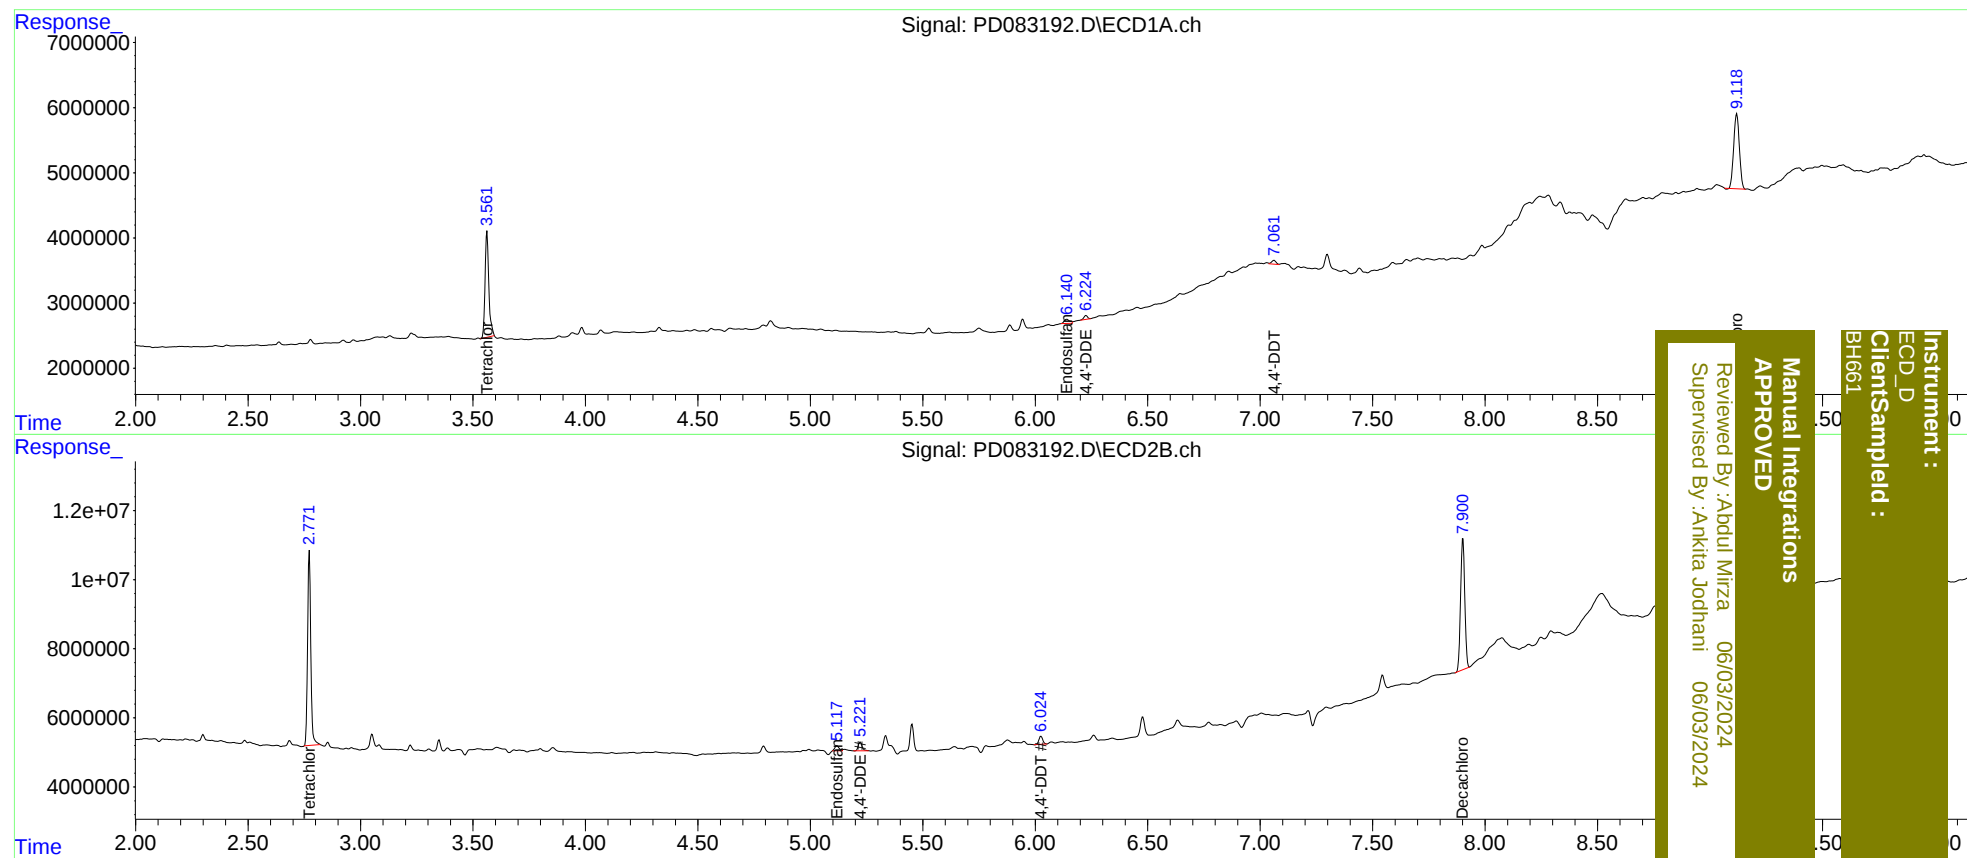

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 06/03/2024
Supervised By: Ankita Jodhani 06/03/2024

Instrument :
ECD_D
ClientSampled :
BH661