

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052919\
 Data File : PD053395.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 May 2019 11:22
 Operator : SM\AJ
 Sample : PB120098BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK98

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 02:08:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052119CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed May 22 06:53:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.317	3.986	17241344	26326219	23.531	26.739
2)	SA Decachlor...	8.016	9.032	26488285	42141514	40.042	40.797
Target Compounds							
13)	MA Dieldrin	0.000	6.502f	0	165528	N.D.	0.131


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052919\
Data File : PD053395.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 May 2019 11:22
Operator : SM\AJ
Sample : PB120098BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 02:08:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052119CLP.M
Quant Title : GC Extractables
QLast Update : Wed May 22 06:53:42 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

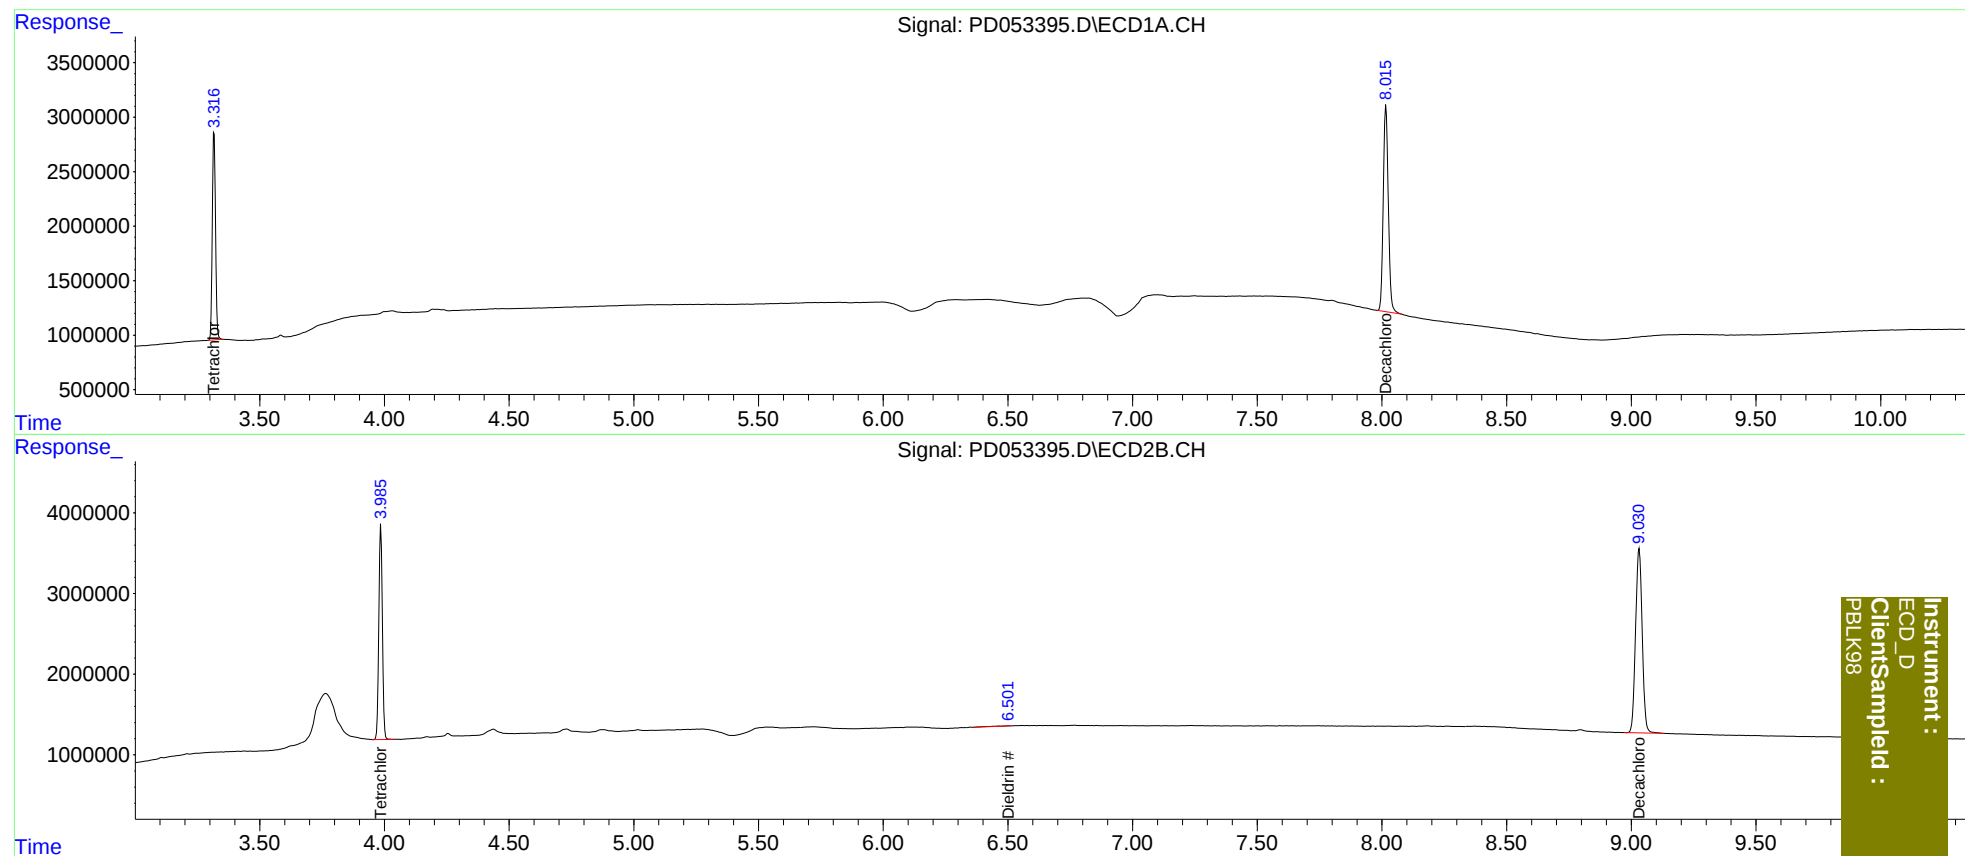


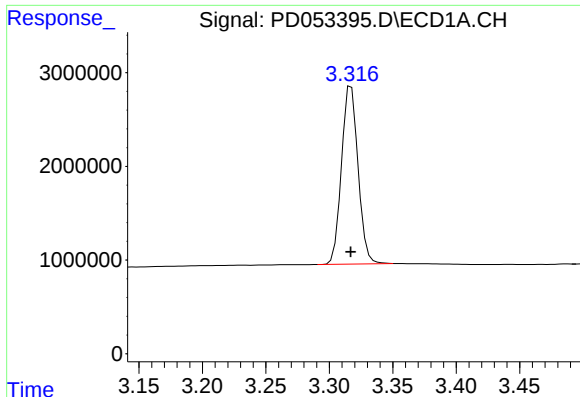

#1 Tetrachloro-m-xylene


R.T.: 3.317 min
Delta R.T.: 0.000 min
Response: 17241344
Conc: 23.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK98

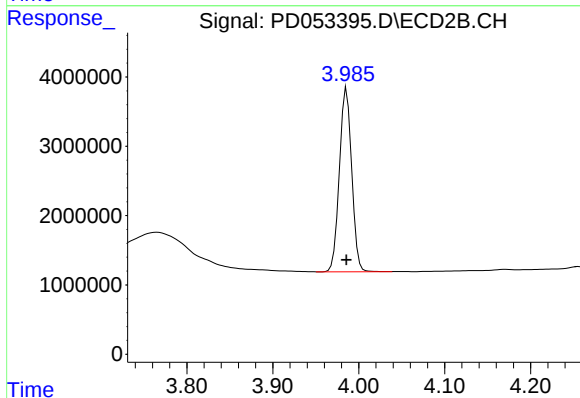


#1 Tetrachloro-m-xylene

R.T.: 3.986 min
Delta R.T.: 0.000 min
Response: 26326219
Conc: 26.74 ng/ml

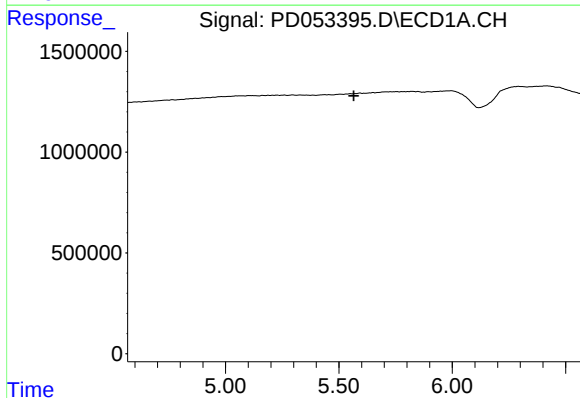


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.565 min
Response: 0
Conc: N.D.

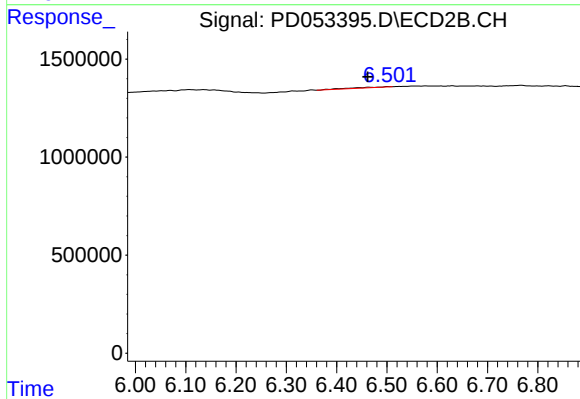

#13 Dieldrin


R.T.: 6.502 min
Delta R.T.: 0.040 min
Response: 165528
Conc: 0.13 ng/ml

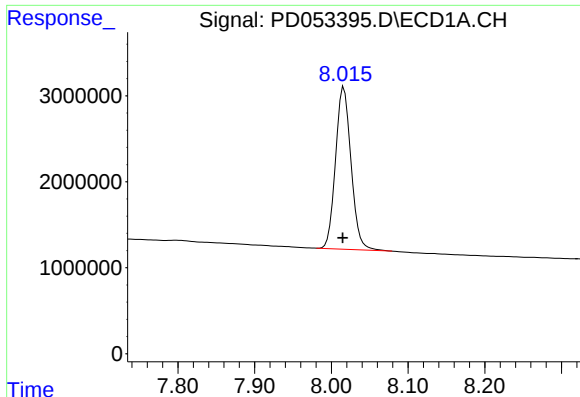

#27 Decachlorobiphenyl

R.T.: 8.016 min
Delta R.T.: 0.001 min
Response: 26488285
Conc: 40.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK98

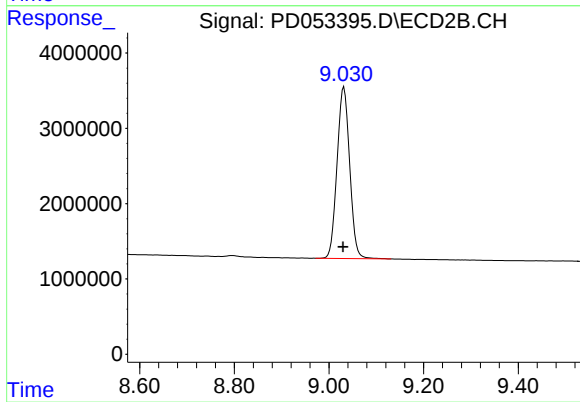

#27 Decachlorobiphenyl

R.T.: 9.032 min
Delta R.T.: 0.002 min
Response: 42141514
Conc: 40.80 ng/ml