

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052920\
 Data File : PD058207.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2020 07:58
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 14:05:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:46:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.866	18188487	26248042	23.273	23.047
28)	SA Decachlor...	7.851	8.852	18613253	23327657	23.279	22.501
Target Compounds							
3)	MA gamma-BHC...	3.924f	0.000	758442	0	0.647	N.D. #
4)	MA Heptachlor	4.192	0.000	35290	0	0.033	N.D. #
5)	MB Aldrin	4.405	0.000	231466	0	0.221	N.D. #
7)	B delta-BHC	4.343	0.000	180618	0	0.158	N.D. #
8)	B Heptachlo...	4.826f	0.000	479522	0	0.491	N.D. #
9)	A Endosulfan I	5.173	0.000	583665	0	0.640	N.D. #
10)	B gamma-Chl...	5.069	0.000	729218	0	0.734	N.D. #
14)	MA Endrin	5.689f	0.000	95704	0	0.120	N.D. #
24)	Chlordane-2	4.501f	0.000	239126	0	7.480	N.D. #
25)	Chlordane-3	5.069	0.000	729218	0	8.136	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052920\
Data File : PD058207.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2020 07:58
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 14:05:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:46:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

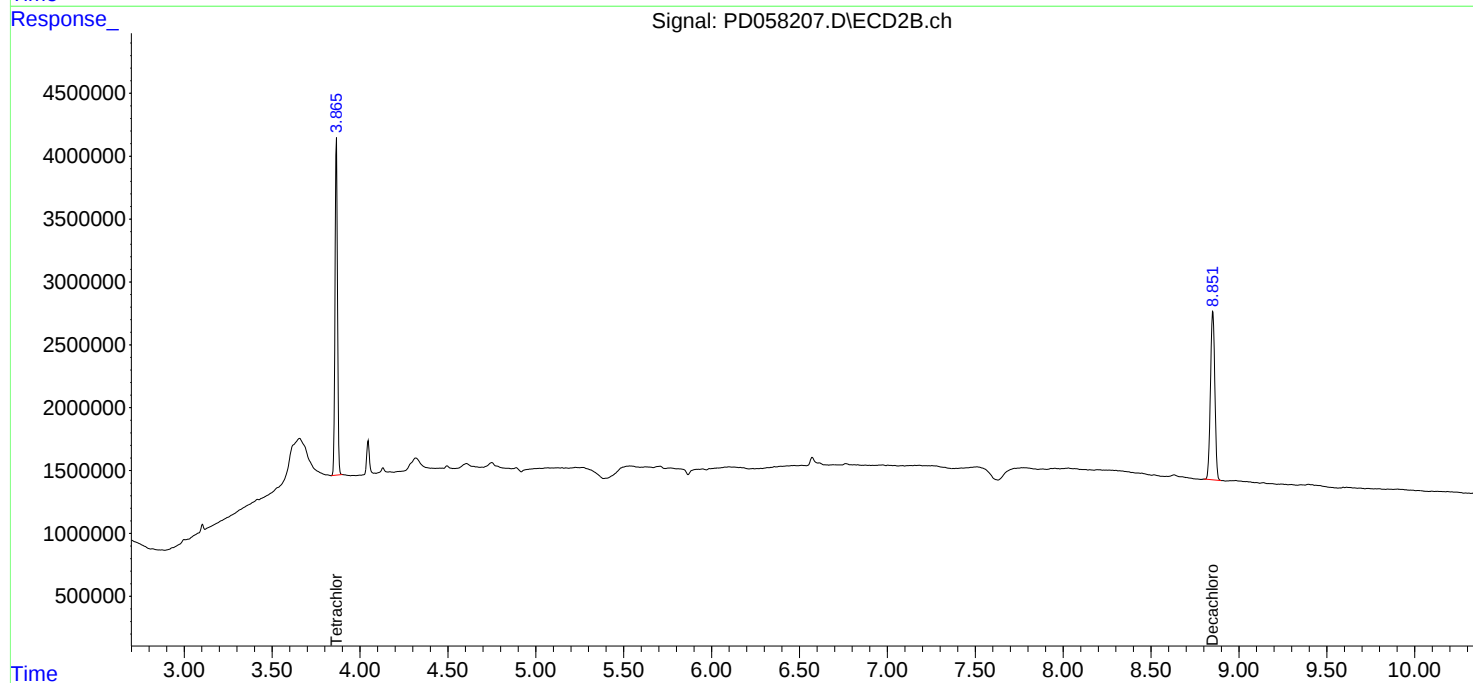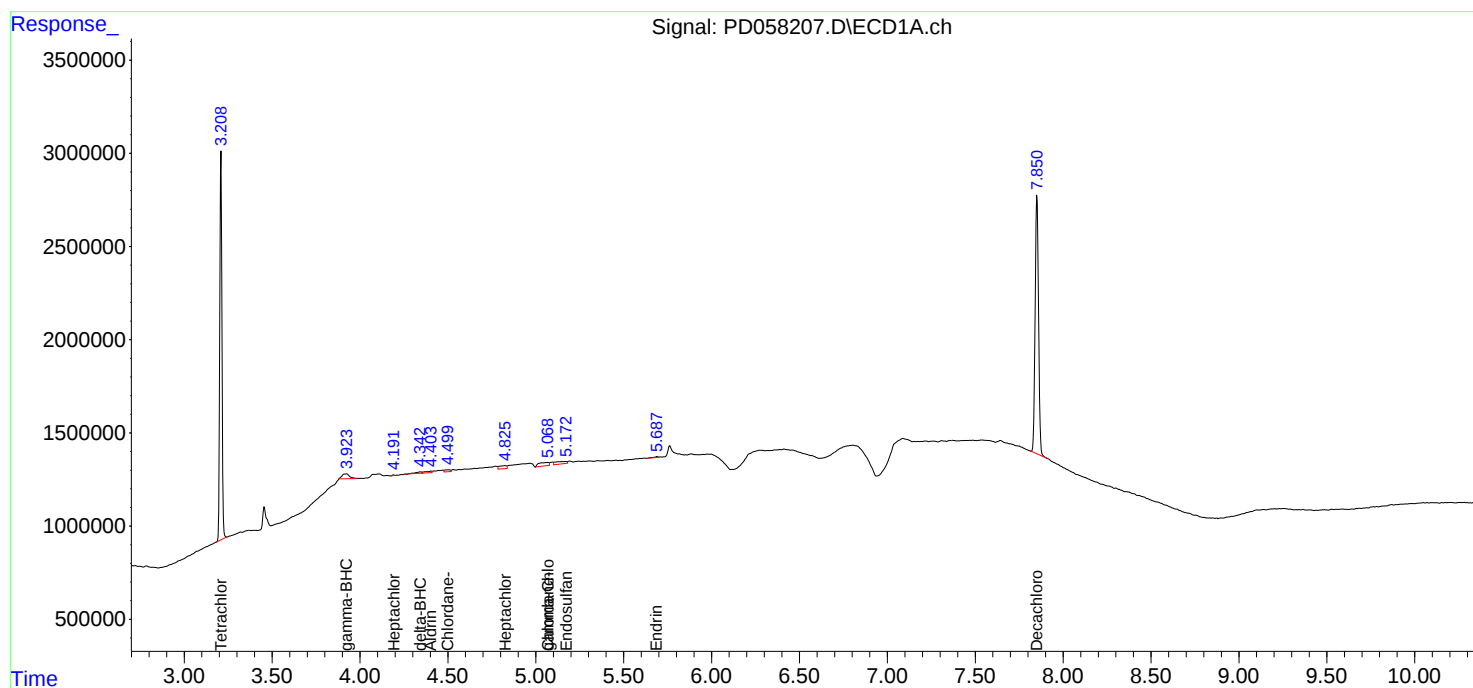


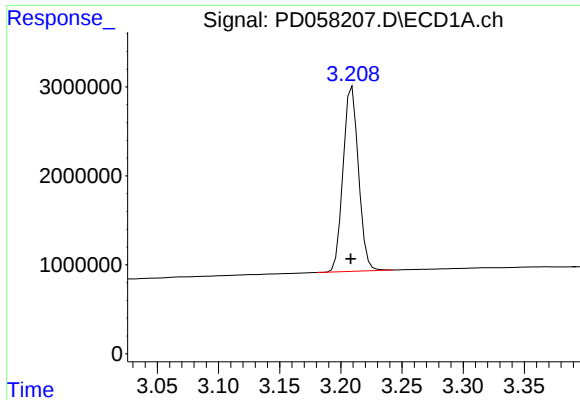

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: 0.001 min
Response: 18188487
Conc: 23.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

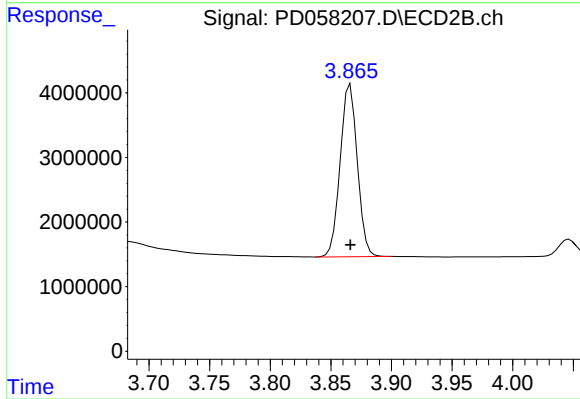


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 26248042
Conc: 23.05 ng/ml

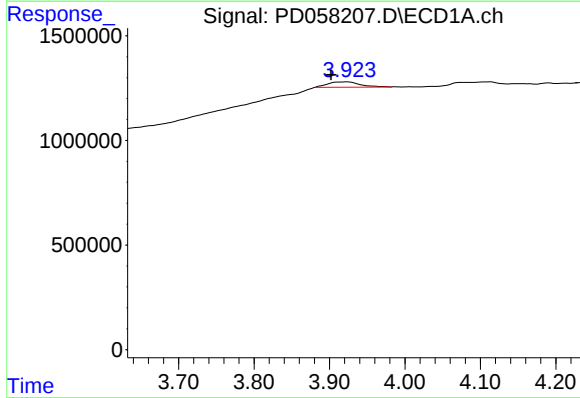


#3 gamma-BHC (Lindane)

R.T.: 3.924 min
Delta R.T.: 0.022 min
Response: 758442
Conc: 0.65 ng/ml

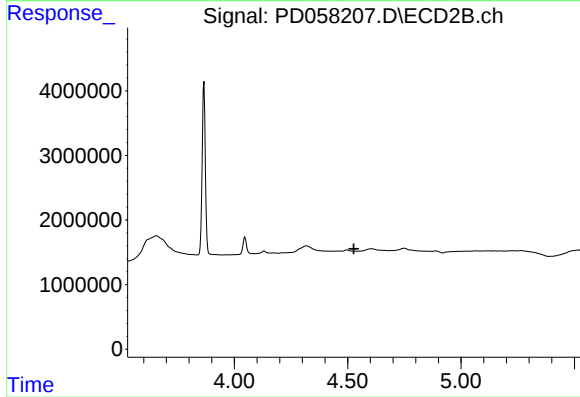

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.527 min
Response: 0
Conc: N.D.

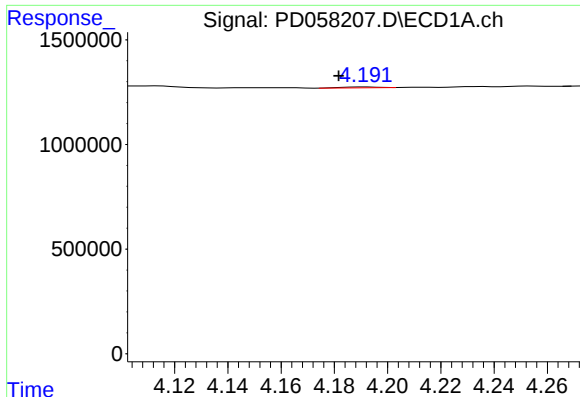

#4 Heptachlor


R.T.: 4.192 min
Delta R.T.: 0.010 min
Response: 35290
Conc: 0.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

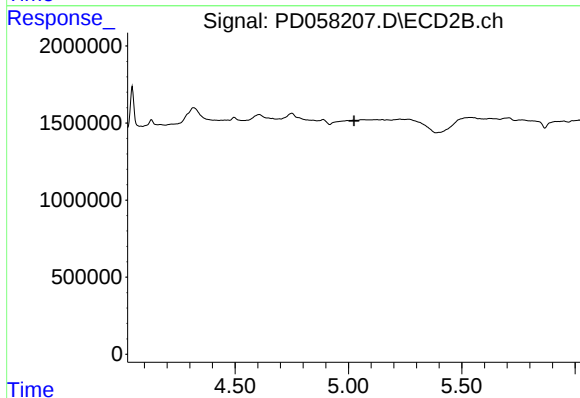


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.026 min
Response: 0
Conc: N.D.

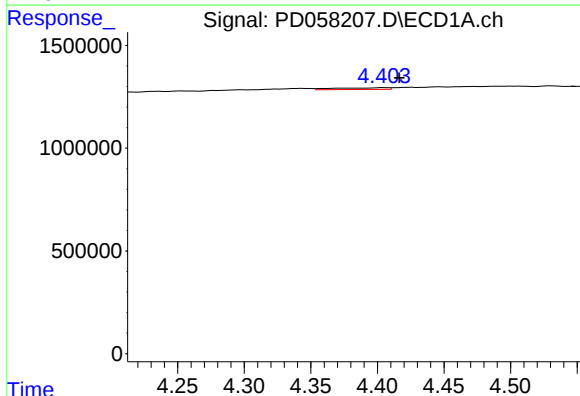


#5 Aldrin

R.T.: 4.405 min
Delta R.T.: -0.011 min
Response: 231466
Conc: 0.22 ng/ml

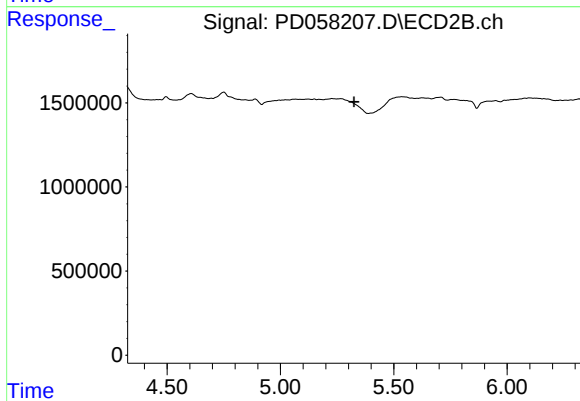

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.325 min
Response: 0
Conc: N.D.

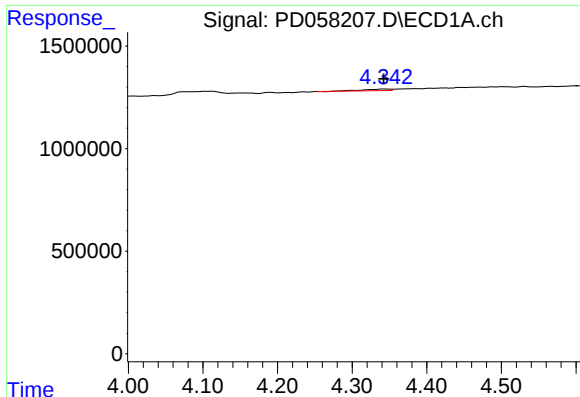

#7 delta-BHC


R.T.: 4.343 min
Delta R.T.: 0.001 min
Response: 180618
Conc: 0.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

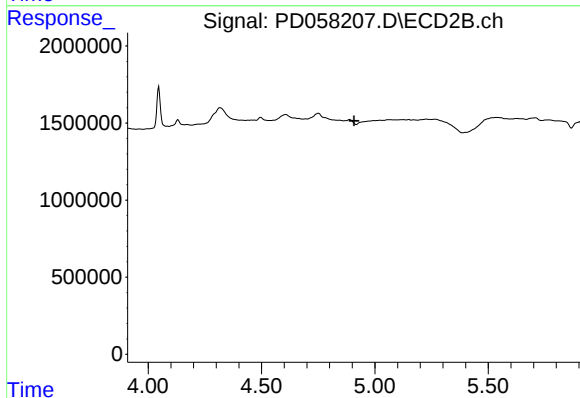


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

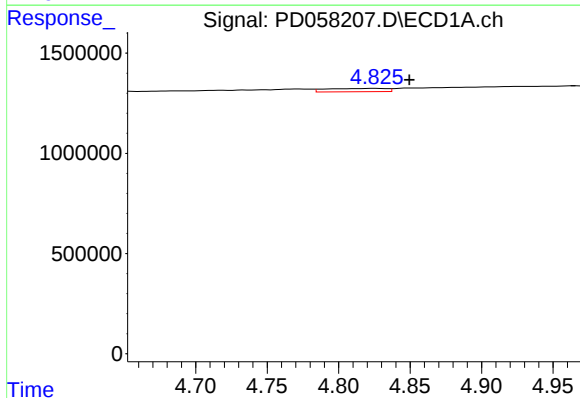


#8 Heptachlor epoxide

R.T.: 4.826 min
Delta R.T.: -0.023 min
Response: 479522
Conc: 0.49 ng/ml

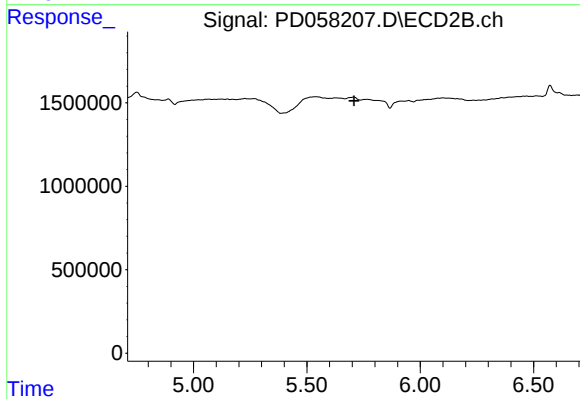

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.708 min
Response: 0
Conc: N.D.

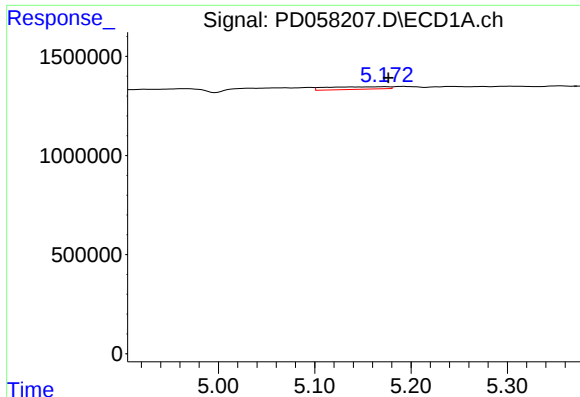

#9 Endosulfan I


R.T.: 5.173 min
Delta R.T.: -0.003 min
Response: 583665
Conc: 0.64 ng/ml

Instrument :
ECD_D
ClientSampleId :

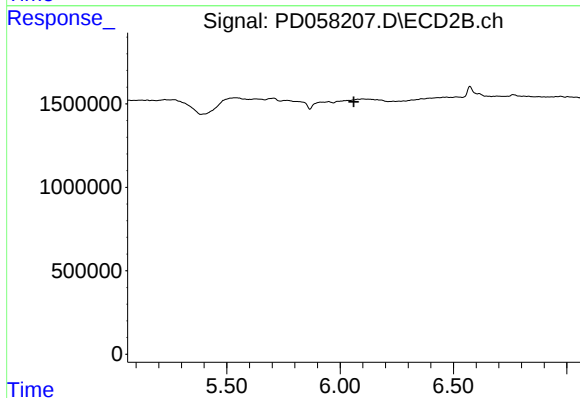


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.060 min
Response: 0
Conc: N.D.

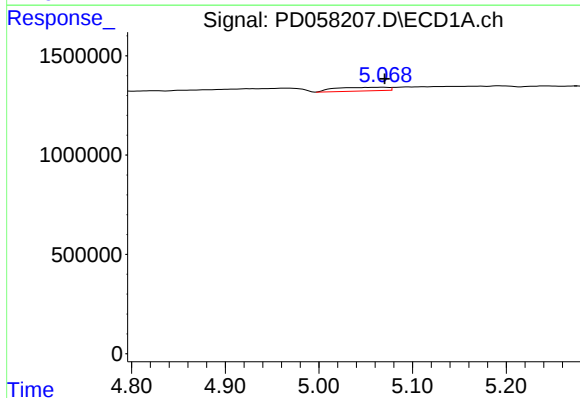


#10 gamma-Chlordane

R.T.: 5.069 min
Delta R.T.: 0.000 min
Response: 729218
Conc: 0.73 ng/ml

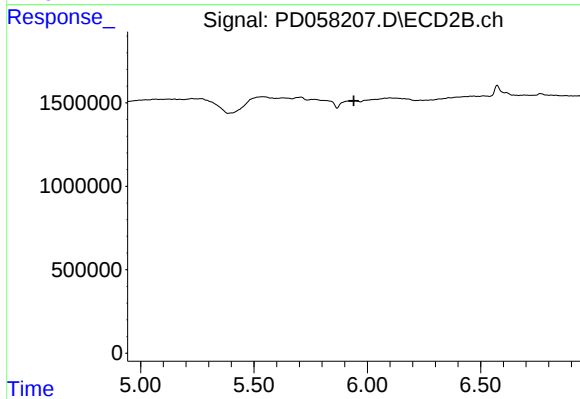

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.940 min
Response: 0
Conc: N.D.

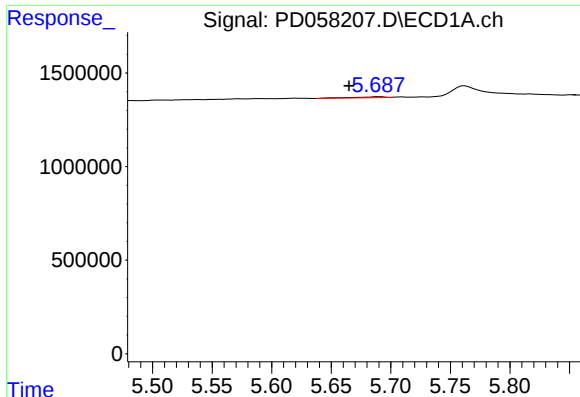

#14 Endrin


R.T.: 5.689 min
Delta R.T.: 0.024 min
Response: 95704
Conc: 0.12 ng/ml

Instrument :
ECD_D
ClientSampleId :

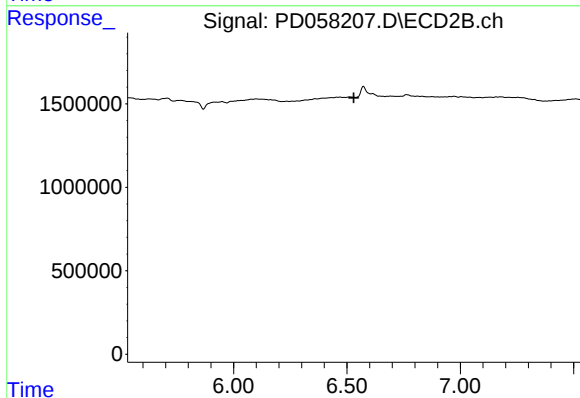


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.530 min
Response: 0
Conc: N.D.

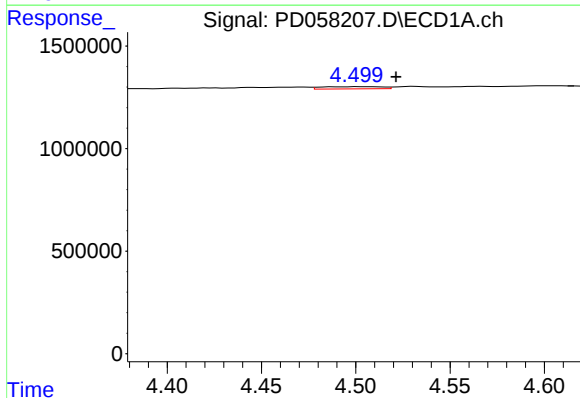


#24 Chlordane-2

R.T.: 4.501 min
Delta R.T.: -0.021 min
Response: 239126
Conc: 7.48 ng/ml

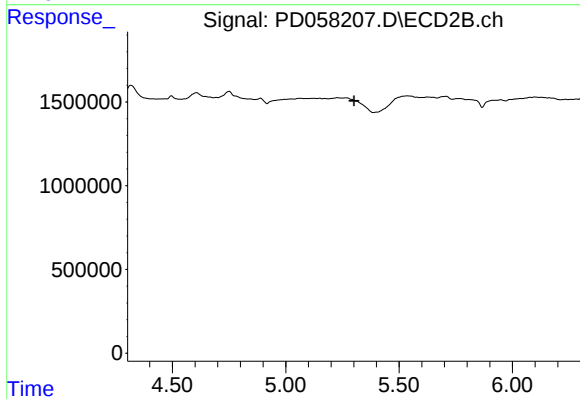

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.302 min
Response: 0
Conc: N.D.

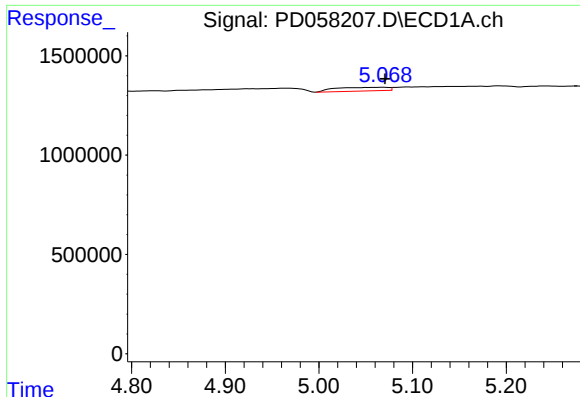

#25 Chlordane-3


R.T.: 5.069 min
Delta R.T.: -0.001 min
Response: 729218
Conc: 8.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

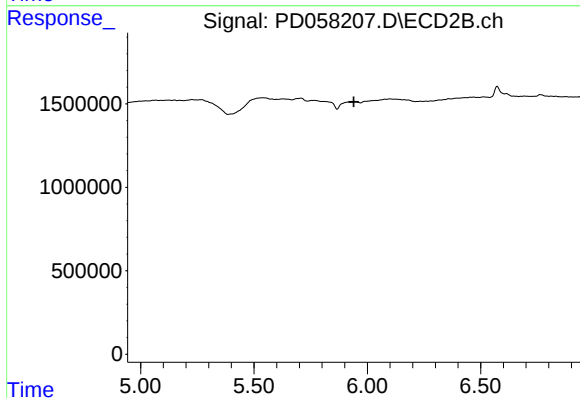


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.941 min
Response: 0
Conc: N.D.

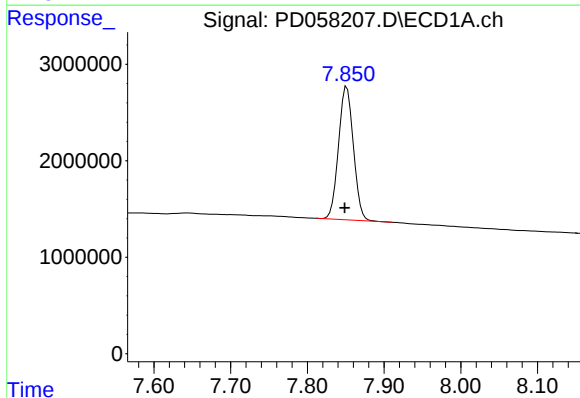

#28 Decachlorobiphenyl

R.T.: 7.851 min
Delta R.T.: 0.003 min
Response: 18613253
Conc: 23.28 ng/ml

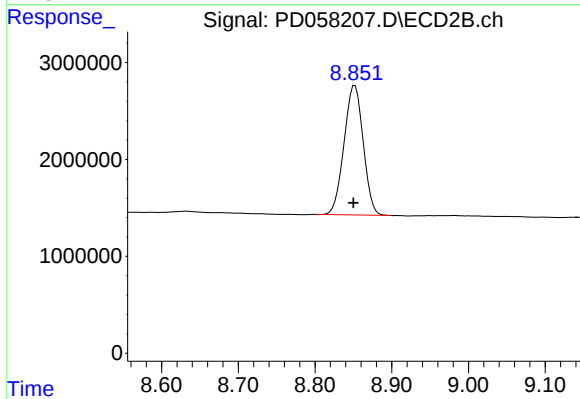

#28 Decachlorobiphenyl

R.T.: 8.852 min
Delta R.T.: 0.002 min
Response: 23327657
Conc: 22.50 ng/ml