

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052920\
 Data File : PD058210.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2020 10:58
 Operator : AJ\MA
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 14:06:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:46:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.867	42610818	53901156	54.522	47.327
28)	SA Decachlor...	7.851	8.852	43289607	52809225	54.140	50.939
Target Compounds							
23)	Chlordane-1	4.038	4.842	13199480	19729954	507.779	498.991
24)	Chlordane-2	4.523	5.303	15674748	22621887	490.303	470.449
25)	Chlordane-3	5.072	5.943	46356557	87329790	517.201	507.871
26)	Chlordane-4	5.127	6.017	43636447	106.8E6	510.735	512.584
27)	Chlordane-5	5.944	6.811	15570727	20577942	576.459	558.175



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052920\
Data File : PD058210.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2020 10:58
Operator : AJ\MA
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 14:06:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:46:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

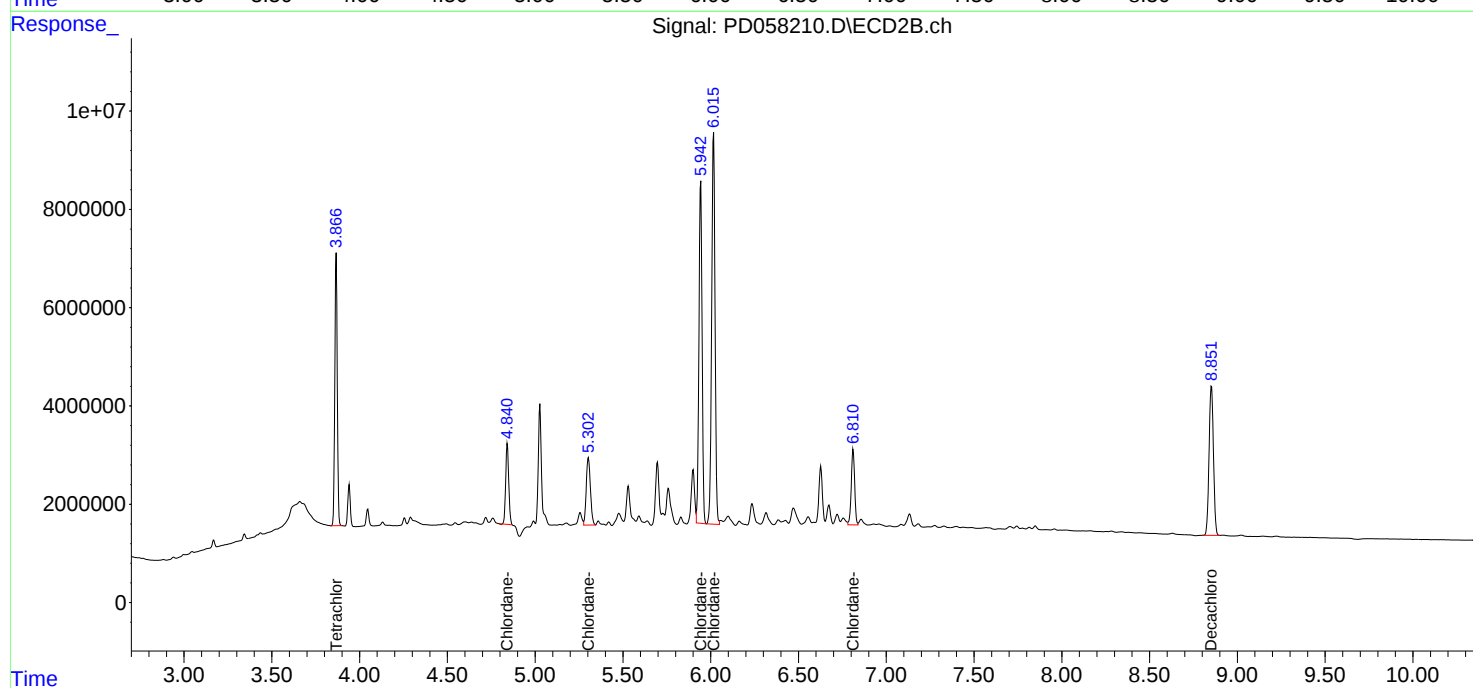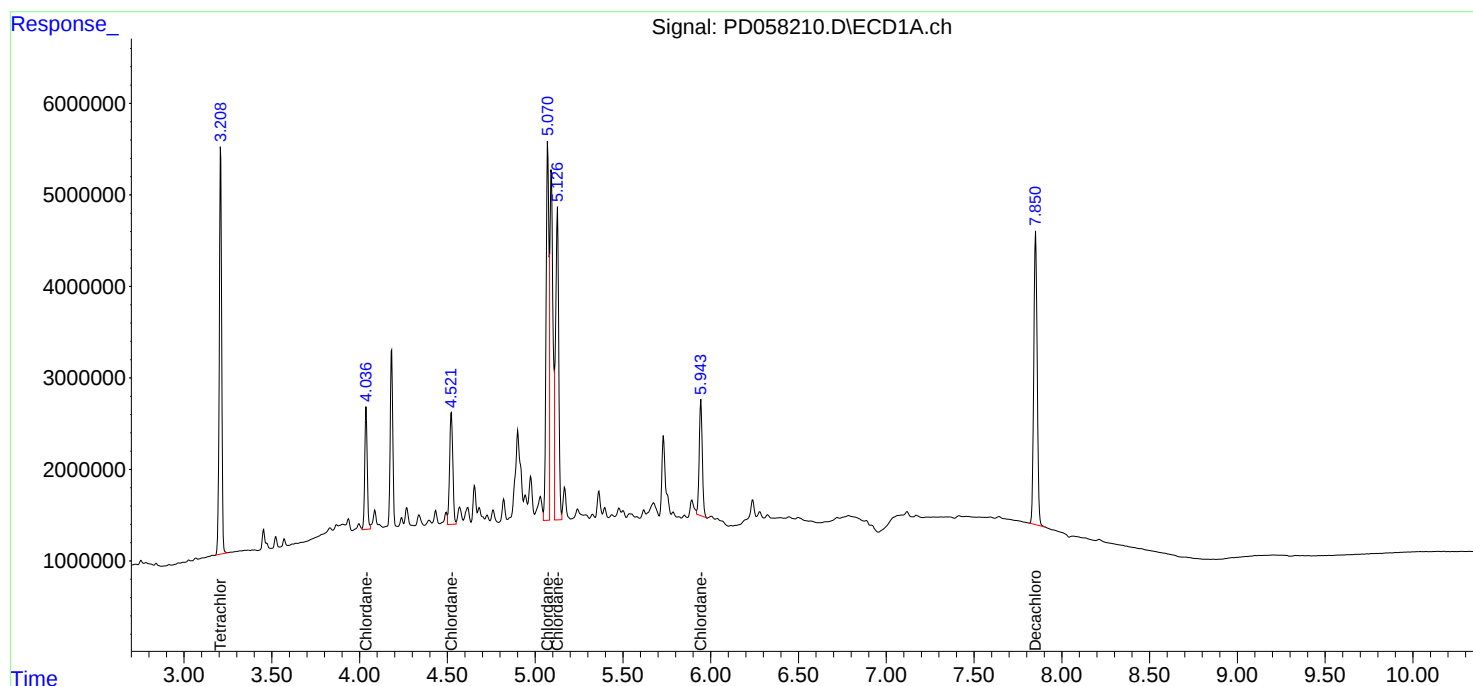


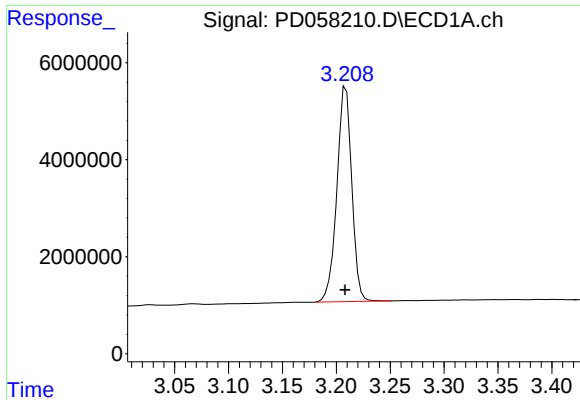

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: 0.001 min
Response: 42610818
Conc: 54.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

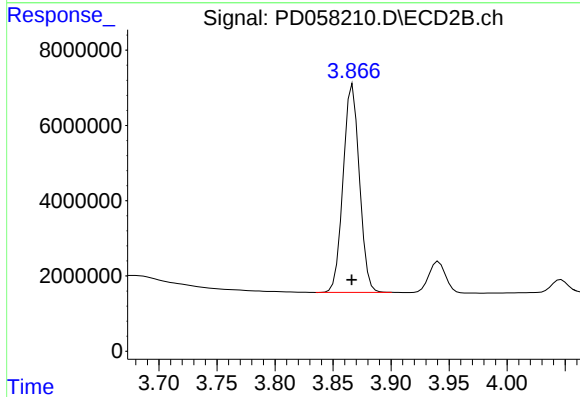


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 53901156
Conc: 47.33 ng/ml

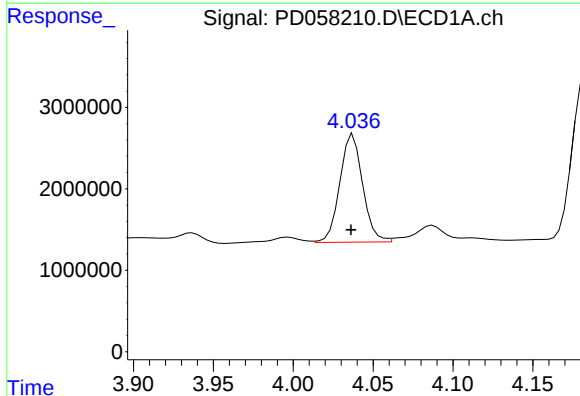


#23 Chlordane-1

R.T.: 4.038 min
Delta R.T.: 0.001 min
Response: 13199480
Conc: 507.78 ng/ml

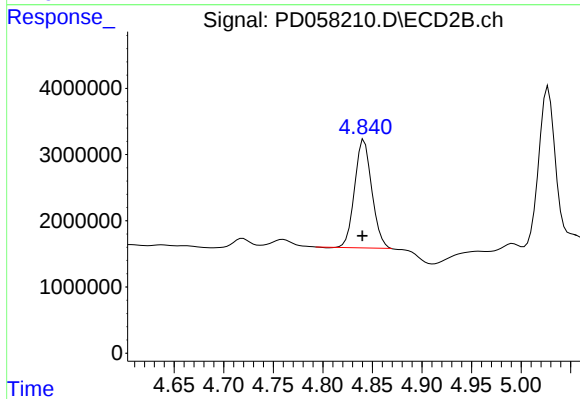

#23 Chlordane-1


R.T.: 4.842 min
Delta R.T.: 0.002 min
Response: 19729954
Conc: 498.99 ng/ml

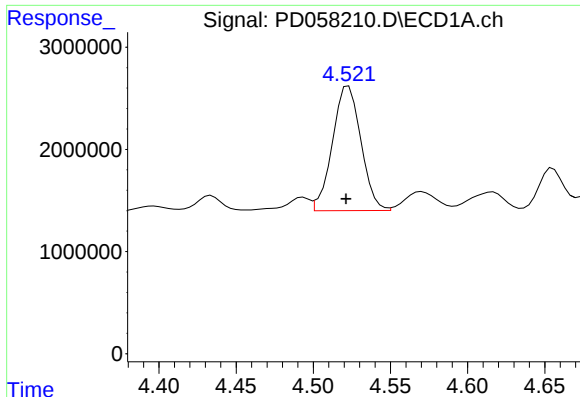

#24 Chlordane-2


R.T.: 4.523 min
Delta R.T.: 0.002 min
Response: 15674748
Conc: 490.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

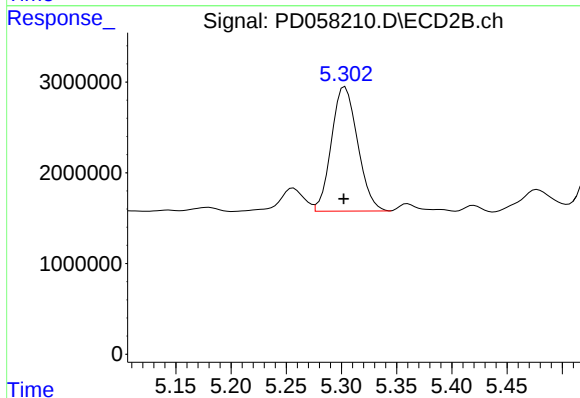


#24 Chlordane-2

R.T.: 5.303 min
Delta R.T.: 0.001 min
Response: 22621887
Conc: 470.45 ng/ml

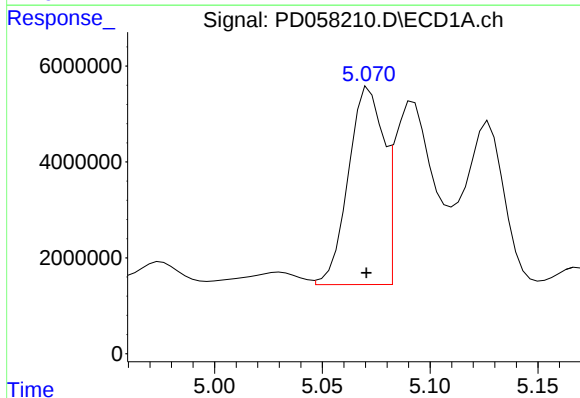


#25 Chlordane-3

R.T.: 5.072 min
Delta R.T.: 0.001 min
Response: 46356557
Conc: 517.20 ng/ml

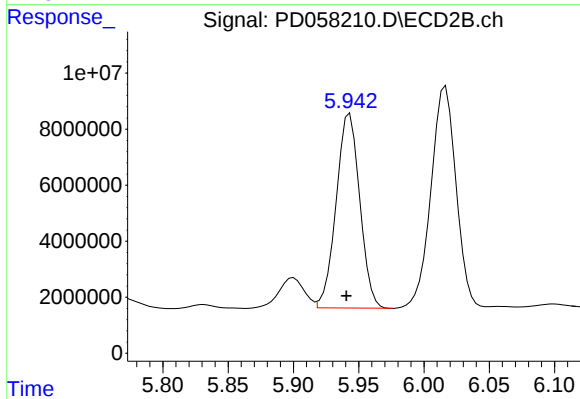

#25 Chlordane-3


R.T.: 5.943 min
Delta R.T.: 0.003 min
Response: 87329790
Conc: 507.87 ng/ml

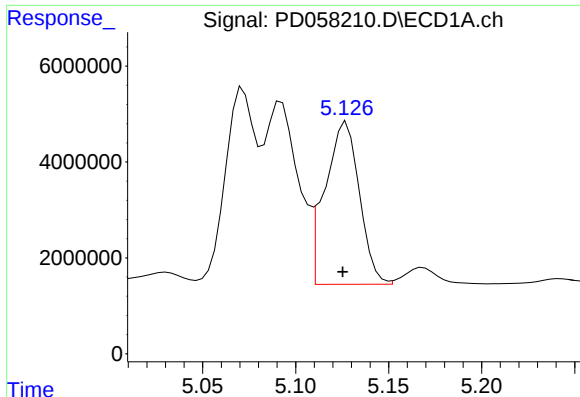

#26 Chlordane-4


R.T.: 5.127 min
Delta R.T.: 0.002 min
Response: 43636447
Conc: 510.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

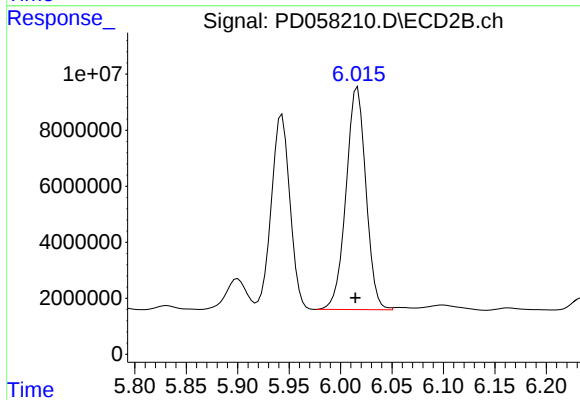


#26 Chlordane-4

R.T.: 6.017 min
Delta R.T.: 0.002 min
Response: 106815871
Conc: 512.58 ng/ml

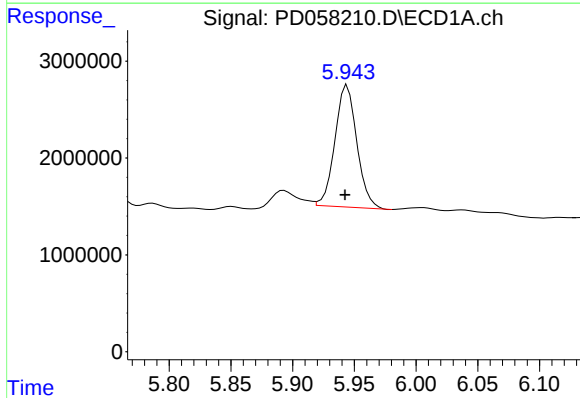


#27 Chlordane-5

R.T.: 5.944 min
Delta R.T.: 0.002 min
Response: 15570727
Conc: 576.46 ng/ml

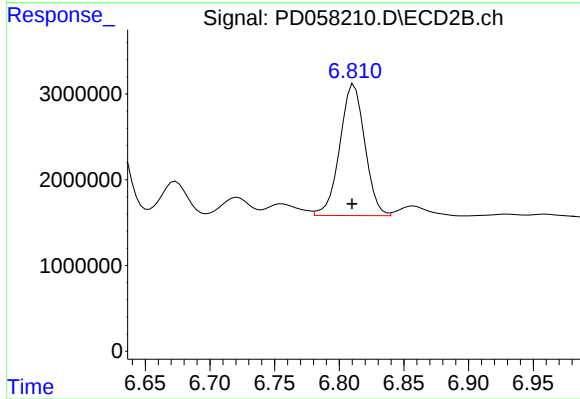

#27 Chlordane-5


R.T.: 6.811 min
Delta R.T.: 0.002 min
Response: 20577942
Conc: 558.17 ng/ml

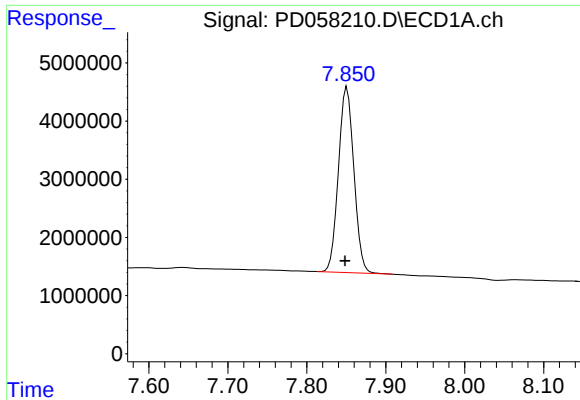

#28 Decachlorobiphenyl

R.T.: 7.851 min
Delta R.T.: 0.002 min
Response: 43289607
Conc: 54.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

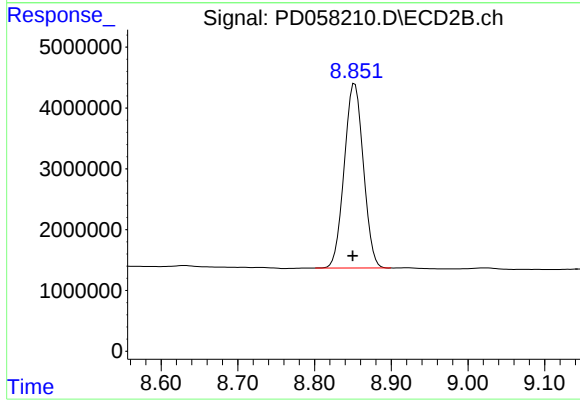

#28 Decachlorobiphenyl

R.T.: 8.852 min
Delta R.T.: 0.003 min
Response: 52809225
Conc: 50.94 ng/ml