

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052920\
 Data File : PD058223.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2020 14:16
 Operator : AJ\MA
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 15:23:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
 Quant Title : GC Extractables
 QLast Update : Thu May 21 13:46:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.867	43767313	55025655	56.002	48.315
28)	SA Decachlor...	7.851	8.853	43696064	53064598	54.649	51.185
Target Compounds							
23)	Chlordane-1	4.037	4.841	13130320	20302807	505.118	513.479
24)	Chlordane-2	4.523	5.303	15910068	23270605	497.663	483.939
25)	Chlordane-3	5.071	5.943	47366525	89501430	528.469	520.500
26)	Chlordane-4	5.127	6.017	44236828	108.7E6	517.762	521.434
27)	Chlordane-5	5.944	6.812	15862443	20996766	587.259	569.536



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052920\
Data File : PD058223.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2020 14:16
Operator : AJ\MA
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 15:23:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052120.M
Quant Title : GC Extractables
QLast Update : Thu May 21 13:46:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

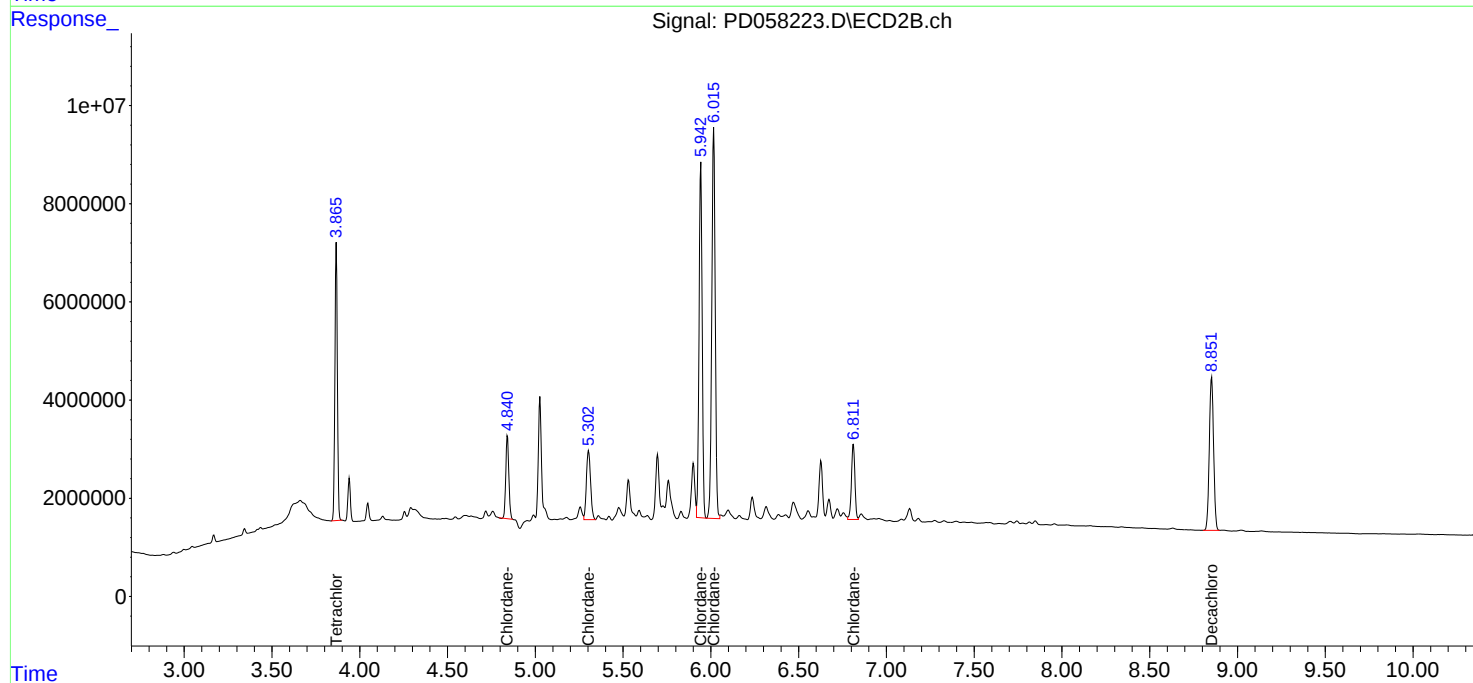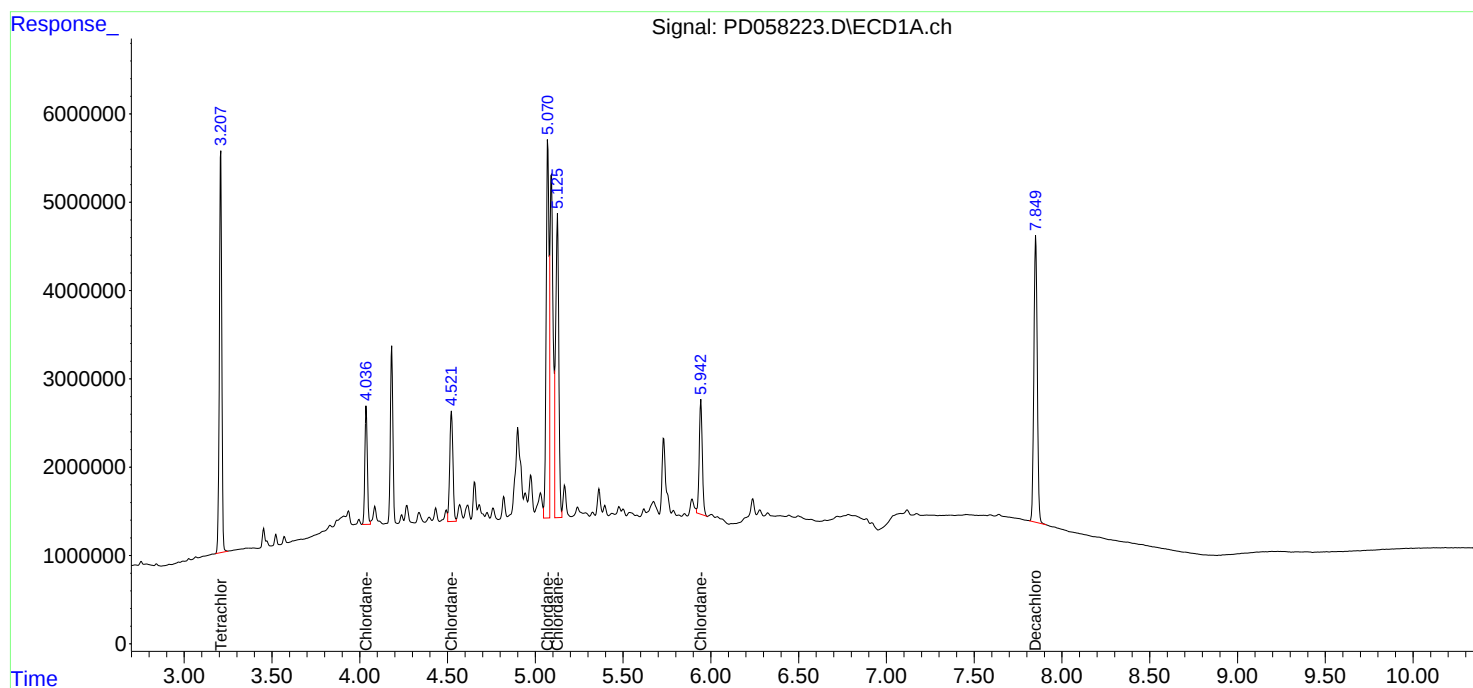


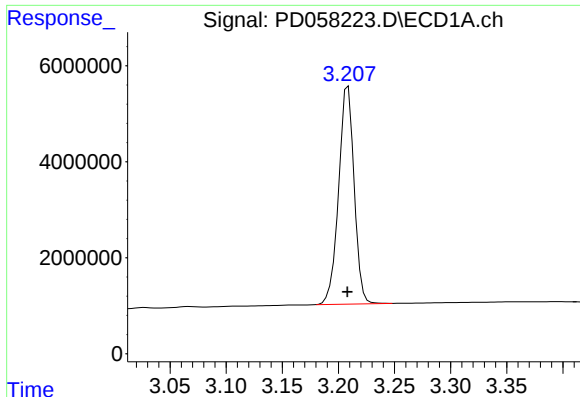

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: 0.000 min
Response: 43767313
Conc: 56.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

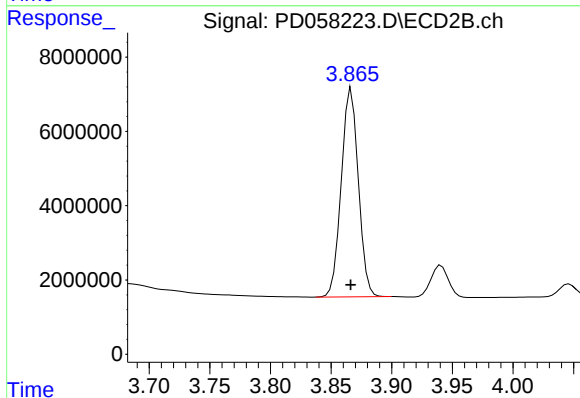


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 55025655
Conc: 48.31 ng/ml

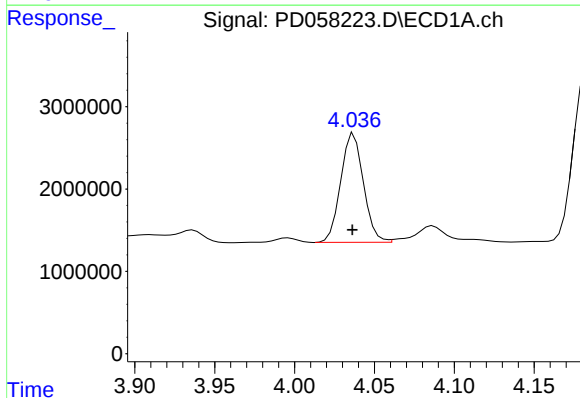


#23 Chlordane-1

R.T.: 4.037 min
Delta R.T.: 0.001 min
Response: 13130320
Conc: 505.12 ng/ml

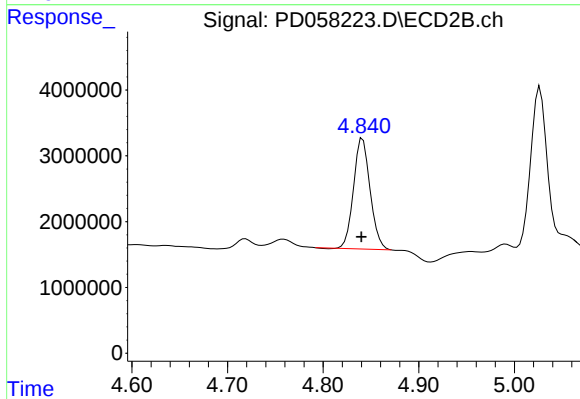

#23 Chlordane-1


R.T.: 4.841 min
Delta R.T.: 0.001 min
Response: 20302807
Conc: 513.48 ng/ml

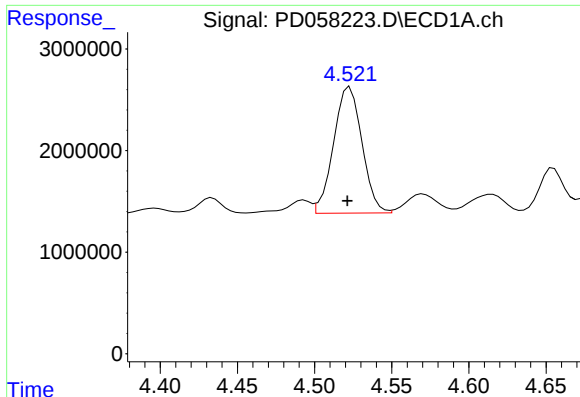

#24 Chlordane-2


R.T.: 4.523 min
Delta R.T.: 0.002 min
Response: 15910068
Conc: 497.66 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

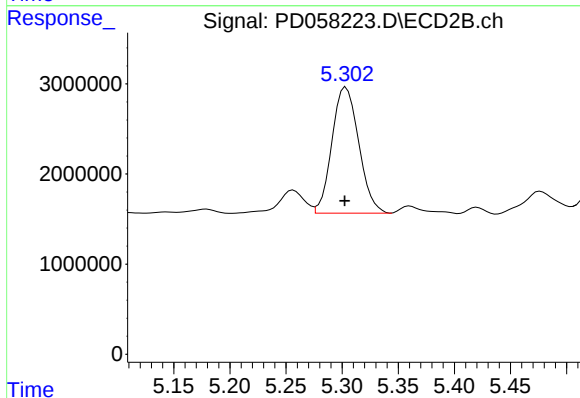


#24 Chlordane-2

R.T.: 5.303 min
Delta R.T.: 0.001 min
Response: 23270605
Conc: 483.94 ng/ml

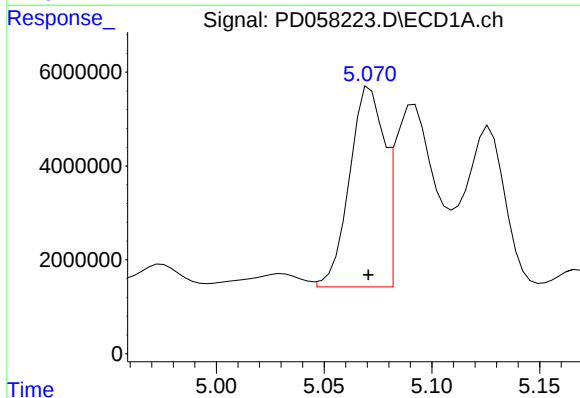


#25 Chlordane-3

R.T.: 5.071 min
Delta R.T.: 0.000 min
Response: 47366525
Conc: 528.47 ng/ml

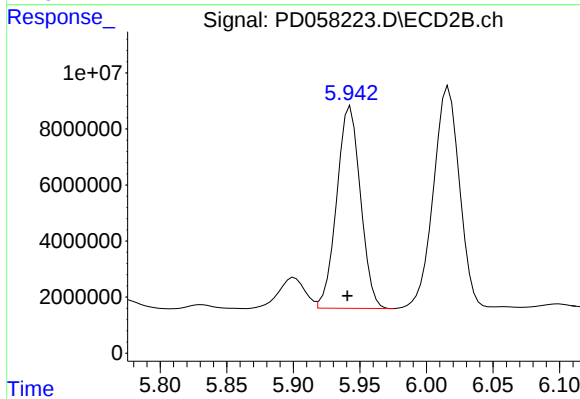

#25 Chlordane-3


R.T.: 5.943 min
Delta R.T.: 0.002 min
Response: 89501430
Conc: 520.50 ng/ml

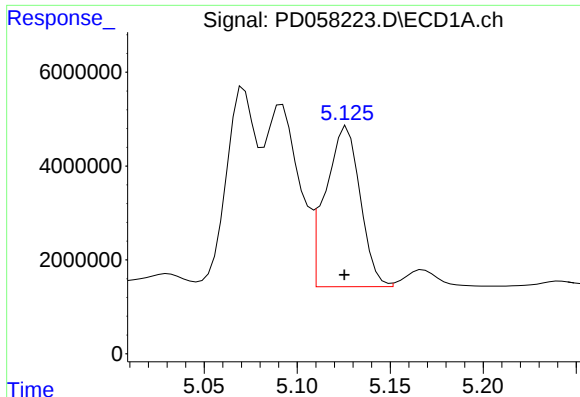

#26 Chlordane-4


R.T.: 5.127 min
Delta R.T.: 0.001 min
Response: 44236828
Conc: 517.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

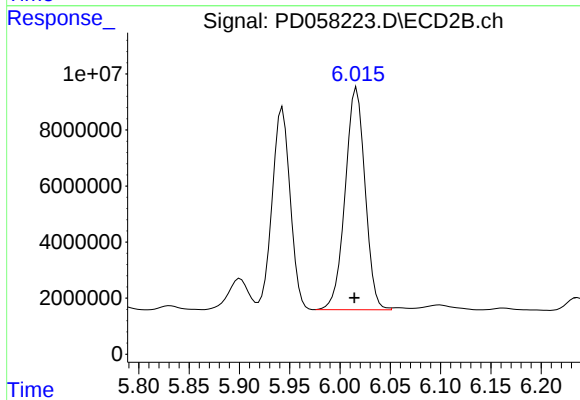


#26 Chlordane-4

R.T.: 6.017 min
Delta R.T.: 0.002 min
Response: 108660219
Conc: 521.43 ng/ml

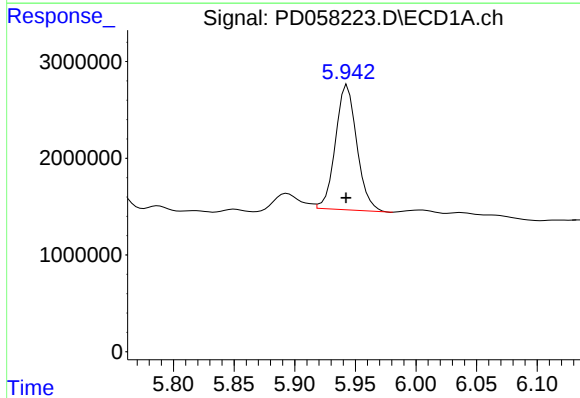


#27 Chlordane-5

R.T.: 5.944 min
Delta R.T.: 0.001 min
Response: 15862443
Conc: 587.26 ng/ml

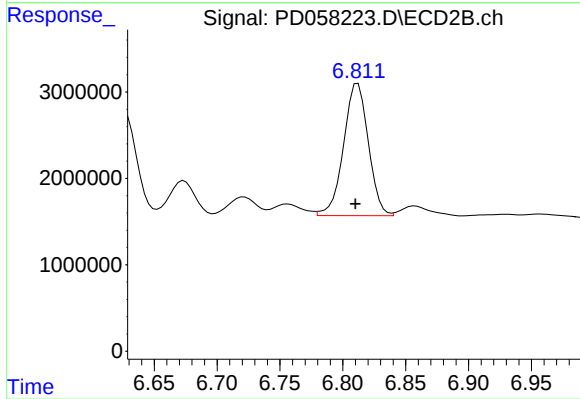

#27 Chlordane-5


R.T.: 6.812 min
Delta R.T.: 0.002 min
Response: 20996766
Conc: 569.54 ng/ml

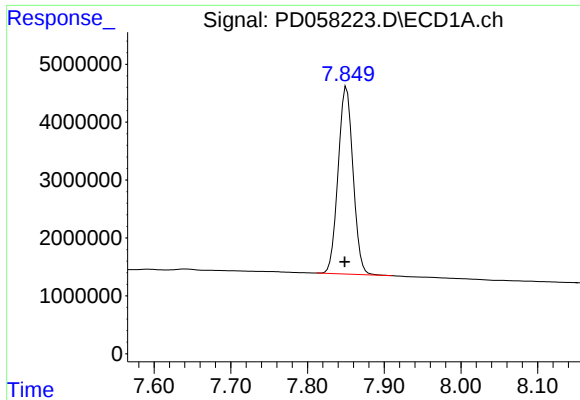

#28 Decachlorobiphenyl

R.T.: 7.851 min
Delta R.T.: 0.002 min
Response: 43696064
Conc: 54.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

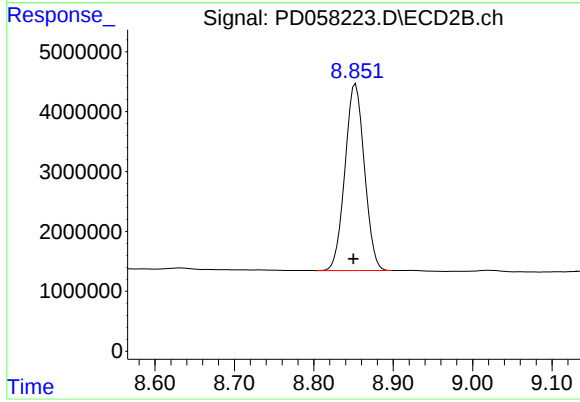

#28 Decachlorobiphenyl

R.T.: 8.853 min
Delta R.T.: 0.003 min
Response: 53064598
Conc: 51.19 ng/ml