

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052924\
 Data File : PD083213.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2024 13:06
 Operator : AR\AJ
 Sample : P2571-23MS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH6A4MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/03/2024
 Supervised By :Ankita Jodhani 06/03/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 13:36:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.773	27393103	80969488	18.314	20.822
27)	SA Decachlor...	9.117	7.901	39913404	95700005	19.913m	24.188
Target Compounds							
2)	A alpha-BHC	4.021	3.273	145.1E6	383.4E6	56.855	61.674
3)	MA gamma-BHC...	4.354	3.602	144.7E6	372.5E6	58.647m	64.379
4)	MA Heptachlor	4.946	3.940	138.8E6	328.1E6	55.134m	58.918
5)	MB Aldrin	5.291	4.219	129.4E6	330.3E6	53.460	59.761
6)	B beta-BHC	4.550	3.898	51543102	134.7E6	47.510m	53.714
7)	B delta-BHC	4.801	4.127	135.1E6	360.1E6	55.176	60.875
8)	B Heptachlo...	5.719	4.721	115.8E6	298.8E6	51.833	58.488
9)	A Endosulfan I	6.106	5.091	111.5E6	211.5E6	53.560	46.901
10)	B trans-Chl...	5.974	4.970	114.0E6	313.7E6	52.665m	63.003
11)	B cis-Chlor...	6.055	5.034	121.1E6	309.0E6	54.210	60.834
12)	B 4,4'-DDE	6.227	5.222	315.9E6	905.6E6	144.834	189.892 #
13)	MA Dieldrin	6.382	5.353	249.3E6	648.1E6	113.426	129.688m
14)	MA Endrin	6.613	5.628	179.1E6	562.8E6	100.436	128.680m#
15)	B Endosulfa...	6.831	5.923	209.1E6	519.7E6	108.532m	123.326
16)	A 4,4'-DDD	6.745	5.776	181.6E6	478.1E6	117.125	127.057
17)	MA 4,4'-DDT	7.061	6.027	316.4E6	755.2E6	196.729	196.670
18)	B Endrin al...	6.962	6.102	136.8E6	332.3E6	98.503	105.372
19)	B Endosulfa...	7.198	6.324	193.4E6	473.2E6	109.580	117.707
20)	A Methoxychlor	7.538	6.602	439.1E6	1063.1E6	507.613	541.790
21)	B Endrin ke...	7.685	6.830	192.3E6	479.7E6	101.993	106.669

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052924\
Data File : PD083213.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2024 13:06
Operator : AR\AJ
Sample : P2571-23MS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 13:36:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

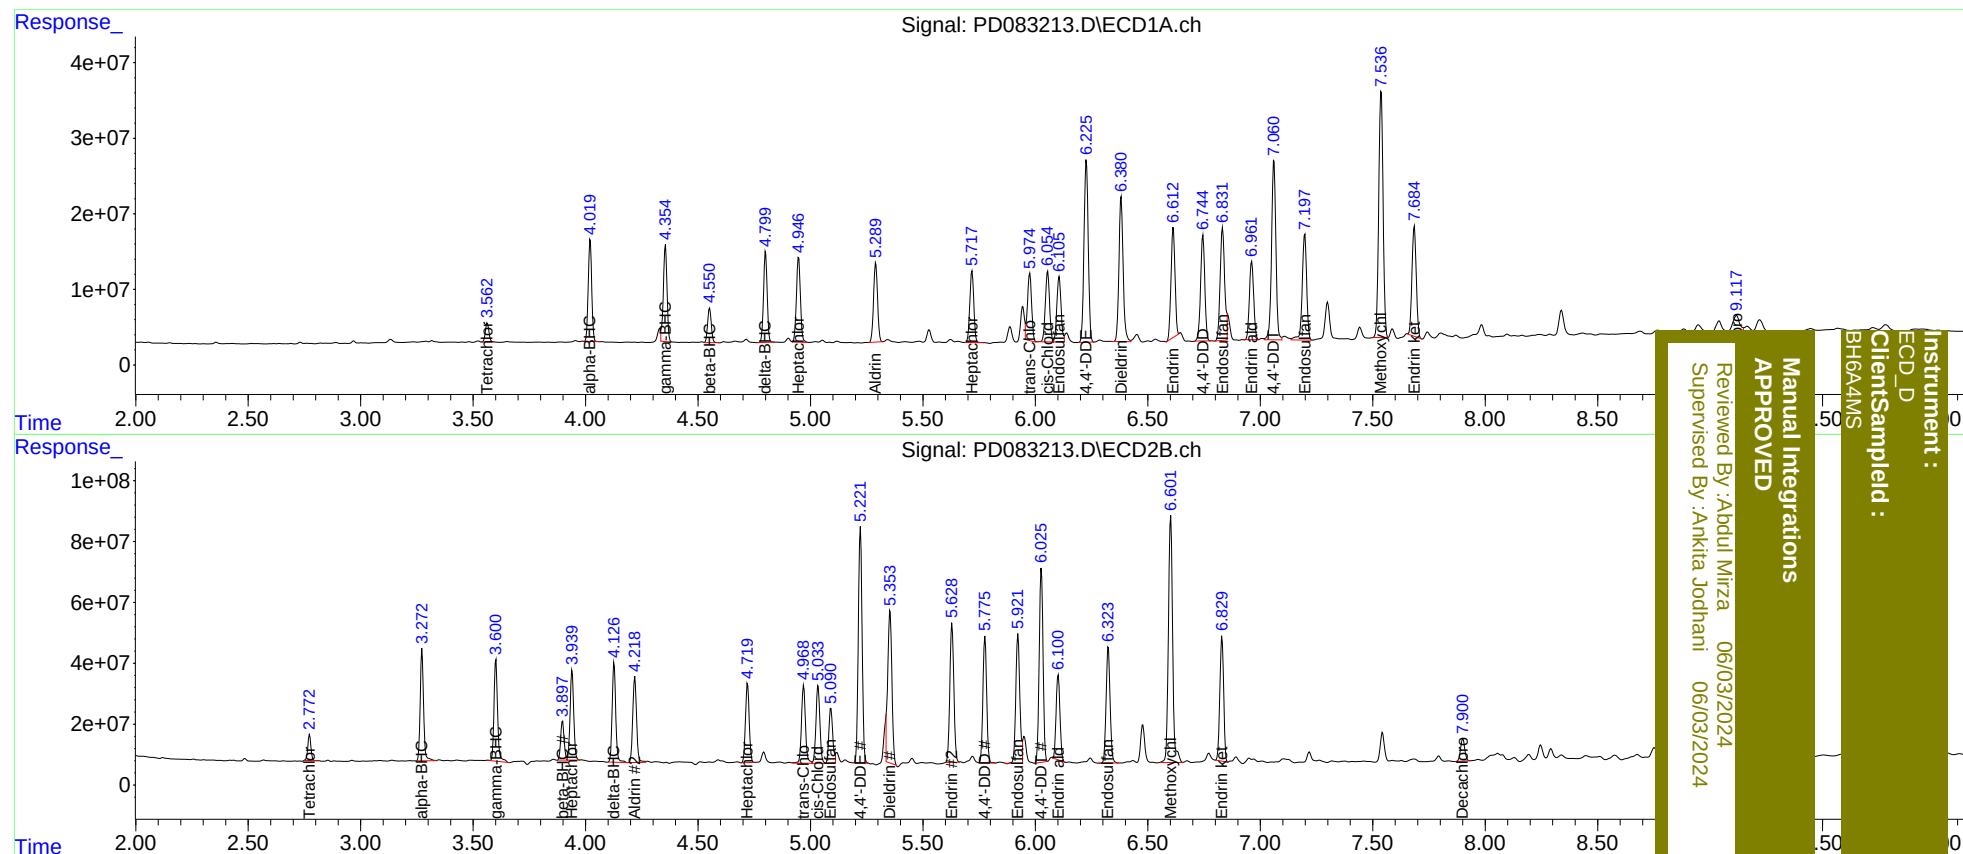

Instrument :
ECD_D
Client Sampled :
BH6A4MS

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/03/2024
Supervised By :Ankita Jodhani 06/03/2024