

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052924\
 Data File : PD083214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2024 13:33
 Operator : AR\AJ
 Sample : P2571-24MSD
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH6A4MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/03/2024
 Supervised By :Ankita Jodhani 06/03/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 10:04:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.773	27033224	79610288	18.073	20.472
27)	SA Decachlor...	9.114	7.900	41454643	95577108	20.682m	24.157
Target Compounds							
2)	A alpha-BHC	4.020	3.273	144.3E6	379.4E6	56.573	61.034
3)	MA gamma-BHC...	4.353	3.602	145.2E6	368.9E6	58.845m	63.746
4)	MA Heptachlor	4.945	3.940	138.3E6	325.7E6	54.914m	58.486
5)	MB Aldrin	5.290	4.219	125.5E6	324.4E6	51.828	58.690
6)	B beta-BHC	4.551	3.898	50068503	134.5E6	46.151	53.642
7)	B delta-BHC	4.799	4.127	134.6E6	357.4E6	54.951	60.405
8)	B Heptachlo...	5.717	4.720	111.4E6	295.0E6	49.885	57.743
9)	A Endosulfan I	6.104	5.091	109.2E6	211.4E6	52.463	46.868
10)	B trans-Chl...	5.973	4.970	110.5E6	309.6E6	51.067m	62.180
11)	B cis-Chlor...	6.054	5.034	118.8E6	304.2E6	53.204	59.887
12)	B 4,4'-DDE	6.226	5.221	312.2E6	897.8E6	143.150	188.262 #
13)	MA Dieldrin	6.381	5.352	243.6E6	656.1E6	110.836	131.299m
14)	MA Endrin	6.612	5.627	173.1E6	560.8E6	97.063	128.225m#
15)	B Endosulfa...	6.830	5.922	227.8E6	513.4E6	118.231	121.819
16)	A 4,4'-DDD	6.743	5.776	177.8E6	474.1E6	114.668	125.986
17)	MA 4,4'-DDT	7.059	6.026	304.2E6	750.1E6	189.127	195.365
18)	B Endrin al...	6.961	6.101	133.9E6	327.3E6	96.401	103.794
19)	B Endosulfa...	7.196	6.323	185.9E6	467.1E6	105.327	116.176
20)	A Methoxychlor	7.536	6.600	428.1E6	1050.6E6	494.884	535.388
21)	B Endrin ke...	7.684	6.828	194.6E6	476.3E6	103.209	105.909

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD052924\
Data File : PD083214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2024 13:33
Operator : AR\AJ
Sample : P2571-24MSD
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 10:04:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

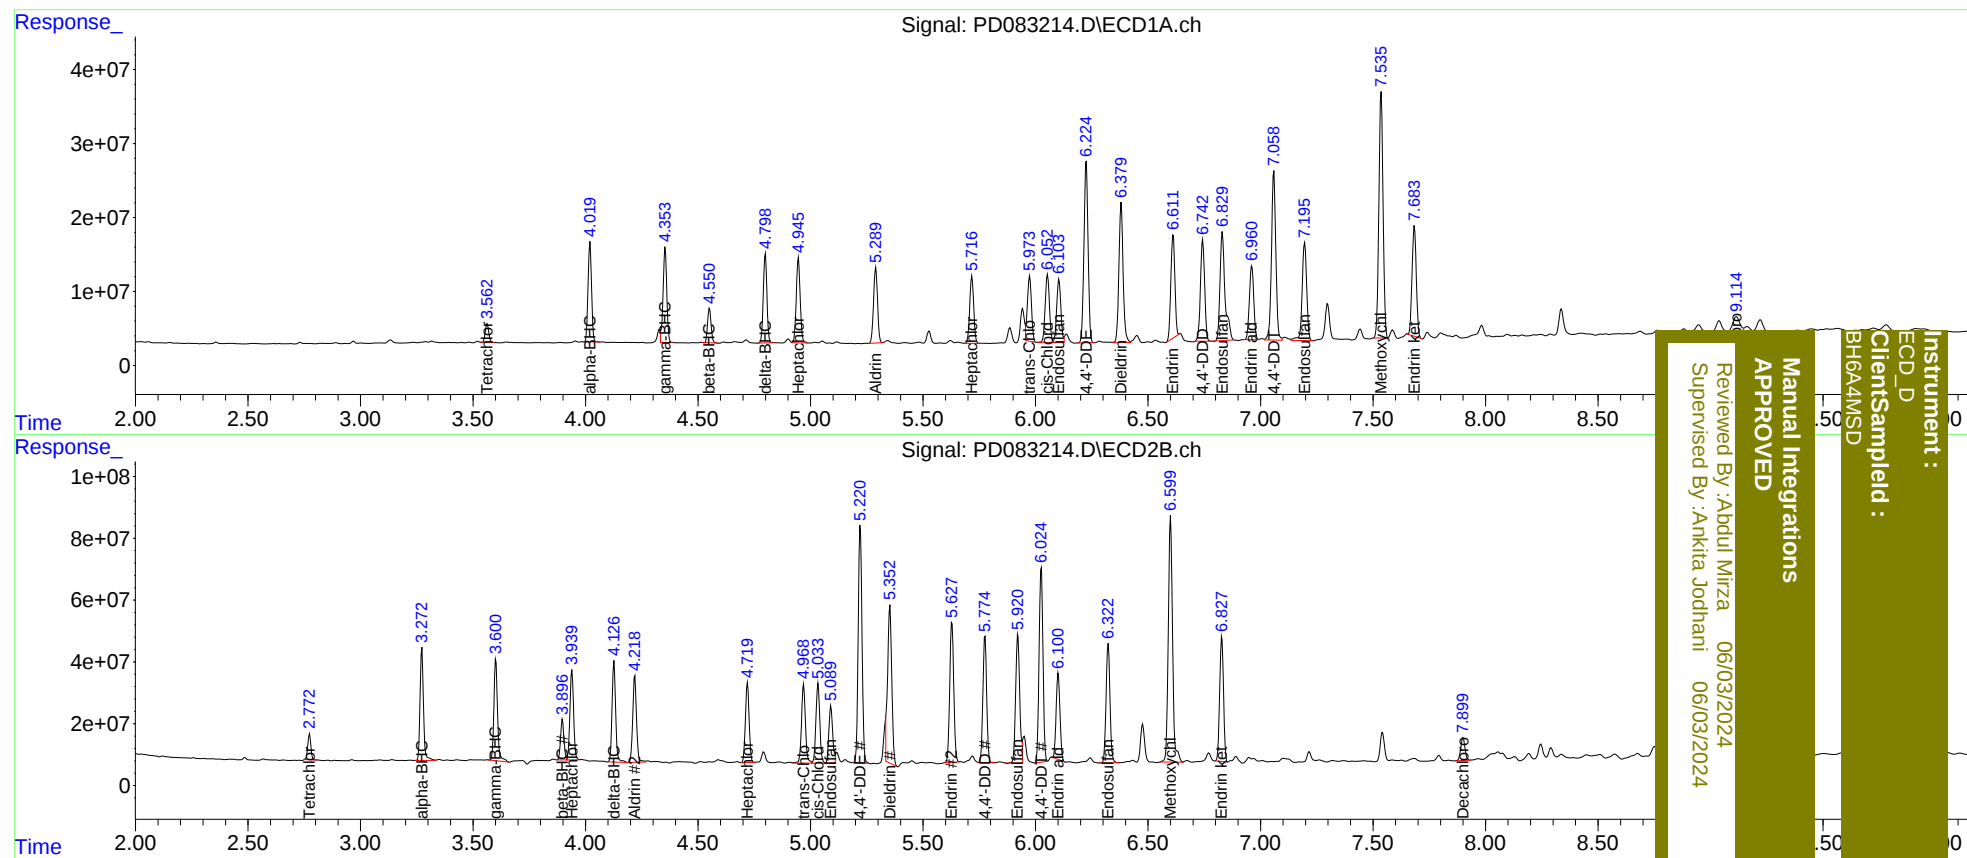

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 06/03/2024
Supervised By: Ankita Jodhani 06/03/2024

Instrument :
ECD_D
Client Sampled :
BH6A4MSD