

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD053024\
 Data File : PD083236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2024 13:14
 Operator : AR\AJ
 Sample : P2588-05MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH5S5MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/31/2024
 Supervised By : Ankita Jodhani 05/31/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 00:28:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.562	2.774	11950525	39210660	7.990m	10.083 #
27)	SA Decachlor...	9.112	7.900	22685616	47903663	11.318m	12.108
Target Compounds							
2)	A alpha-BHC	4.020	3.273	114.2E6	307.1E6	44.759	49.399
3)	MA gamma-BHC...	4.353	3.601	111.6E6	296.5E6	45.216m	51.242
4)	MA Heptachlor	4.946	3.940	112.4E6	269.9E6	44.652m	48.478
5)	MB Aldrin	5.290	4.219	104.4E6	261.9E6	43.128	47.388
6)	B beta-BHC	4.550	3.898	39652568	109.6E6	36.550m	43.693
7)	B delta-BHC	4.800	4.127	105.8E6	299.6E6	43.200	50.649
8)	B Heptachlo...	5.718	4.720	92932057	243.5E6	41.615	47.668
9)	A Endosulfan I	6.105	5.091	91472735	155.0E6	43.959	34.368
10)	B trans-Chl...	5.973	4.968	90515349	244.9E6	41.814m	49.182m
11)	B cis-Chlor...	6.054	5.033	97624190	259.1E6	43.711	51.018
12)	B 4,4'-DDE	6.226	5.221	150.2E6	454.8E6	68.873	95.361 #
13)	MA Dieldrin	6.380	5.352	204.7E6	513.3E6	93.146m	102.723m
14)	MA Endrin	6.612	5.628	158.6E6	446.5E6	88.955	102.085
15)	B Endosulfa...	6.831	5.920	158.1E6	409.1E6	82.043	97.084m
16)	A 4,4'-DDD	6.745	5.775	140.8E6	358.3E6	90.781	95.235
17)	MA 4,4'-DDT	7.061	6.026	157.8E6	385.2E6	98.134	100.331
18)	B Endrin al...	6.961	6.101	112.4E6	265.7E6	80.926	84.263
19)	B Endosulfa...	7.196	6.323	159.1E6	405.6E6	90.125	100.888
20)	A Methoxychlor	7.537	6.601	367.5E6	850.9E6	424.799	433.620
21)	B Endrin ke...	7.685	6.828	152.5E6	373.3E6	80.888	83.009

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD053024\
Data File : PD083236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2024 13:14
Operator : AR\AJ
Sample : P2588-05MS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 00:28:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

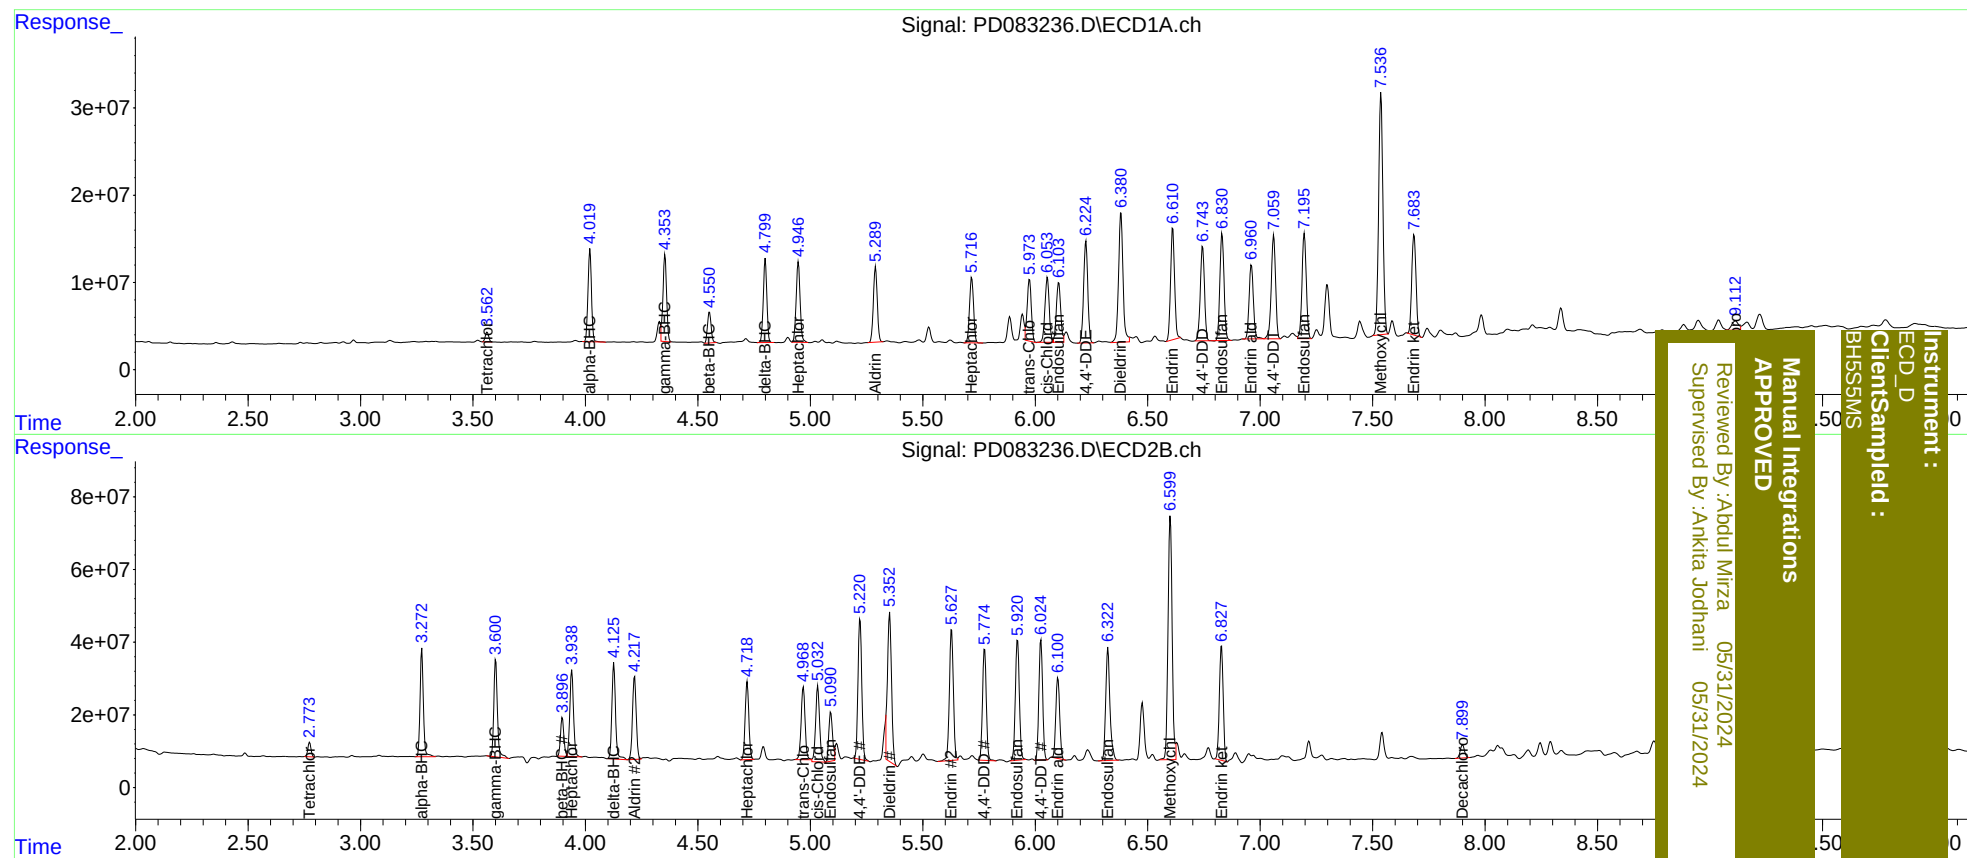

Instrument :
ECD_D
ClientSampled :
BHSSMS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 05/31/2024
Supervised By: Ankita Jodhani 05/31/2024