

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD053024\
 Data File : PD083237.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2024 13:40
 Operator : AR\AJ
 Sample : P2588-06MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH5S5MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/31/2024
 Supervised By :Ankita Jodhani 05/31/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 00:29:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.562	2.774	11580018	38818999	7.742m	9.983 #
27)	SA Decachlor...	9.113	7.901	21582317	46201200	10.767m	11.677
Target Compounds							
2)	A alpha-BHC	4.020	3.273	111.0E6	300.6E6	43.502m	48.354
3)	MA gamma-BHC...	4.354	3.602	110.6E6	291.3E6	44.800m	50.340
4)	MA Heptachlor	4.946	3.940	106.9E6	263.3E6	42.454m	47.277
5)	MB Aldrin	5.291	4.219	102.0E6	256.2E6	42.119	46.350
6)	B beta-BHC	4.551	3.898	38625548	108.1E6	35.603m	43.091
7)	B delta-BHC	4.800	4.127	104.0E6	293.3E6	42.469	49.586
8)	B Heptachlo...	5.719	4.720	90997987	236.9E6	40.749	46.366
9)	A Endosulfan I	6.106	5.092	89171402	152.7E6	42.853	33.852
10)	B trans-Chl...	5.975	4.969	87845183	237.9E6	40.581m	47.771m
11)	B cis-Chlor...	6.055	5.034	95324983	255.6E6	42.682	50.330
12)	B 4,4'-DDE	6.227	5.222	147.6E6	447.6E6	67.676	93.857 #
13)	MA Dieldrin	6.381	5.353	201.7E6	497.6E6	91.754m	99.576m
14)	MA Endrin	6.613	5.630	152.9E6	440.8E6	85.727	100.781
15)	B Endosulfa...	6.833	5.922	155.2E6	408.6E6	80.544	96.963m
16)	A 4,4'-DDD	6.746	5.777	137.7E6	350.2E6	88.765	93.063
17)	MA 4,4'-DDT	7.061	6.027	156.9E6	379.7E6	97.531	98.879
18)	B Endrin al...	6.963	6.103	110.4E6	260.4E6	79.460	82.579
19)	B Endosulfa...	7.198	6.325	156.6E6	398.7E6	88.743	99.169
20)	A Methoxychlor	7.539	6.602	360.1E6	841.6E6	416.271	428.917
21)	B Endrin ke...	7.687	6.830	150.2E6	368.3E6	79.664	81.895

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD053024\
Data File : PD083237.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2024 13:40
Operator : AR\AJ
Sample : P2588-06MSD
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 00:29:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

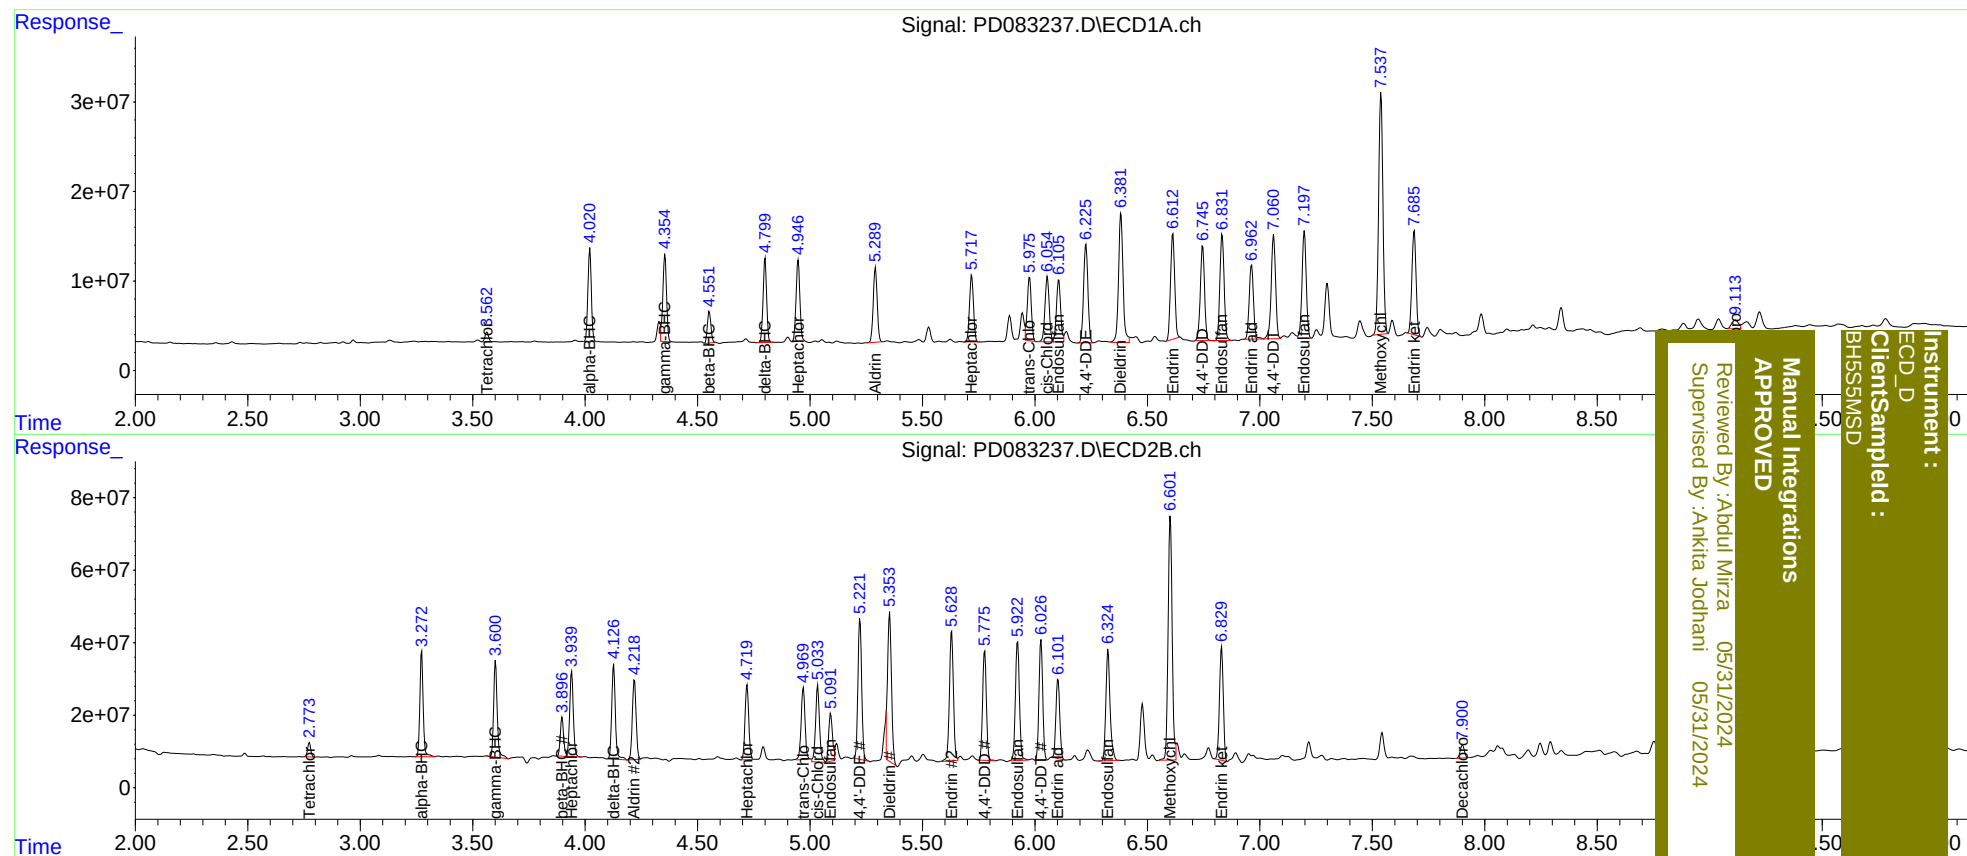

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/31/2024
Supervised By: Ankita Jodhani 05/31/2024

Instrument :
ECD_D
Client Sampled :
BHSSMSD