

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD053024\
 Data File : PD083252.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2024 19:48
 Operator : AR\AJ
 Sample : P2588-17
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH6E2

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/31/2024
 Supervised By :Ankita Jodhani 05/31/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 00:37:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.563	2.773	14492790	47114911	9.689	12.116 #
27) SA Decachlor...	9.115	7.901	14536839	36335323	7.252m	9.184 #
Target Compounds						
9) A Endosulfan I	6.138	5.116	3486635	11711671	1.676	2.597m#
13) MA Dieldrin	6.401	5.359	2321384	8514706	1.056	1.704m#
16) A 4,4'-DDD	6.730	5.776	2271779	5088162	1.465m	1.352m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD053024\
Data File : PD083252.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2024 19:48
Operator : AR\AJ
Sample : P2588-17
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 00:37:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

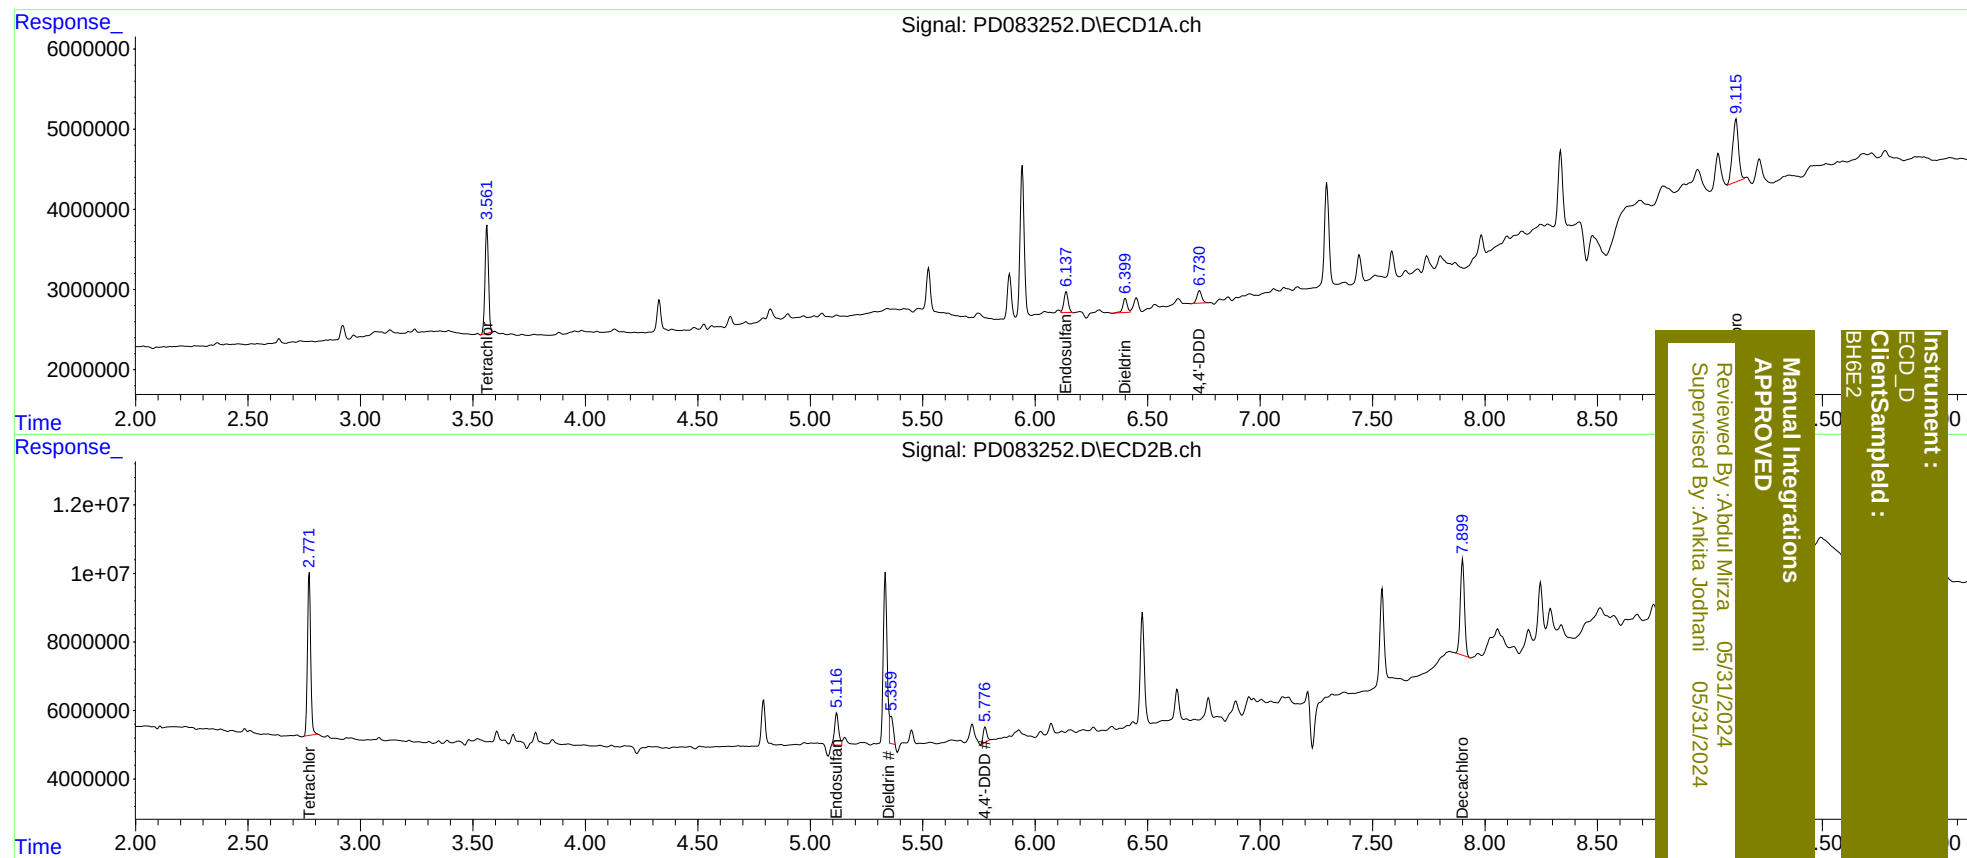

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/31/2024
Supervised By: Ankita Jodhani 05/31/2024

Instrument :
ECD_D
ClientSampled :
BH6E2