

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD053024\
 Data File : PD083235.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2024 12:47
 Operator : AR\AJ
 Sample : P2588-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH5S5

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/31/2024
 Supervised By : Ankita Jodhani 05/31/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 00:28:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.562	2.772	13373304	46776547	8.941m	12.029m#
2)	SA Decachlor...	9.111	7.900	23643682	54703558	11.796m	13.826
Target Compounds							
9)	A Endosulfan I	6.138	5.116	18762022	58695431	9.016m	13.015m#
13)	MA Dieldrin	6.403	5.359	12292013	34621652	5.593m	6.928m
16)	A 4,4'-DDD	6.731	5.775	8674900	14091627	5.593m	3.745m#
17)	MA 4,4'-DDT	7.061	6.023	10359166	23516070	6.441	6.124m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD053024\
Data File : PD083235.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2024 12:47
Operator : AR\AJ
Sample : P2588-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 00:28:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

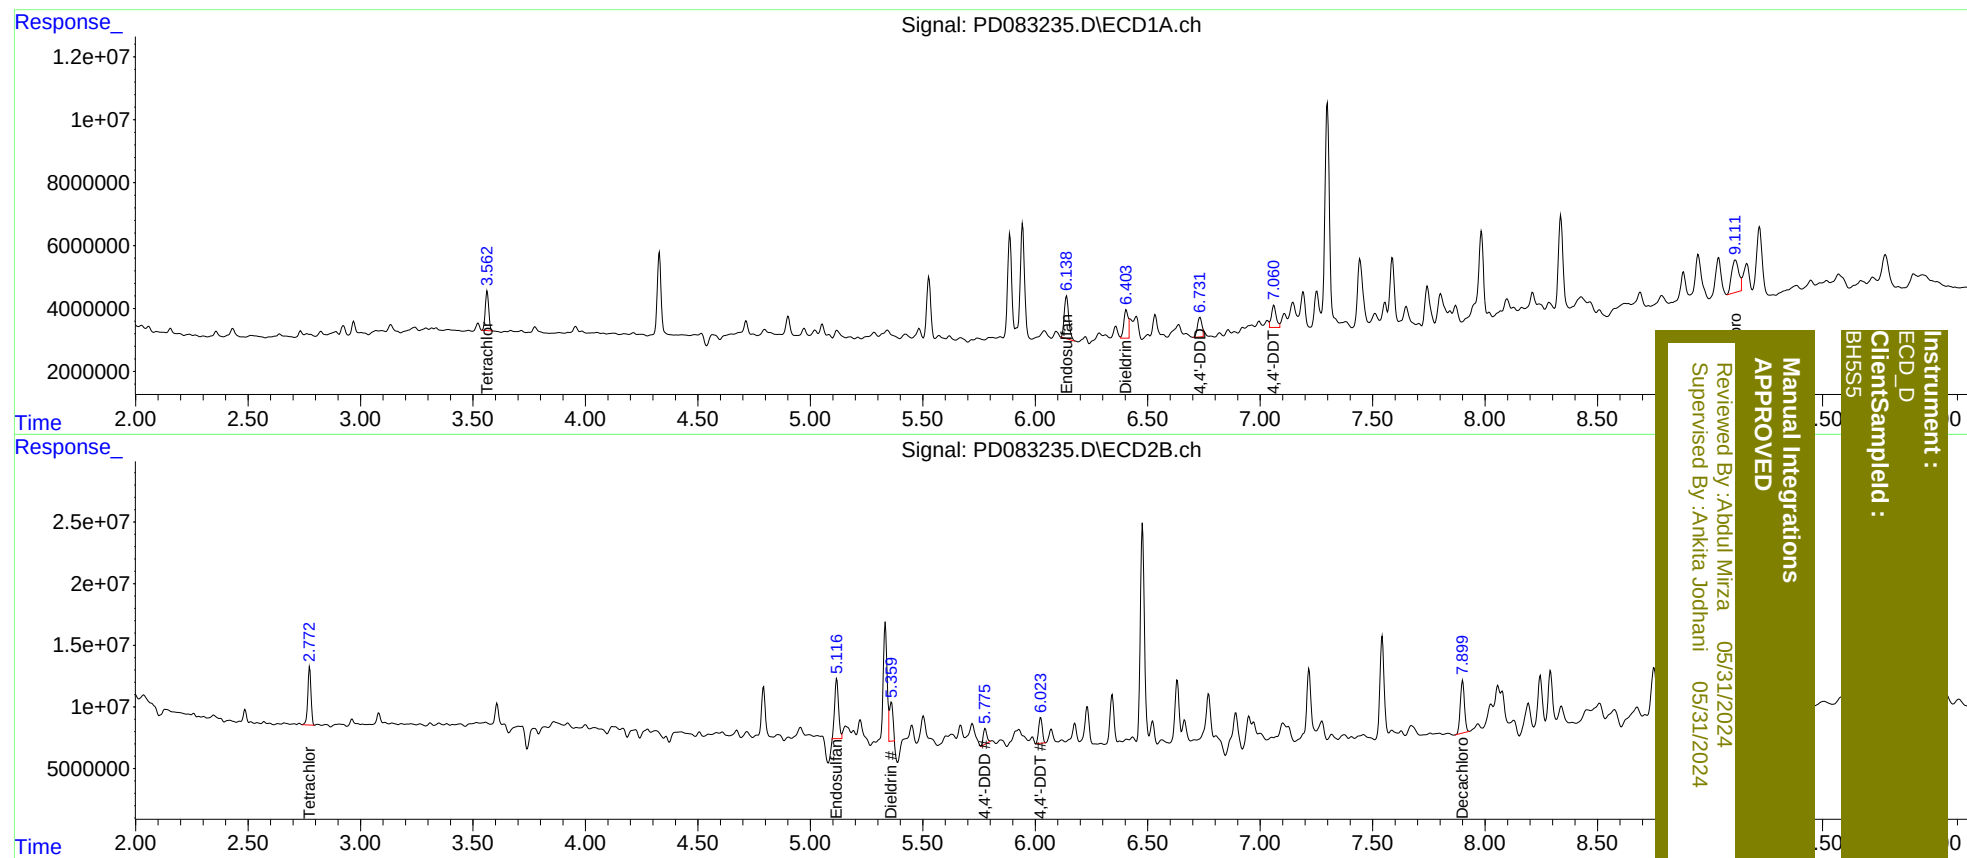

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/31/2024
Supervised By: Ankita Jodhani 05/31/2024

Instrument :
ECD_D
ClientSampled :
BH555