

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD053024\
 Data File : PD083238.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2024 14:07
 Operator : AR\AJ
 Sample : P2588-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH5S7

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/31/2024
 Supervised By : Ankita Jodhani 05/31/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 00:29:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 17 05:17:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.562	2.773	6478218	22304068	4.331m	5.736 #
2) SA Decachlor...	9.118	7.902	8104265	22180772	4.043m	5.606 #
Target Compounds						
9) A Endosulfan I	6.139	5.117	5452064	15154300	2.620m	3.360m#
13) MA Dieldrin	6.404	5.361	2523824	10807806	1.148	2.163m#
16) A 4,4'-DDD	6.732	5.778	2784973	4632847	1.796m	1.231m#
17) MA 4,4'-DDT	7.065	6.024	1671968	3608484	1.040m	0.940m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD053024\
Data File : PD083238.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2024 14:07
Operator : AR\AJ
Sample : P2588-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 00:29:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051924CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 17 05:17:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

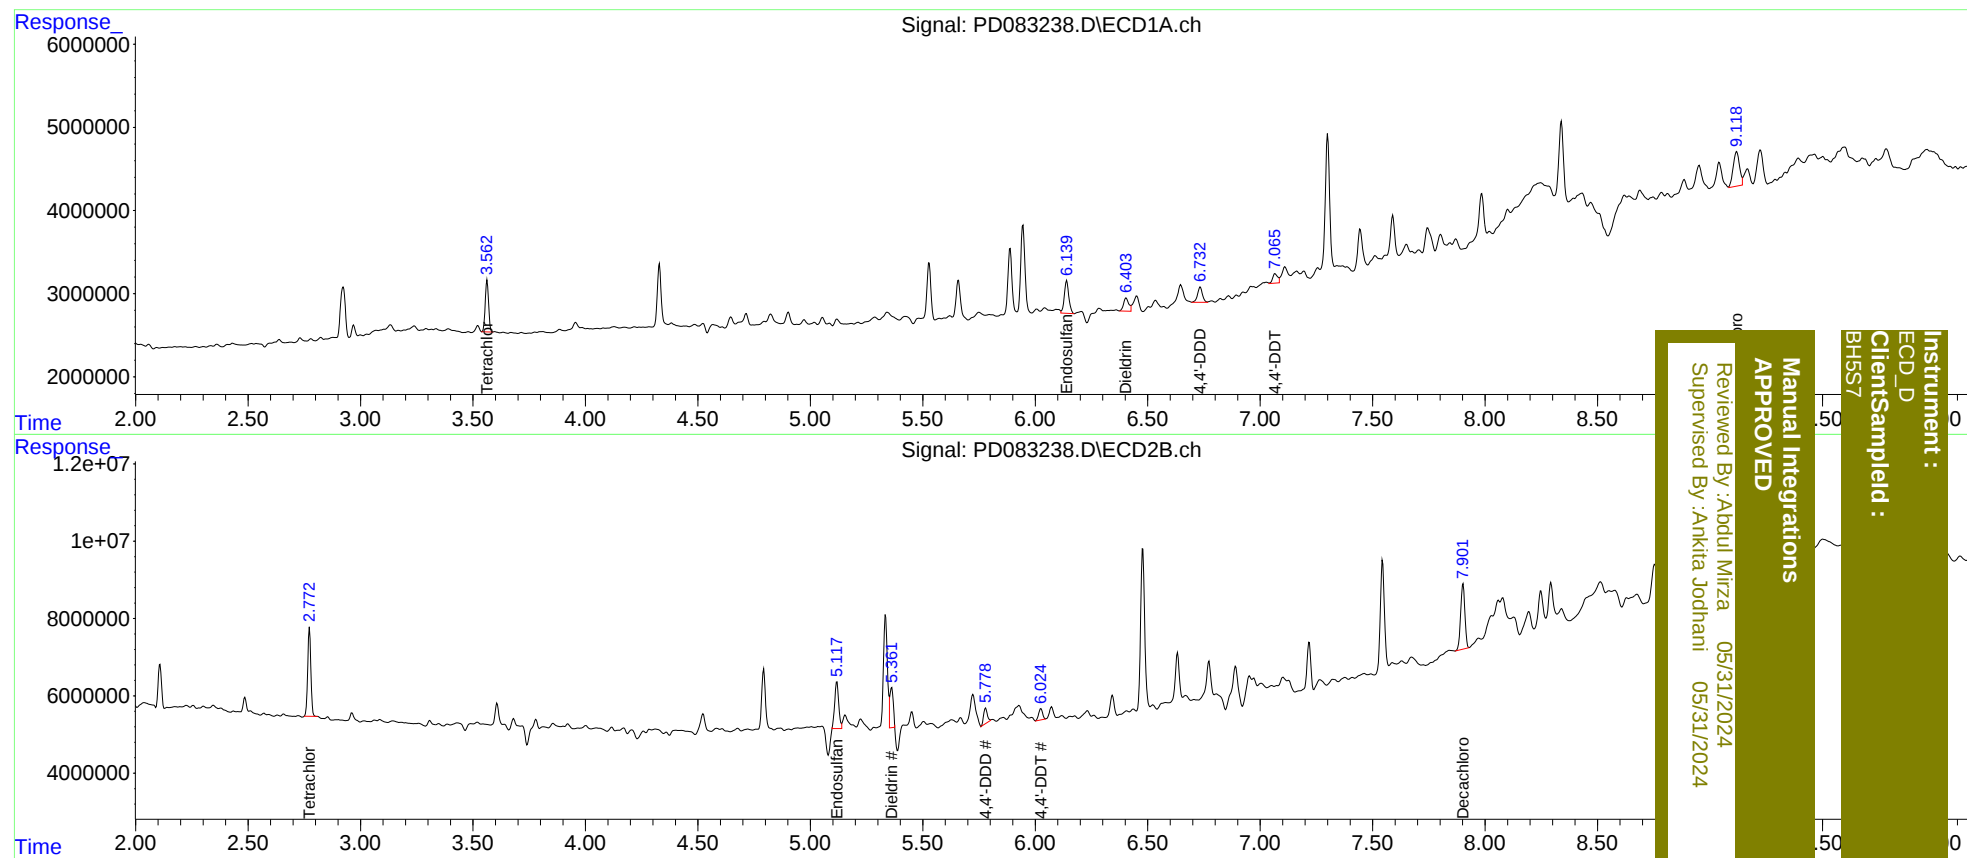

Reviewed By: Abdul Mirza 05/31/2024
Supervised By: Ankita Jodhani 05/31/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BH557