

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD053119\
 Data File : PD053463.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 May 2019 14:45
 Operator : SM\AJ
 Sample : PB120225BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK25

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 23:19:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052119CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed May 22 06:53:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.317	3.986	16791379	25056248	22.917	25.449
2)	SA Decachlor...	8.016	9.030	26283285	39677177	39.733	38.411
Target Compounds							
6)	B beta-BHC	0.000	4.871f	0	449010	N.D.	0.765
7)	B delta-BHC	0.000	5.018	0	480190	N.D.	0.395


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD053119\
Data File : PD053463.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 May 2019 14:45
Operator : SM\AJ
Sample : PB120225BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 23:19:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052119CLP.M
Quant Title : GC Extractables
QLast Update : Wed May 22 06:53:42 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

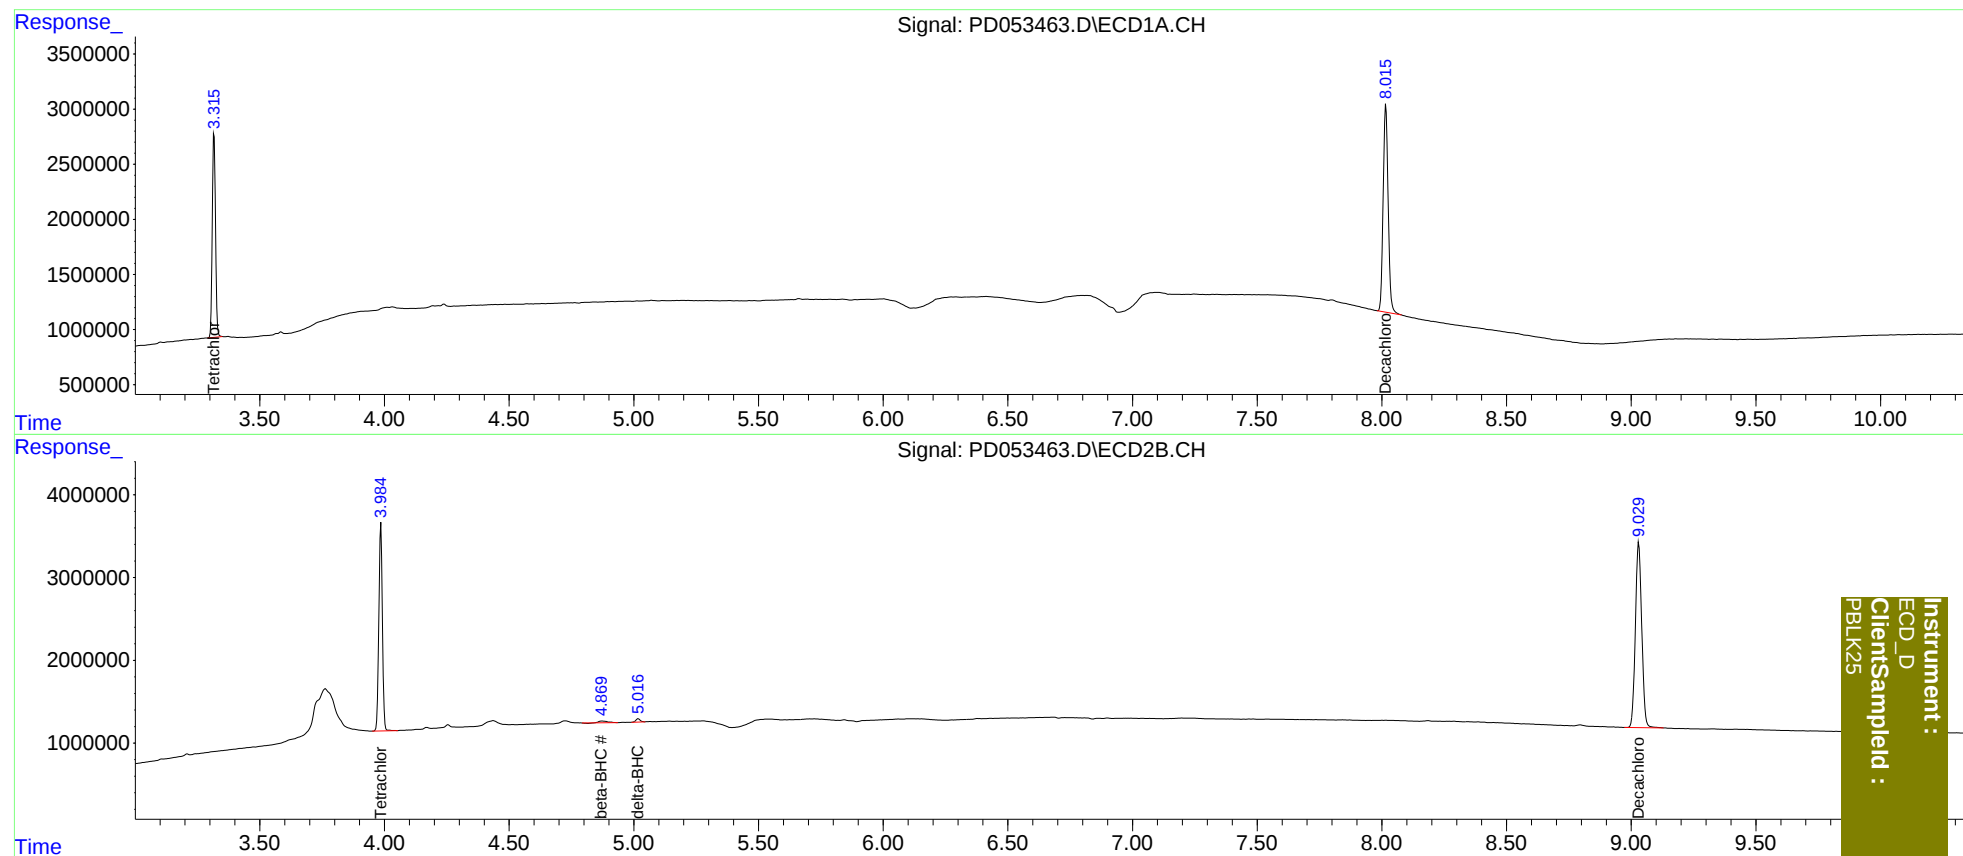


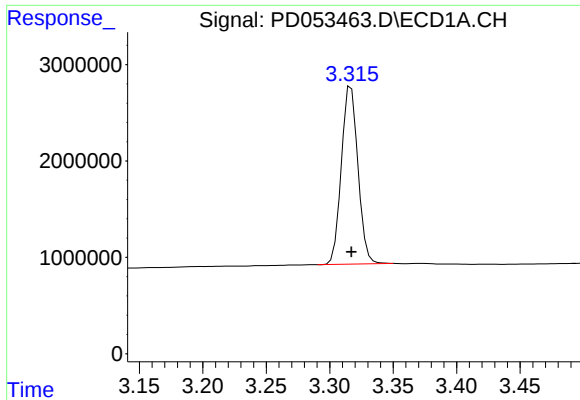

#1 Tetrachloro-m-xylene


R.T.: 3.317 min
Delta R.T.: 0.000 min
Response: 16791379
Conc: 22.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK25

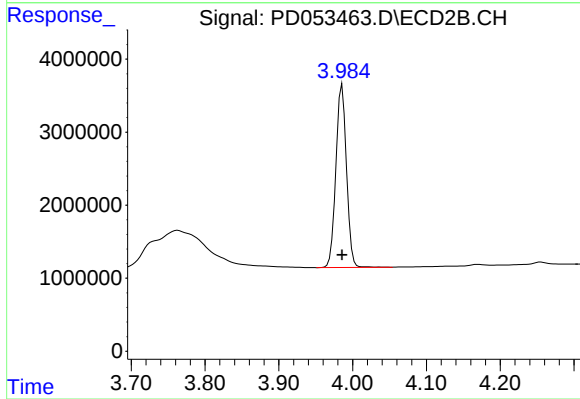


#1 Tetrachloro-m-xylene

R.T.: 3.986 min
Delta R.T.: 0.000 min
Response: 25056248
Conc: 25.45 ng/ml

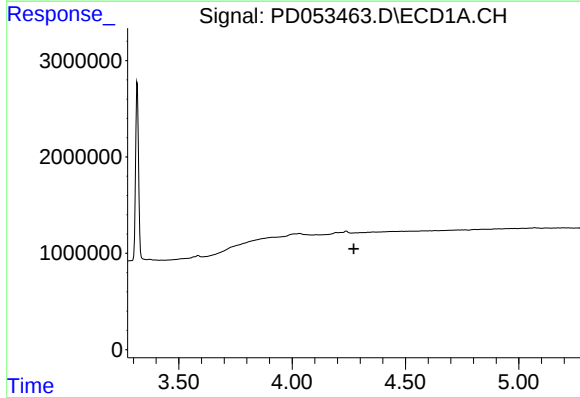


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.272 min
Response: 0
Conc: N.D.

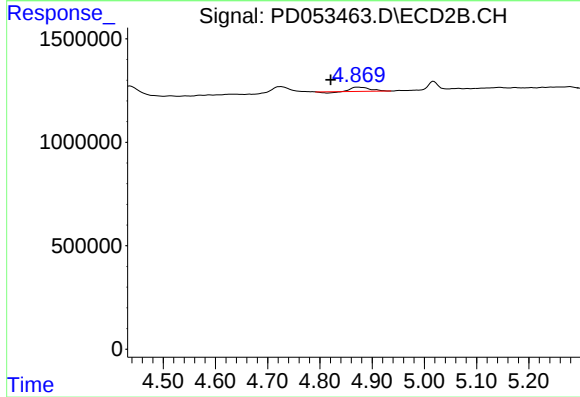

#6 beta-BHC


R.T.: 4.871 min
Delta R.T.: 0.050 min
Response: 449010
Conc: 0.77 ng/ml

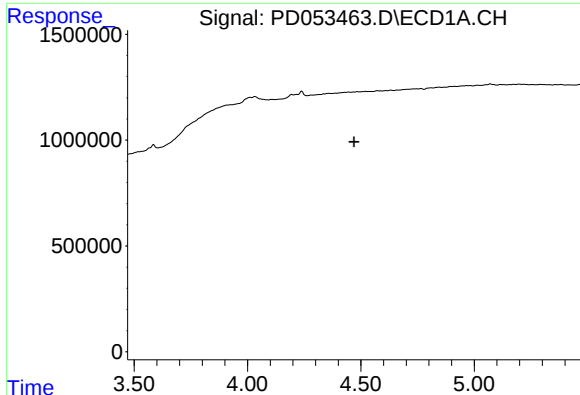

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.470 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PBLK25

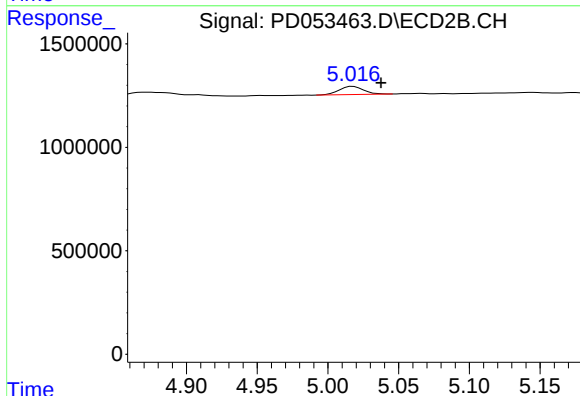


#7 delta-BHC

R.T.: 5.018 min
Delta R.T.: -0.020 min
Response: 480190
Conc: 0.39 ng/ml

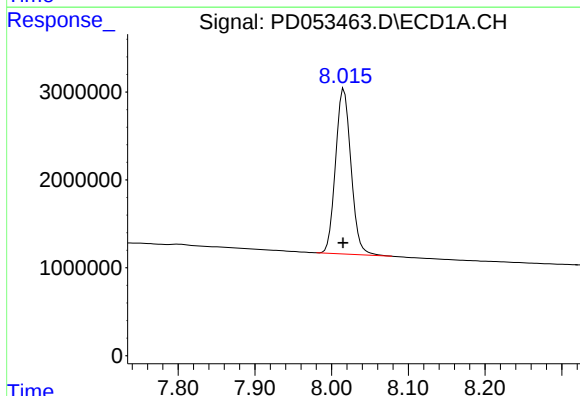

#27 Decachlorobiphenyl

R.T.: 8.016 min
Delta R.T.: 0.001 min
Response: 26283285
Conc: 39.73 ng/ml

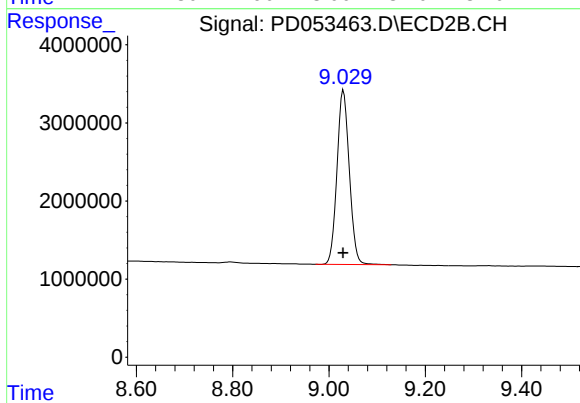

#27 Decachlorobiphenyl

R.T.: 9.030 min
Delta R.T.: 0.000 min
Response: 39677177
Conc: 38.41 ng/ml