

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060120\
 Data File : PD058227.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2020 09:38
 Operator : AJ\MA
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 12:47:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060120.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 01 12:24:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.215	3.866	14994936	22628244	19.156	18.945
28)	SA Decachlor...	7.857	8.853	16560324	23546286	19.277	19.657
Target Compounds							
7)	B delta-BHC	0.000	4.889f	0	929315	N.D.	0.597 #
9)	A Endosulfan I	5.186	6.062	7100414	11572954	8.587	8.695
10)	B gamma-Chl...	5.078	5.942	8136774	12901684	8.878	8.955
12)	B 4,4'-DDE	5.304	6.174	16978951	24738003	17.642	17.682
13)	MA Dieldrin	5.423	6.317	10232193	21312407	17.640	16.995
15)	B Endosulfa...	5.949	0.000	109788	0	0.166	N.D. #
19)	B Endosulfa...	6.326	7.088	10751513	19067606	17.330	17.254
20)	A Methoxychlor	6.594	7.416	17989044	39325114	87.274	84.367
21)	B Endrin ke...	6.806	7.553	10297778	20124540	17.363	16.853
25)	Chlordane-3	5.078	5.942	8136774	12901684	97.318	73.738
27)	Chlordane-5	5.949	0.000	109788	0	5.684	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060120\
Data File : PD058227.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2020 09:38
Operator : AJ\MA
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 12:47:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060120.M
Quant Title : GC Extractables
QLast Update : Mon Jun 01 12:24:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

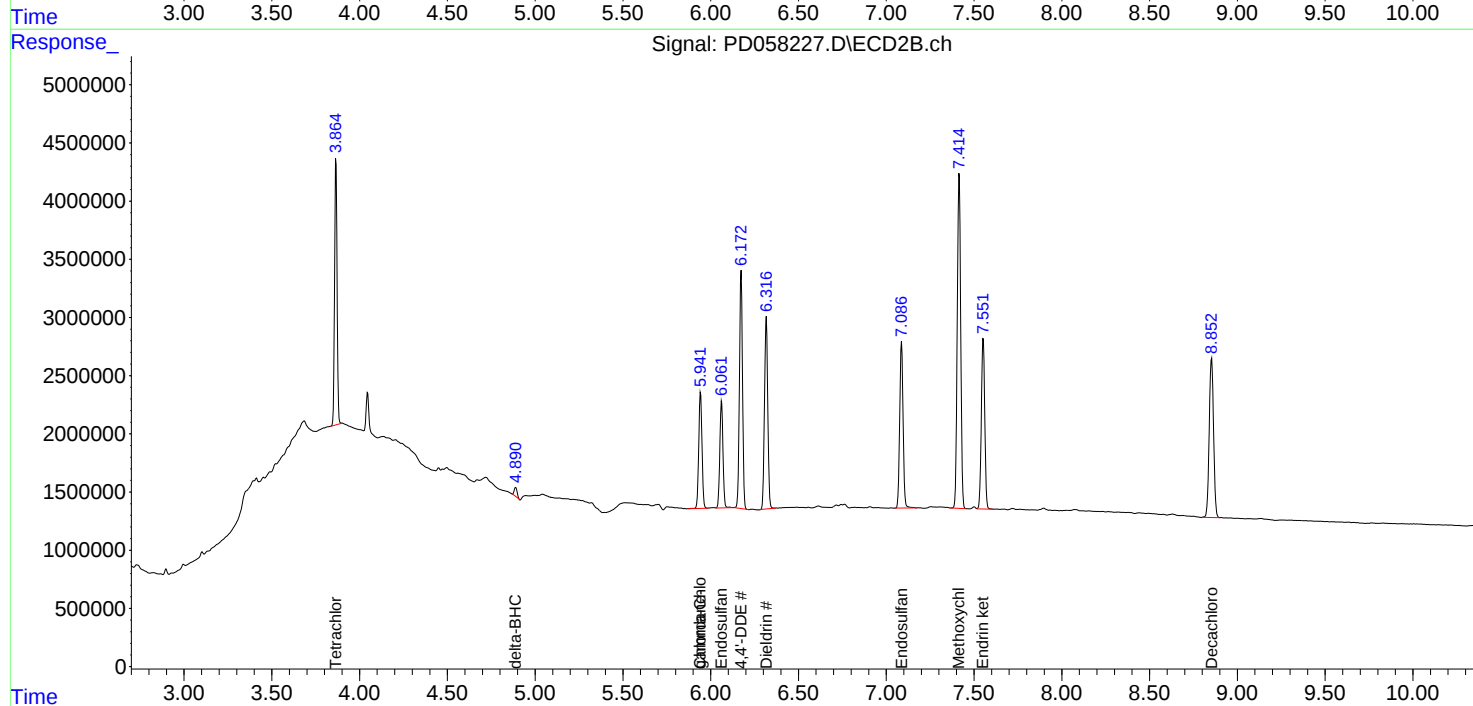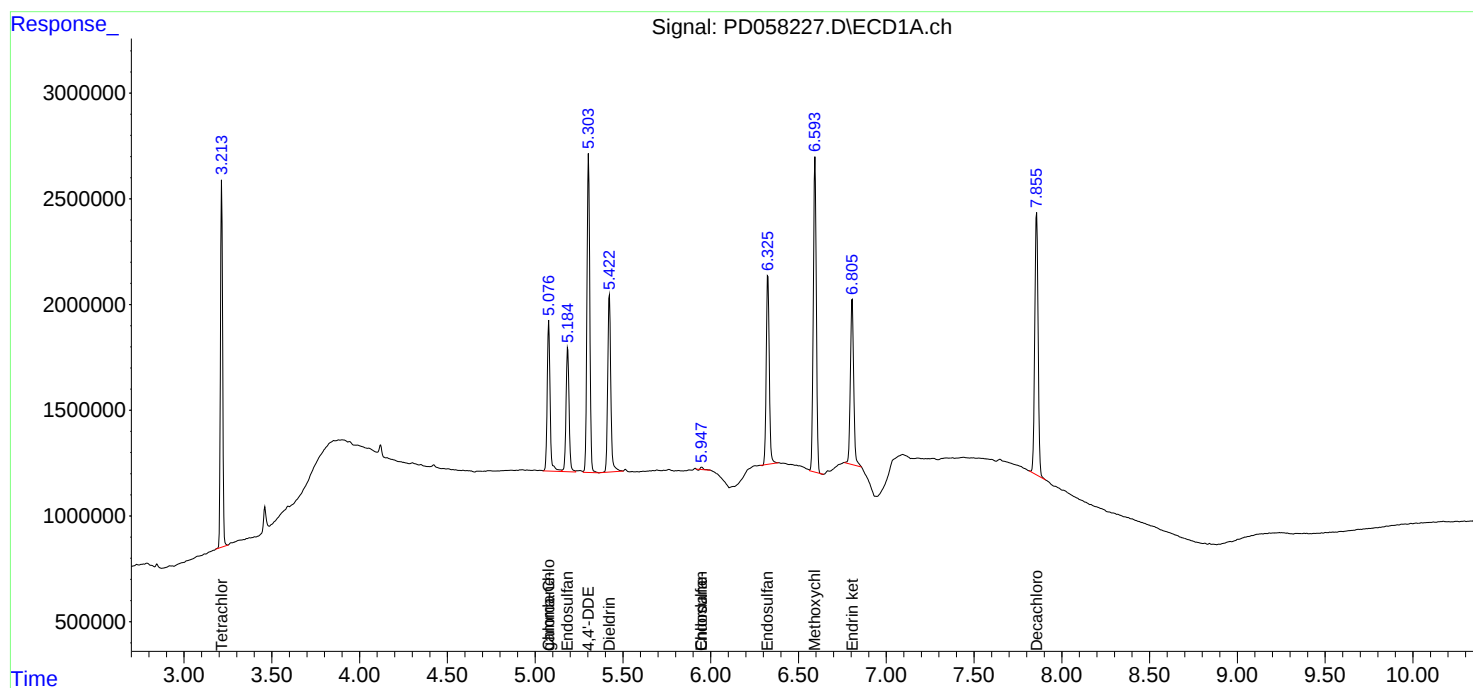


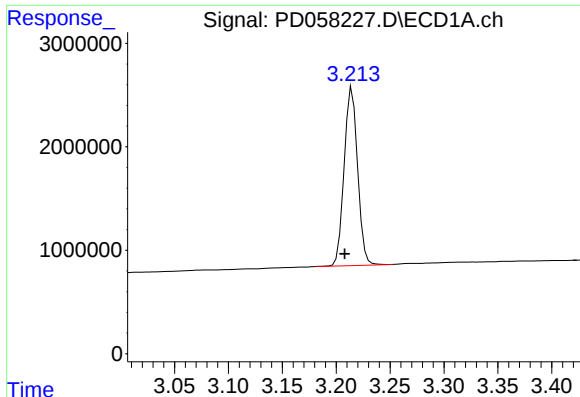

#1 Tetrachloro-m-xylene


R.T.: 3.215 min
Delta R.T.: 0.007 min
Response: 14994936
Conc: 19.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

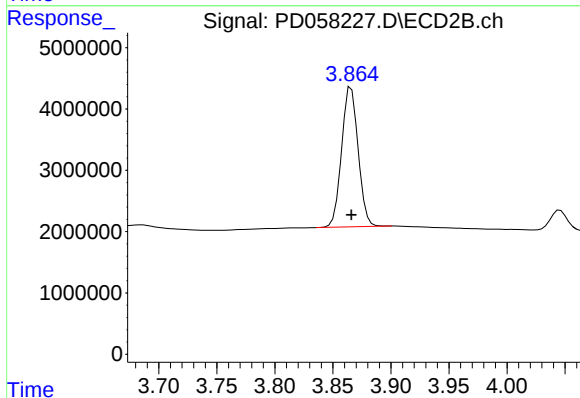


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 22628244
Conc: 18.95 ng/ml

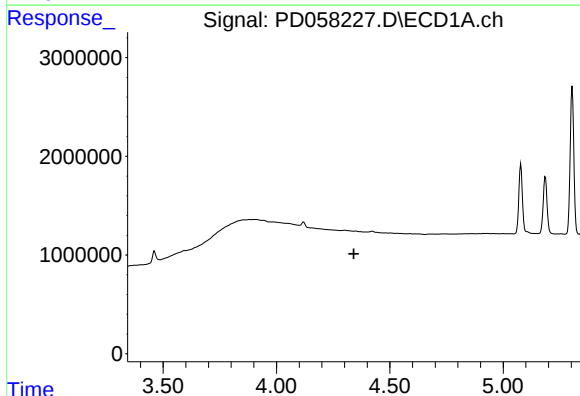


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.342 min
Response: 0
Conc: N.D.

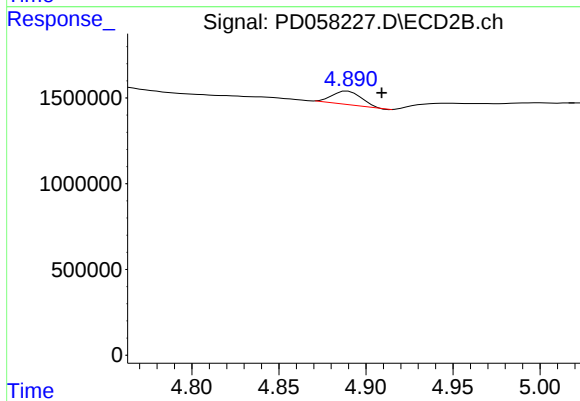

#7 delta-BHC


R.T.: 4.889 min
Delta R.T.: -0.020 min
Response: 929315
Conc: 0.60 ng/ml

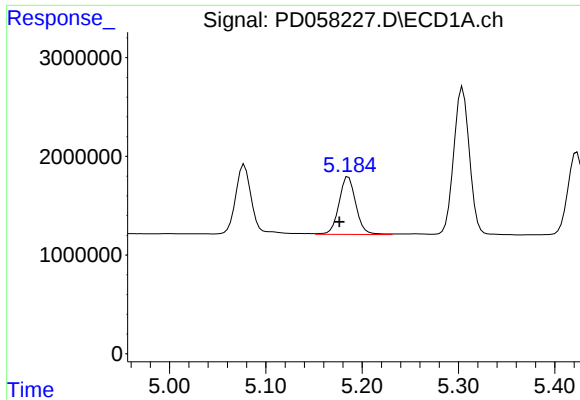

#9 Endosulfan I


R.T.: 5.186 min
Delta R.T.: 0.009 min
Response: 7100414
Conc: 8.59 ng/ml

Instrument :
ECD_D
ClientSampleId :

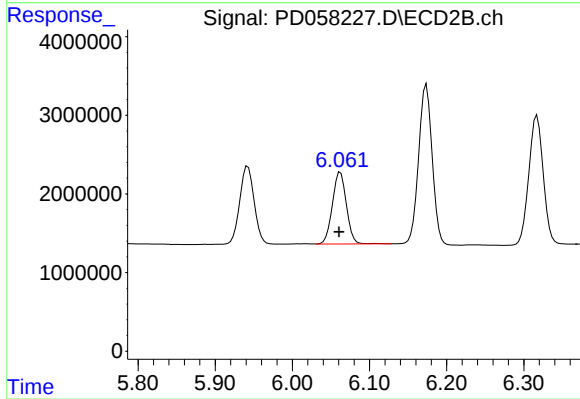


#9 Endosulfan I

R.T.: 6.062 min
Delta R.T.: 0.002 min
Response: 11572954
Conc: 8.69 ng/ml

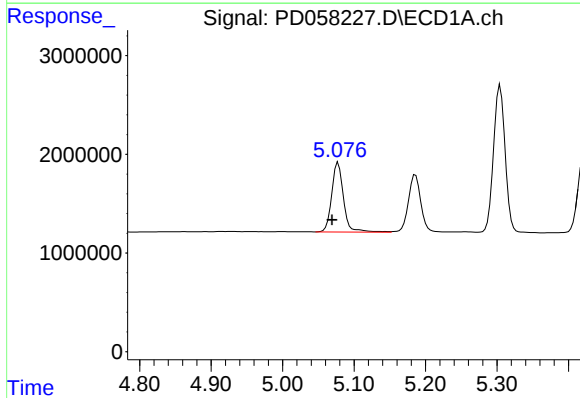


#10 gamma-Chlordane

R.T.: 5.078 min
Delta R.T.: 0.009 min
Response: 8136774
Conc: 8.88 ng/ml

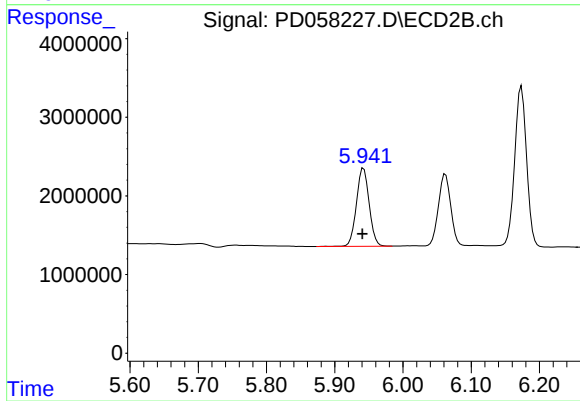

#10 gamma-Chlordane


R.T.: 5.942 min
Delta R.T.: 0.002 min
Response: 12901684
Conc: 8.96 ng/ml

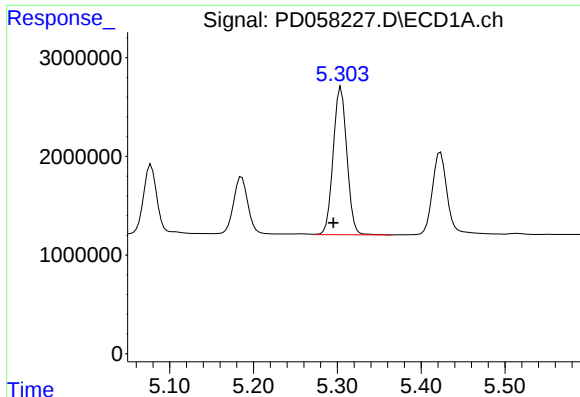

#12 4,4'-DDE


R.T.: 5.304 min
Delta R.T.: 0.009 min
Response: 16978951
Conc: 17.64 ng/ml

Instrument :
ECD_D
ClientSampleId :

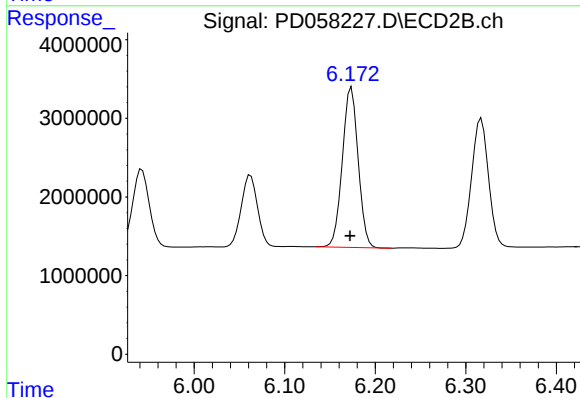


#12 4,4'-DDE

R.T.: 6.174 min
Delta R.T.: 0.001 min
Response: 24738003
Conc: 17.68 ng/ml

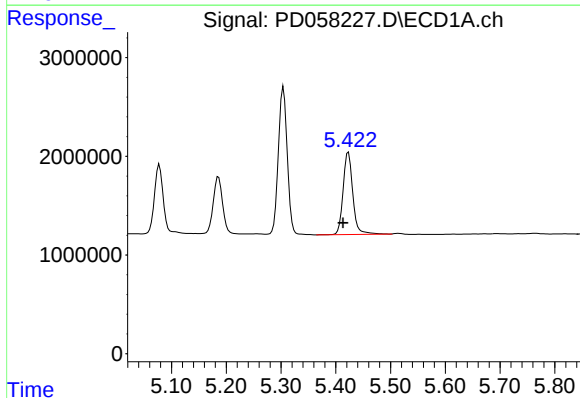


#13 Dieldrin

R.T.: 5.423 min
Delta R.T.: 0.010 min
Response: 10232193
Conc: 17.64 ng/ml

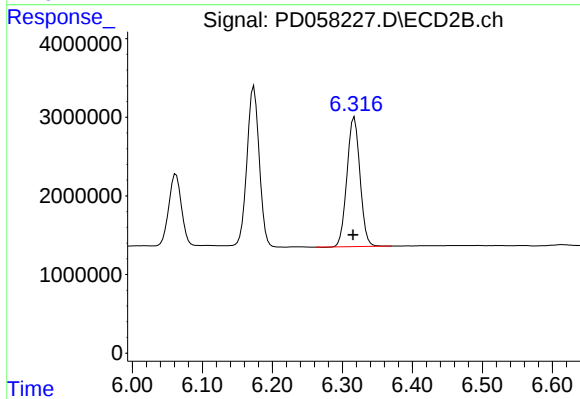

#13 Dieldrin


R.T.: 6.317 min
Delta R.T.: 0.002 min
Response: 21312407
Conc: 16.99 ng/ml

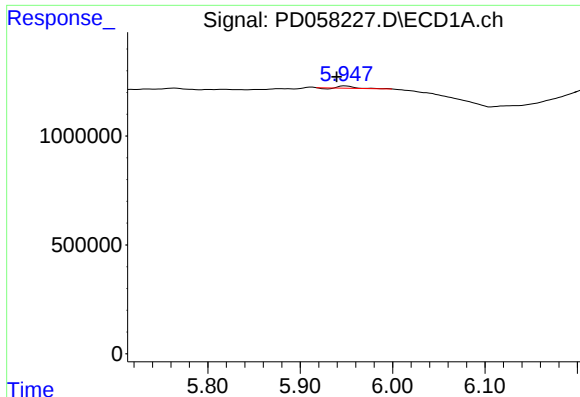

#15 Endosulfan II


R.T.: 5.949 min
Delta R.T.: 0.009 min
Response: 109788
Conc: 0.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

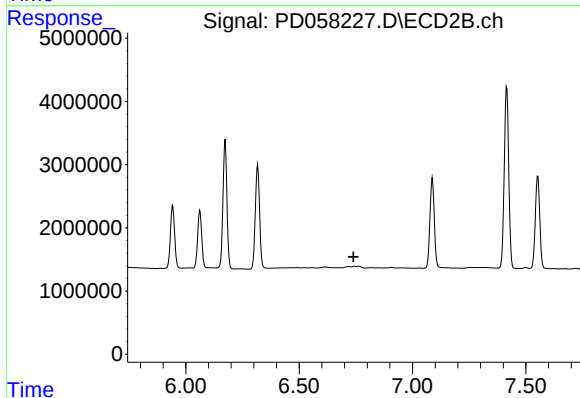


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.740 min
Response: 0
Conc: N.D.

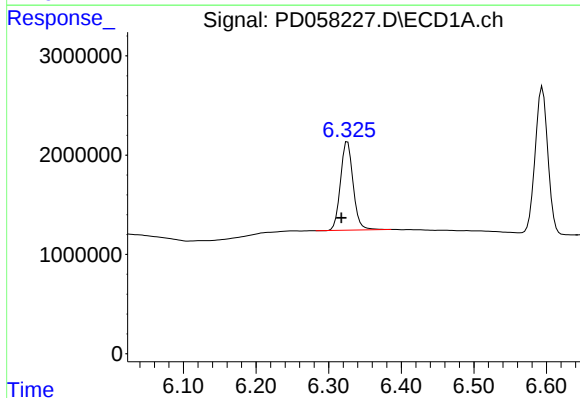


#19 Endosulfan Sulfate

R.T.: 6.326 min
Delta R.T.: 0.008 min
Response: 10751513
Conc: 17.33 ng/ml

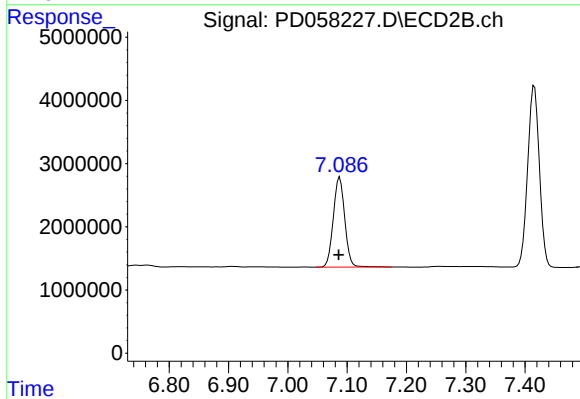

#19 Endosulfan Sulfate


R.T.: 7.088 min
Delta R.T.: 0.002 min
Response: 19067606
Conc: 17.25 ng/ml

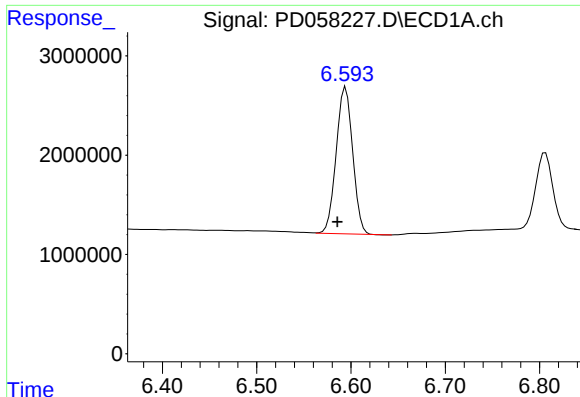

#20 Methoxychlor


R.T.: 6.594 min
Delta R.T.: 0.009 min
Response: 17989044
Conc: 87.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

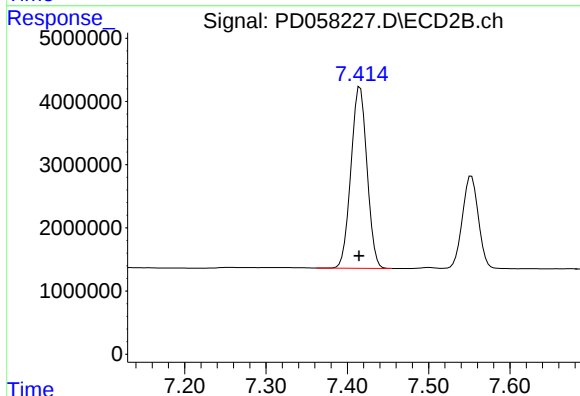


#20 Methoxychlor

R.T.: 7.416 min
Delta R.T.: 0.001 min
Response: 39325114
Conc: 84.37 ng/ml

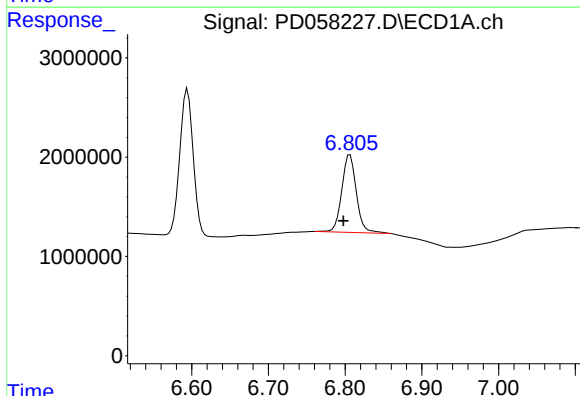


#21 Endrin ketone

R.T.: 6.806 min
Delta R.T.: 0.008 min
Response: 10297778
Conc: 17.36 ng/ml

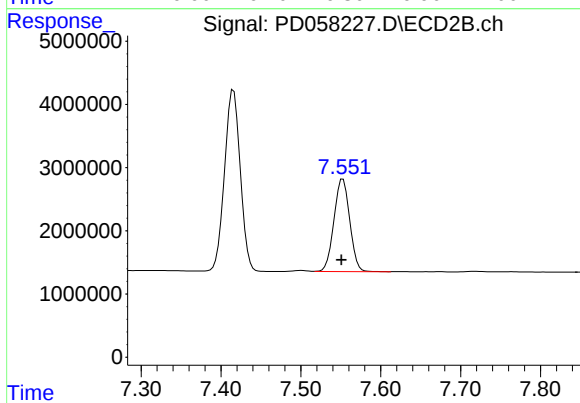

#21 Endrin ketone


R.T.: 7.553 min
Delta R.T.: 0.002 min
Response: 20124540
Conc: 16.85 ng/ml

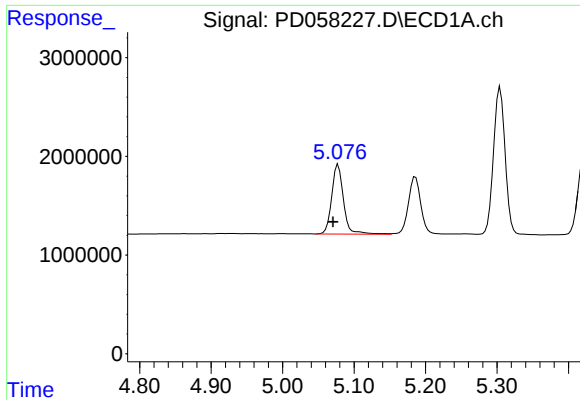

#25 Chlordane-3


R.T.: 5.078 min
Delta R.T.: 0.007 min
Response: 8136774
Conc: 97.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

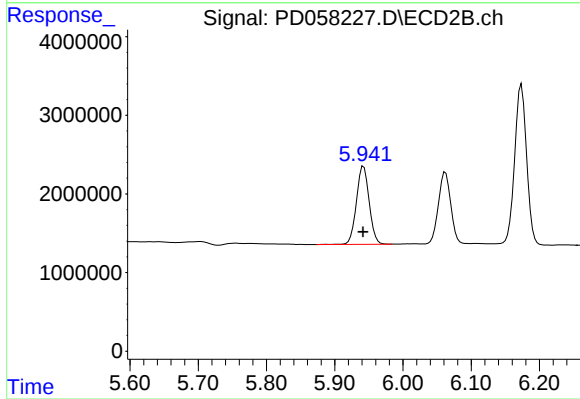


#25 Chlordane-3

R.T.: 5.942 min
Delta R.T.: 0.000 min
Response: 12901684
Conc: 73.74 ng/ml

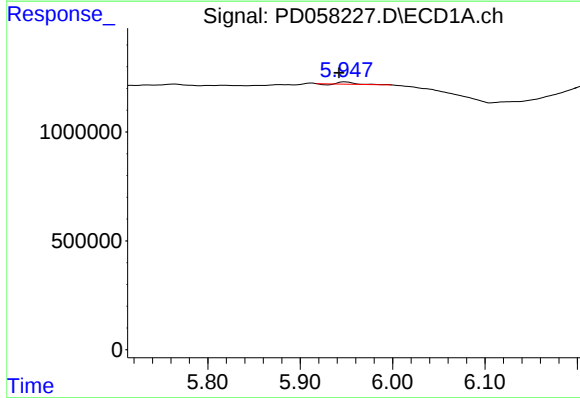


#27 Chlordane-5

R.T.: 5.949 min
Delta R.T.: 0.006 min
Response: 109788
Conc: 5.68 ng/ml

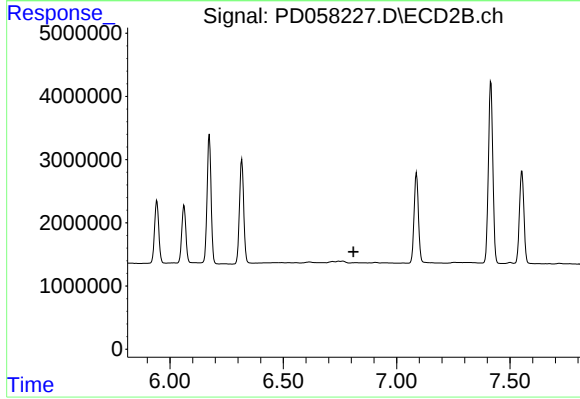

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.810 min
Response: 0
Conc: N.D.

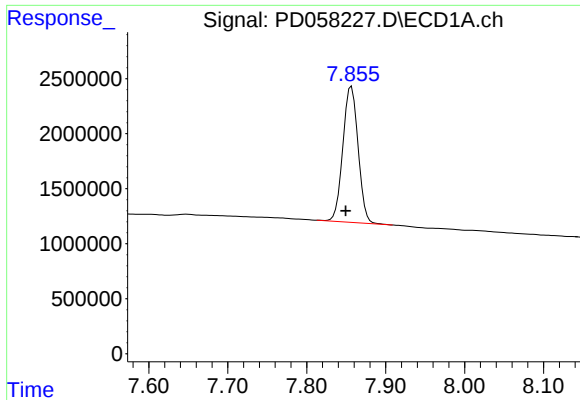

#28 Decachlorobiphenyl

R.T.: 7.857 min
Delta R.T.: 0.007 min
Response: 16560324
Conc: 19.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

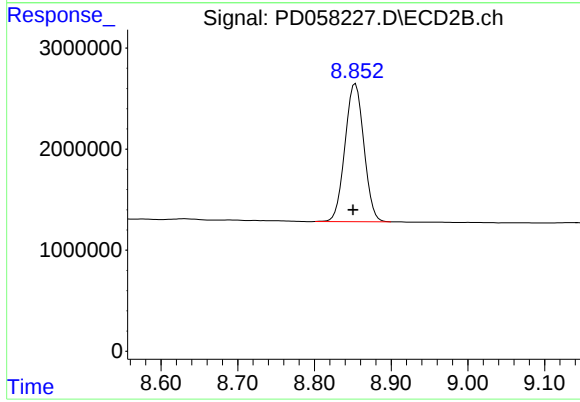

#28 Decachlorobiphenyl

R.T.: 8.853 min
Delta R.T.: 0.003 min
Response: 23546286
Conc: 19.66 ng/ml