

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060120\
 Data File : PD058248.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2020 16:39
 Operator : AJ\MA
 Sample : L2505-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 03:34:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060120.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 01 12:24:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.866	19171968	27435415	24.492	22.970
28)	SA Decachlor...	7.850	8.852	18379164	25381192	21.394	21.189
Target Compounds							
3)	MA gamma-BHC...	3.910	0.000	1851727	0	1.608	N.D. #
4)	MA Heptachlor	4.195	0.000	463205	0	0.648	N.D. #
6)	B beta-BHC	4.160	0.000	608248	0	1.297	N.D. #
7)	B delta-BHC	4.337	4.887f	505192	2192444	0.458	1.408 #
8)	B Heptachlo...	0.000	5.702	0	3370431	N.D.	2.410 #
12)	B 4,4'-DDE	0.000	6.163	0	768759	N.D.	0.549 #
15)	B Endosulfa...	0.000	6.765f	0	508681	N.D.	0.404 #
19)	B Endosulfa...	6.293f	0.000	1415783	0	2.282	N.D. #
20)	A Methoxychlor	6.582	7.419	108046	2048974	0.524	4.396 #
21)	B Endrin ke...	6.803	0.000	904617	0	1.525	N.D. #
23)	Chlordane-1	4.054f	0.000	1540324	0	76.183	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060120\
Data File : PD058248.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2020 16:39
Operator : AJ\MA
Sample : L2505-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 03:34:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060120.M
Quant Title : GC Extractables
QLast Update : Mon Jun 01 12:24:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

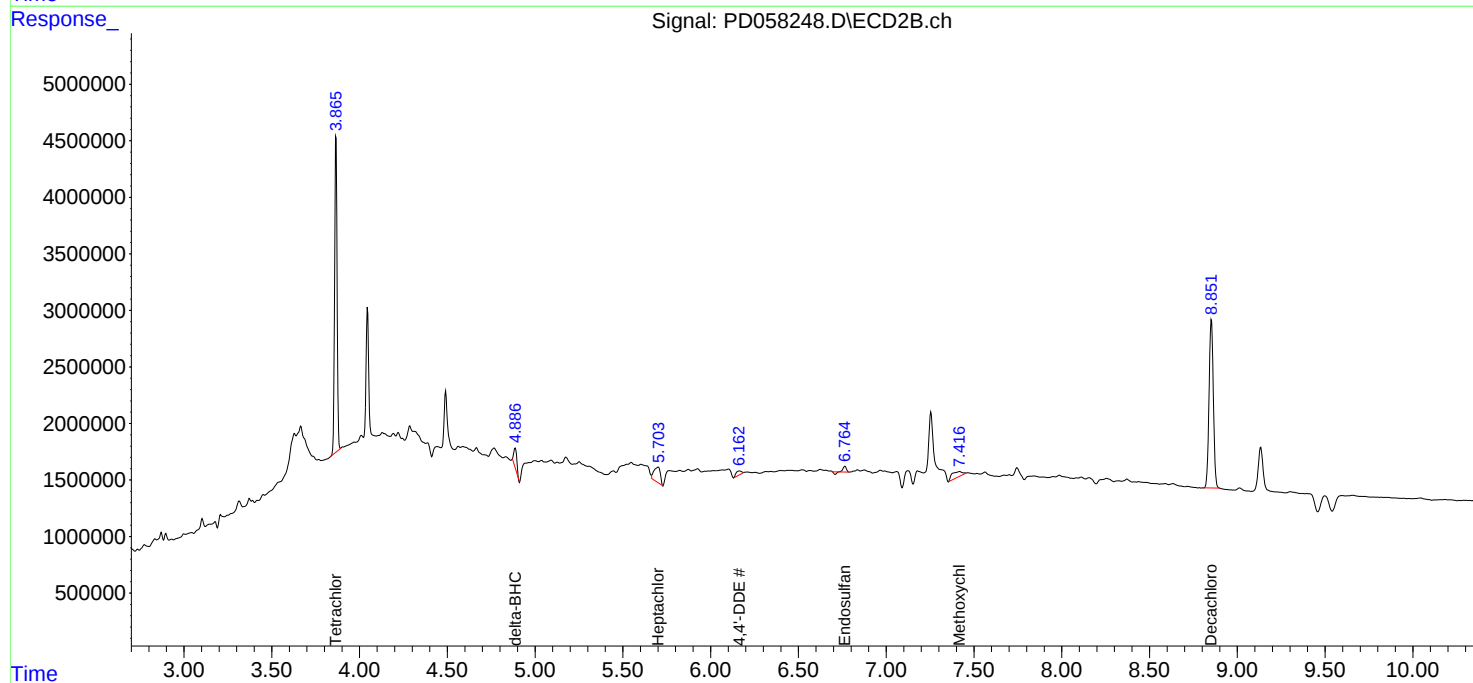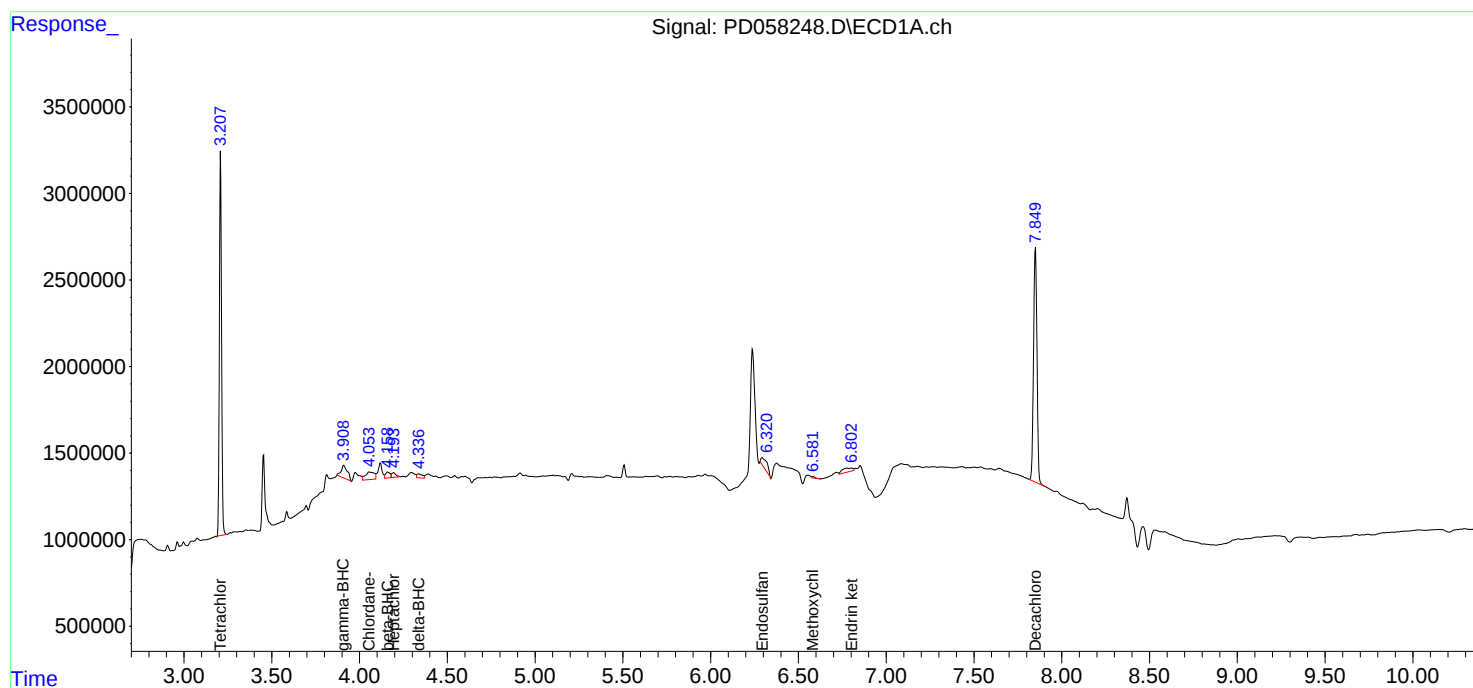


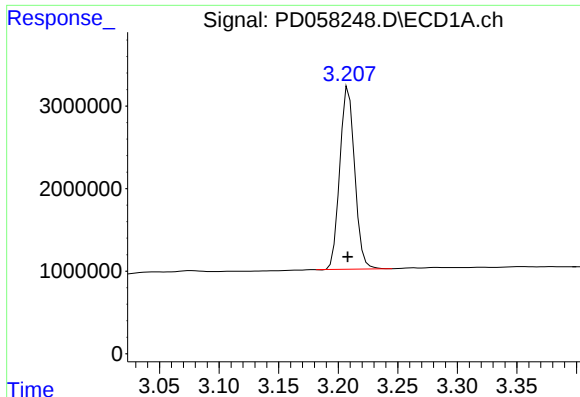

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: 0.000 min
Response: 19171968
Conc: 24.49 ng/ml

Instrument :
ECD_D
ClientSampleId :

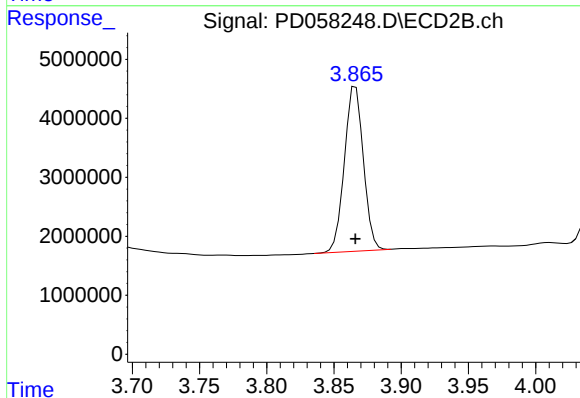


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 27435415
Conc: 22.97 ng/ml

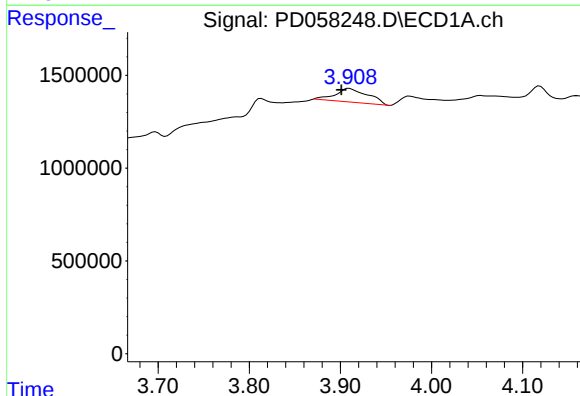


#3 gamma-BHC (Lindane)

R.T.: 3.910 min
Delta R.T.: 0.008 min
Response: 1851727
Conc: 1.61 ng/ml

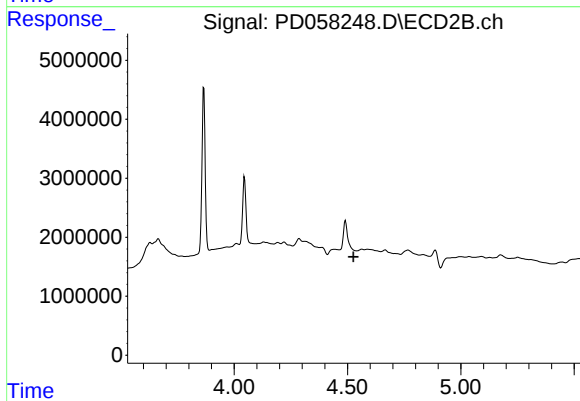

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.527 min
Response: 0
Conc: N.D.

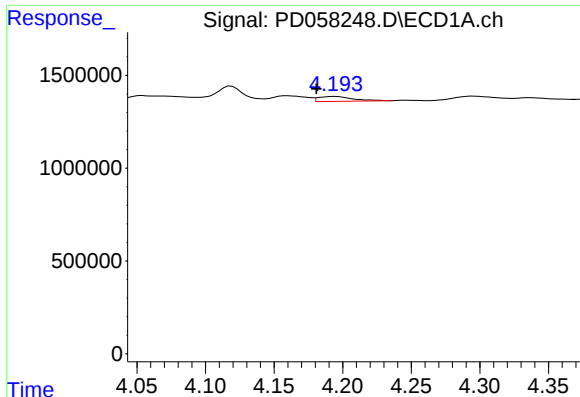

#4 Heptachlor


R.T.: 4.195 min
Delta R.T.: 0.014 min
Response: 463205
Conc: 0.65 ng/ml

Instrument :
ECD_D
ClientSampleId :

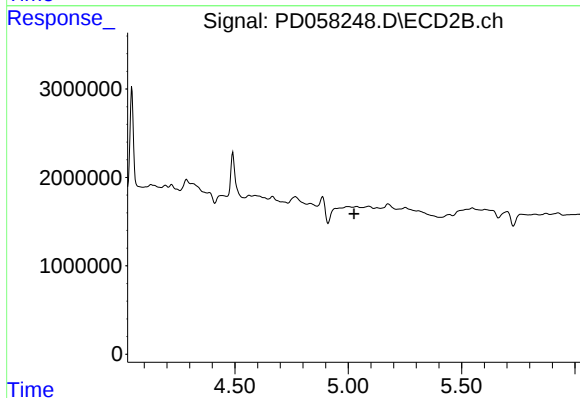


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.026 min
Response: 0
Conc: N.D.

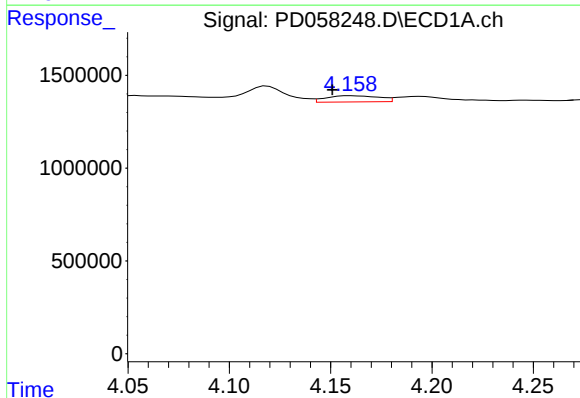


#6 beta-BHC

R.T.: 4.160 min
Delta R.T.: 0.009 min
Response: 608248
Conc: 1.30 ng/ml

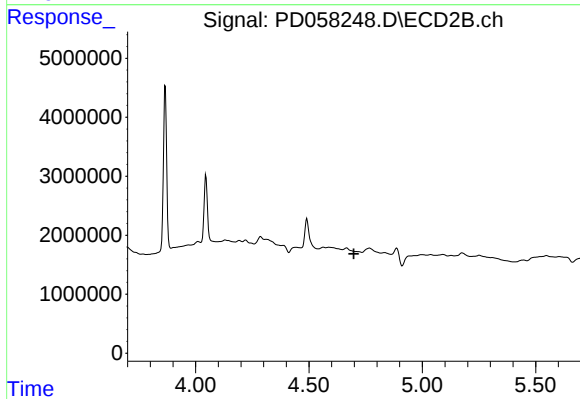

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.698 min
Response: 0
Conc: N.D.

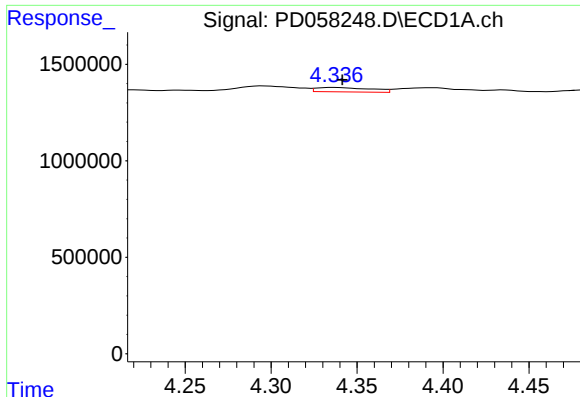

#7 delta-BHC


R.T.: 4.337 min
Delta R.T.: -0.004 min
Response: 505192
Conc: 0.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

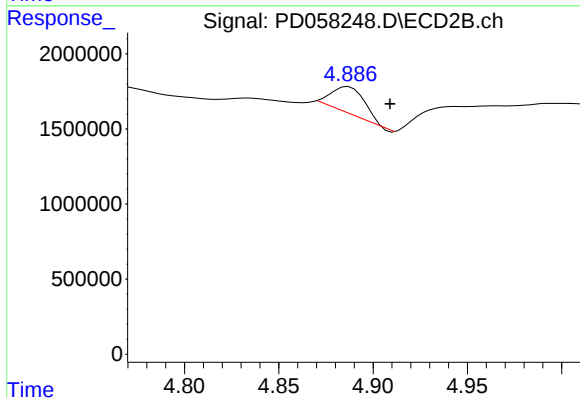


#7 delta-BHC

R.T.: 4.887 min
Delta R.T.: -0.022 min
Response: 2192444
Conc: 1.41 ng/ml

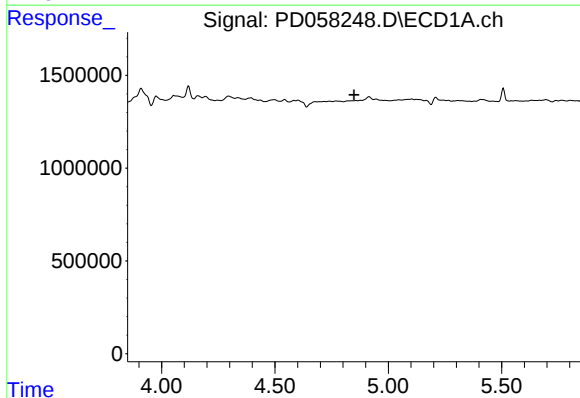


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.849 min
Response: 0
Conc: N.D.

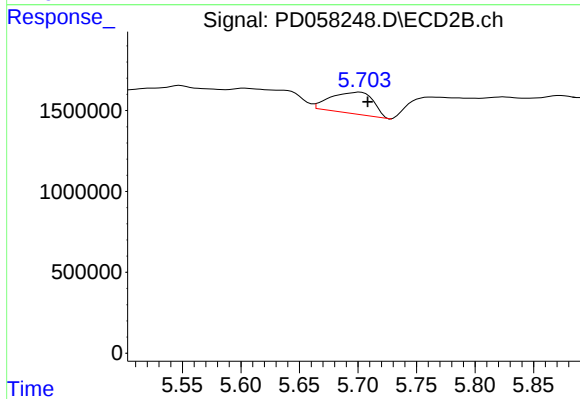

#8 Heptachlor epoxide


R.T.: 5.702 min
Delta R.T.: -0.007 min
Response: 3370431
Conc: 2.41 ng/ml

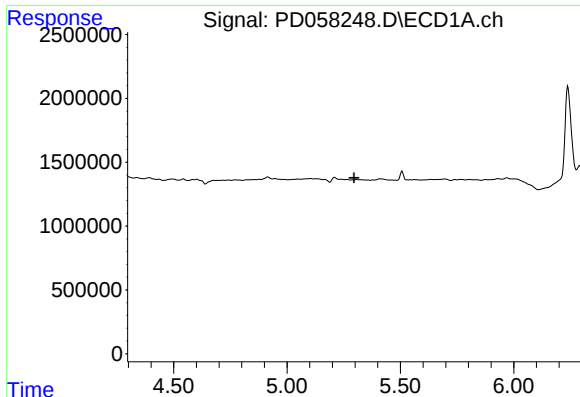

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.295 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

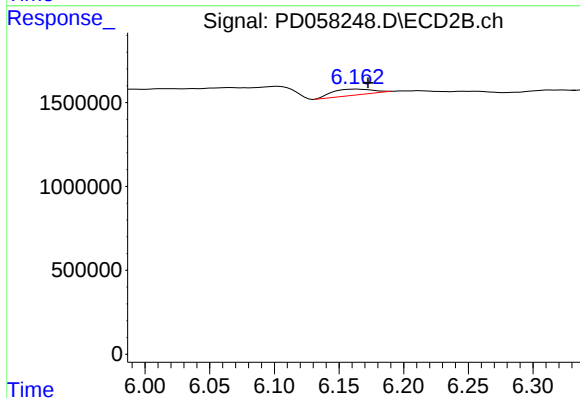


#12 4,4'-DDE

R.T.: 6.163 min
Delta R.T.: -0.009 min
Response: 768759
Conc: 0.55 ng/ml

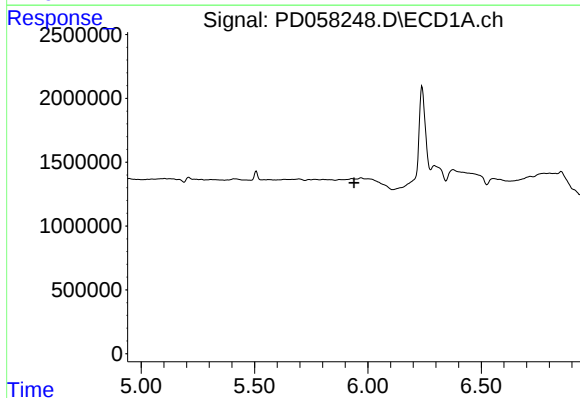


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.939 min
Response: 0
Conc: N.D.

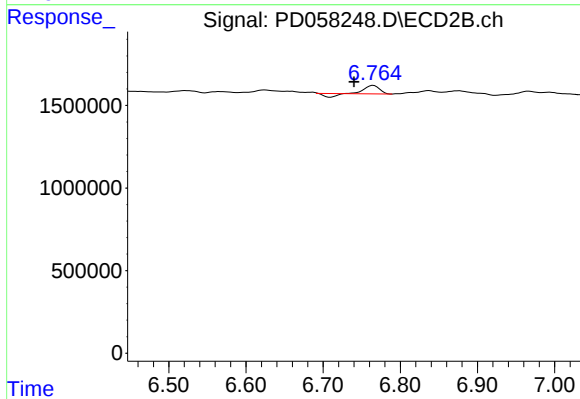

#15 Endosulfan II


R.T.: 6.765 min
Delta R.T.: 0.025 min
Response: 508681
Conc: 0.40 ng/ml

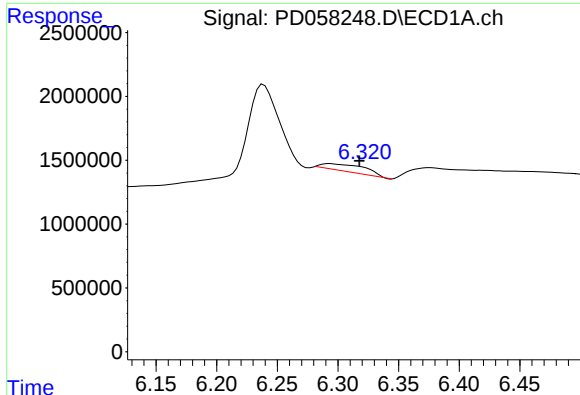

#19 Endosulfan Sulfate


R.T.: 6.293 min
Delta R.T.: -0.024 min
Response: 1415783
Conc: 2.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

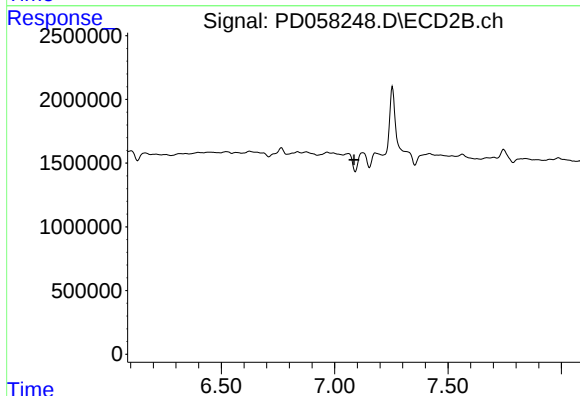


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.086 min
Response: 0
Conc: N.D.

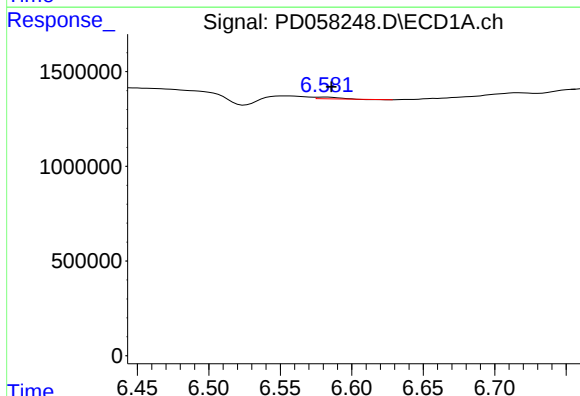


#20 Methoxychlor

R.T.: 6.582 min
Delta R.T.: -0.004 min
Response: 108046
Conc: 0.52 ng/ml

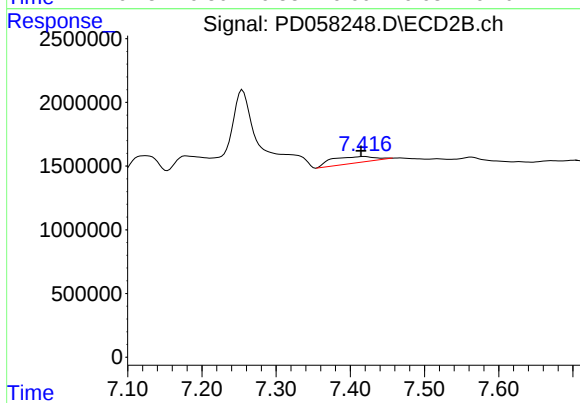

#20 Methoxychlor


R.T.: 7.419 min
Delta R.T.: 0.004 min
Response: 2048974
Conc: 4.40 ng/ml

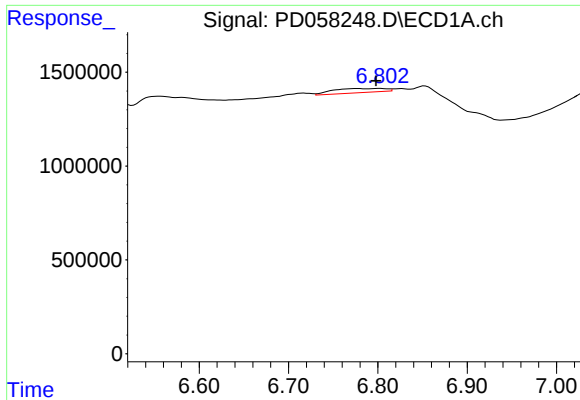

#21 Endrin ketone


R.T.: 6.803 min
Delta R.T.: 0.005 min
Response: 904617
Conc: 1.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

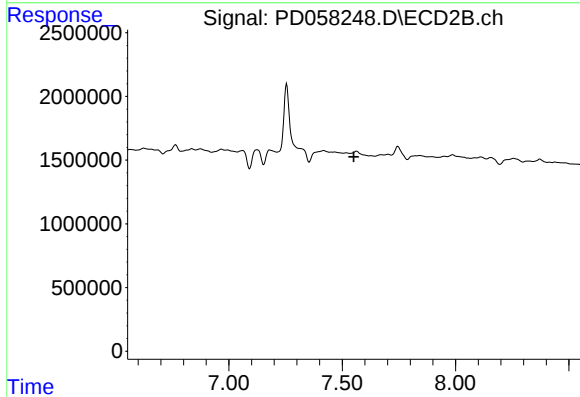


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.551 min
Response: 0
Conc: N.D.

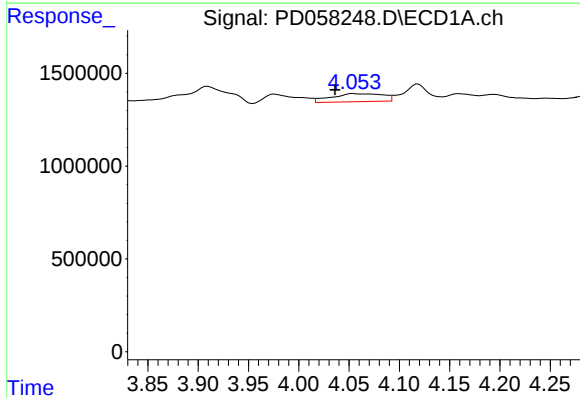


#23 Chlordane-1

R.T.: 4.054 min
Delta R.T.: 0.018 min
Response: 1540324
Conc: 76.18 ng/ml

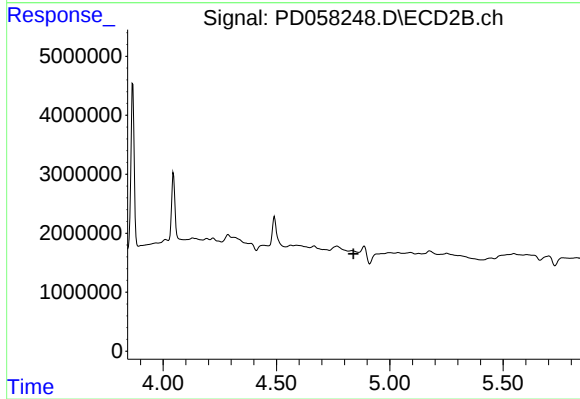

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.840 min
Response: 0
Conc: N.D.

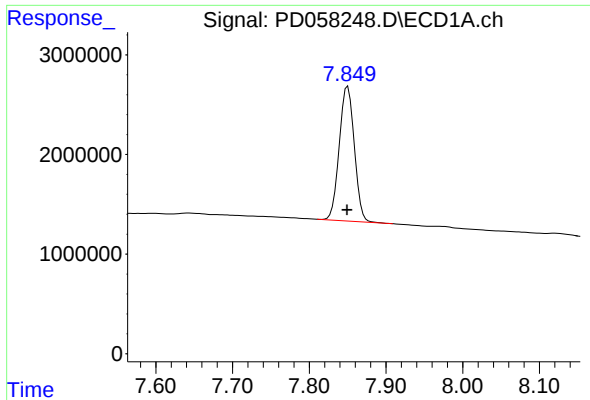

#28 Decachlorobiphenyl

R.T.: 7.850 min
Delta R.T.: 0.000 min
Response: 18379164
Conc: 21.39 ng/ml

Instrument :
ECD_D
ClientSampleId :

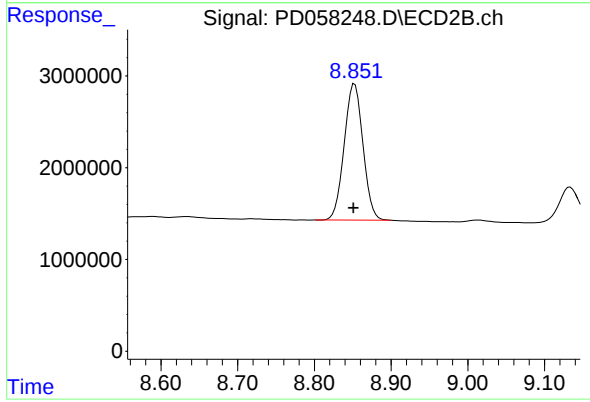

#28 Decachlorobiphenyl

R.T.: 8.852 min
Delta R.T.: 0.002 min
Response: 25381192
Conc: 21.19 ng/ml