

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060120\
 Data File : PD058234.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2020 11:17
 Operator : AJ\MA
 Sample : PTOXICC1000
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 12:29:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX060120.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 01 12:29:02 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.209	3.866	79613438	117.9E6	102.105	101.495
7) SA Decachlor...	7.849	8.850	84333279	111.0E6	99.290	96.611
Target Compounds						
2) Toxaphene-1	5.596	6.407	5410397	12200261	967.122	937.923
3) Toxaphene-2	5.971	6.699	9890165	12864328	1030.802	934.369
4) Toxaphene-3	6.213	6.986	9102774	30809147	996.094	954.898
5) Toxaphene-4	6.350	7.069	4254498	18683637	1025.170	946.638
6) Toxaphene-5	6.630	7.480	3523876	13406250	1103.684	889.679

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060120\
Data File : PD058234.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2020 11:17
Operator : AJ\MA
Sample : PTOXICC1000
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 12:29:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX060120.M
Quant Title : GC Extractables
QLast Update : Mon Jun 01 12:29:02 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

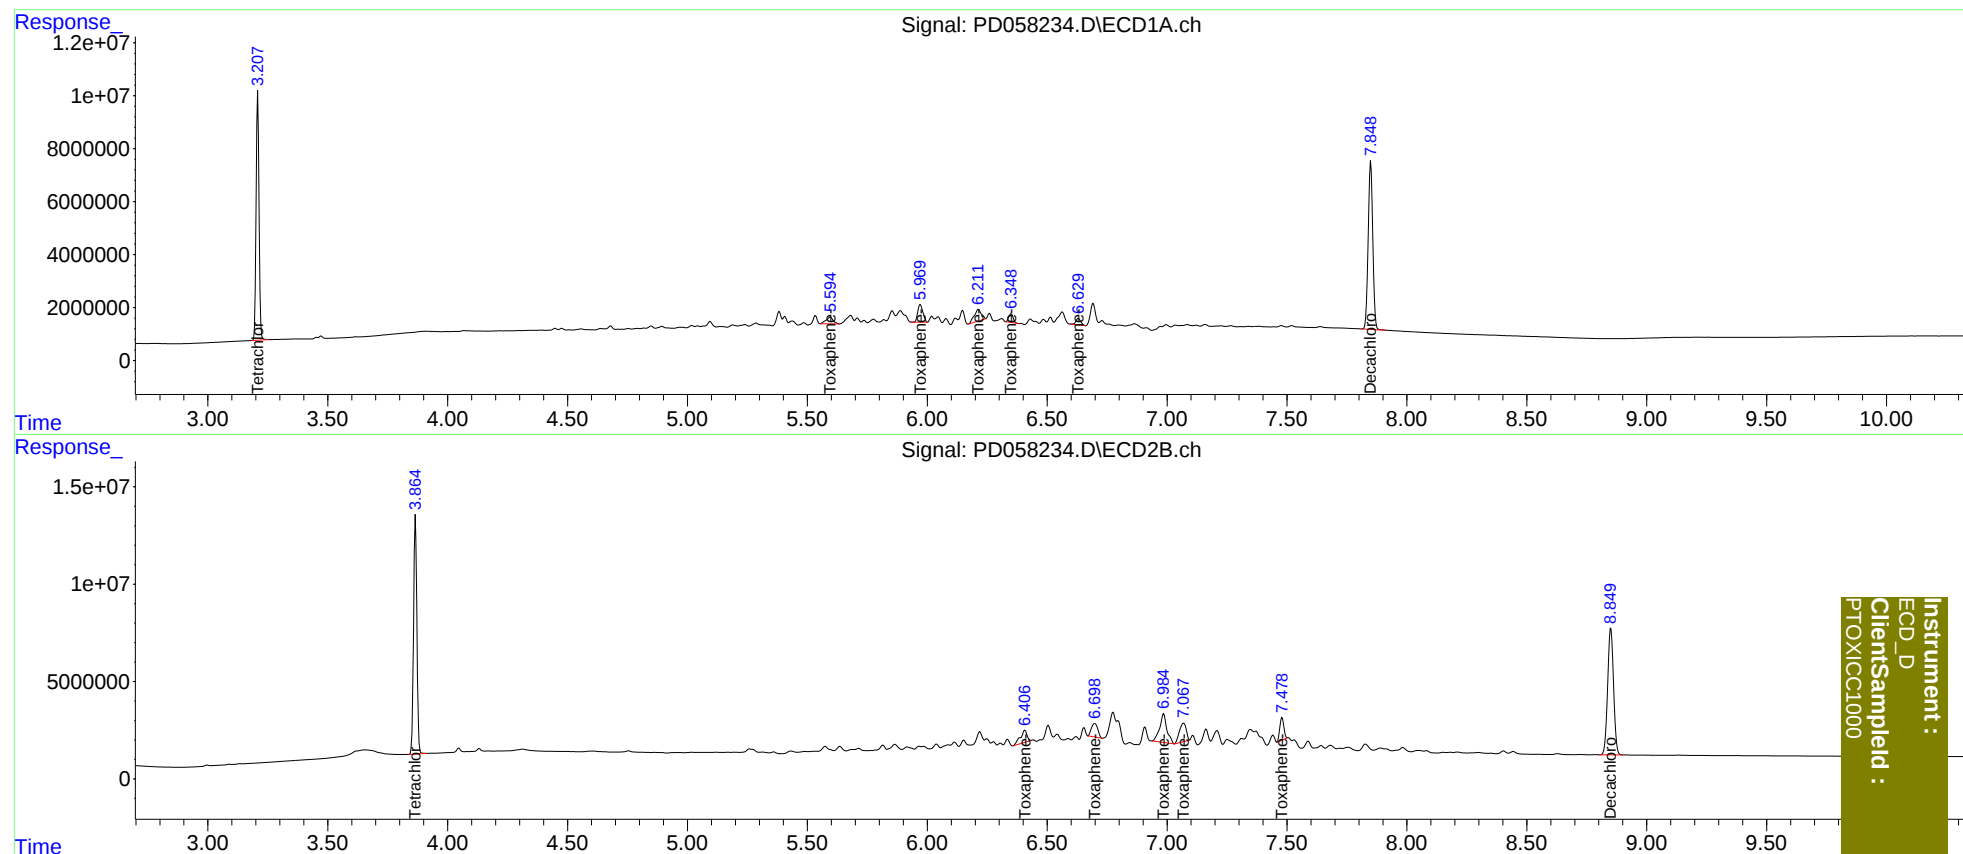

Instrument :
ECD_D
ClientSample :
PTOXICC1000