

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060120\
 Data File : PD058233.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2020 11:03
 Operator : AJ\MA
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 12:21:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060120.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 01 12:20:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.866	38935680	55213444	50.000	50.000
28)	SA Decachlor...	7.849	8.851	39892828	54085609	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.036	4.840	10109322	19371563	500.000	500.000
24)	Chlordane-2	4.522	5.302	10078007	21772790	500.000	500.000
25)	Chlordane-3	5.071	5.941	41804896	87483198	500.000	500.000
26)	Chlordane-4	5.126	6.015	39493302	105.6E6	500.000	500.000
27)	Chlordane-5	5.942	6.810	9657546	18750210	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060120\
Data File : PD058233.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2020 11:03
Operator : AJ\MA
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 12:21:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060120.M
Quant Title : GC Extractables
QLast Update : Mon Jun 01 12:20:46 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

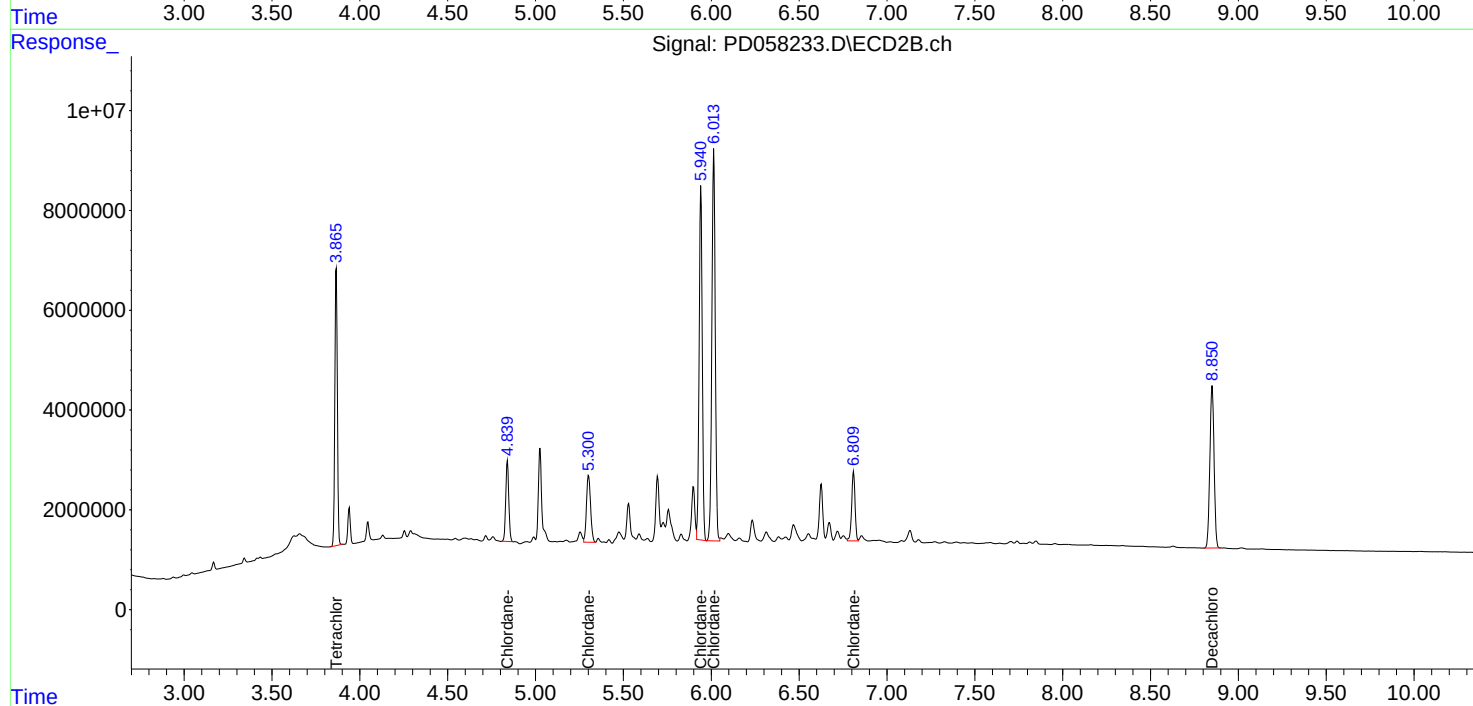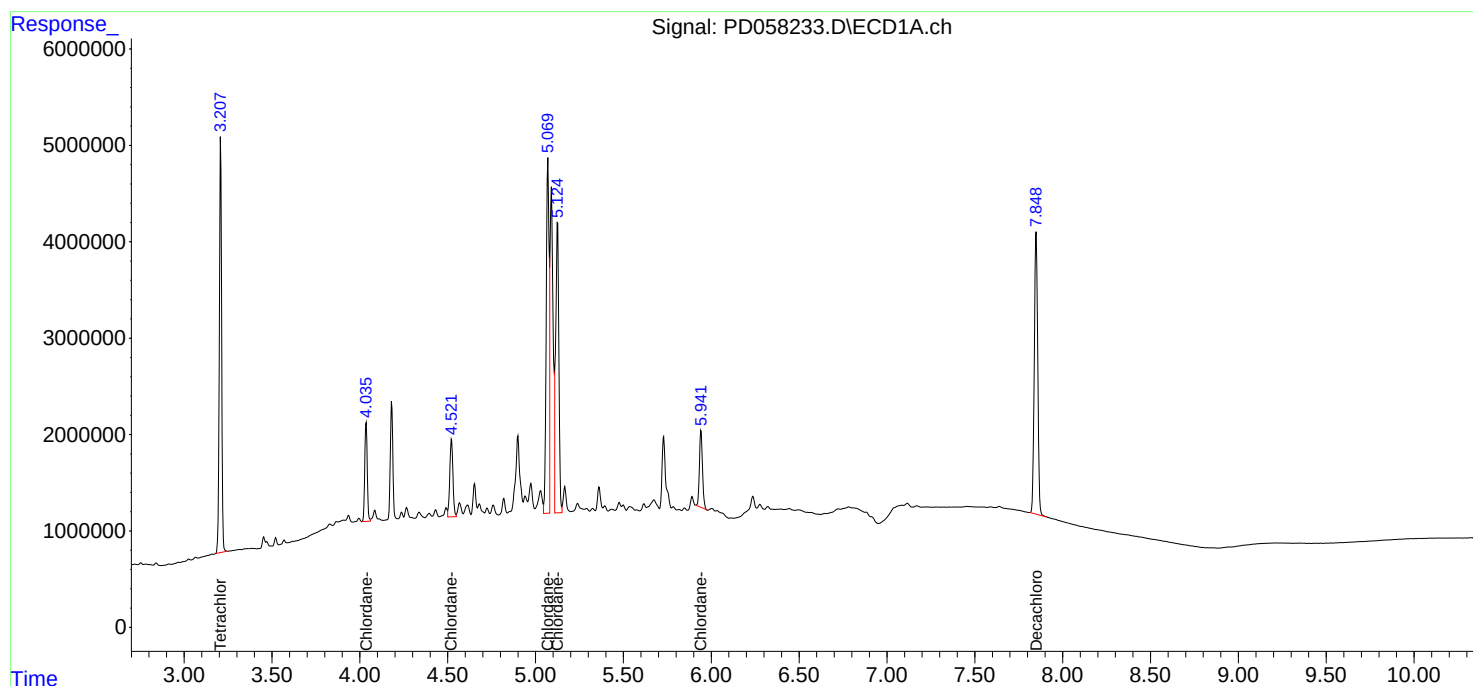


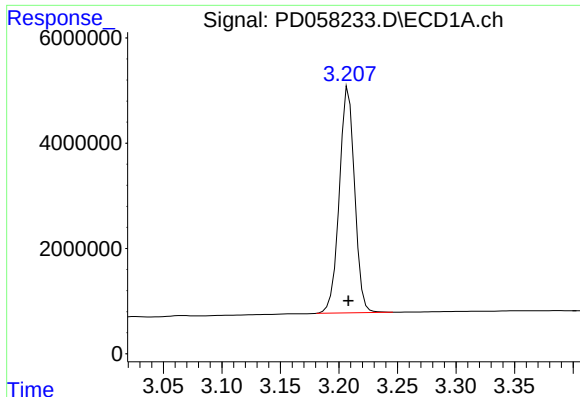

#1 Tetrachloro-m-xylene


R.T.: 3.208 min
Delta R.T.: 0.000 min
Response: 38935680
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

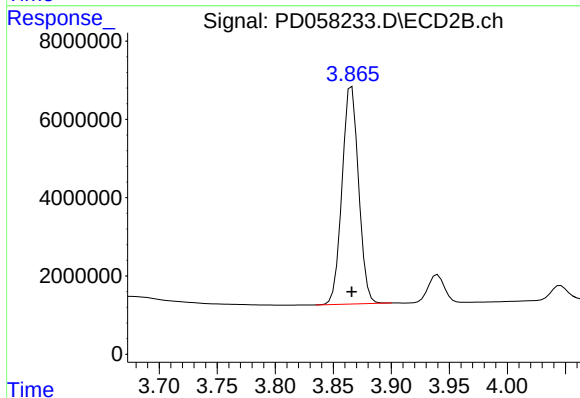


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 55213444
Conc: 50.00 ng/ml

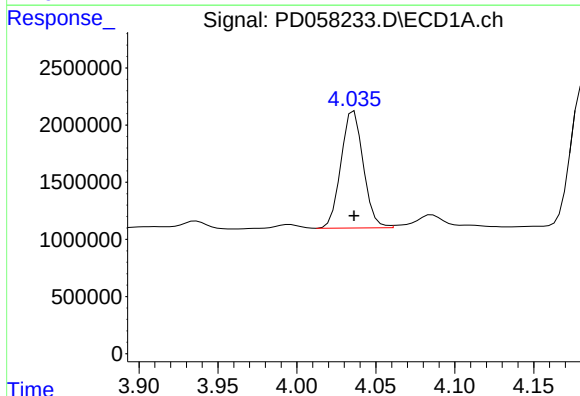


#23 Chlordane-1

R.T.: 4.036 min
Delta R.T.: 0.000 min
Response: 10109322
Conc: 500.00 ng/ml

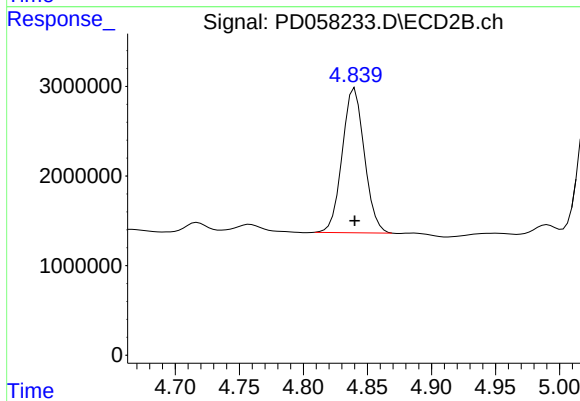

#23 Chlordane-1


R.T.: 4.840 min
Delta R.T.: 0.000 min
Response: 19371563
Conc: 500.00 ng/ml

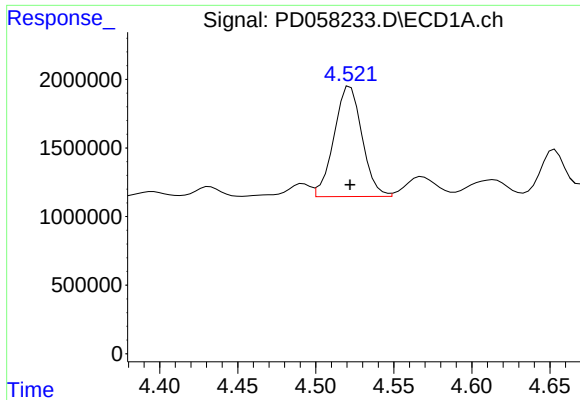

#24 Chlordane-2


R.T.: 4.522 min
Delta R.T.: 0.000 min
Response: 10078007
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

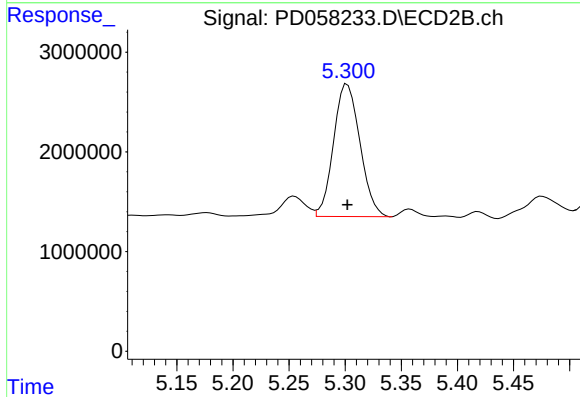


#24 Chlordane-2

R.T.: 5.302 min
Delta R.T.: 0.000 min
Response: 21772790
Conc: 500.00 ng/ml

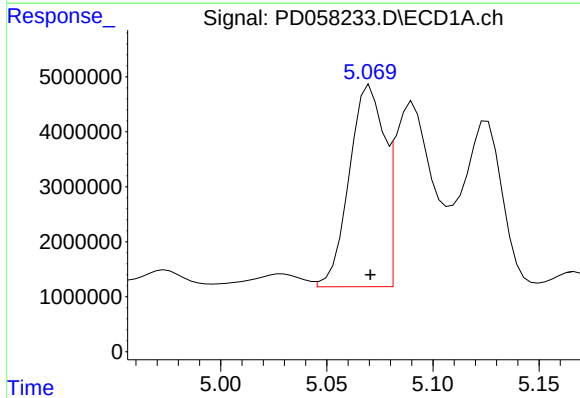


#25 Chlordane-3

R.T.: 5.071 min
Delta R.T.: 0.000 min
Response: 41804896
Conc: 500.00 ng/ml

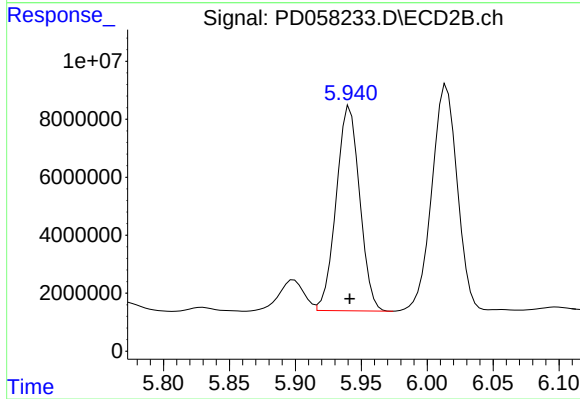

#25 Chlordane-3


R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 87483198
Conc: 500.00 ng/ml

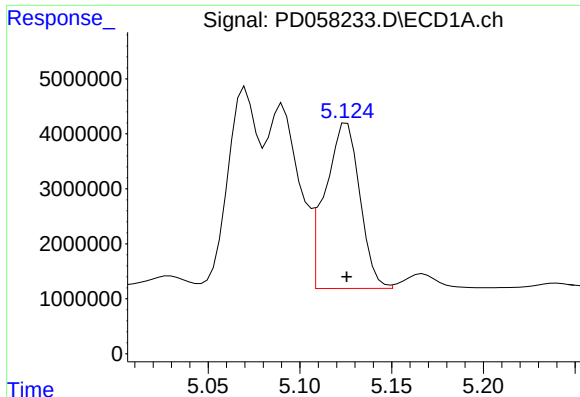

#26 Chlordane-4


R.T.: 5.126 min
Delta R.T.: 0.000 min
Response: 39493302
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

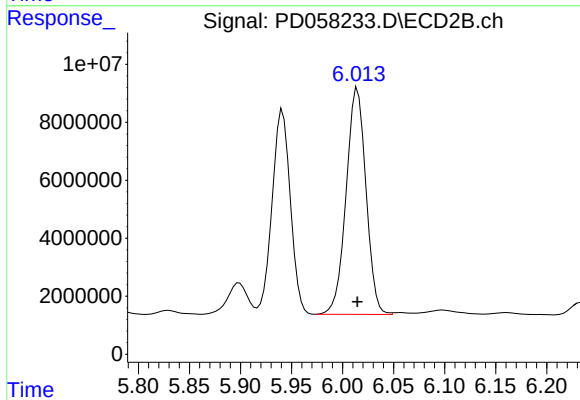


#26 Chlordane-4

R.T.: 6.015 min
Delta R.T.: 0.000 min
Response: 105621854
Conc: 500.00 ng/ml

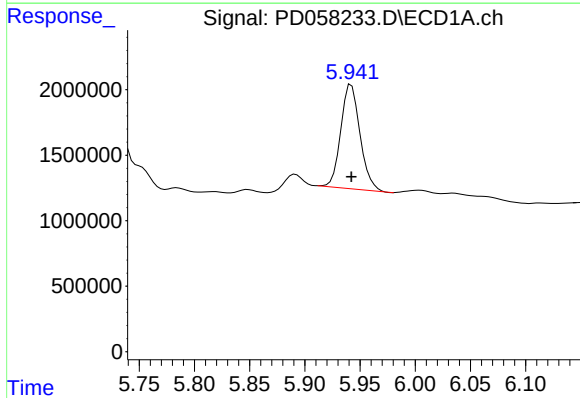


#27 Chlordane-5

R.T.: 5.942 min
Delta R.T.: 0.000 min
Response: 9657546
Conc: 500.00 ng/ml

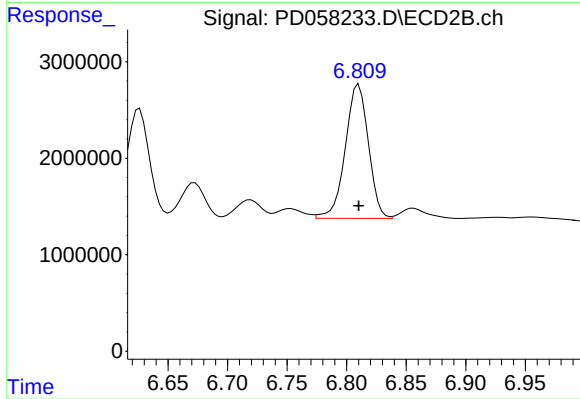

#27 Chlordane-5


R.T.: 6.810 min
Delta R.T.: 0.000 min
Response: 18750210
Conc: 500.00 ng/ml

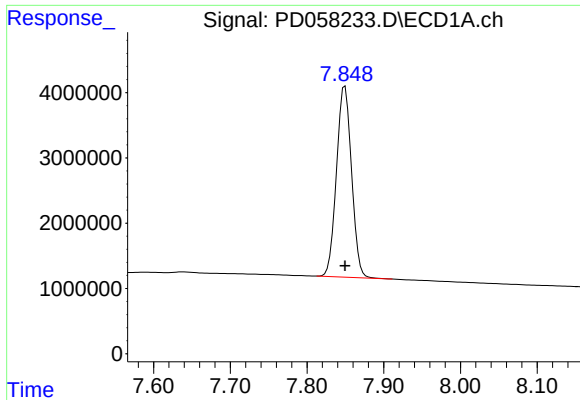

#28 Decachlorobiphenyl

R.T.: 7.849 min
Delta R.T.: 0.000 min
Response: 39892828
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

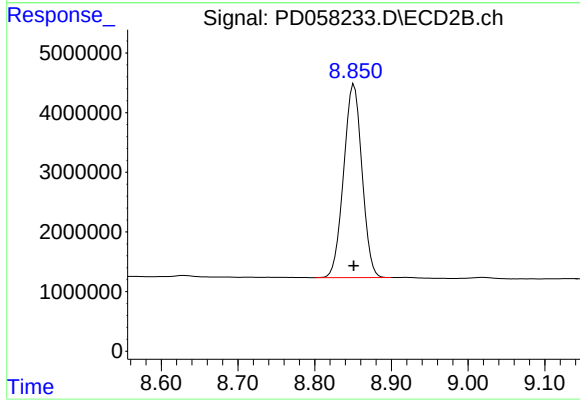

#28 Decachlorobiphenyl

R.T.: 8.851 min
Delta R.T.: 0.000 min
Response: 54085609
Conc: 50.00 ng/ml