

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060120\
 Data File : PD058256.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2020 18:32
 Operator : AJ\MA
 Sample : L2797-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TEST-HOLE-3-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 03:36:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060120.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 01 12:24:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.867	17976469	25928244	22.965	21.708
28)	SA Decachlor...	7.850	8.851	19724557	26254466	22.960	21.918

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060120\
Data File : PD058256.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2020 18:32
Operator : AJ\MA
Sample : L2797-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TEST-HOLE-3-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 03:36:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060120.M
Quant Title : GC Extractables
QLast Update : Mon Jun 01 12:24:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

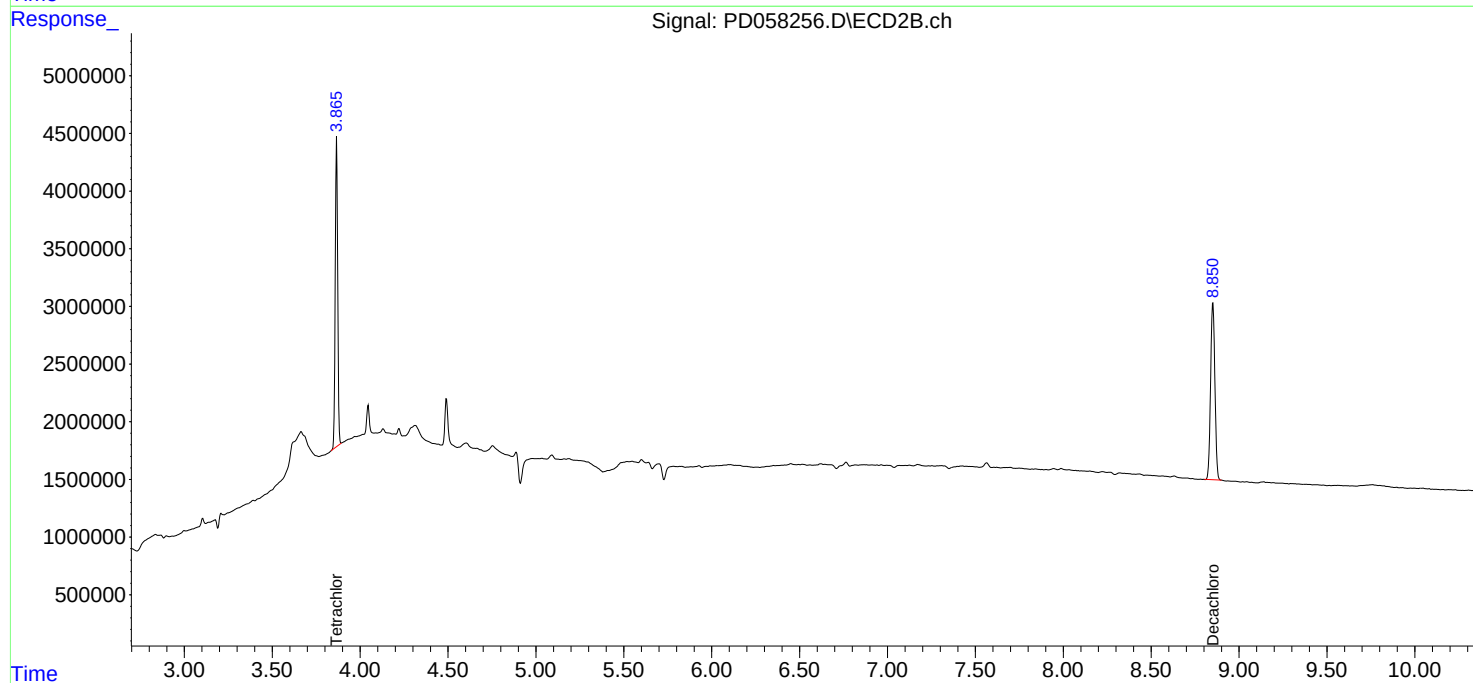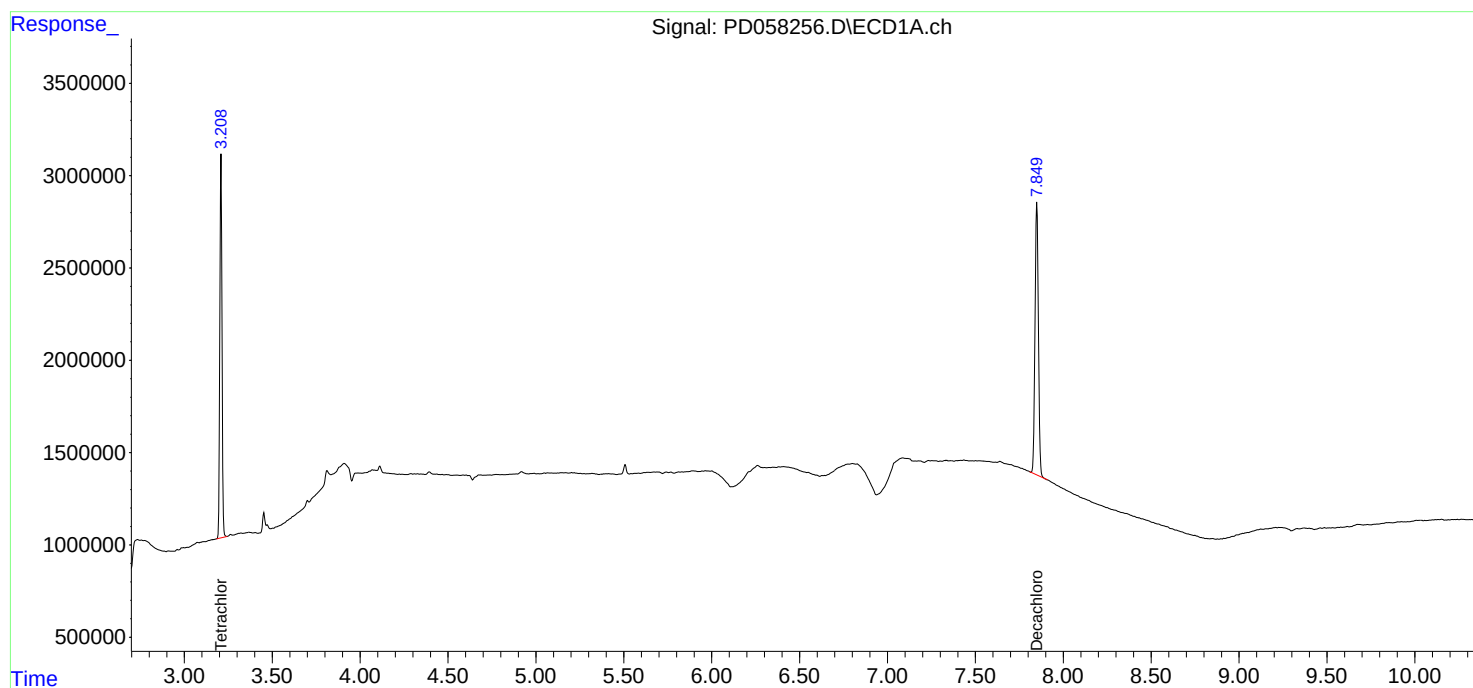


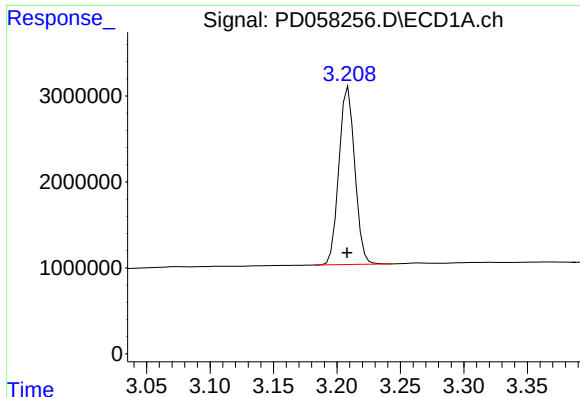

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: 0.001 min
Response: 17976469
Conc: 22.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
TEST-HOLE-3-COMP

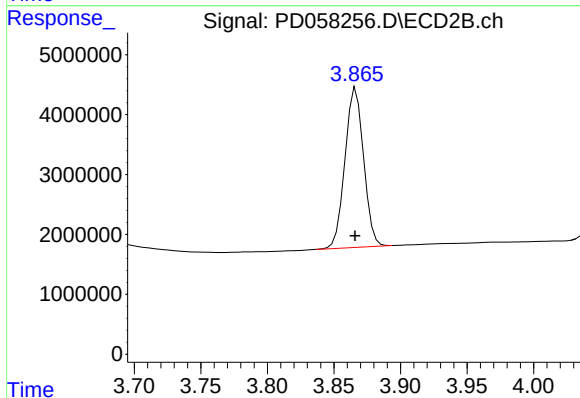


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 25928244
Conc: 21.71 ng/ml

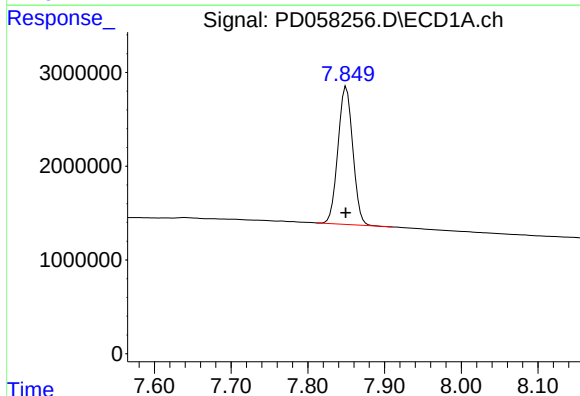

#28 Decachlorobiphenyl

R.T.: 7.850 min
Delta R.T.: 0.000 min
Response: 19724557
Conc: 22.96 ng/ml

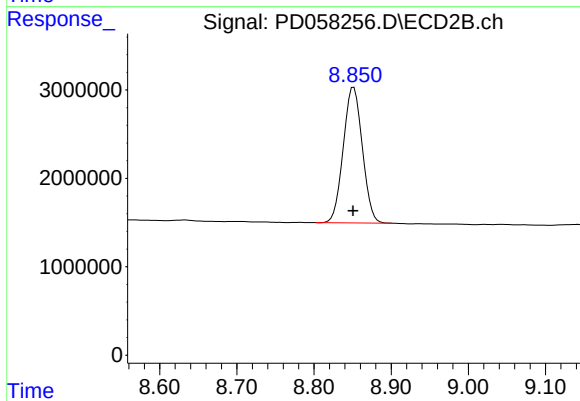

#28 Decachlorobiphenyl

R.T.: 8.851 min
Delta R.T.: 0.000 min
Response: 26254466
Conc: 21.92 ng/ml