

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060220\
 Data File : PD058262.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2020 10:09
 Operator : AJ\MA
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 14:29:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX060120.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 01 12:37:23 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.210	3.866	37470657	52439418	47.999	44.919
7) SA Decachlor...	7.852	8.852	39767551	54270843	47.211	45.931
Target Compounds						
2) Toxaphene-1	5.597	6.409	3152881	5481734	566.135	420.757 #
3) Toxaphene-2	5.973	6.700	5500316	5980362	557.922	422.464
4) Toxaphene-3	6.215	6.987	5313522	14012009	594.836	433.611 #
5) Toxaphene-4	6.352	7.071	2493879	8333751	594.138	430.450 #
6) Toxaphene-5	6.633	7.482	1706255	6097190	548.540	414.816

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060220\
Data File : PD058262.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2020 10:09
Operator : AJ\MA
Sample : PTOXCCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 14:29:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX060120.M
Quant Title : GC Extractables
QLast Update : Mon Jun 01 12:37:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

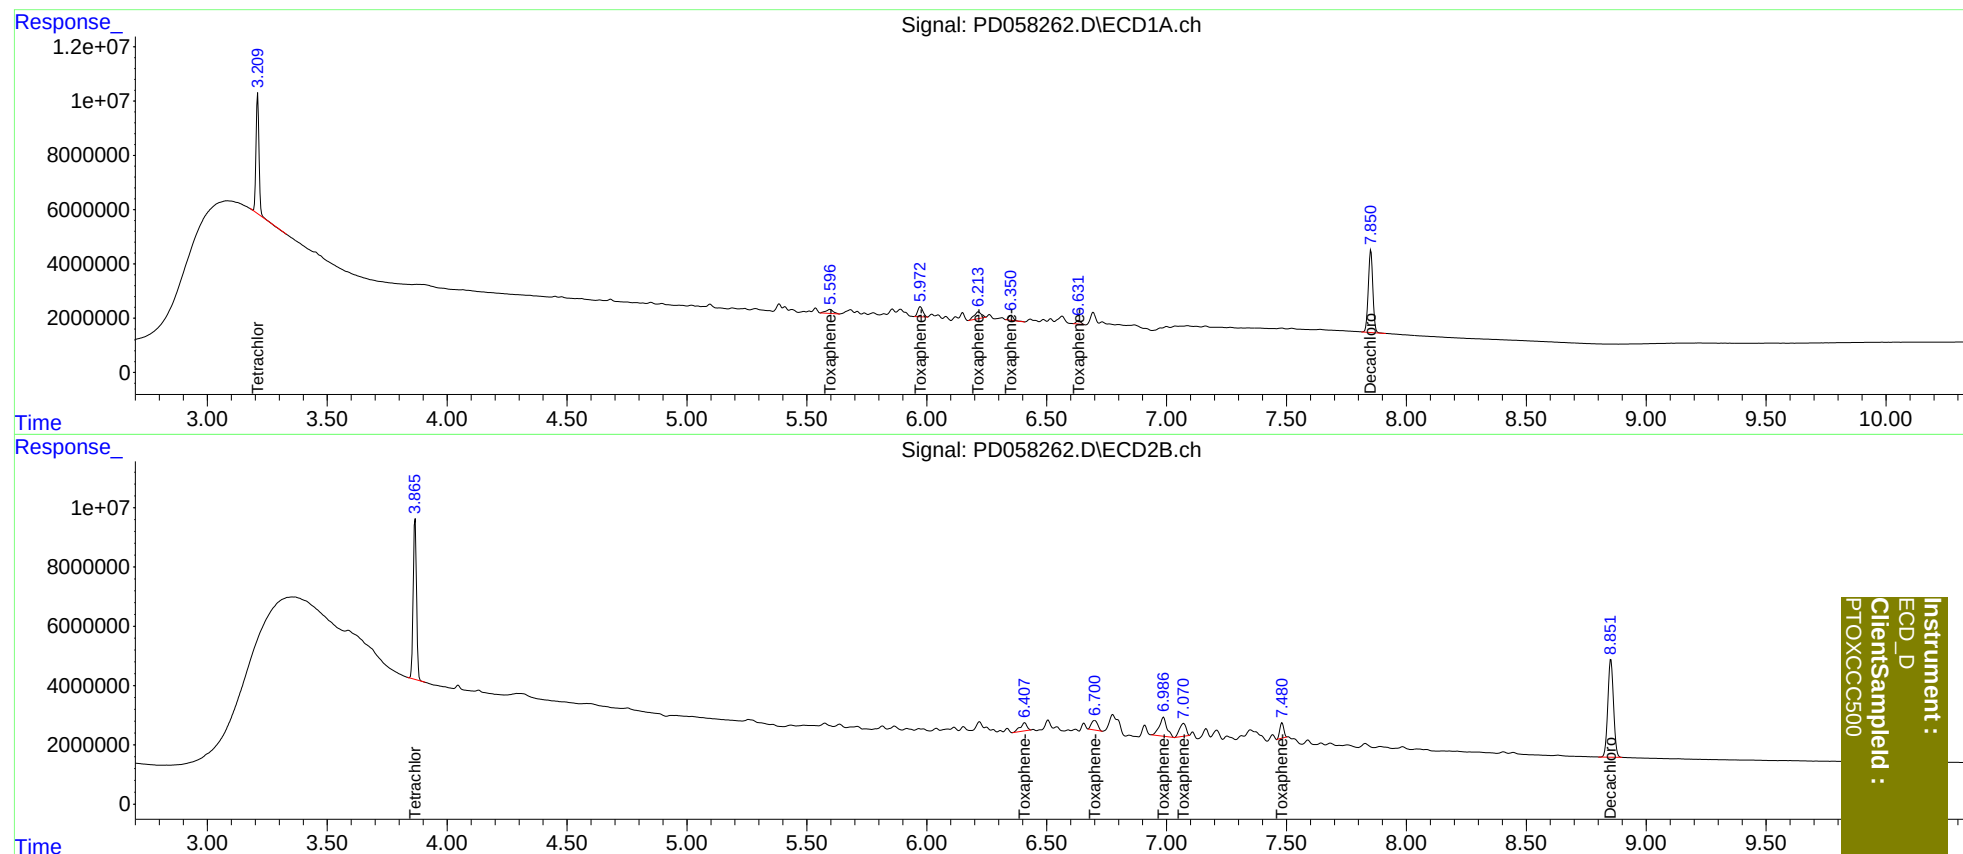

Instrument :
ECD_D
ClientSampled :
PTOXCCC500