

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060220\
 Data File : PD058265.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2020 12:15
 Operator : AJ\MA
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Manual Integrations
 APPROVED

mohammad
 6/3/2020 1:14:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 14:30:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX060120.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 01 12:37:23 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.209	3.866	34007625	47803772	43.563m	40.948
7) SA Decachlor...	7.854	8.854	35856283	48541439	42.568	41.082
Target Compounds						
2) Toxaphene-1	5.600	6.409	3311330	5745289	594.586	440.987 #
3) Toxaphene-2	5.975	6.700	5637312	6425792	571.818	453.930
4) Toxaphene-3	6.217	6.988	5248066	14682900	587.508	454.373
5) Toxaphene-4	6.353	7.071	2452399	8918795	584.255	460.669
6) Toxaphene-5	6.635	7.482	1588073	7038425	510.546	478.852

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060220\
Data File : PD058265.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2020 12:15
Operator : AJ\MA
Sample : PTOXCCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 14:30:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX060120.M
Quant Title : GC Extractables
QLast Update : Mon Jun 01 12:37:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

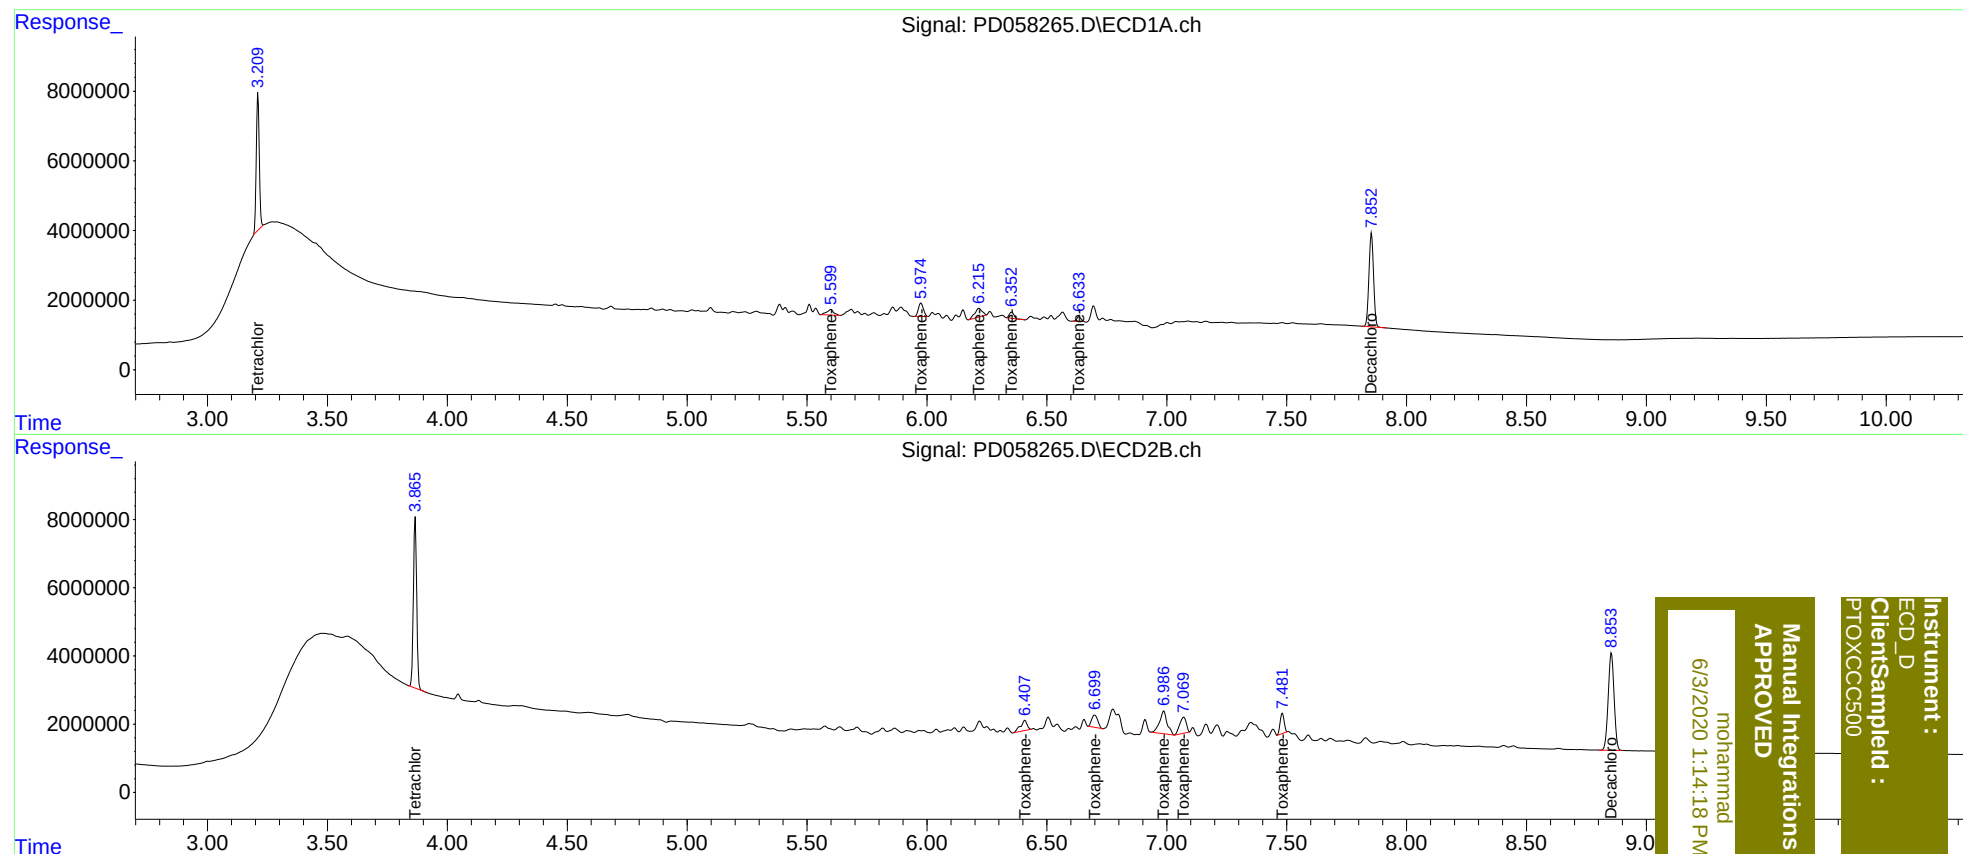

Manual Integrations
APPROVED

mohammad
6/3/2020 1:14:18 PM

Instrument :
ECD_D
ClientSampled :
PTOXCCC500