

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060221\
 Data File : PD063358.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 12:52
 Operator : AR\AJ
 Sample : PTOXICC1000
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 01:15:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 01:14:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.439	3.970	138.6E6	1310.3E6	102.643	99.012
7) SA Decachlor...	8.194	9.024	158.0E6	1368.0E6	100.666	98.508
Target Compounds						
2) Toxaphene-1	5.694	6.542	10324359	162.3E6	994.173	1014.079
3) Toxaphene-2	6.177	7.050	12521071	139.2E6	1079.504	1027.545
4) Toxaphene-3	6.296	7.126	28262306	389.1E6	1064.659	977.221
5) Toxaphene-4	6.543	7.212	30587507	252.0E6	1110.432	1000.837
6) Toxaphene-5	7.030	7.625	31963817	183.7E6	1018.536	1040.433

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060221\
Data File : PD063358.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 12:52
Operator : AR\AJ
Sample : PTOXICC1000
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 01:15:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 01:14:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

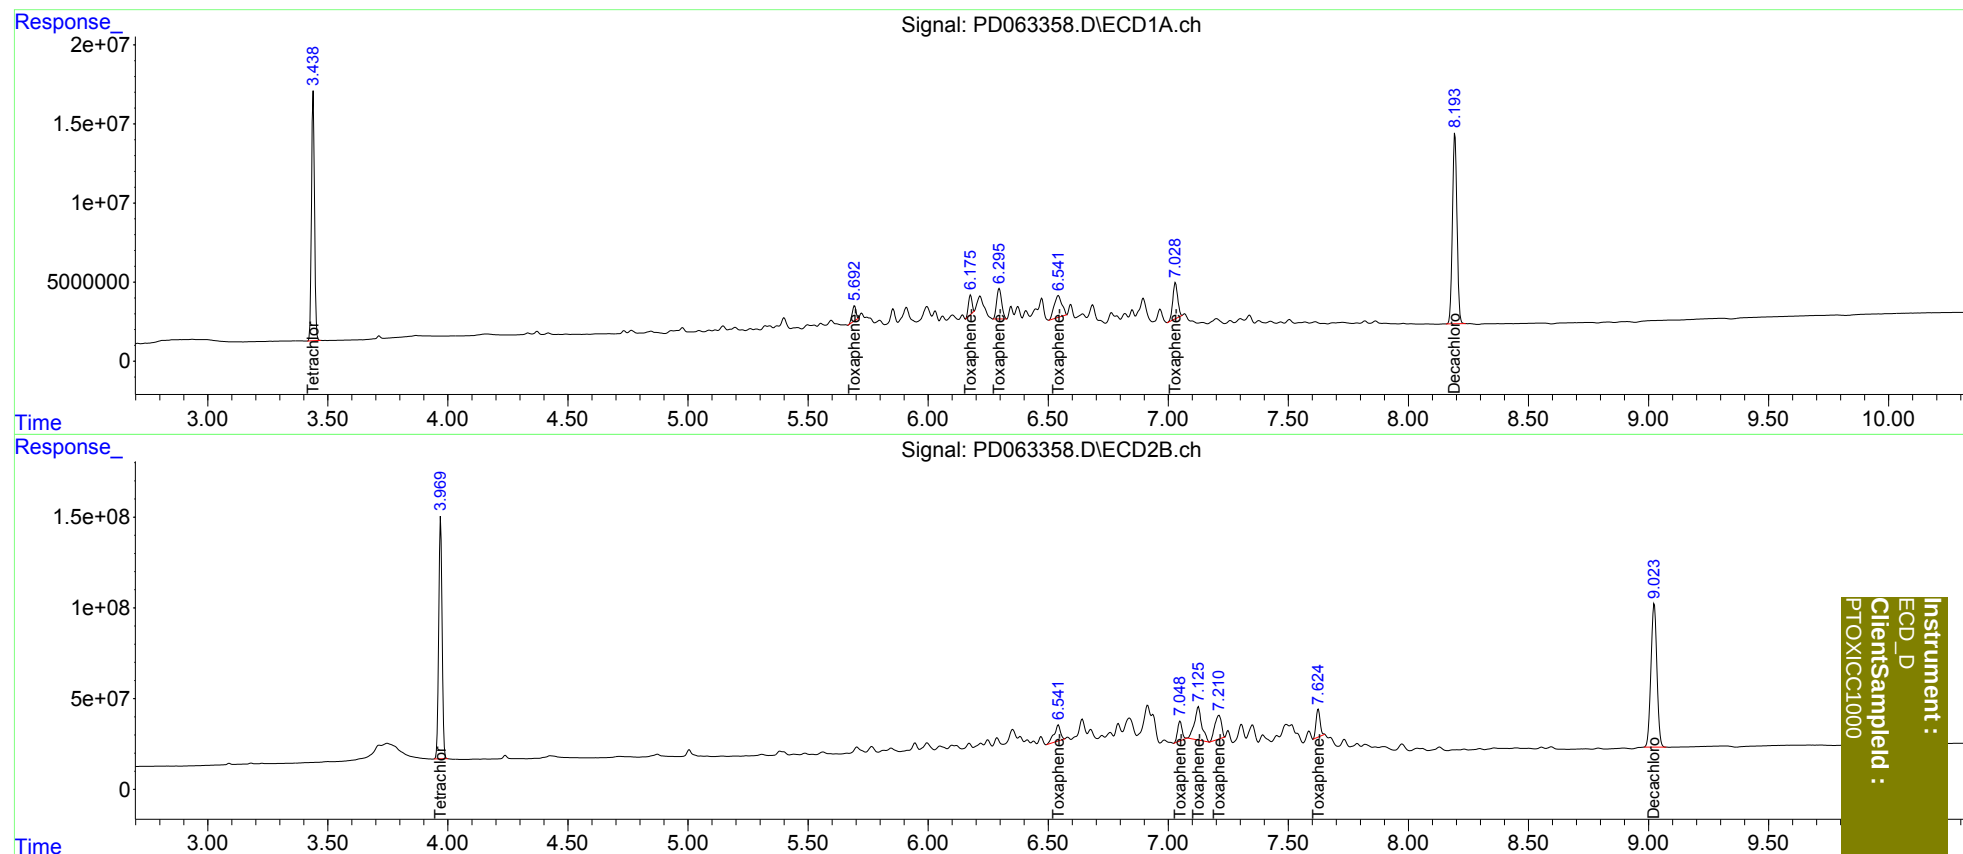

Instrument :
ECD_D
Client Sample :
PTOXICC1000