

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060221\
 Data File : PD063347.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 10:15
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 01:37:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 01:33:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.971	31892996	292.9E6	23.048	21.864
28)	SA Decachlor...	8.194	9.024	35442592	323.1E6	22.536	23.385
Target Compounds							
9)	A Endosulfan I	5.489	6.196	17995364	210.1E6	10.918	12.333
10)	B gamma-Chl...	5.377	6.074	19357527	224.7E6	10.839	12.094
12)	B 4,4'-DDE	5.599	6.303	39869732	442.6E6	22.930	24.357
13)	MA Dieldrin	5.732	6.452	40408321	447.6E6	23.006	24.728
19)	B Endosulfa...	6.645	7.226	28340239	348.6E6	22.175	22.988
20)	A Methoxychlor	6.903	7.549	82941535	767.8E6	103.993	103.669
21)	B Endrin ke...	7.137	7.696	38946818	348.6E6	21.953	23.843



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060221\
Data File : PD063347.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 10:15
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 01:37:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 01:33:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

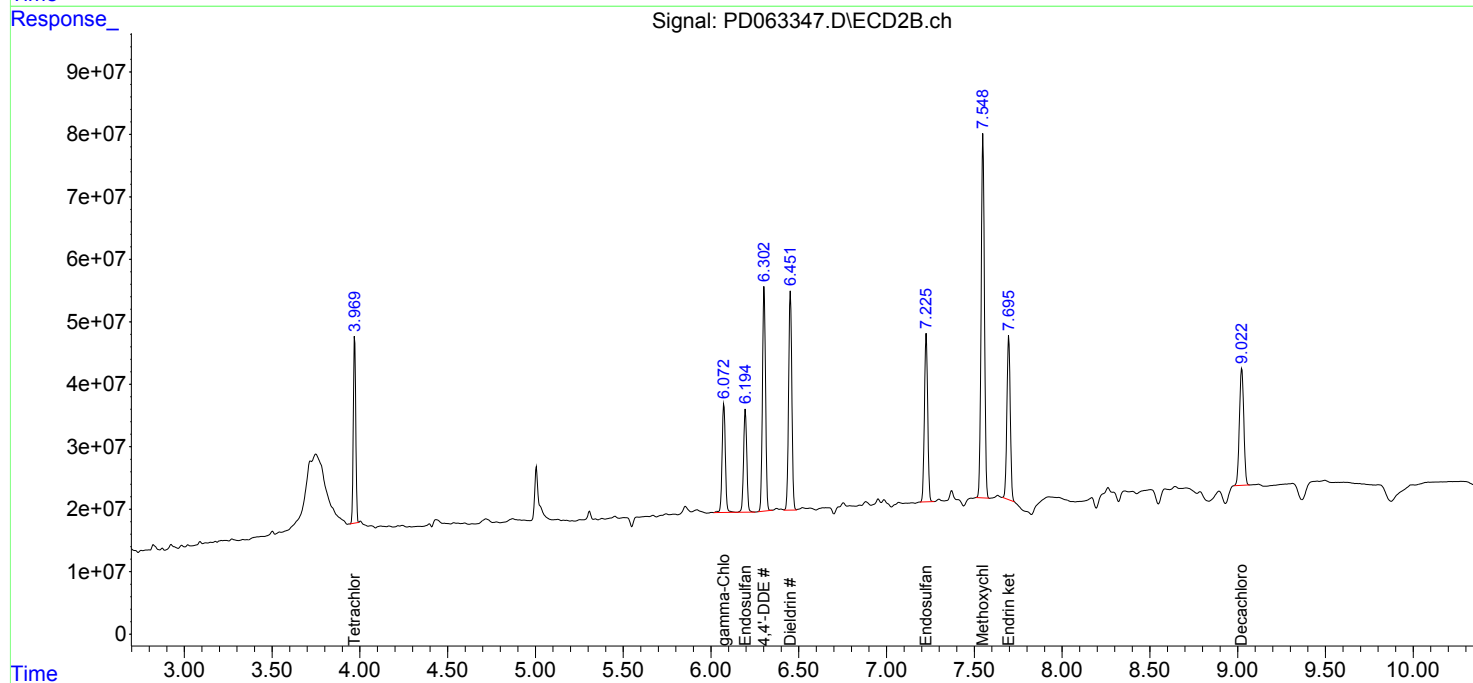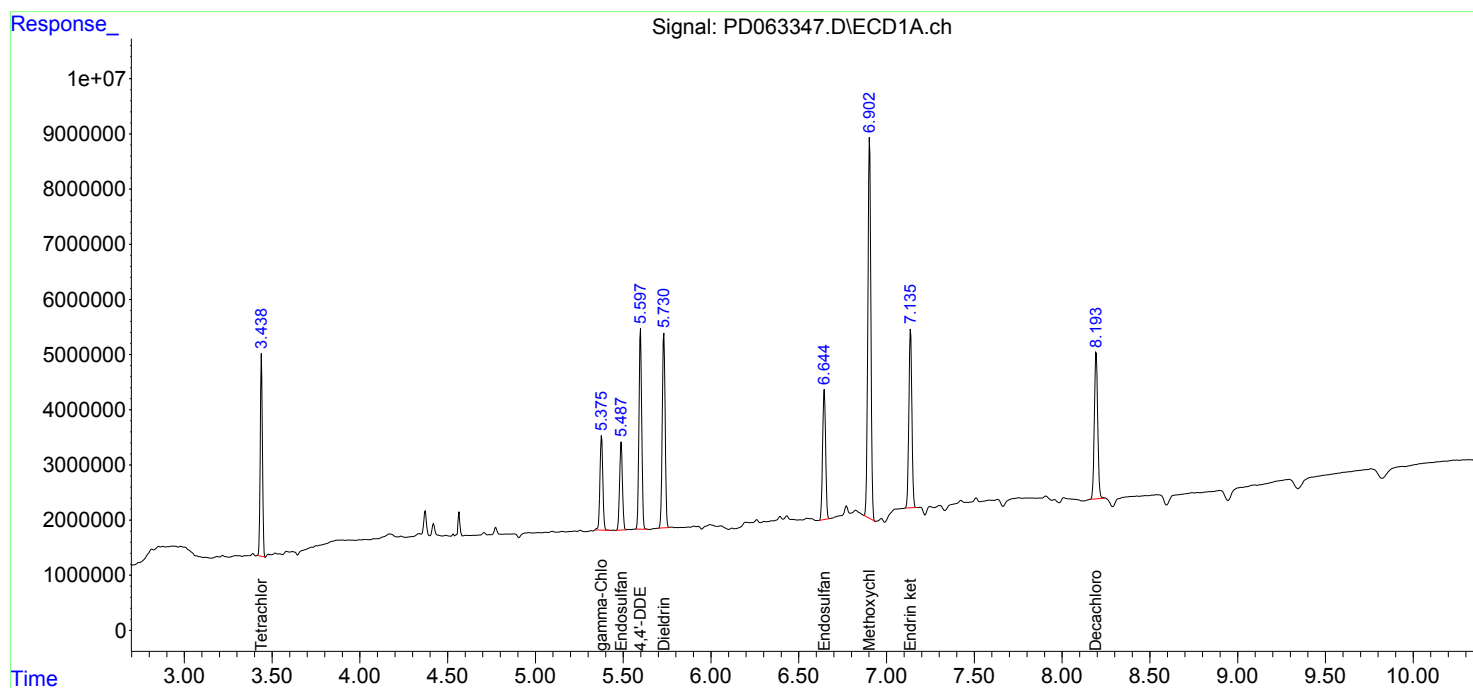


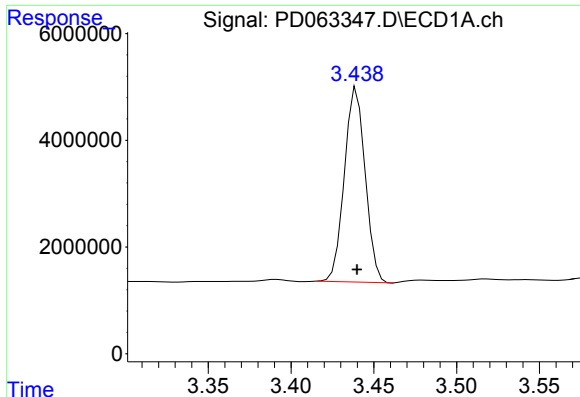

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 31892996
Conc: 23.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

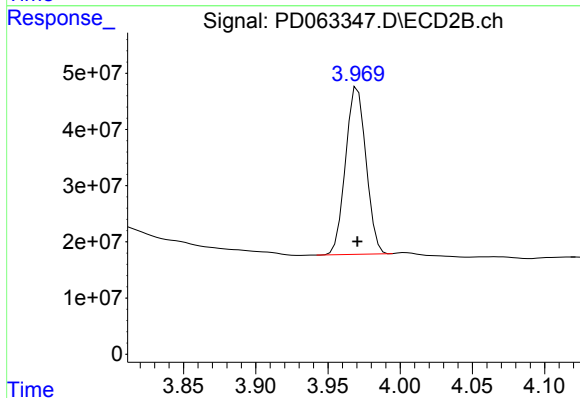


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 292948977
Conc: 21.86 ng/ml

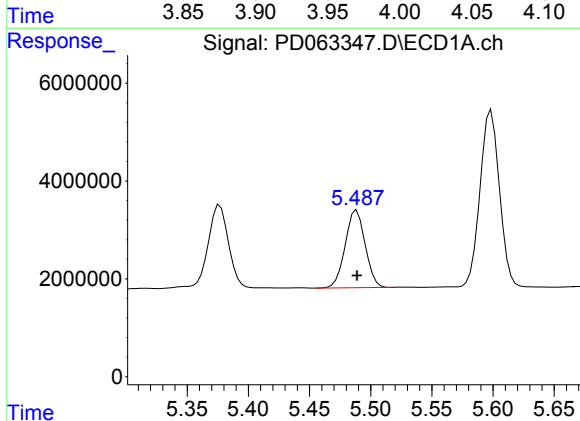


#9 Endosulfan I

R.T.: 5.489 min
Delta R.T.: 0.000 min
Response: 17995364
Conc: 10.92 ng/ml

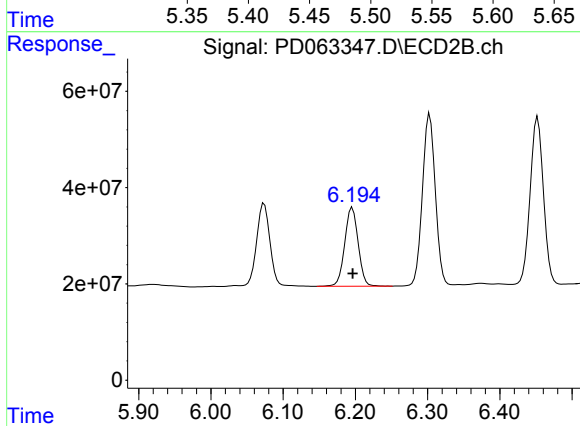

#9 Endosulfan I


R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 210139709
Conc: 12.33 ng/ml

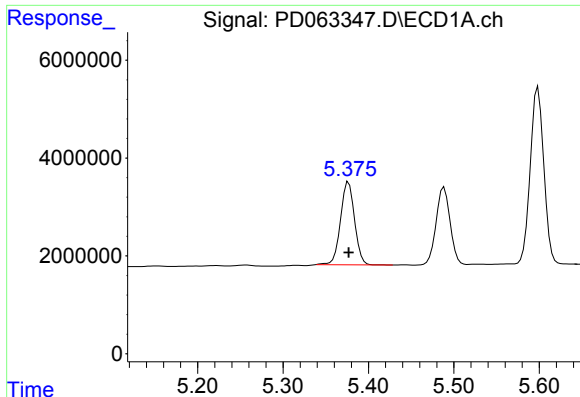

#10 gamma-Chlordane


R.T.: 5.377 min
Delta R.T.: 0.000 min
Response: 19357527
Conc: 10.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

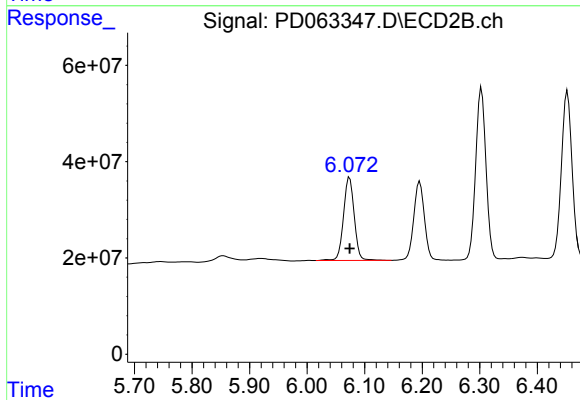


#10 gamma-Chlordane

R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 224662605
Conc: 12.09 ng/ml

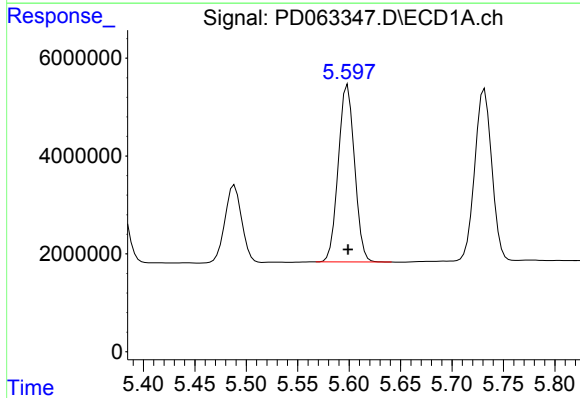


#12 4,4'-DDE

R.T.: 5.599 min
Delta R.T.: 0.000 min
Response: 39869732
Conc: 22.93 ng/ml

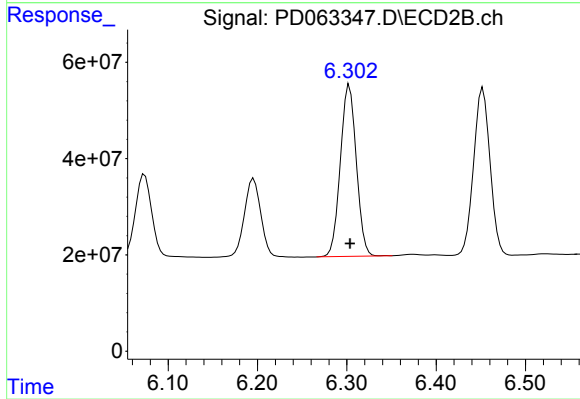

#12 4,4'-DDE


R.T.: 6.303 min
Delta R.T.: 0.000 min
Response: 442639474
Conc: 24.36 ng/ml

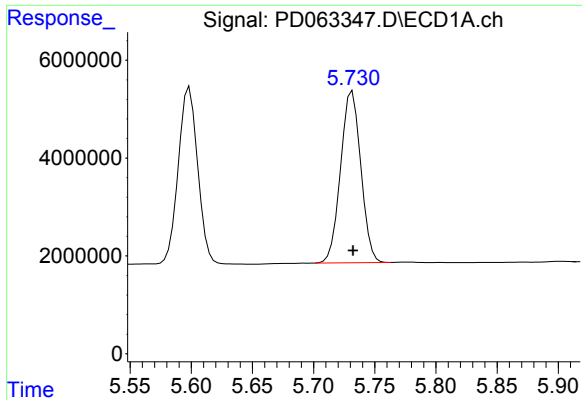

#13 Dieldrin


R.T.: 5.732 min
Delta R.T.: 0.000 min
Response: 40408321
Conc: 23.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

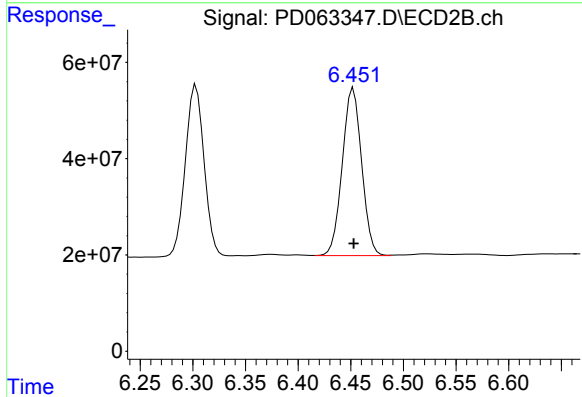


#13 Dieldrin

R.T.: 6.452 min
Delta R.T.: 0.000 min
Response: 447637476
Conc: 24.73 ng/ml

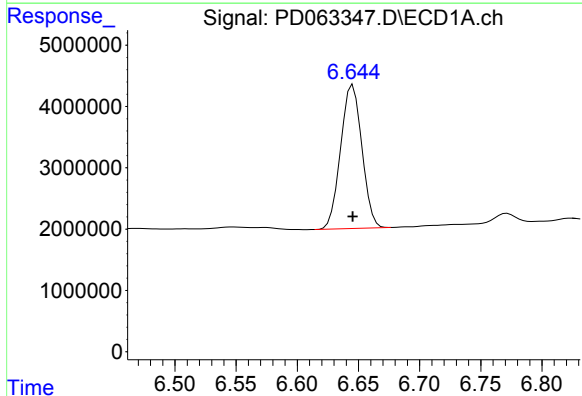


#19 Endosulfan Sulfate

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 28340239
Conc: 22.18 ng/ml

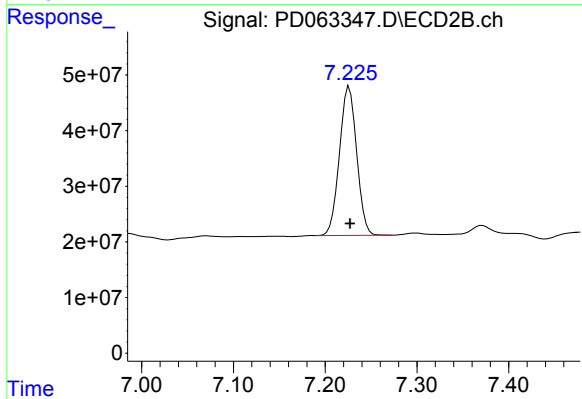

#19 Endosulfan Sulfate


R.T.: 7.226 min
Delta R.T.: 0.000 min
Response: 348603153
Conc: 22.99 ng/ml

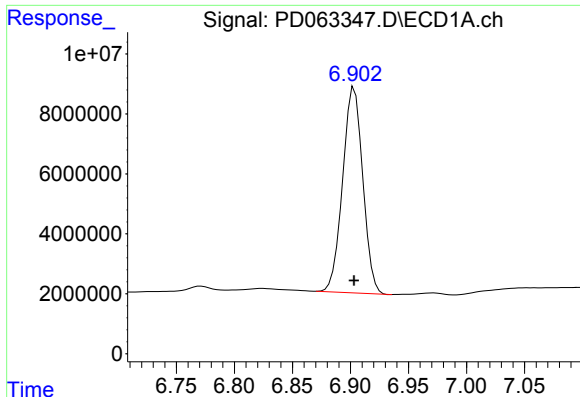

#20 Methoxychlor


R.T.: 6.903 min
Delta R.T.: 0.000 min
Response: 82941535
Conc: 103.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

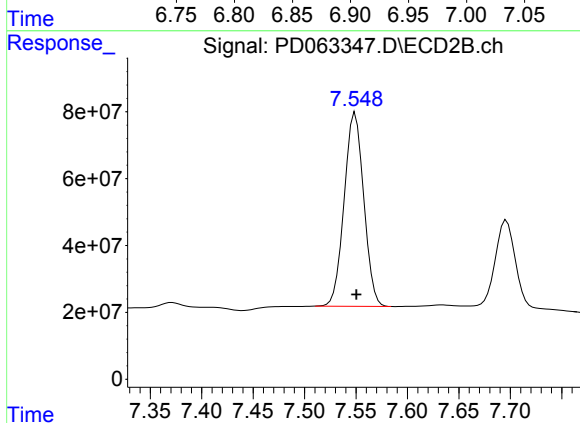


#20 Methoxychlor

R.T.: 7.549 min
Delta R.T.: 0.000 min
Response: 767846001
Conc: 103.67 ng/ml

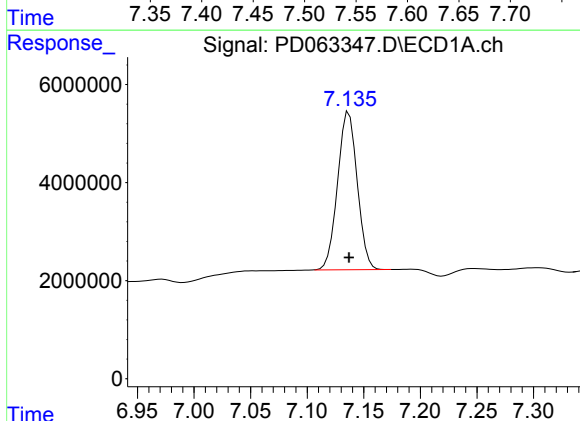


#21 Endrin ketone

R.T.: 7.137 min
Delta R.T.: 0.000 min
Response: 38946818
Conc: 21.95 ng/ml

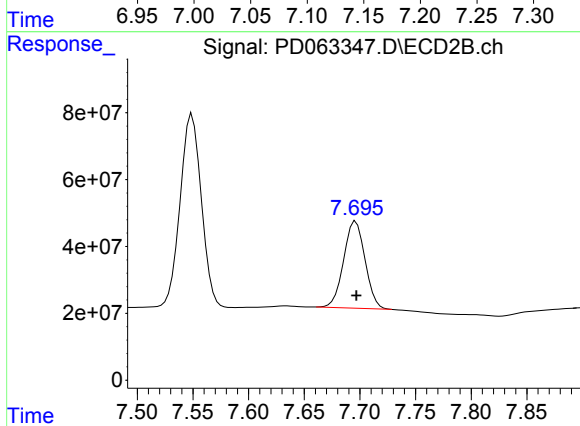

#21 Endrin ketone


R.T.: 7.696 min
Delta R.T.: 0.000 min
Response: 348631703
Conc: 23.84 ng/ml

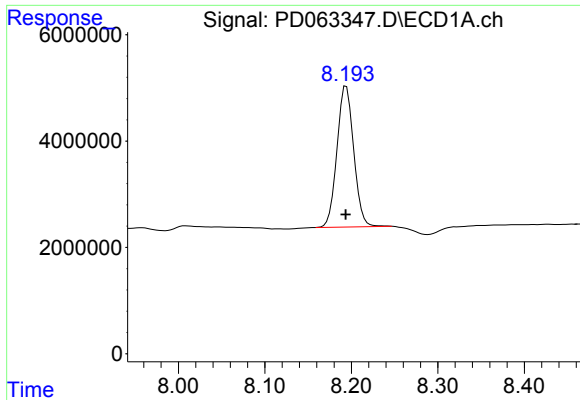

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 35442592
Conc: 22.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

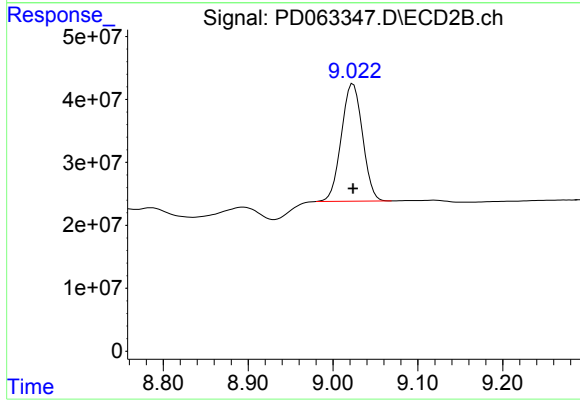

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 323145910
Conc: 23.38 ng/ml