

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060221\
 Data File : PD063353.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 11:42
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 12:57:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 12:56:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	3.971	160.0E6	1278.8E6	101.439	94.126
28)	SA Decachlor...	8.198	9.025	149.3E6	1226.6E6	93.376	87.241
Target Compounds							
23)	Chlordane-1	4.311	4.963	46944257	540.9E6	982.007	940.305
24)	Chlordane-2	4.813	5.429	54288218	499.8E6	953.058	915.353
25)	Chlordane-3	5.382	6.075	173.3E6	2295.7E6	1010.832	941.336
26)	Chlordane-4	5.439	6.149	140.1E6	2629.4E6	990.017	935.942
27)	Chlordane-5	6.276	6.953	55335880	494.1E6	985.543	946.641



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060221\
Data File : PD063353.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 11:42
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 12:57:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 12:56:45 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

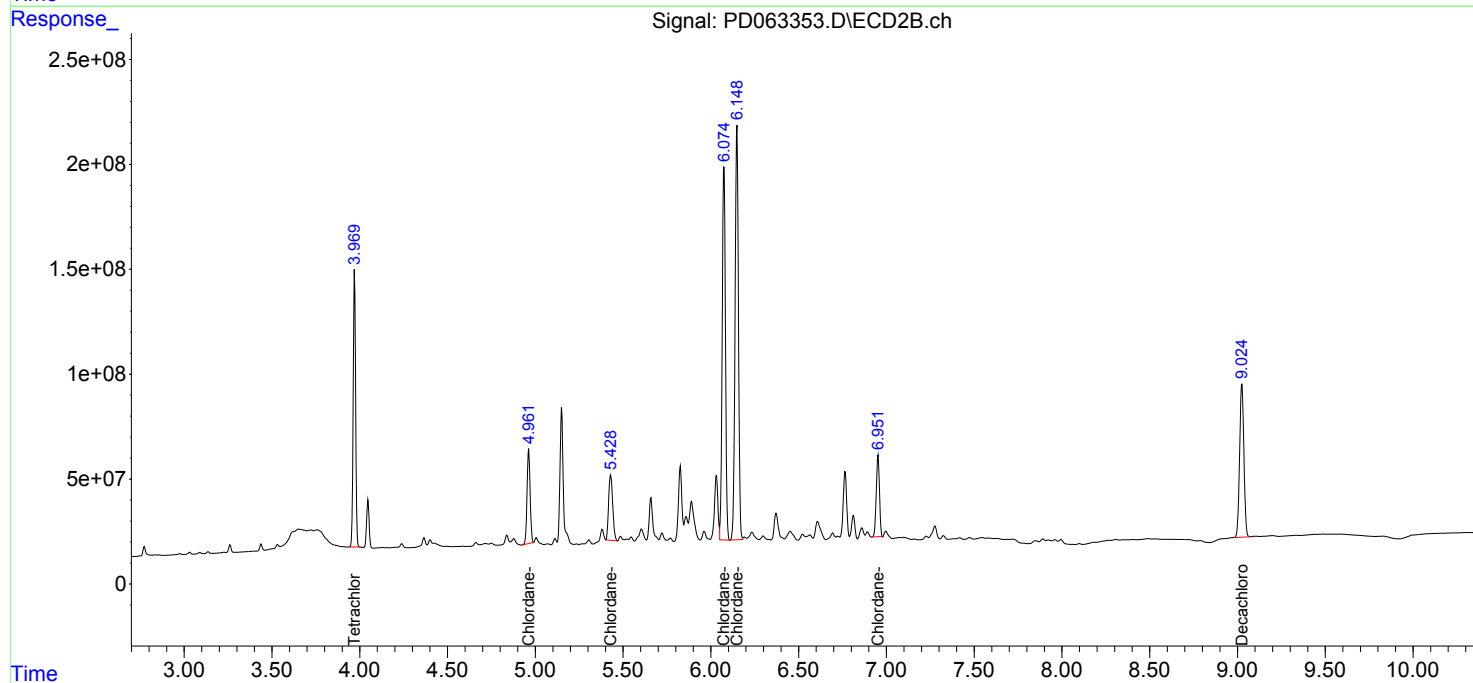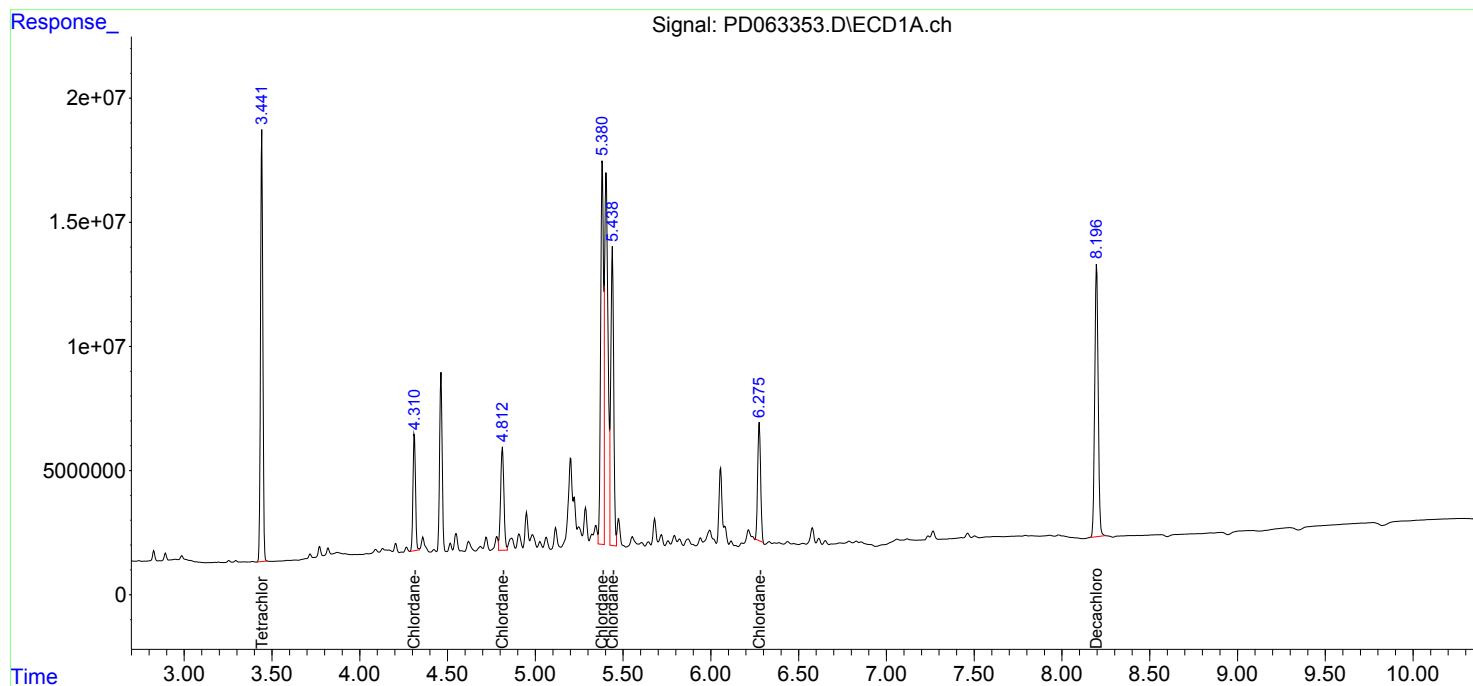


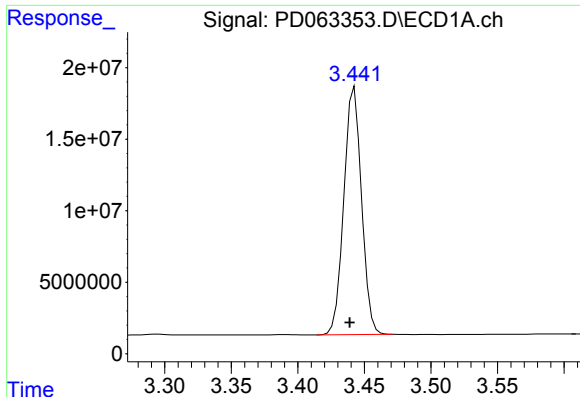

#1 Tetrachloro-m-xylene


R.T.: 3.443 min
Delta R.T.: 0.004 min
Response: 160009785
Conc: 101.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

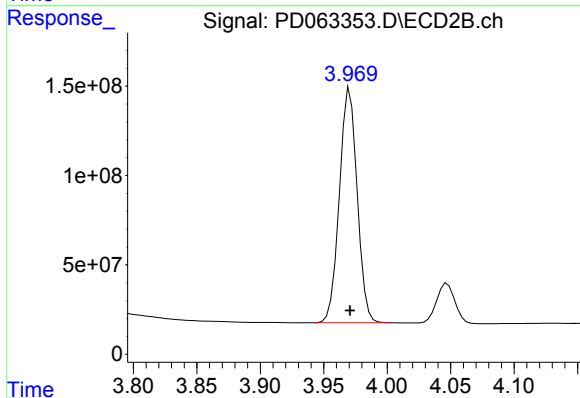


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 1278751450
Conc: 94.13 ng/ml

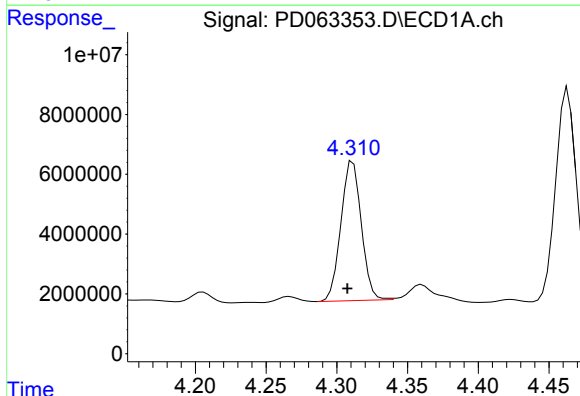


#23 Chlordane-1

R.T.: 4.311 min
Delta R.T.: 0.004 min
Response: 46944257
Conc: 982.01 ng/ml

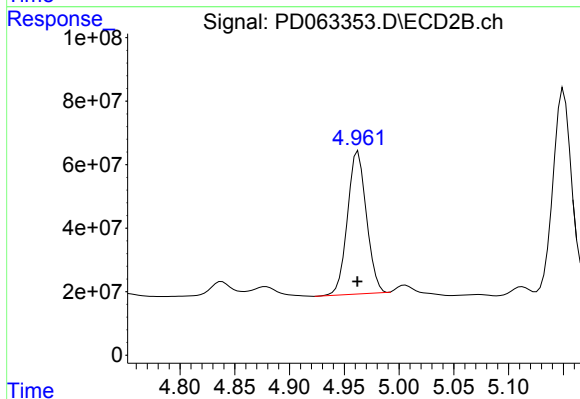

#23 Chlordane-1


R.T.: 4.963 min
Delta R.T.: 0.000 min
Response: 540898970
Conc: 940.30 ng/ml

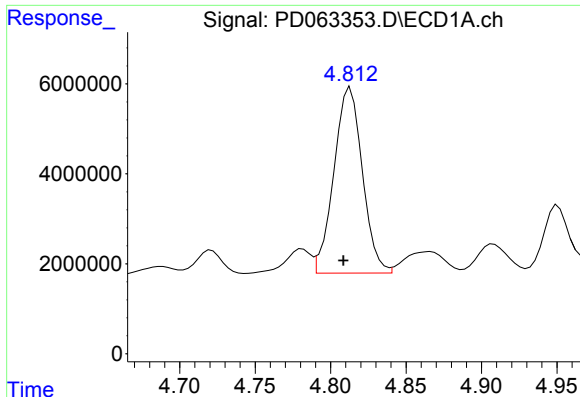

#24 Chlordane-2


R.T.: 4.813 min
Delta R.T.: 0.005 min
Response: 54288218
Conc: 953.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

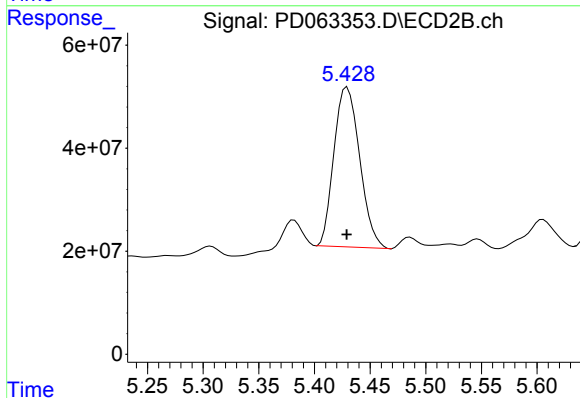


#24 Chlordane-2

R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 499814779
Conc: 915.35 ng/ml

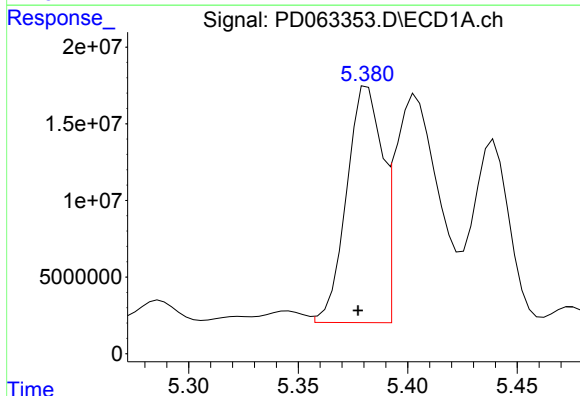


#25 Chlordane-3

R.T.: 5.382 min
Delta R.T.: 0.004 min
Response: 173258903
Conc: 1010.83 ng/ml

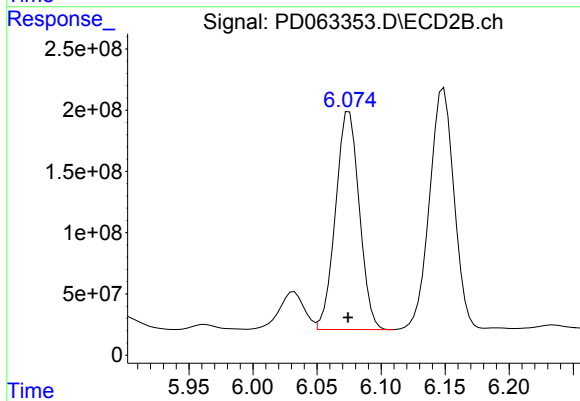

#25 Chlordane-3


R.T.: 6.075 min
Delta R.T.: 0.001 min
Response: 2295668247
Conc: 941.34 ng/ml

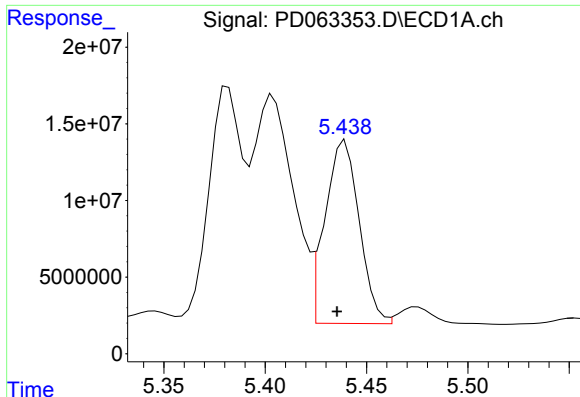

#26 Chlordane-4


R.T.: 5.439 min
Delta R.T.: 0.004 min
Response: 140089479
Conc: 990.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

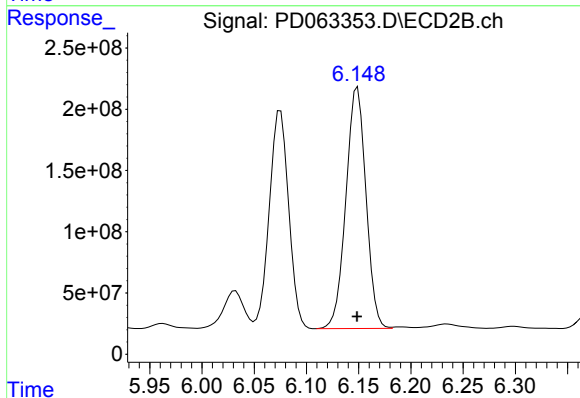


#26 Chlordane-4

R.T.: 6.149 min
Delta R.T.: 0.000 min
Response: 2629398282
Conc: 935.94 ng/ml

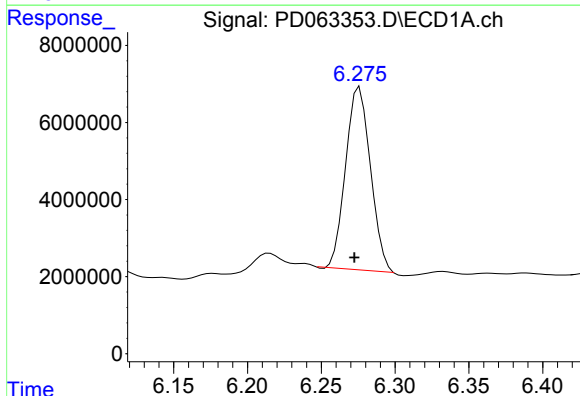


#27 Chlordane-5

R.T.: 6.276 min
Delta R.T.: 0.004 min
Response: 55335880
Conc: 985.54 ng/ml

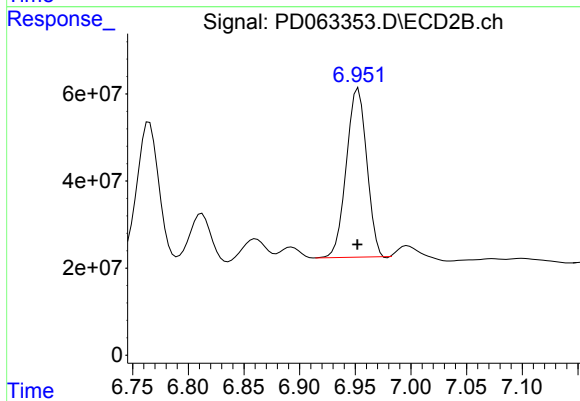

#27 Chlordane-5


R.T.: 6.953 min
Delta R.T.: 0.001 min
Response: 494068142
Conc: 946.64 ng/ml

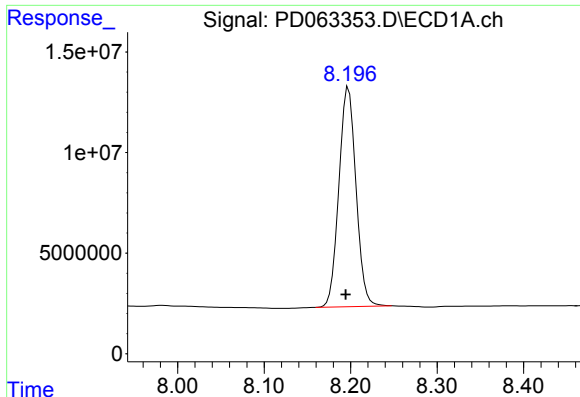

#28 Decachlorobiphenyl

R.T.: 8.198 min
Delta R.T.: 0.003 min
Response: 149315612
Conc: 93.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

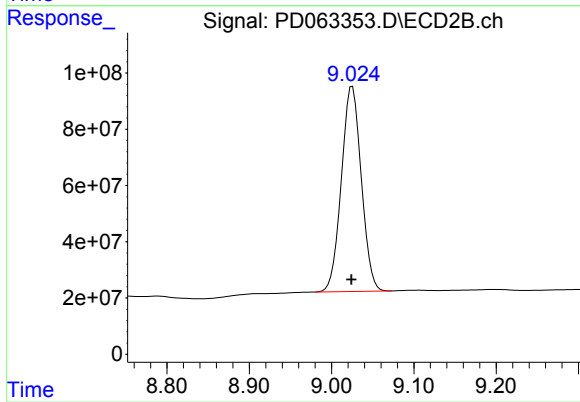

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.001 min
Response: 1226611567
Conc: 87.24 ng/ml