

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060221\
 Data File : PD063354.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 11:56
 Operator : AR\AJ
 Sample : PCHLORICC750 (Sig #1); PCHLORICC500 (Sig #2)
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 12:57:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 12:56:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.970	118.2E6	980.7E6	74.947	72.187
28)	SA Decachlor...	8.194	9.024	112.6E6	996.0E6	70.437	70.842
Target Compounds							
23)	Chlordane-1	4.307	4.962	35392078	418.7E6	740.352	727.841
24)	Chlordane-2	4.809	5.428	41145617	389.6E6	722.333	713.447
25)	Chlordane-3	5.378	6.074	129.3E6	1764.1E6	754.103	723.367
26)	Chlordane-4	5.436	6.148	105.0E6	2025.7E6	741.860	721.039
27)	Chlordane-5	6.272	6.951	41714233	379.6E6	742.939	727.274



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060221\
Data File : PD063354.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 11:56
Operator : AR\AJ
Sample : PCHLORICC750 (Sig #1); PCHLORICC500 (Sig #2)
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleID :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 12:57:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 12:56:45 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

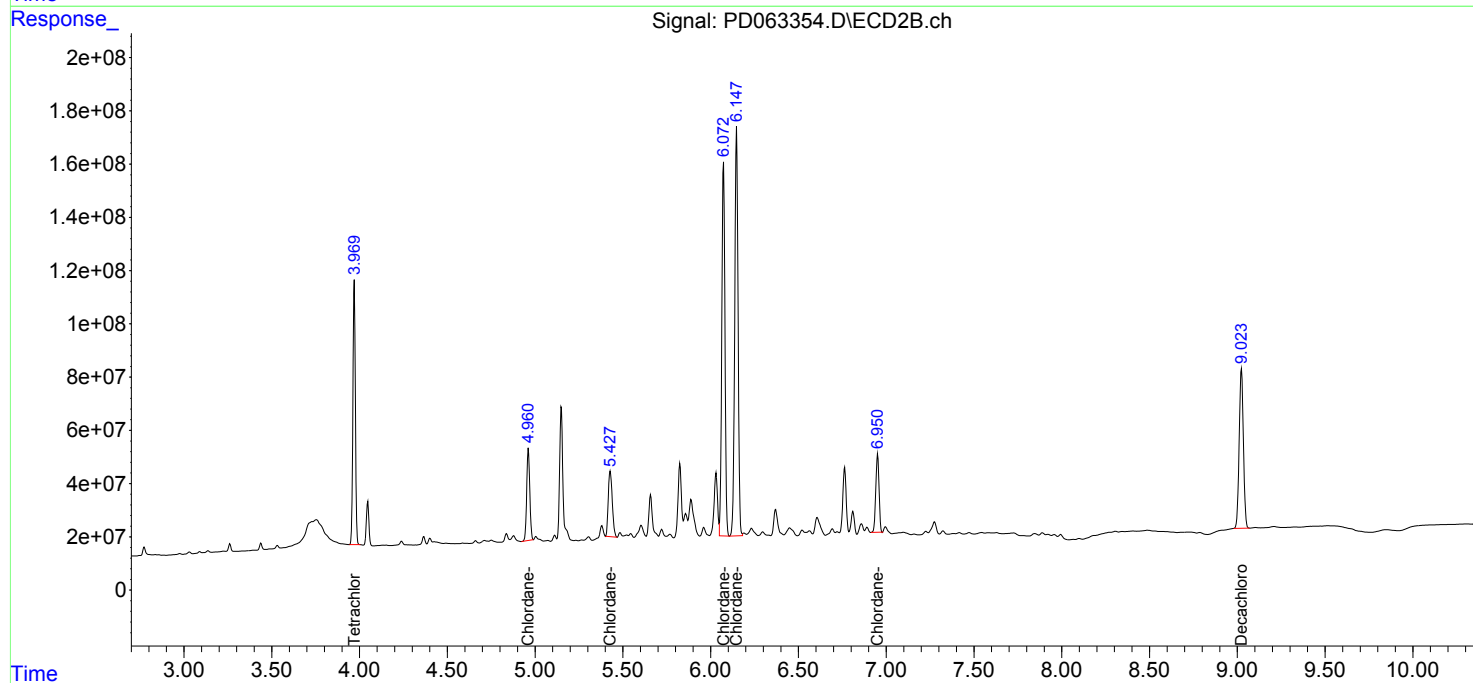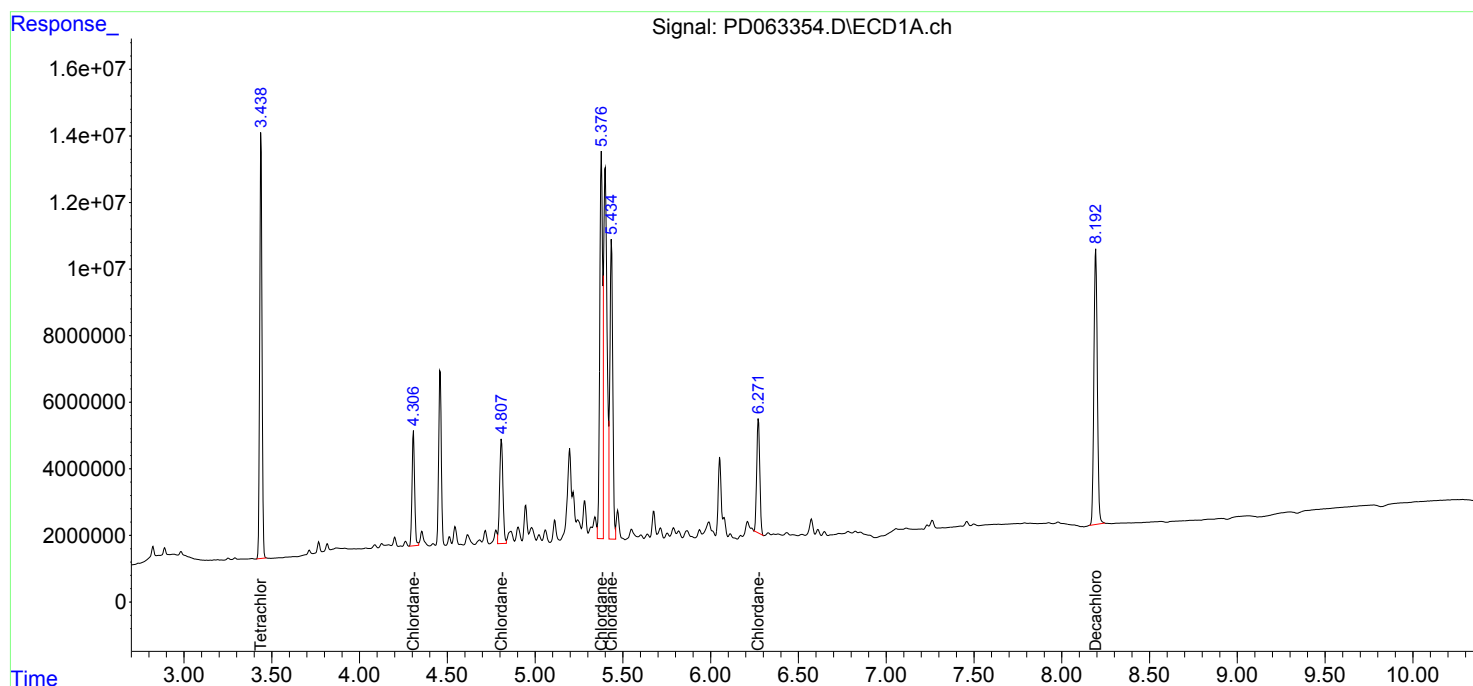


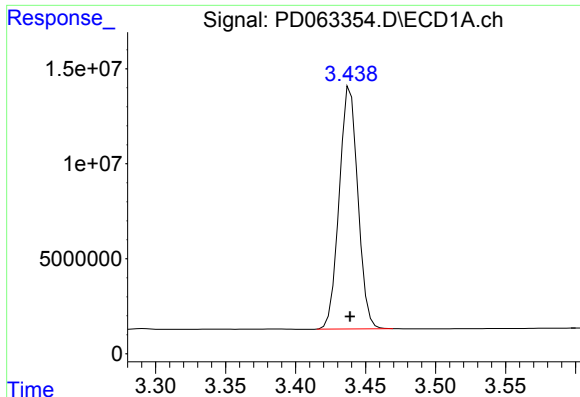

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 118222082
Conc: 74.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

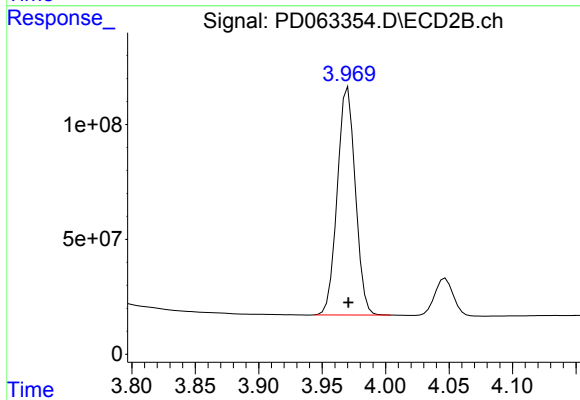


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 980694297
Conc: 72.19 ng/ml

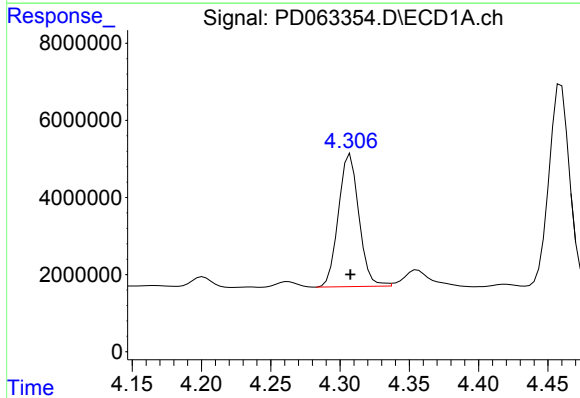


#23 Chlordane-1

R.T.: 4.307 min
Delta R.T.: 0.000 min
Response: 35392078
Conc: 740.35 ng/ml

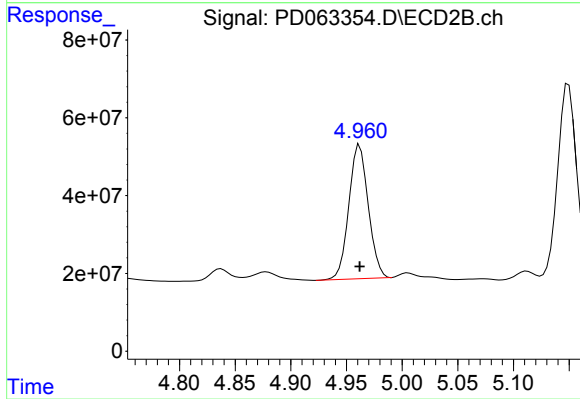

#23 Chlordane-1


R.T.: 4.962 min
Delta R.T.: 0.000 min
Response: 418681896
Conc: 727.84 ng/ml

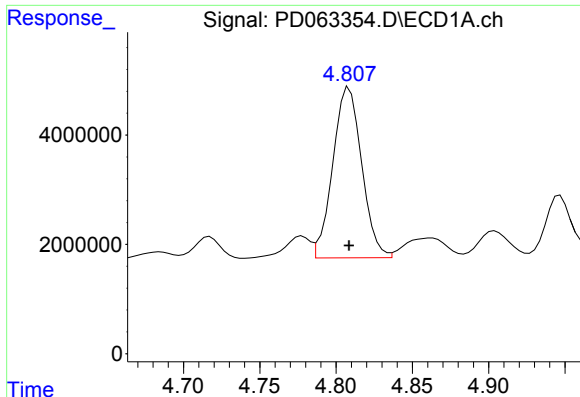

#24 Chlordane-2


R.T.: 4.809 min
Delta R.T.: 0.000 min
Response: 41145617
Conc: 722.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

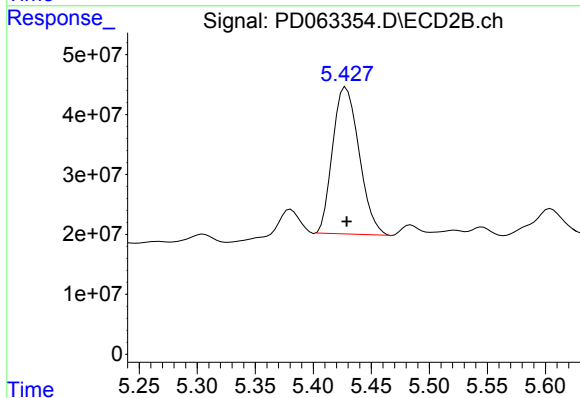


#24 Chlordane-2

R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 389567023
Conc: 713.45 ng/ml

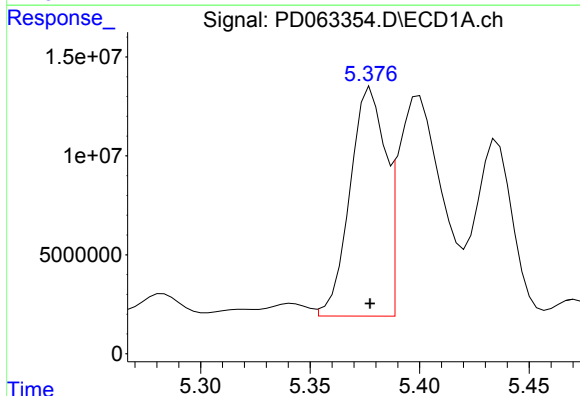


#25 Chlordane-3

R.T.: 5.378 min
Delta R.T.: 0.000 min
Response: 129254848
Conc: 754.10 ng/ml

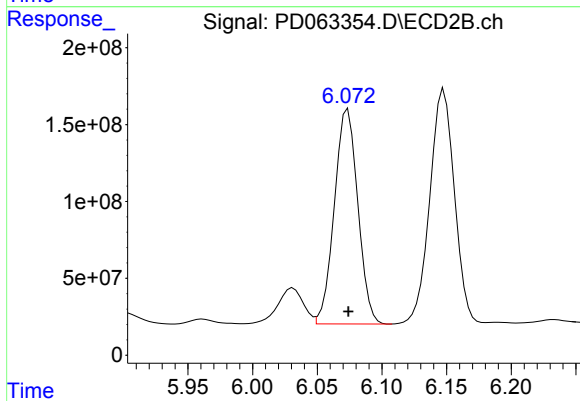

#25 Chlordane-3


R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 1764099779
Conc: 723.37 ng/ml

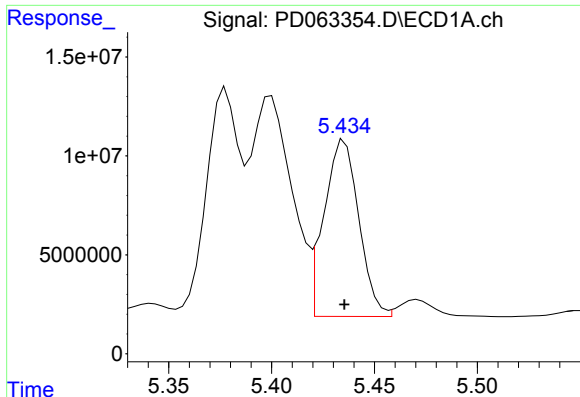

#26 Chlordane-4


R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 104974726
Conc: 741.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

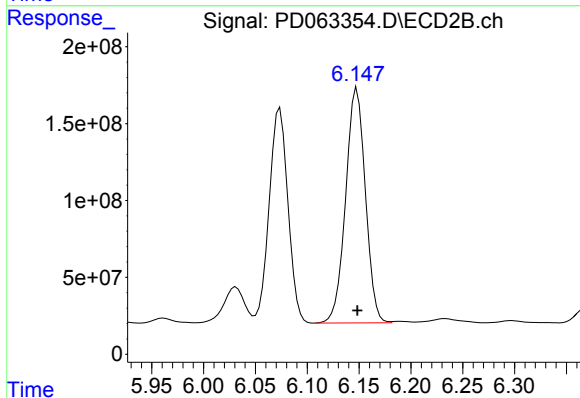


#26 Chlordane-4

R.T.: 6.148 min
Delta R.T.: 0.000 min
Response: 2025660105
Conc: 721.04 ng/ml

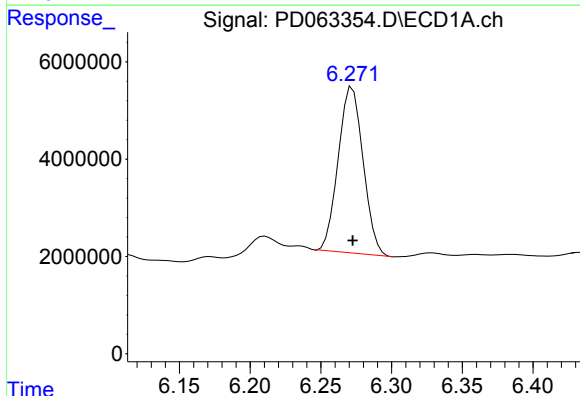


#27 Chlordane-5

R.T.: 6.272 min
Delta R.T.: 0.000 min
Response: 41714233
Conc: 742.94 ng/ml

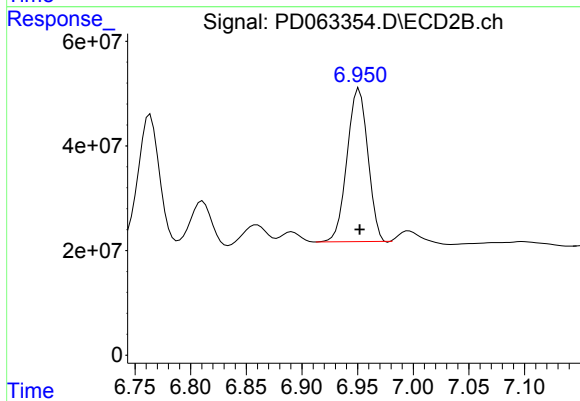

#27 Chlordane-5


R.T.: 6.951 min
Delta R.T.: 0.000 min
Response: 379576527
Conc: 727.27 ng/ml

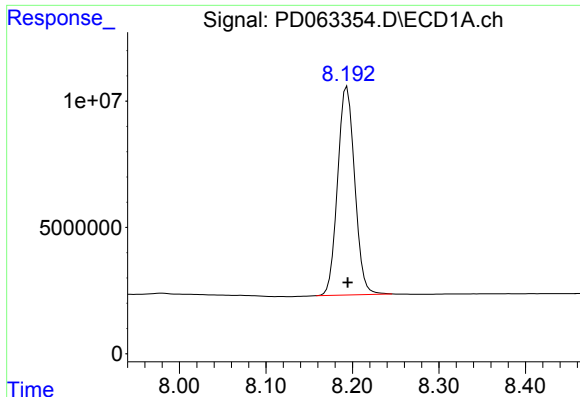

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 112634586
Conc: 70.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

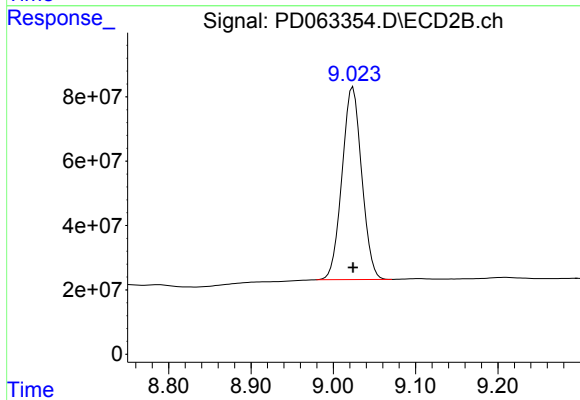

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 996045787
Conc: 70.84 ng/ml