

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060221\
 Data File : PD063355.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 12:10
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 12:57:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 12:56:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.971	78870127	679.3E6	50.000	50.000
28)	SA Decachlor...	8.194	9.024	79953682	703.0E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.308	4.962	23902200	287.6E6	500.000	500.000
24)	Chlordane-2	4.808	5.429	28481057	273.0E6	500.000	500.000
25)	Chlordane-3	5.377	6.074	85701113	1219.4E6	500.000	500.000
26)	Chlordane-4	5.435	6.149	70751068	1404.7E6	500.000	500.000
27)	Chlordane-5	6.272	6.952	28073808	261.0E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060221\
Data File : PD063355.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 12:10
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 12:57:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 12:56:45 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

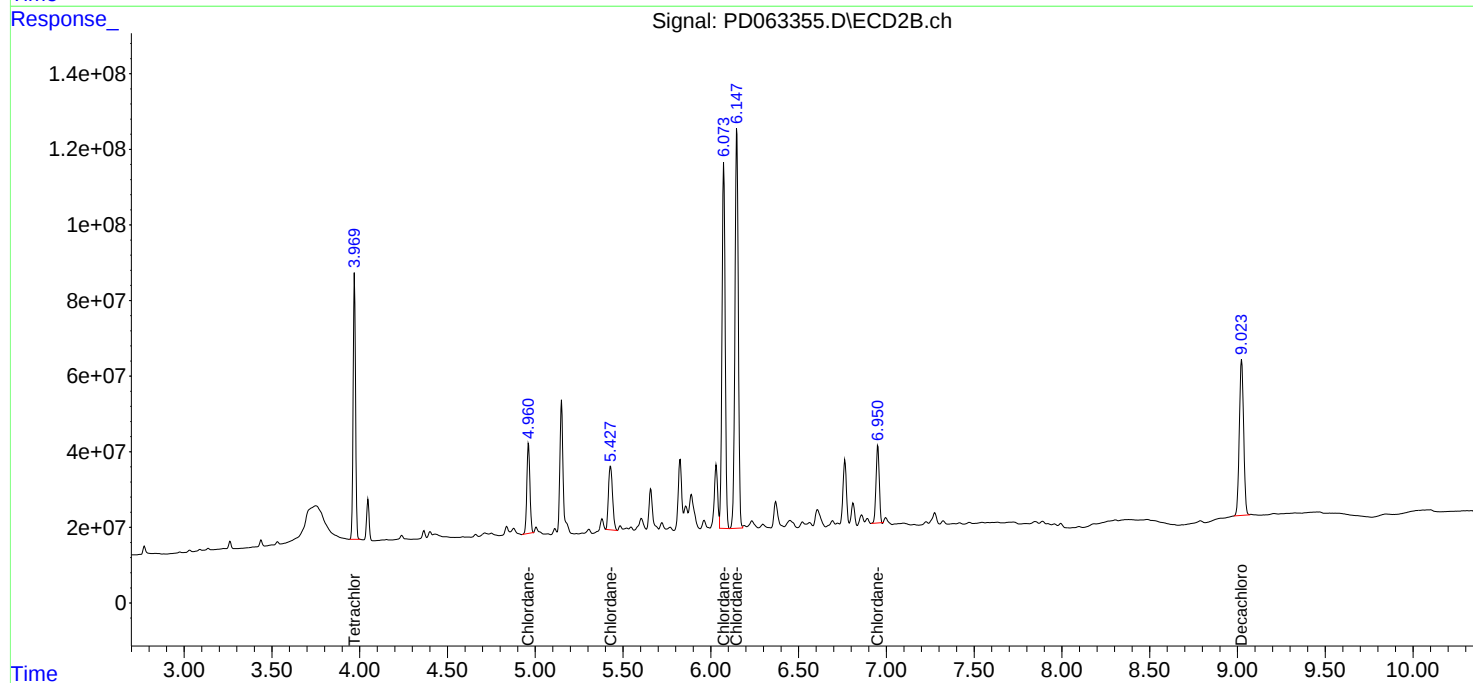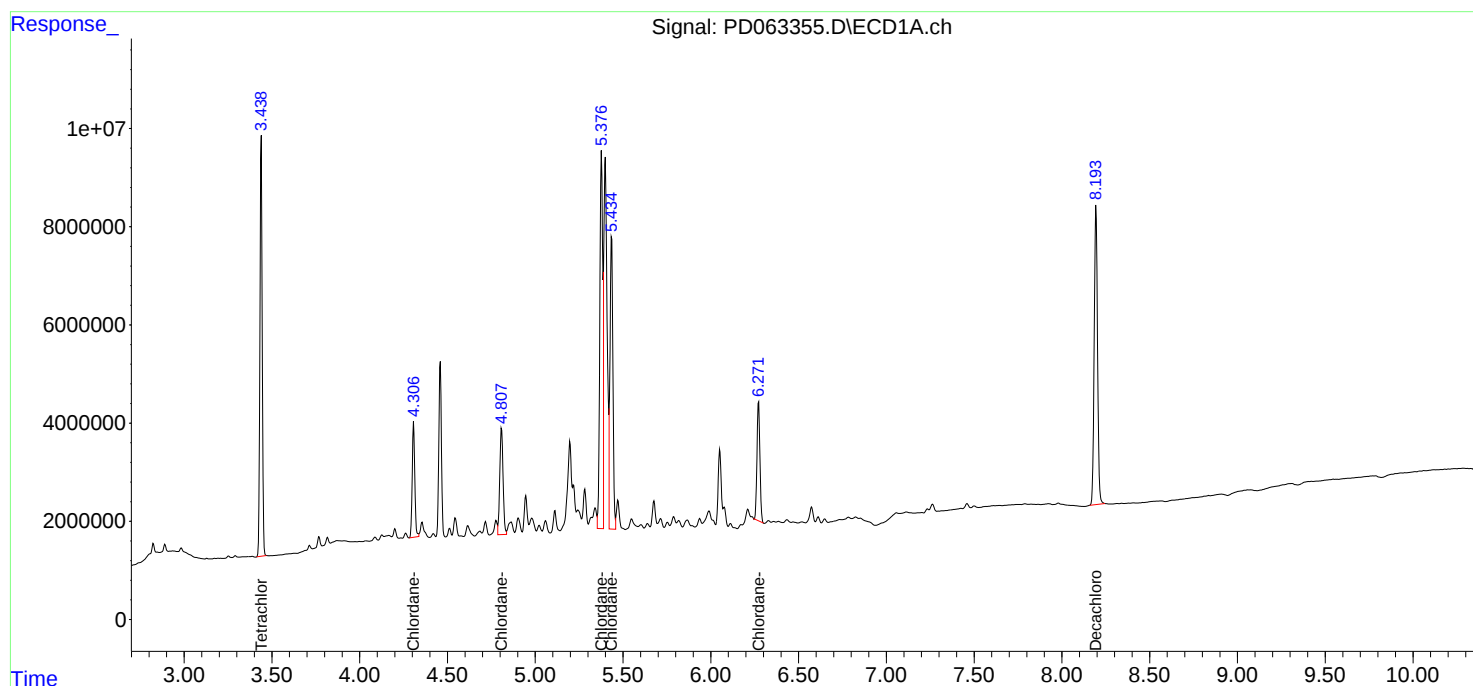


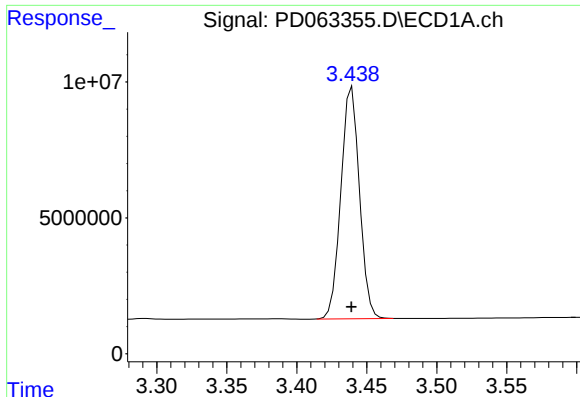

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 78870127
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

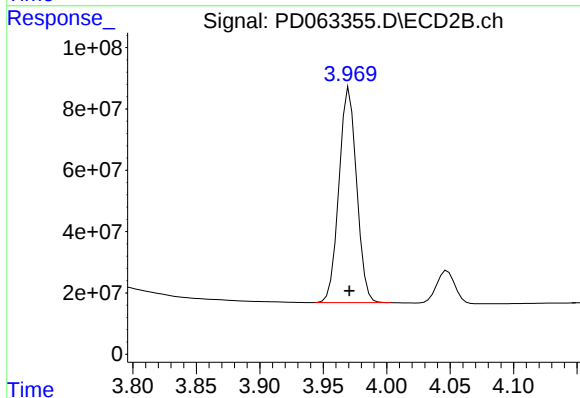


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 679272995
Conc: 50.00 ng/ml

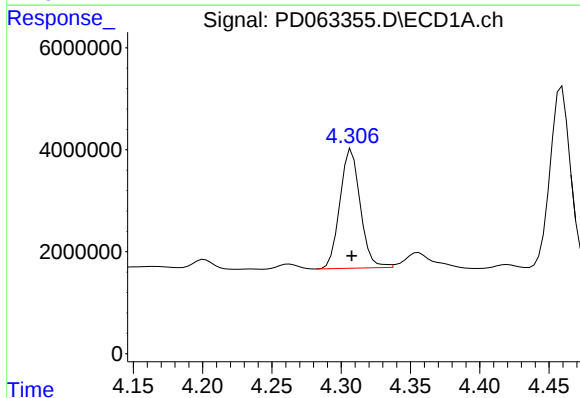


#23 Chlordane-1

R.T.: 4.308 min
Delta R.T.: 0.000 min
Response: 23902200
Conc: 500.00 ng/ml

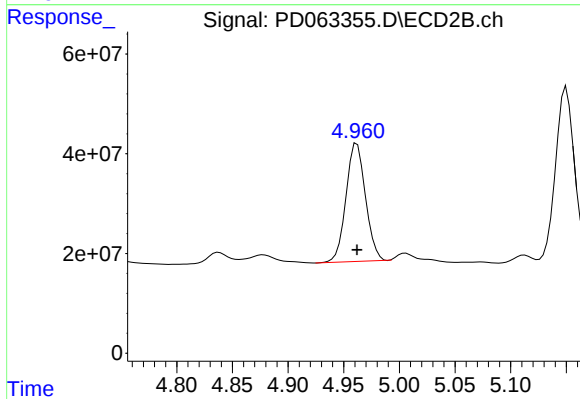

#23 Chlordane-1


R.T.: 4.962 min
Delta R.T.: 0.000 min
Response: 287618971
Conc: 500.00 ng/ml

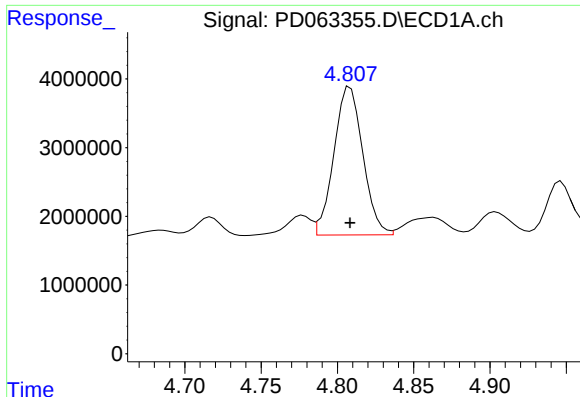

#24 Chlordane-2


R.T.: 4.808 min
Delta R.T.: 0.000 min
Response: 28481057
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

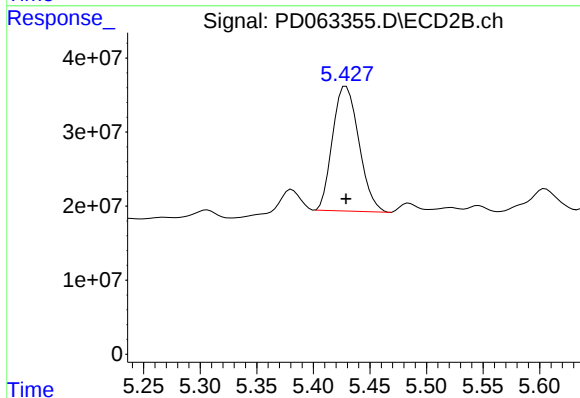


#24 Chlordane-2

R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 273017625
Conc: 500.00 ng/ml

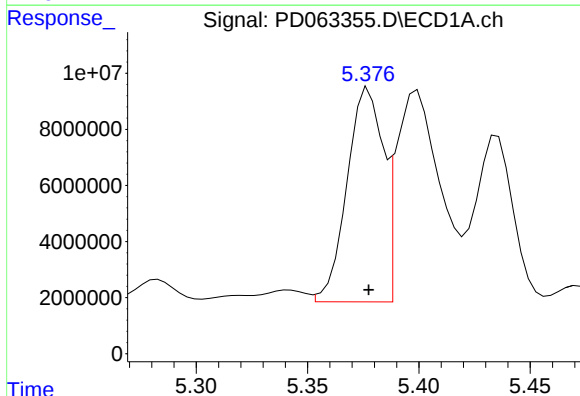


#25 Chlordane-3

R.T.: 5.377 min
Delta R.T.: 0.000 min
Response: 85701113
Conc: 500.00 ng/ml

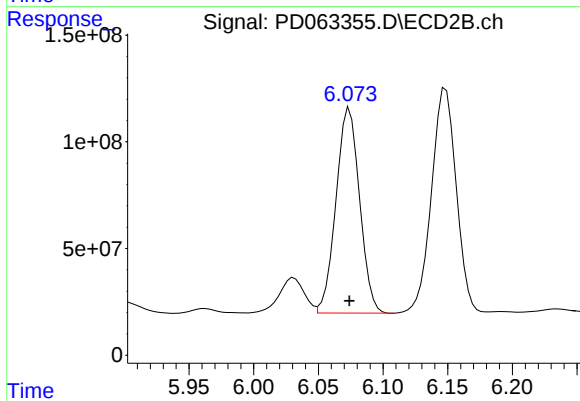

#25 Chlordane-3


R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 1219367266
Conc: 500.00 ng/ml

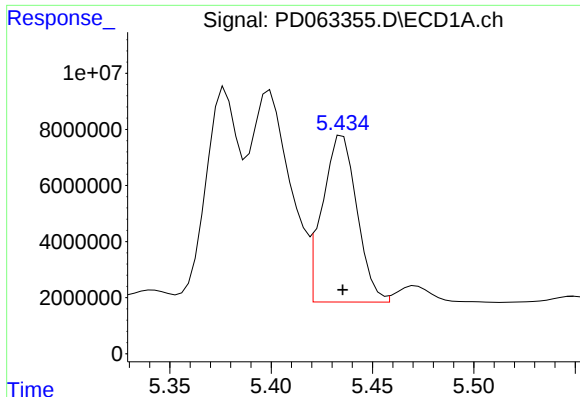

#26 Chlordane-4


R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 70751068
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

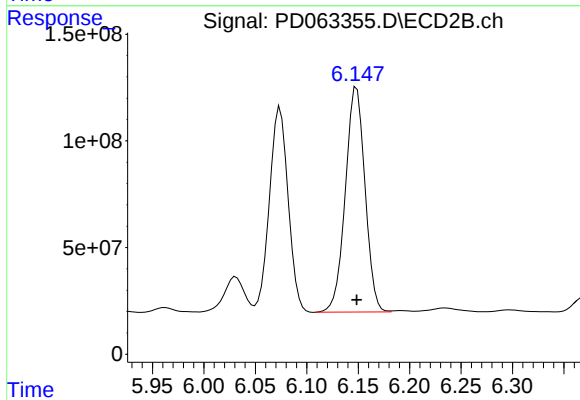


#26 Chlordane-4

R.T.: 6.149 min
Delta R.T.: 0.000 min
Response: 1404680467
Conc: 500.00 ng/ml

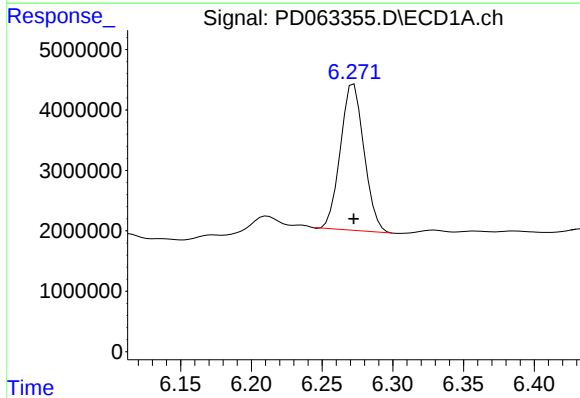


#27 Chlordane-5

R.T.: 6.272 min
Delta R.T.: 0.000 min
Response: 28073808
Conc: 500.00 ng/ml

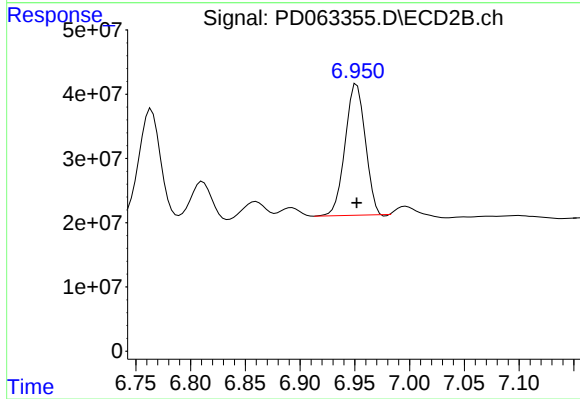

#27 Chlordane-5


R.T.: 6.952 min
Delta R.T.: 0.000 min
Response: 260958508
Conc: 500.00 ng/ml

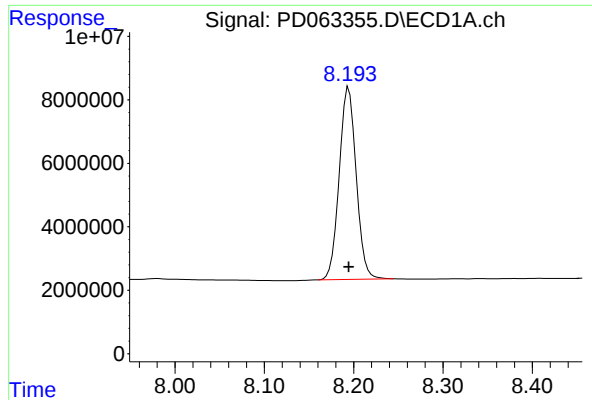

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 79953682
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

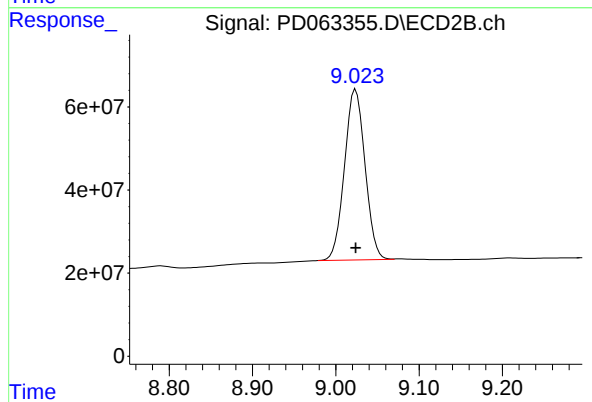

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 703001780
Conc: 50.00 ng/ml