

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060221\
 Data File : PD063356.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 12:24
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 12:58:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 12:56:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.970	38877931	351.9E6	24.647	25.903
28)	SA Decachlor...	8.193	9.023	40939235	374.2E6	25.602	26.612
Target Compounds							
23)	Chlordane-1	4.307	4.961	12010419	145.0E6	251.241	252.065
24)	Chlordane-2	4.809	5.428	14881124	143.1E6	261.246	261.982
25)	Chlordane-3	5.377	6.074	42257277	626.5E6	246.539	256.875
26)	Chlordane-4	5.435	6.148	34783402	726.0E6	245.815	258.431
27)	Chlordane-5	6.272	6.951	13496176	133.9E6	240.370	256.622



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060221\
Data File : PD063356.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 12:24
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 12:58:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 12:56:45 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

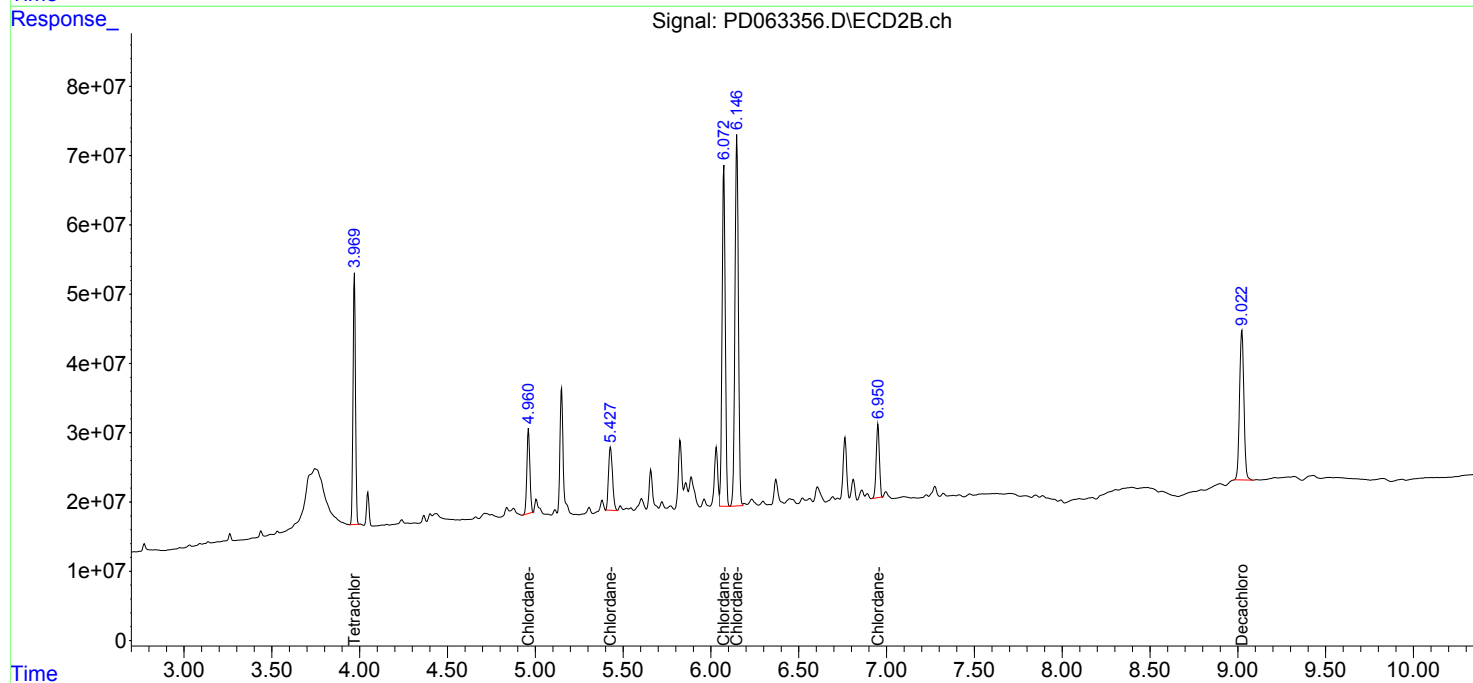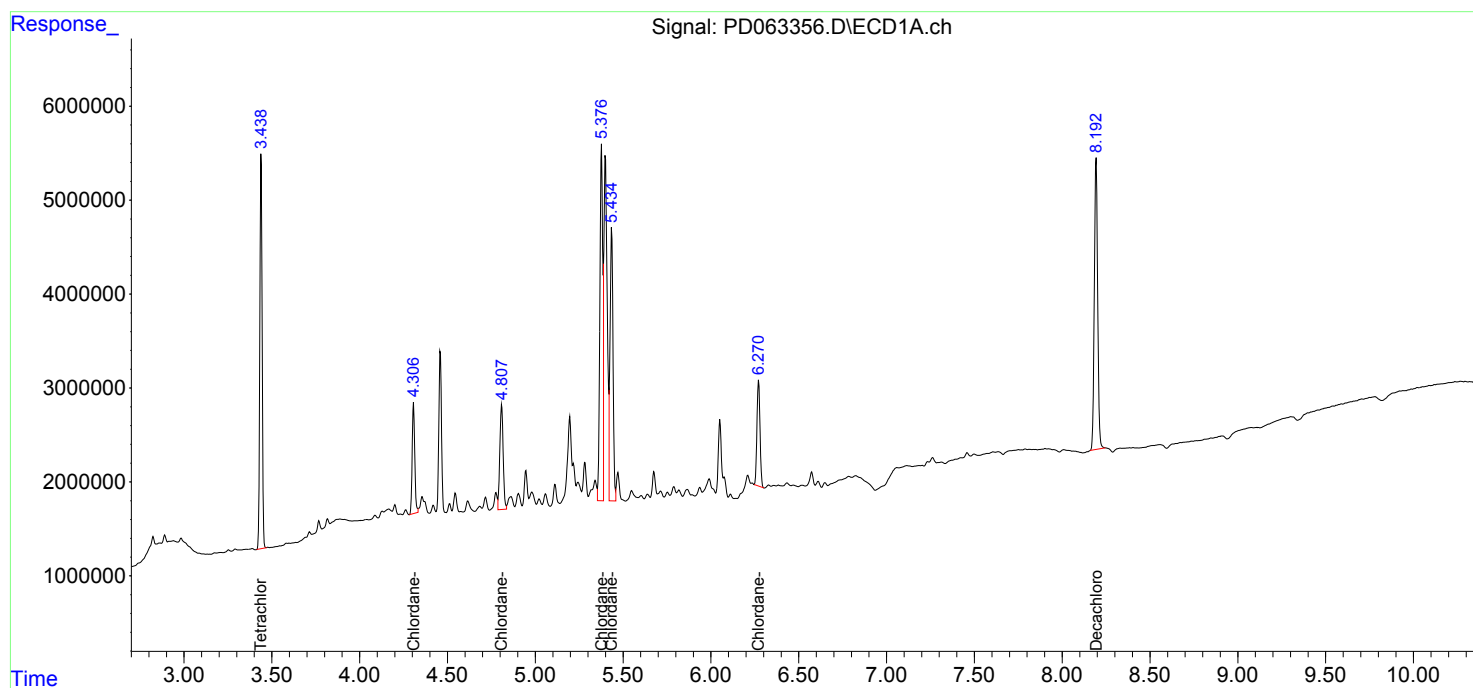


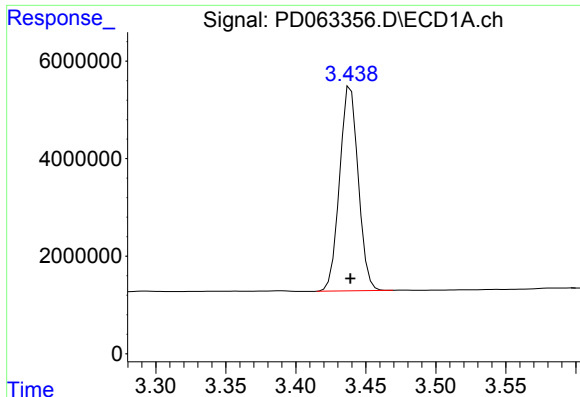

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 38877931
Conc: 24.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

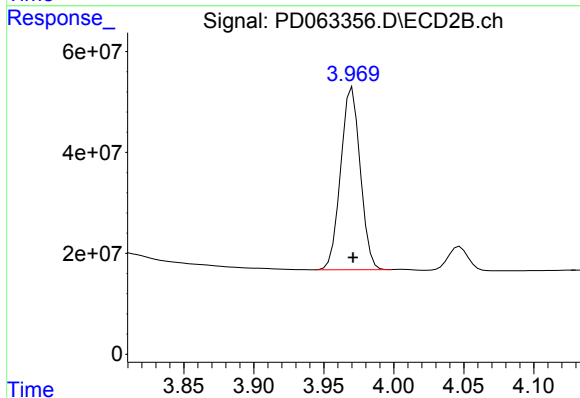


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 351900507
Conc: 25.90 ng/ml

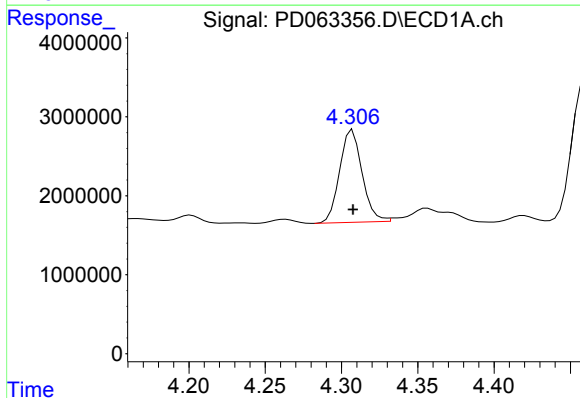


#23 Chlordane-1

R.T.: 4.307 min
Delta R.T.: 0.000 min
Response: 12010419
Conc: 251.24 ng/ml

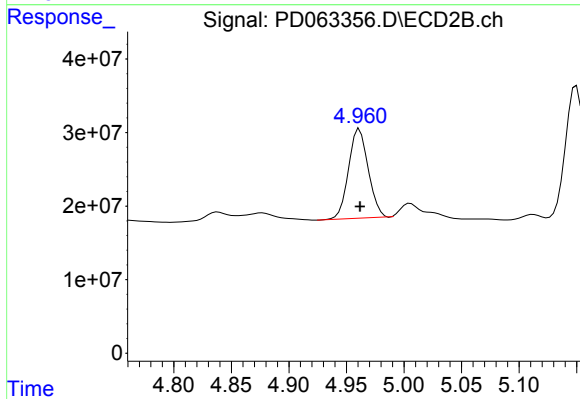

#23 Chlordane-1


R.T.: 4.961 min
Delta R.T.: 0.000 min
Response: 144997216
Conc: 252.06 ng/ml

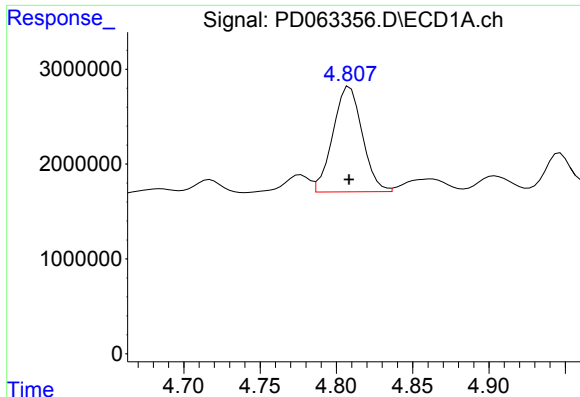

#24 Chlordane-2


R.T.: 4.809 min
Delta R.T.: 0.000 min
Response: 14881124
Conc: 261.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

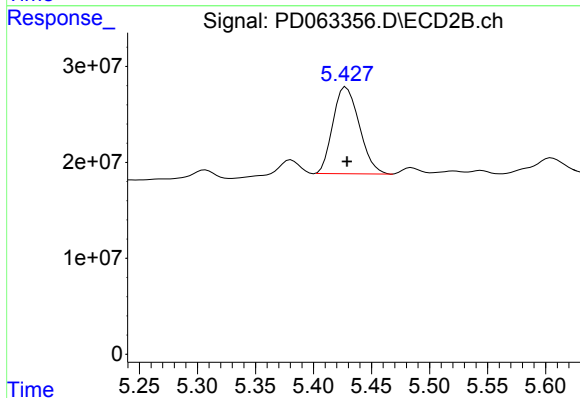


#24 Chlordane-2

R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 143051202
Conc: 261.98 ng/ml

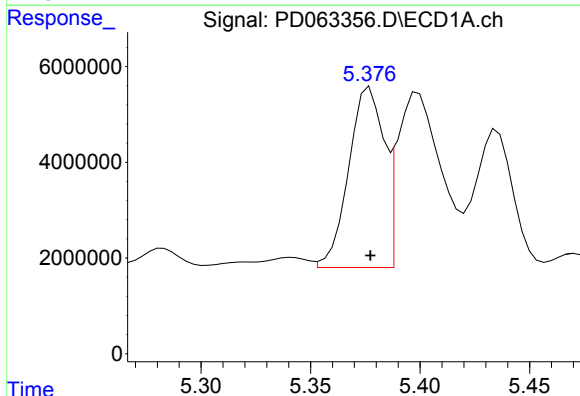


#25 Chlordane-3

R.T.: 5.377 min
Delta R.T.: 0.000 min
Response: 42257277
Conc: 246.54 ng/ml

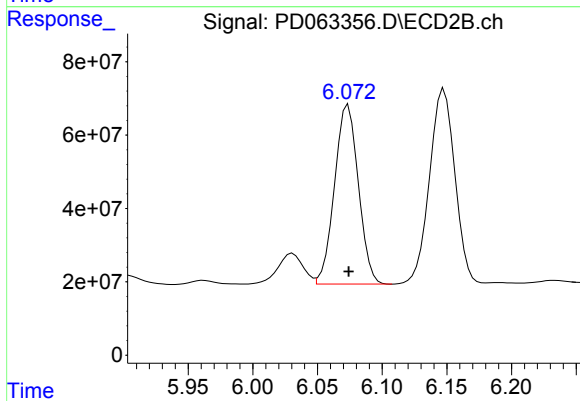

#25 Chlordane-3


R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 626450388
Conc: 256.88 ng/ml

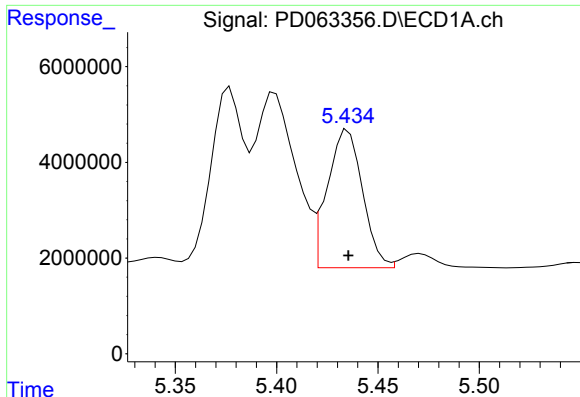

#26 Chlordane-4


R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 34783402
Conc: 245.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

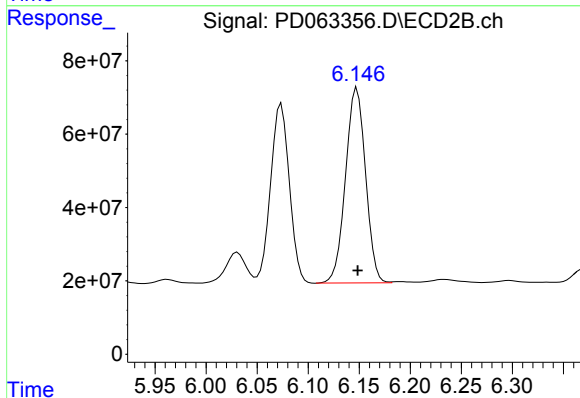


#26 Chlordane-4

R.T.: 6.148 min
Delta R.T.: 0.000 min
Response: 726025510
Conc: 258.43 ng/ml

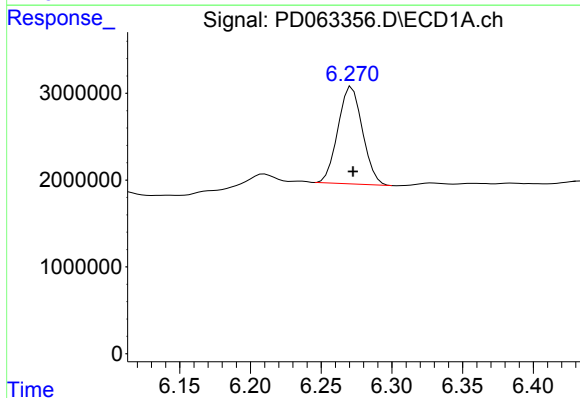


#27 Chlordane-5

R.T.: 6.272 min
Delta R.T.: 0.000 min
Response: 13496176
Conc: 240.37 ng/ml

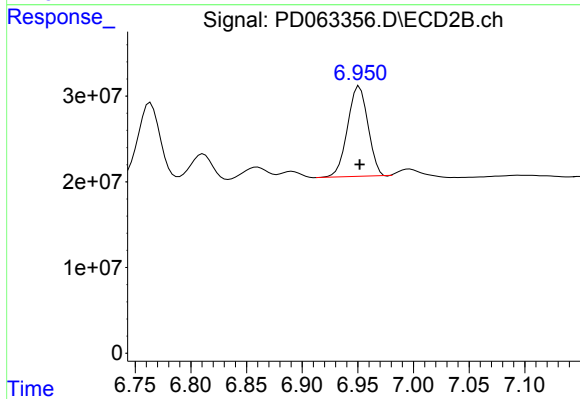

#27 Chlordane-5


R.T.: 6.951 min
Delta R.T.: 0.000 min
Response: 133935568
Conc: 256.62 ng/ml

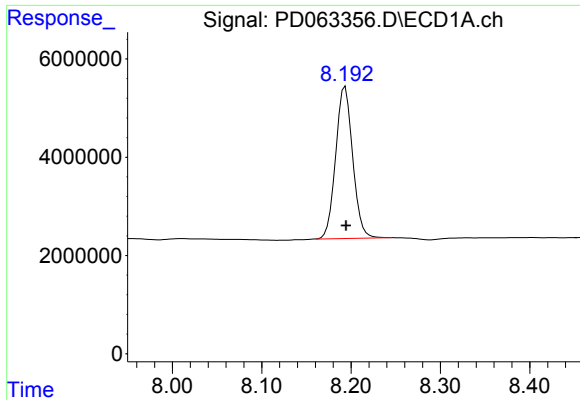

#28 Decachlorobiphenyl

R.T.: 8.193 min
Delta R.T.: -0.001 min
Response: 40939235
Conc: 25.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

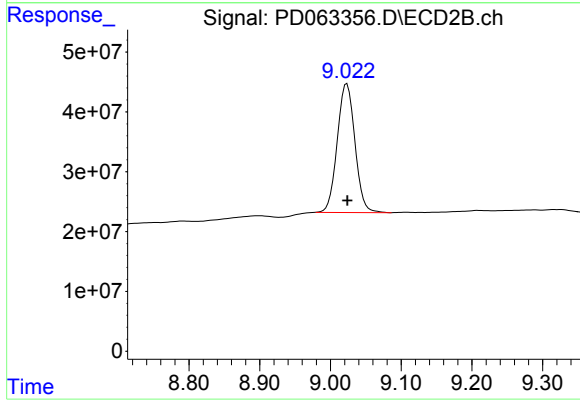

#28 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: 0.000 min
Response: 374172379
Conc: 26.61 ng/ml