

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060221\
 Data File : PD063364.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 14:17
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICPD060221

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 01:25:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 00:19:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.971	79285813	676.8E6	50.105	49.018
28)	SA Decachlor...	8.196	9.024	81369418	709.5E6	50.739	48.794
Target Compounds							
23)	Chlordane-1	4.309	4.962	24814436	300.7E6	511.173	519.936
24)	Chlordane-2	4.810	5.429	28823467	276.8E6	494.211	494.718
25)	Chlordane-3	5.379	6.074	88369015	1236.4E6	519.546	500.462
26)	Chlordane-4	5.437	6.149	71964685	1421.2E6	516.314	497.216
27)	Chlordane-5	6.273	6.953	28550733	277.4E6	515.756	530.890



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060221\
Data File : PD063364.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 14:17
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD060221

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 01:25:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 00:19:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

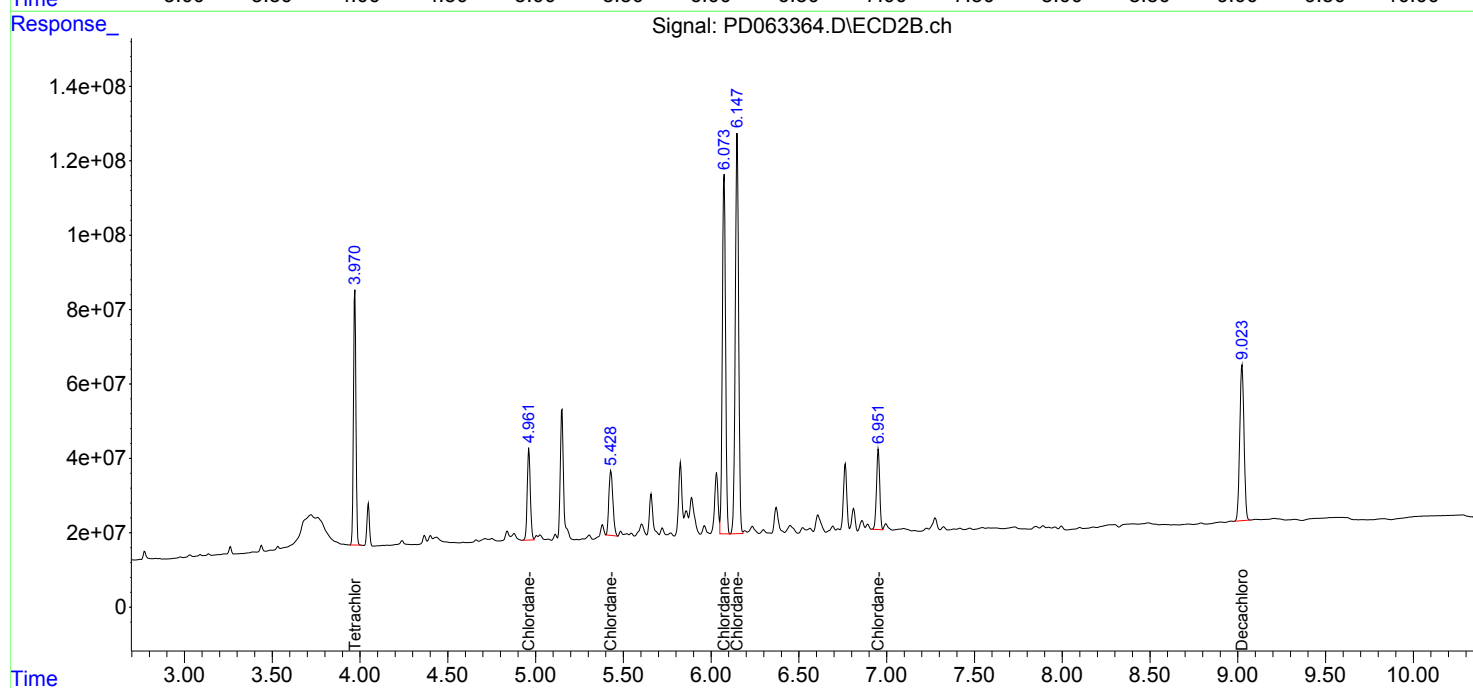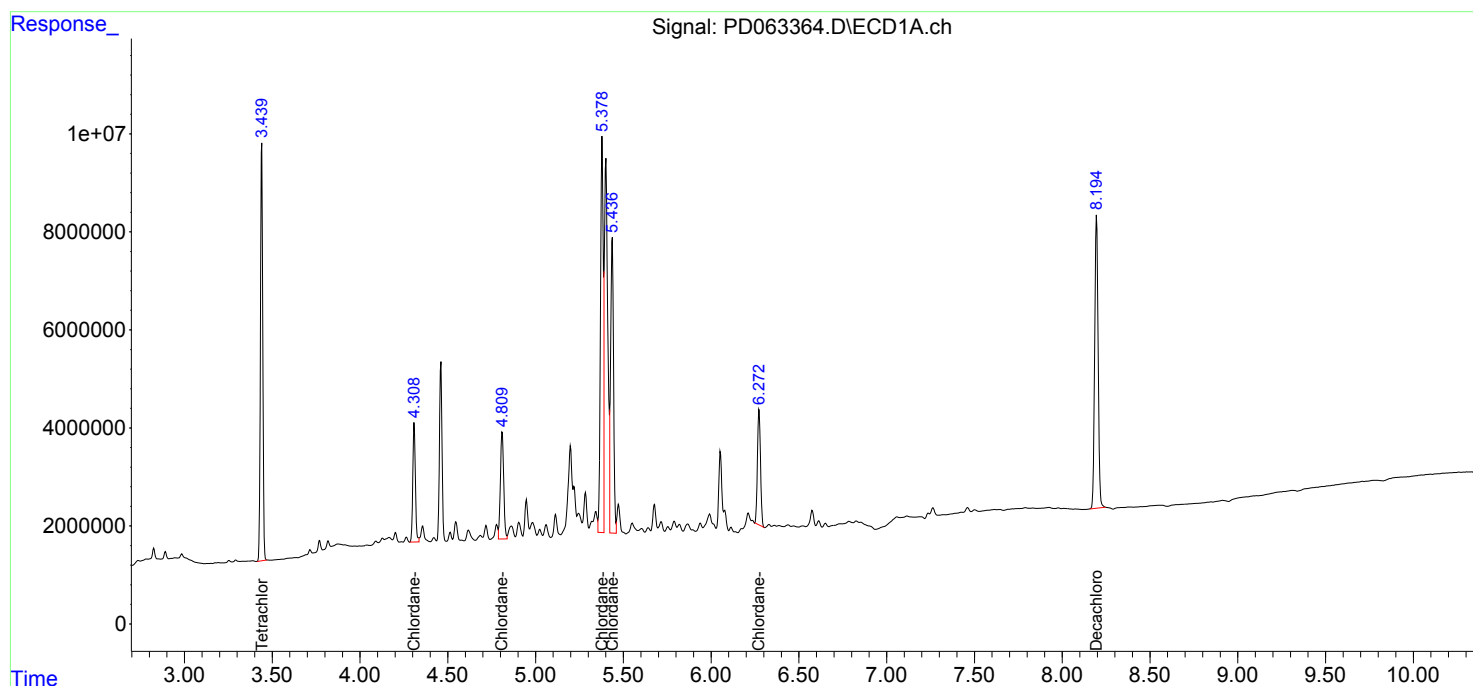


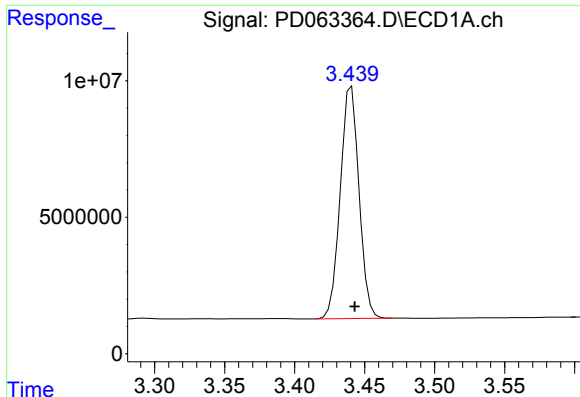

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: -0.002 min
Response: 79285813
Conc: 50.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD060221

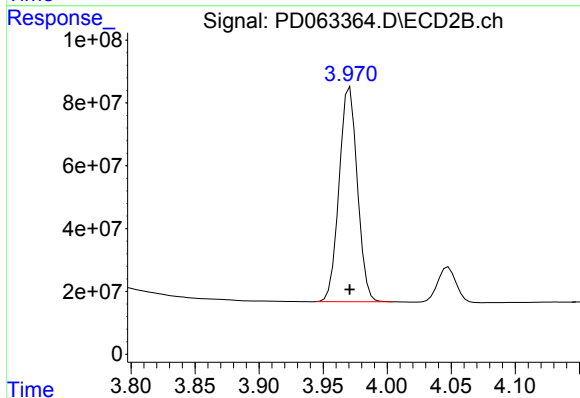


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 676790990
Conc: 49.02 ng/ml

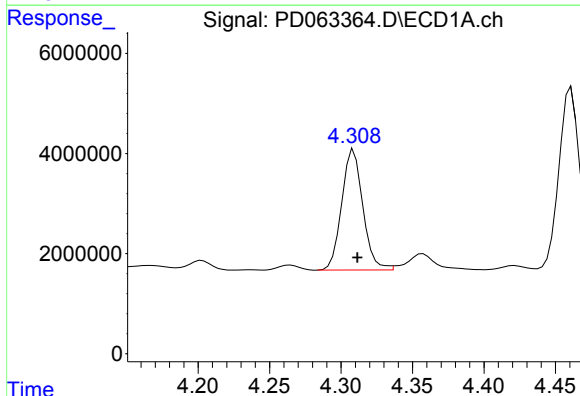


#23 Chlordane-1

R.T.: 4.309 min
Delta R.T.: -0.002 min
Response: 24814436
Conc: 511.17 ng/ml

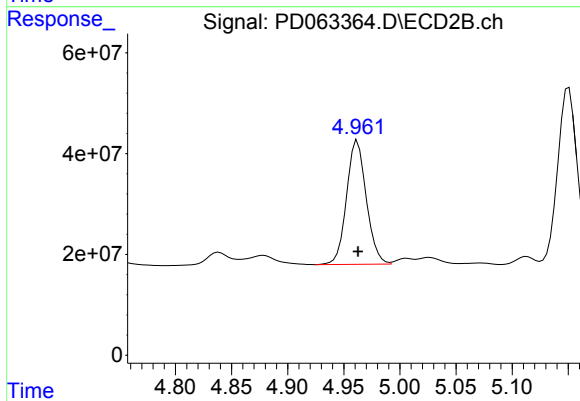

#23 Chlordane-1


R.T.: 4.962 min
Delta R.T.: 0.000 min
Response: 300748109
Conc: 519.94 ng/ml

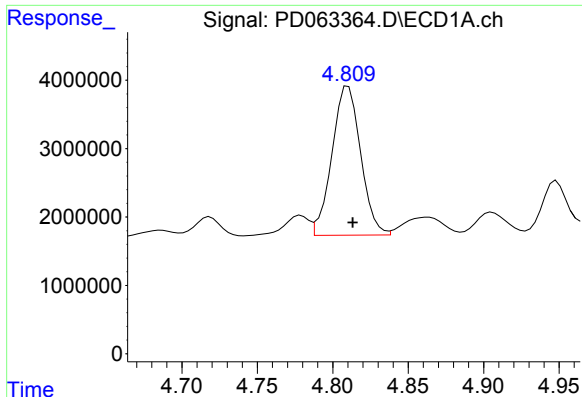

#24 Chlordane-2


R.T.: 4.810 min
Delta R.T.: -0.003 min
Response: 28823467
Conc: 494.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD060221

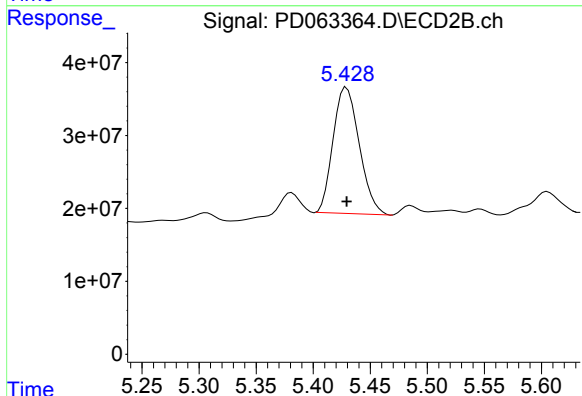


#24 Chlordane-2

R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 276779221
Conc: 494.72 ng/ml

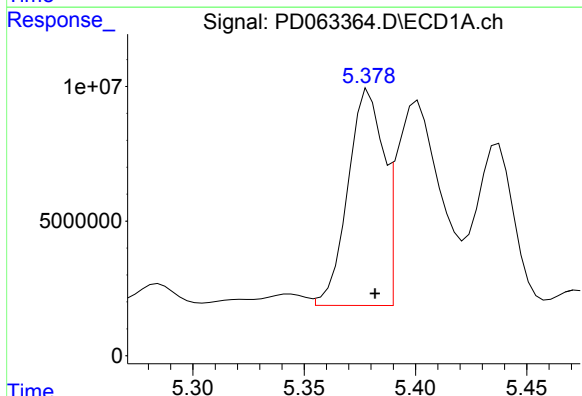


#25 Chlordane-3

R.T.: 5.379 min
Delta R.T.: -0.003 min
Response: 88369015
Conc: 519.55 ng/ml

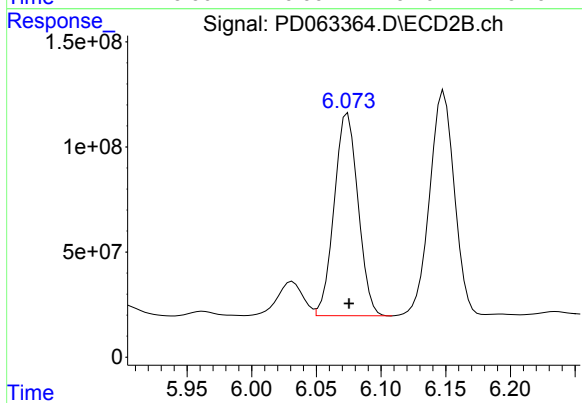

#25 Chlordane-3


R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 1236444825
Conc: 500.46 ng/ml

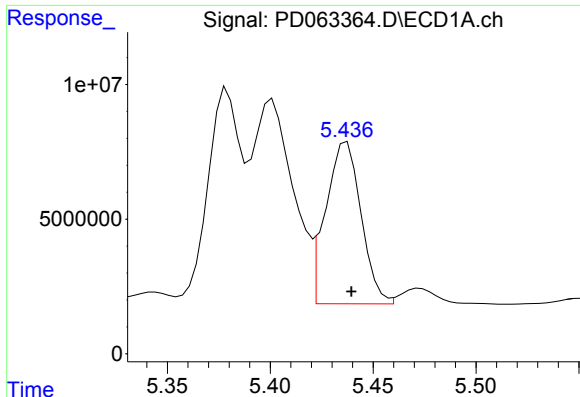

#26 Chlordane-4


R.T.: 5.437 min
Delta R.T.: -0.002 min
Response: 71964685
Conc: 516.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD060221

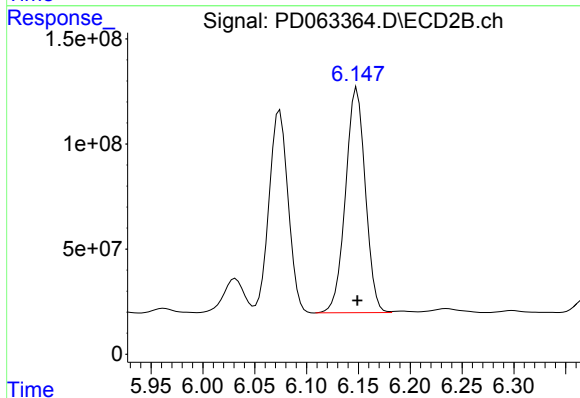


#26 Chlordane-4

R.T.: 6.149 min
Delta R.T.: 0.000 min
Response: 1421193215
Conc: 497.22 ng/ml

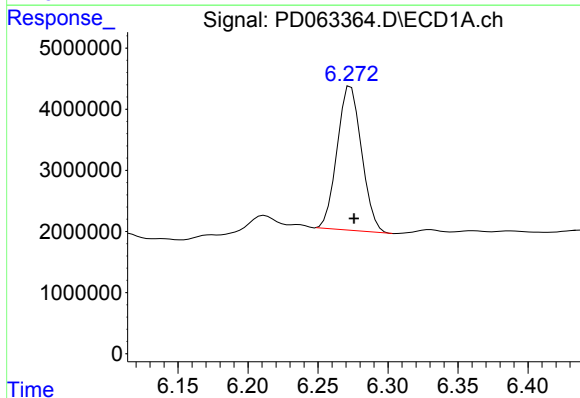


#27 Chlordane-5

R.T.: 6.273 min
Delta R.T.: -0.002 min
Response: 28550733
Conc: 515.76 ng/ml

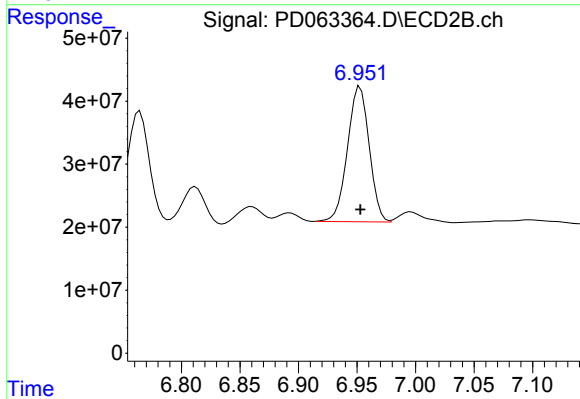

#27 Chlordane-5


R.T.: 6.953 min
Delta R.T.: 0.000 min
Response: 277391562
Conc: 530.89 ng/ml

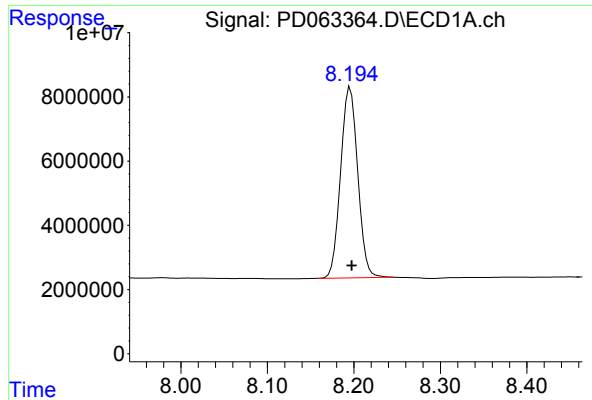

#28 Decachlorobiphenyl

R.T.: 8.196 min
Delta R.T.: -0.002 min
Response: 81369418
Conc: 50.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD060221

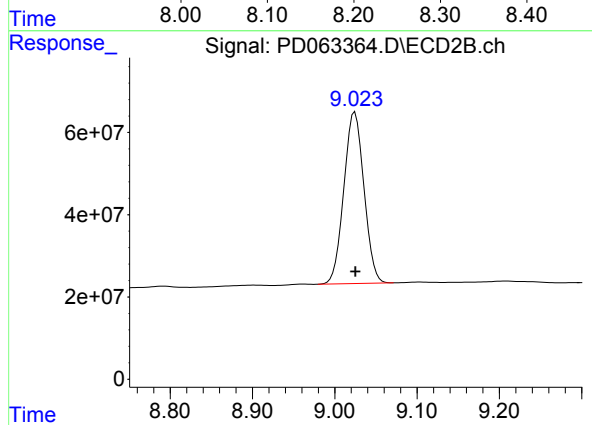

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 709463622
Conc: 48.79 ng/ml