

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060319\
 Data File : PD053470.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Jun 2019 8:43
 Operator : SM\AJ
 Sample : PIBLK31
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK31

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 04:09:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052119CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed May 22 06:53:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.317	3.985	16388954	24023160	22.368	24.400
27) SA Decachlor...	8.017	9.030	25749135	39805564	38.925	38.536
Target Compounds						
3) MA gamma-BHC...	0.000	4.633	0	80656	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060319\
Data File : PD053470.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Jun 2019 8:43
Operator : SM\AJ
Sample : PIBLK31
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK31

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 04:09:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052119CLP.M
Quant Title : GC Extractables
QLast Update : Wed May 22 06:53:42 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

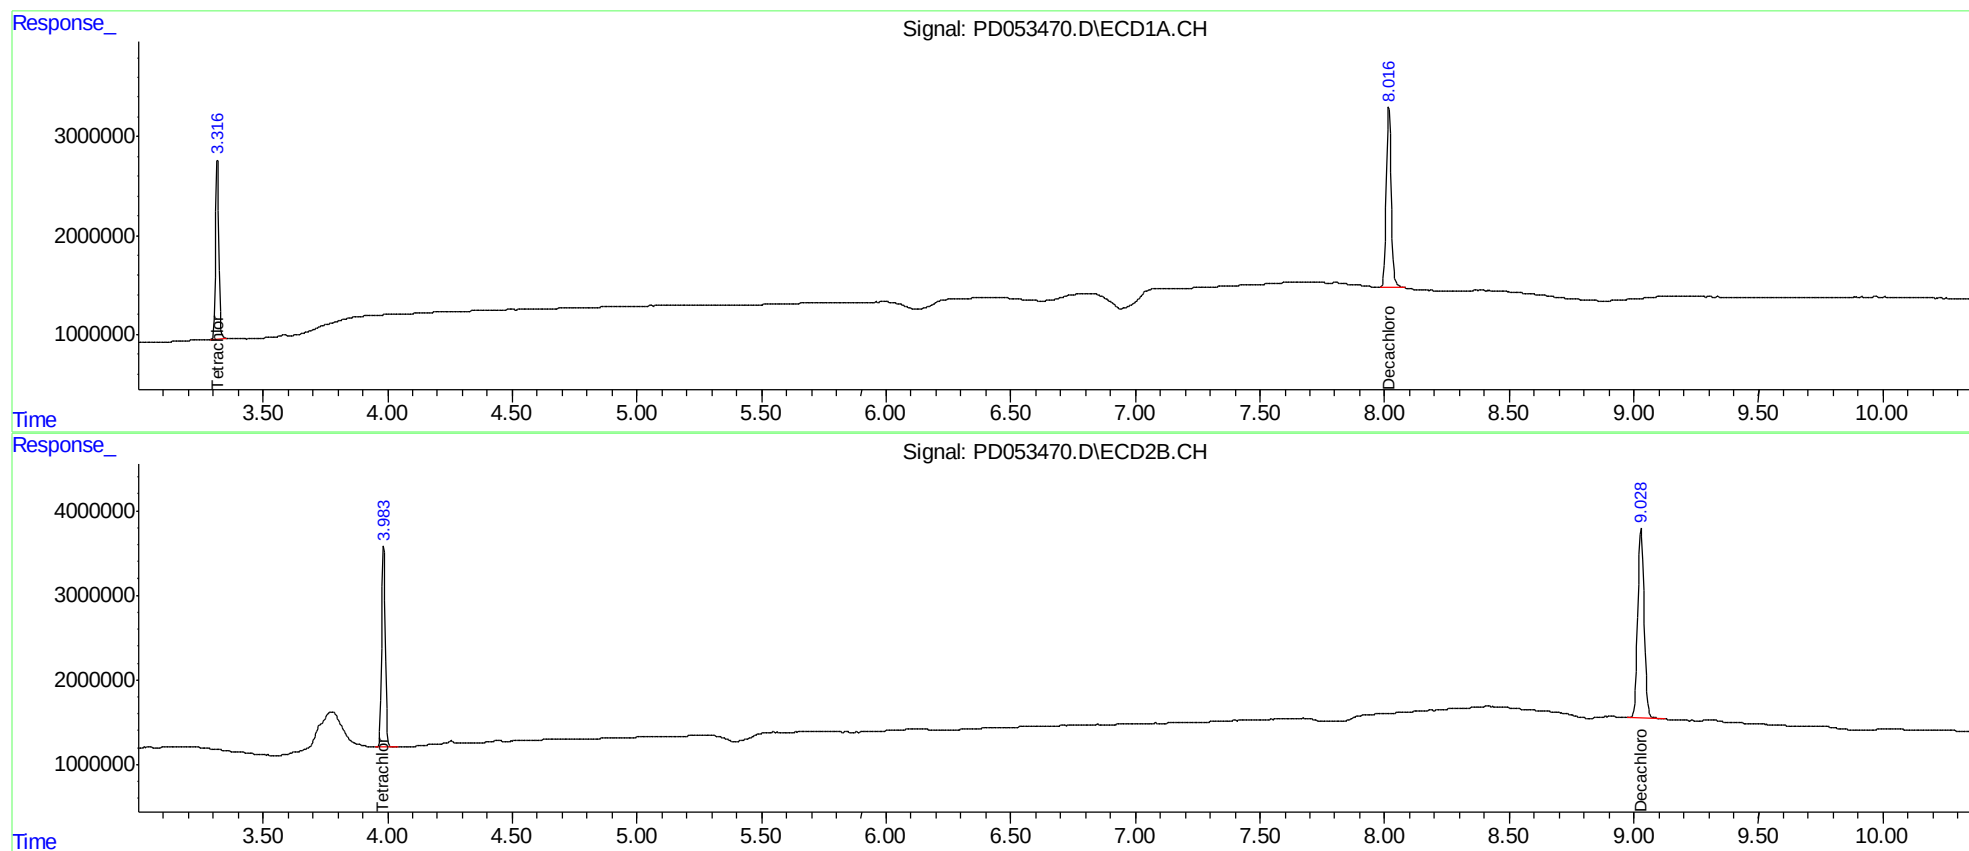


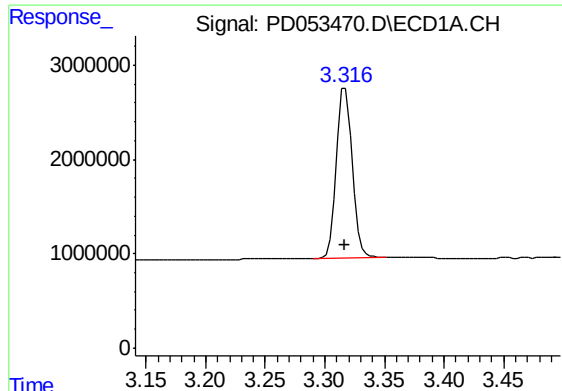

#1 Tetrachloro-m-xylene


R.T.: 3.317 min
Delta R.T.: 0.000 min
Response: 16388954
Conc: 22.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK31

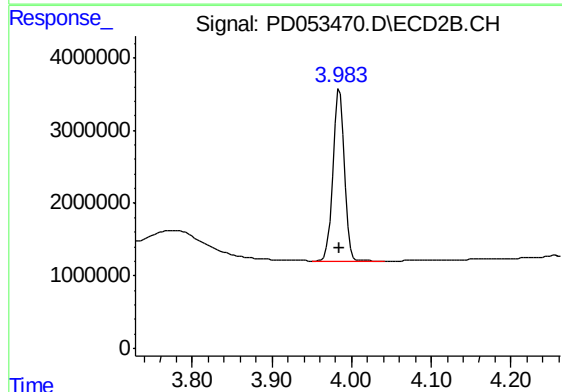


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 24023160
Conc: 24.40 ng/ml

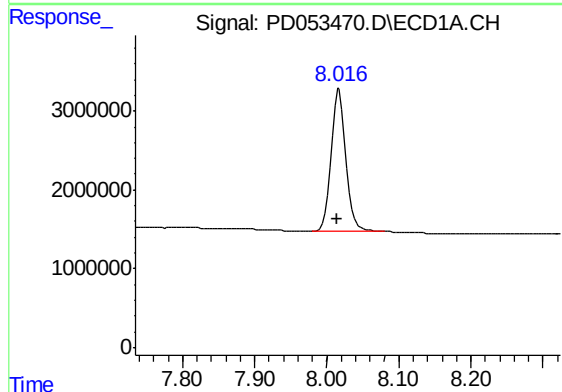

#27 Decachlorobiphenyl

R.T.: 8.017 min
Delta R.T.: 0.002 min
Response: 25749135
Conc: 38.93 ng/ml

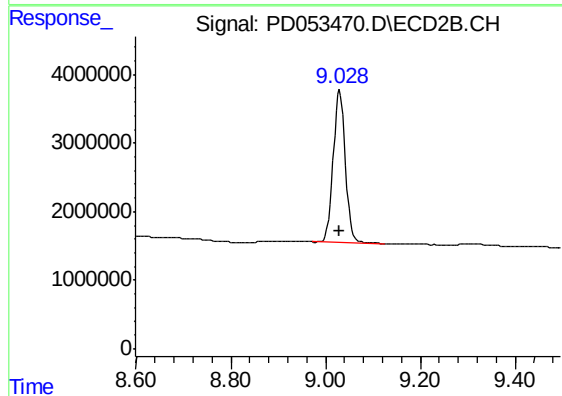

#27 Decachlorobiphenyl

R.T.: 9.030 min
Delta R.T.: 0.000 min
Response: 39805564
Conc: 38.54 ng/ml