

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060321\
 Data File : PD063374.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 17:17
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 05:49:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 05:48:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.970	7146757	76050026	5.215	5.348
27)	SA Decachlor...	8.194	9.024	17263787	163.8E6	10.577	11.196
Target Compounds							
2)	A alpha-BHC	3.875	4.358	9714275	117.3E6	4.774	5.274
3)	MA gamma-BHC...	4.158	4.642	10526100	108.5E6	5.322	5.267
4)	MA Heptachlor	4.459	5.150	9690558	110.9E6	4.994	5.284
9)	A Endosulfan I	5.488	6.196	8220049	95490855	5.027	5.302
13)	MA Dieldrin	5.731	6.453	17873209	205.7E6	9.489	10.661
14)	MA Endrin	5.989	6.670	15984029	169.3E6	9.848	10.562
16)	A 4,4'-DDD	6.115	6.793	13805846	158.4E6	9.254	10.307
17)	MA 4,4'-DDT	6.356	7.092	13477093	159.9E6	8.764	10.323
20)	A Methoxychlor	6.902	7.550	43015519	402.0E6	50.851	54.625


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060321\
Data File : PD063374.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 17:17
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 05:49:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 05:48:53 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

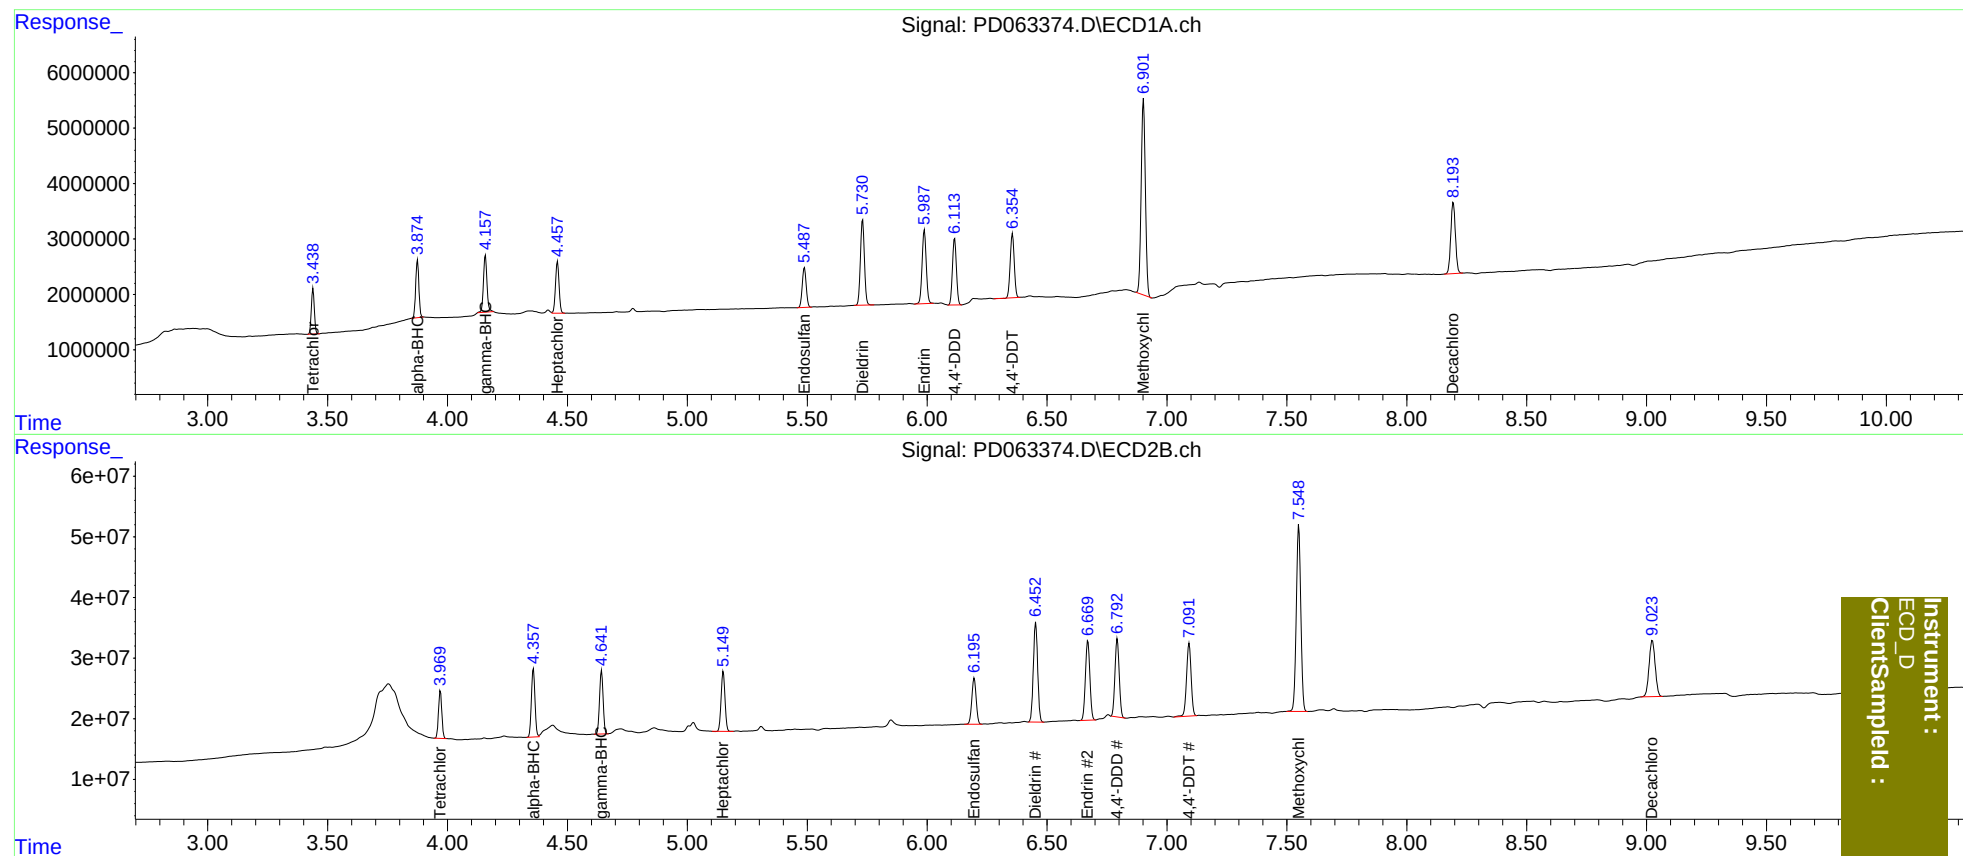


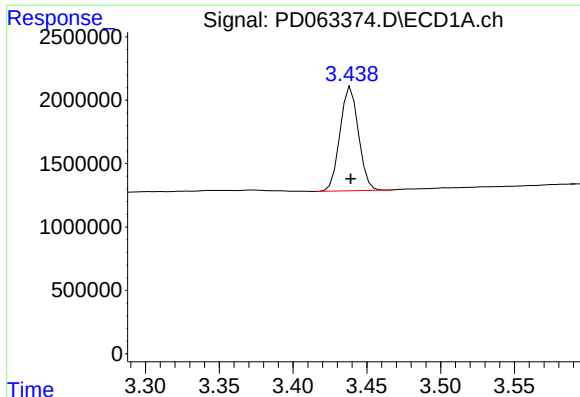

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 7146757
Conc: 5.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

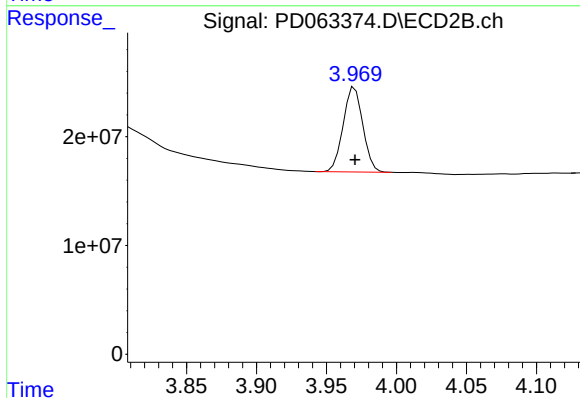


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 76050026
Conc: 5.35 ng/ml

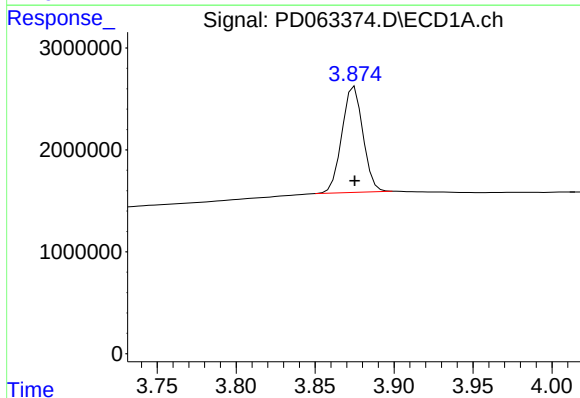


#2 alpha-BHC

R.T.: 3.875 min
Delta R.T.: 0.000 min
Response: 9714275
Conc: 4.77 ng/ml

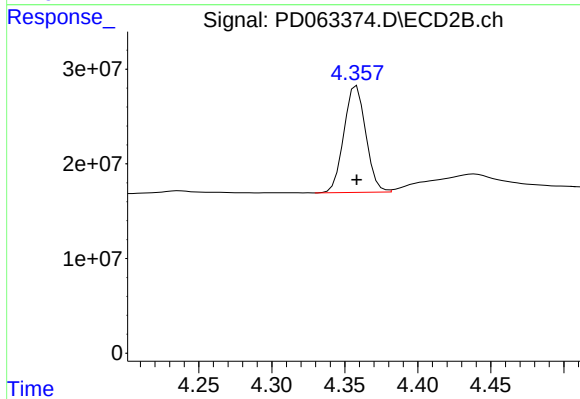

#2 alpha-BHC


R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 117293981
Conc: 5.27 ng/ml

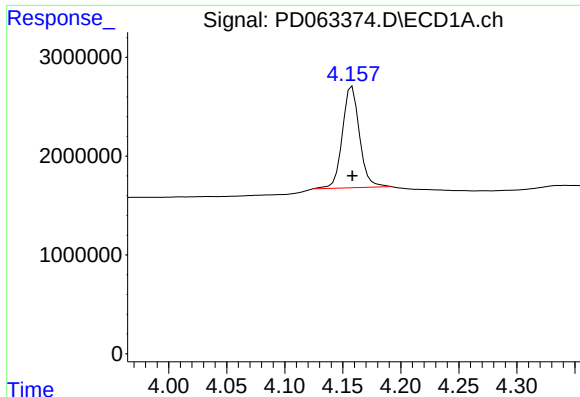

#3 gamma-BHC (Lindane)


R.T.: 4.158 min
Delta R.T.: 0.000 min
Response: 10526100
Conc: 5.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

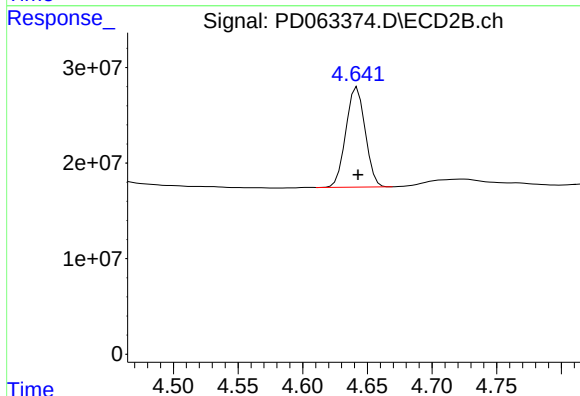


#3 gamma-BHC (Lindane)

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 108522703
Conc: 5.27 ng/ml

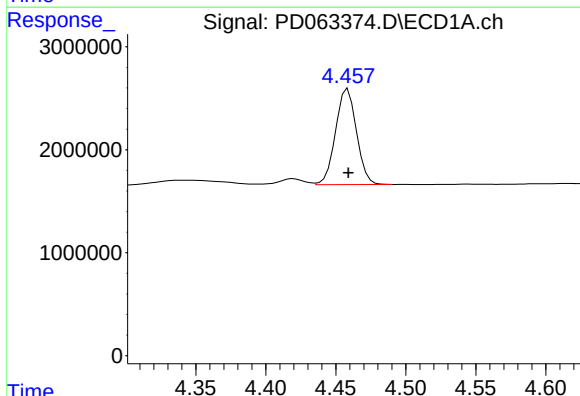


#4 Heptachlor

R.T.: 4.459 min
Delta R.T.: 0.000 min
Response: 9690558
Conc: 4.99 ng/ml

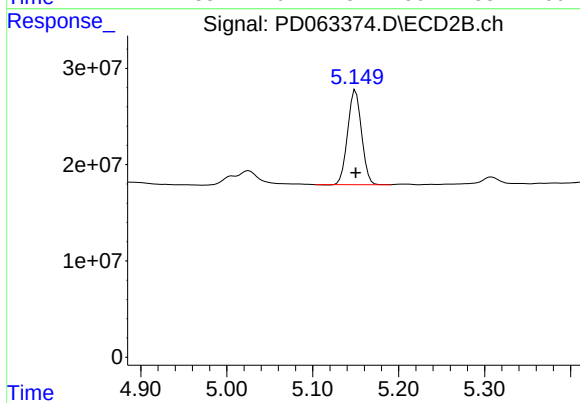

#4 Heptachlor


R.T.: 5.150 min
Delta R.T.: 0.000 min
Response: 110926656
Conc: 5.28 ng/ml

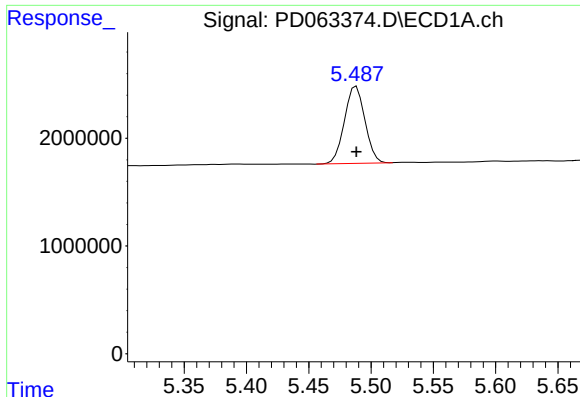

#9 Endosulfan I


R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 8220049
Conc: 5.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

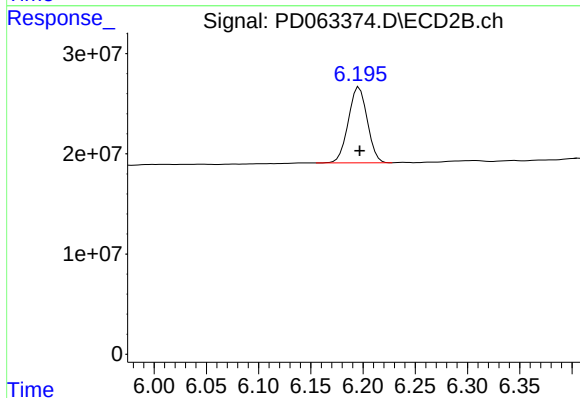


#9 Endosulfan I

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 95490855
Conc: 5.30 ng/ml

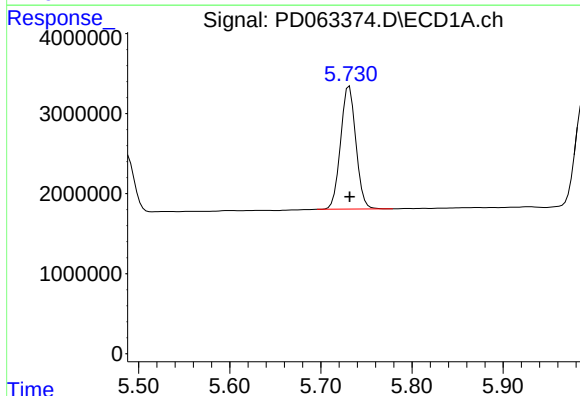


#13 Dieldrin

R.T.: 5.731 min
Delta R.T.: 0.000 min
Response: 17873209
Conc: 9.49 ng/ml

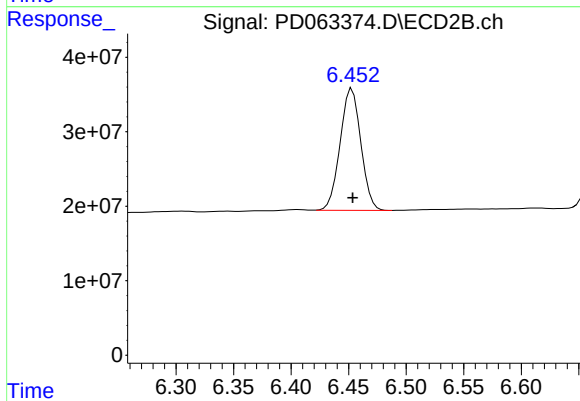

#13 Dieldrin


R.T.: 6.453 min
Delta R.T.: 0.000 min
Response: 205714810
Conc: 10.66 ng/ml

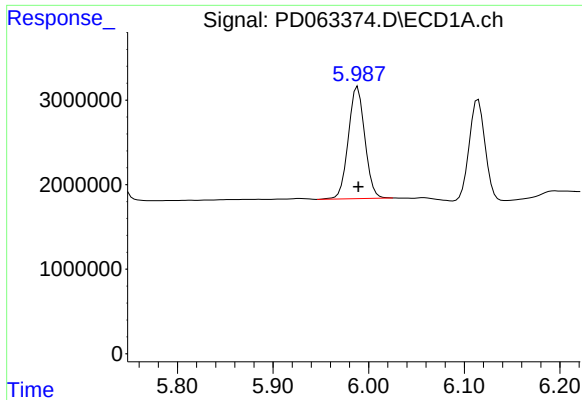

#14 Endrin


R.T.: 5.989 min
Delta R.T.: 0.000 min
Response: 15984029
Conc: 9.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

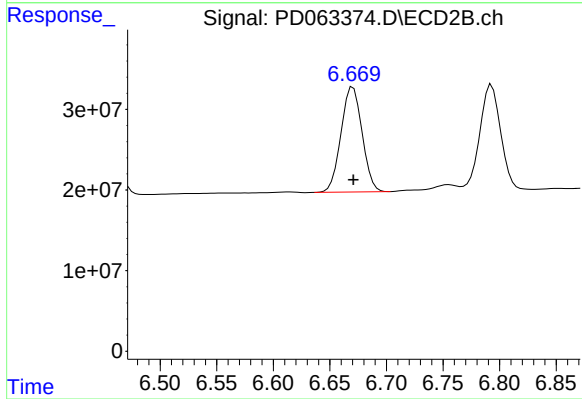


#14 Endrin

R.T.: 6.670 min
Delta R.T.: 0.000 min
Response: 169280838
Conc: 10.56 ng/ml

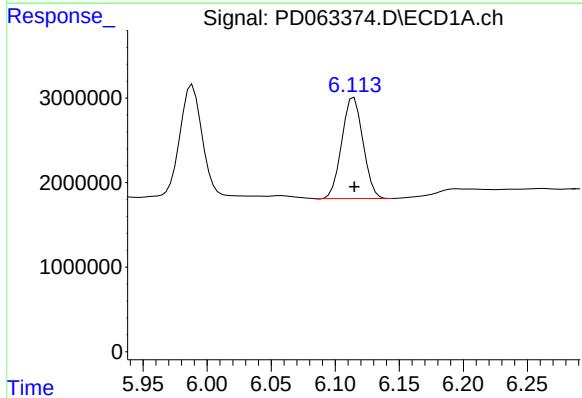


#16 4,4'-DDD

R.T.: 6.115 min
Delta R.T.: 0.000 min
Response: 13805846
Conc: 9.25 ng/ml

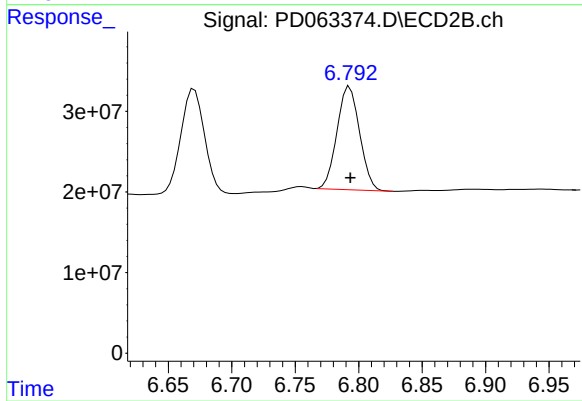

#16 4,4'-DDD


R.T.: 6.793 min
Delta R.T.: 0.000 min
Response: 158353391
Conc: 10.31 ng/ml

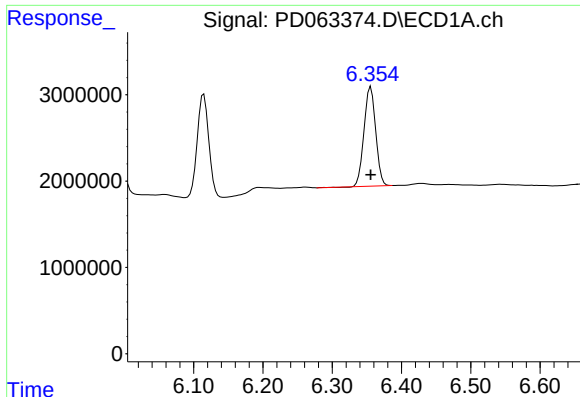

#17 4,4'-DDT


R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 13477093
Conc: 8.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

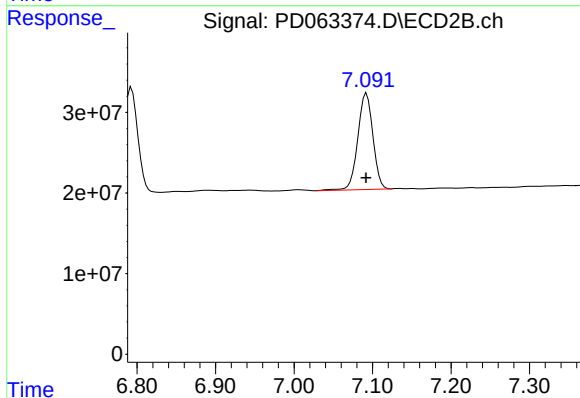


#17 4,4'-DDT

R.T.: 7.092 min
Delta R.T.: 0.000 min
Response: 159929105
Conc: 10.32 ng/ml

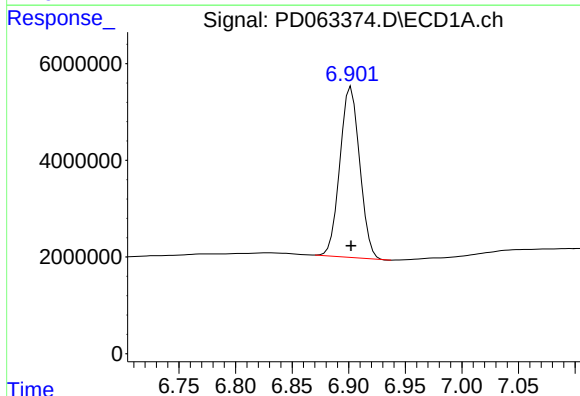


#20 Methoxychlor

R.T.: 6.902 min
Delta R.T.: 0.000 min
Response: 43015519
Conc: 50.85 ng/ml

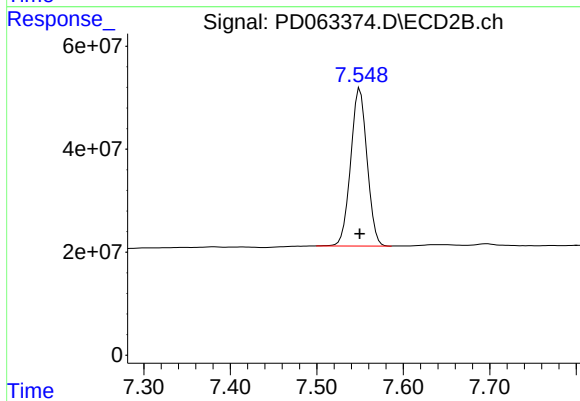

#20 Methoxychlor


R.T.: 7.550 min
Delta R.T.: 0.000 min
Response: 401960031
Conc: 54.62 ng/ml

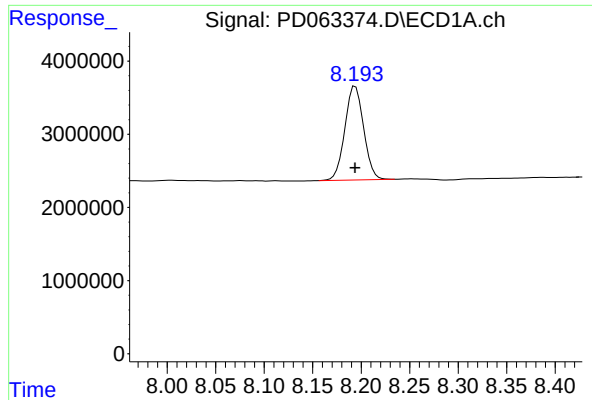

#27 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 17263787
Conc: 10.58 ng/ml

Instrument :
ECD_D
ClientSampleId :

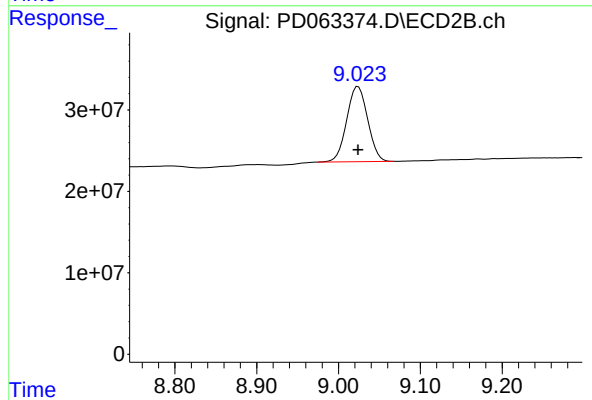

#27 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 163775964
Conc: 11.20 ng/ml