

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060321\
 Data File : PD063380.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 18:40
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 05:50:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 05:48:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.970	52573011	527.0E6	38.363	37.059
27)	SA Decachlor...	8.194	9.024	123.0E6	1088.7E6	75.378	74.423
Target Compounds							
2)	A alpha-BHC	3.875	4.358	81930161	838.7E6	40.260	37.712
3)	MA gamma-BHC...	4.159	4.642	77564173	775.5E6	39.219	37.634
4)	MA Heptachlor	4.459	5.150	76525021	783.6E6	39.433	37.322
9)	A Endosulfan I	5.489	6.196	64616643	674.8E6	39.519	37.463
13)	MA Dieldrin	5.732	6.453	150.7E6	1449.4E6	80.028	75.117
14)	MA Endrin	5.989	6.670	128.6E6	1203.9E6	79.233	75.114
16)	A 4,4'-DDD	6.115	6.793	119.7E6	1164.4E6	80.233	75.785
17)	MA 4,4'-DDT	6.356	7.092	125.5E6	1182.8E6	81.616	76.345
20)	A Methoxychlor	6.904	7.551	318.8E6	2686.6E6	376.847	365.101


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060321\
Data File : PD063380.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 18:40
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 05:50:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 05:48:53 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

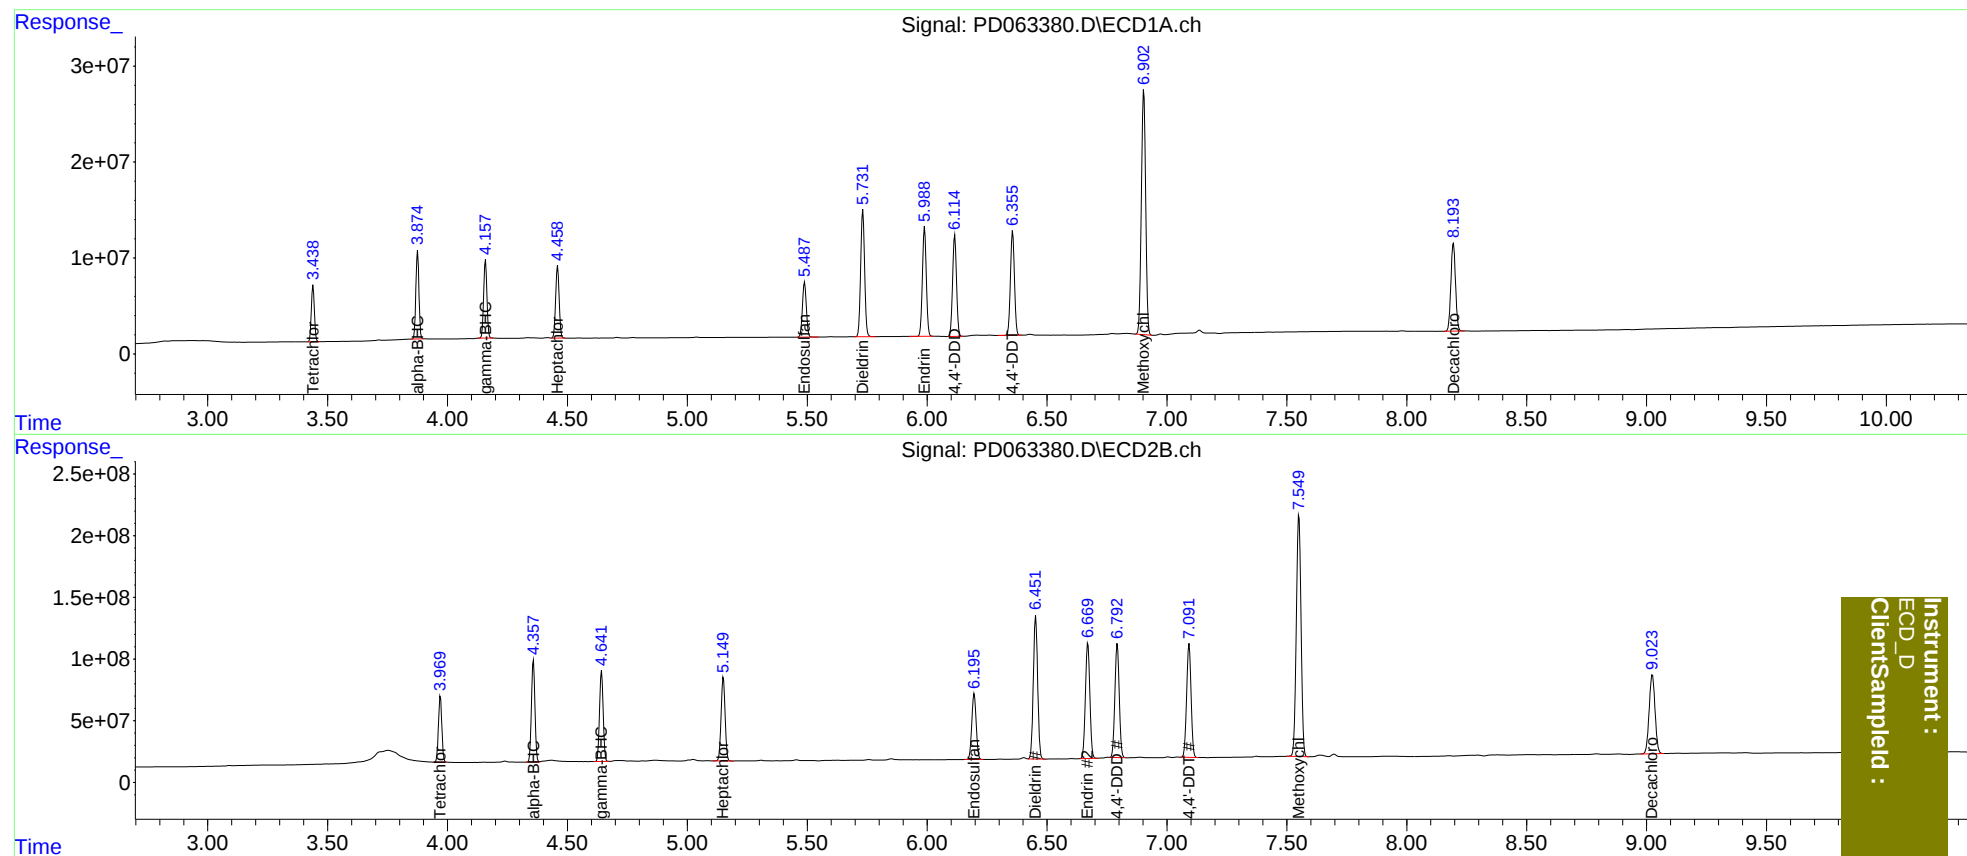


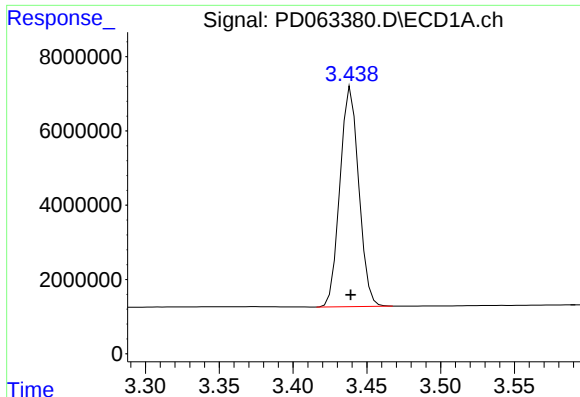

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 52573011
Conc: 38.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

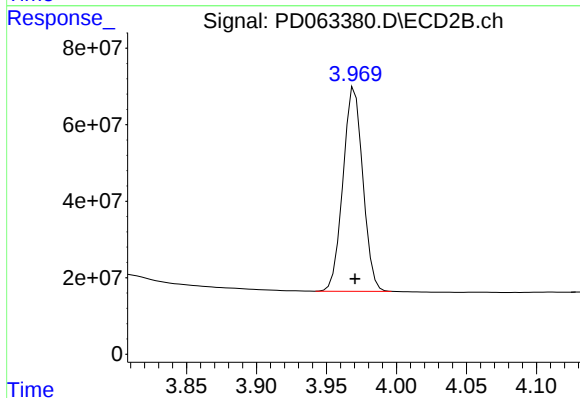


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 526974644
Conc: 37.06 ng/ml

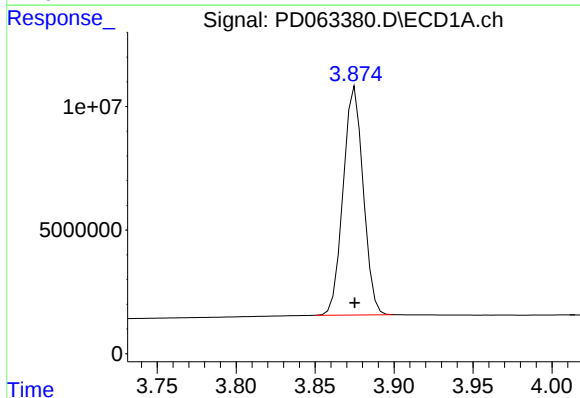


#2 alpha-BHC

R.T.: 3.875 min
Delta R.T.: 0.000 min
Response: 81930161
Conc: 40.26 ng/ml

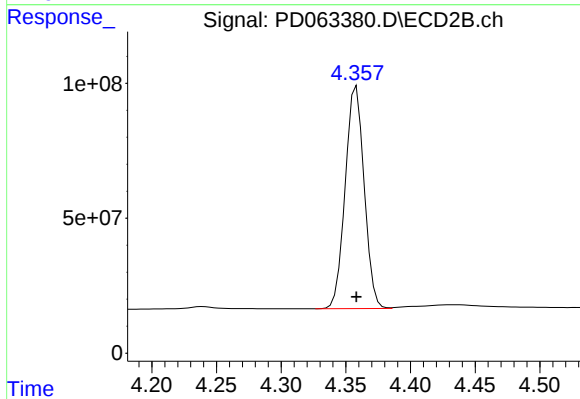

#2 alpha-BHC


R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 838691132
Conc: 37.71 ng/ml

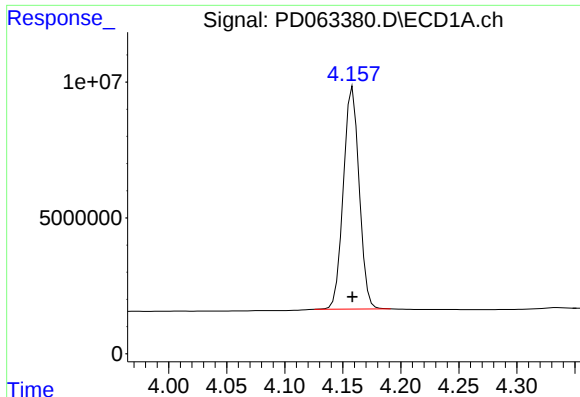

#3 gamma-BHC (Lindane)


R.T.: 4.159 min
Delta R.T.: 0.000 min
Response: 77564173
Conc: 39.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

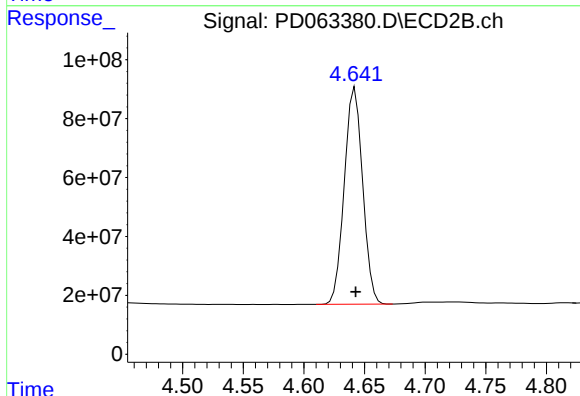


#3 gamma-BHC (Lindane)

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 775481915
Conc: 37.63 ng/ml

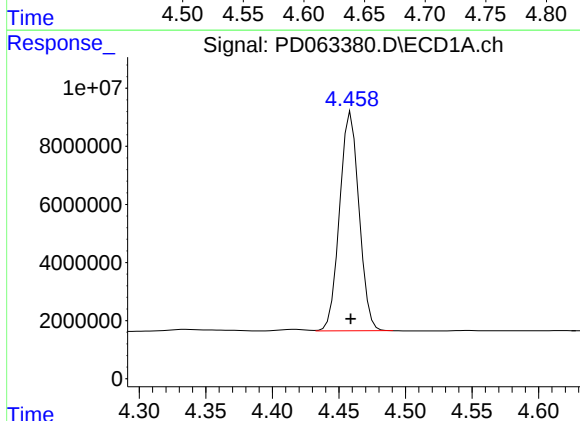


#4 Heptachlor

R.T.: 4.459 min
Delta R.T.: 0.000 min
Response: 76525021
Conc: 39.43 ng/ml

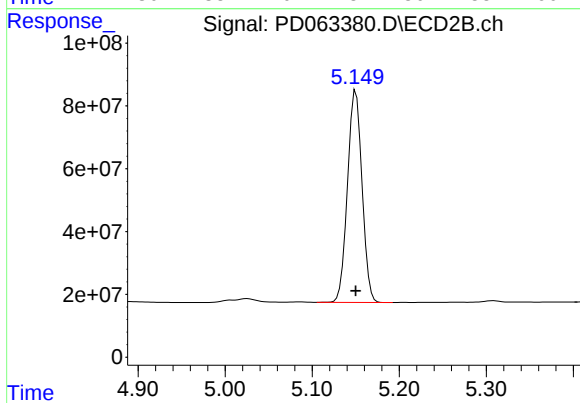

#4 Heptachlor


R.T.: 5.150 min
Delta R.T.: 0.000 min
Response: 783568250
Conc: 37.32 ng/ml

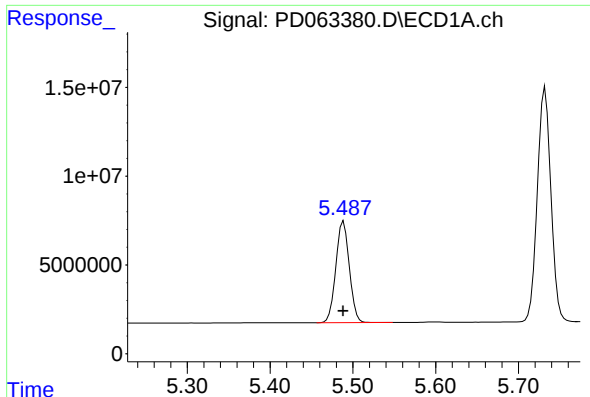

#9 Endosulfan I


R.T.: 5.489 min
Delta R.T.: 0.000 min
Response: 64616643
Conc: 39.52 ng/ml

Instrument :
ECD_D
ClientSampleId :

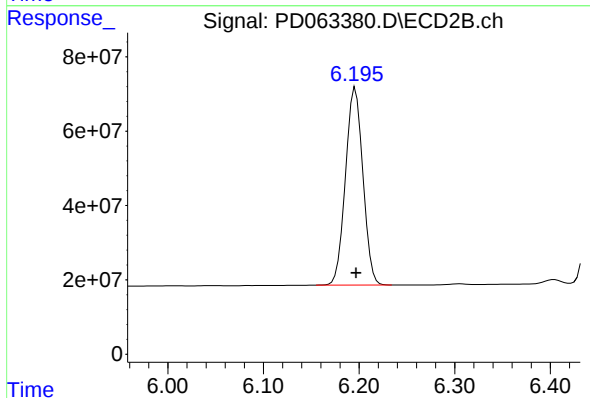


#9 Endosulfan I

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 674781046
Conc: 37.46 ng/ml

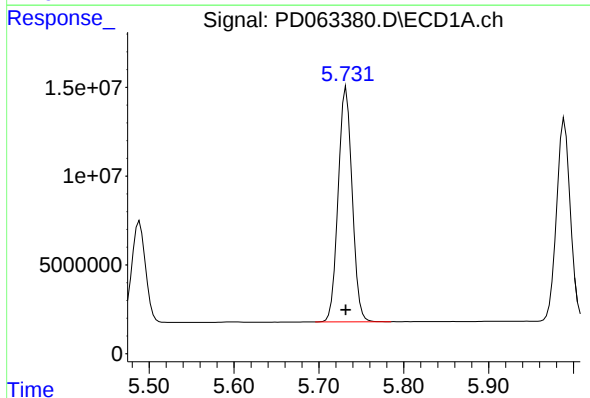


#13 Dieldrin

R.T.: 5.732 min
Delta R.T.: 0.000 min
Response: 150742452
Conc: 80.03 ng/ml

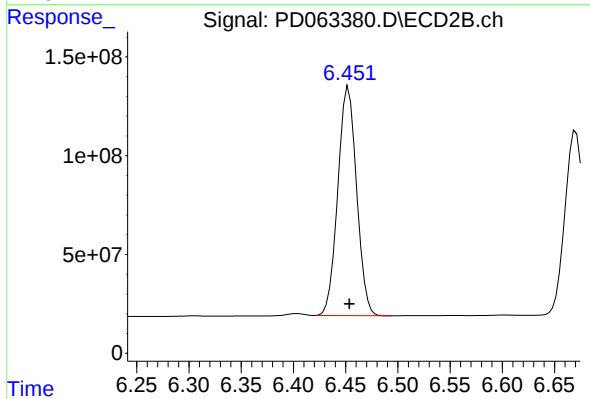

#13 Dieldrin


R.T.: 6.453 min
Delta R.T.: 0.000 min
Response: 1449418295
Conc: 75.12 ng/ml

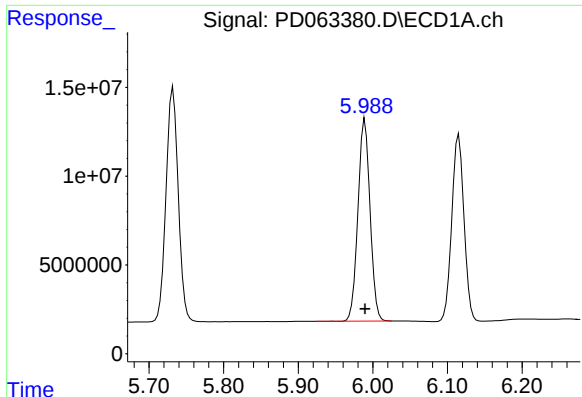

#14 Endrin


R.T.: 5.989 min
Delta R.T.: 0.000 min
Response: 128595013
Conc: 79.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

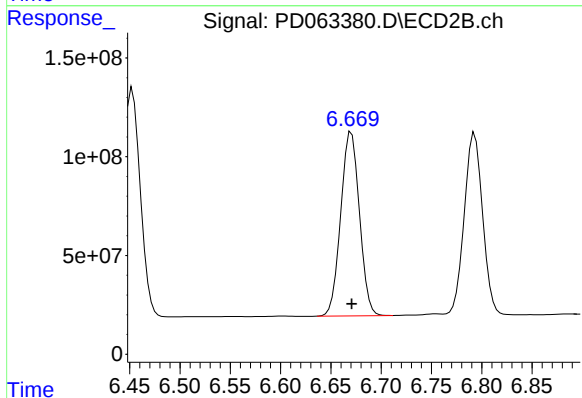


#14 Endrin

R.T.: 6.670 min
Delta R.T.: 0.000 min
Response: 1203910227
Conc: 75.11 ng/ml

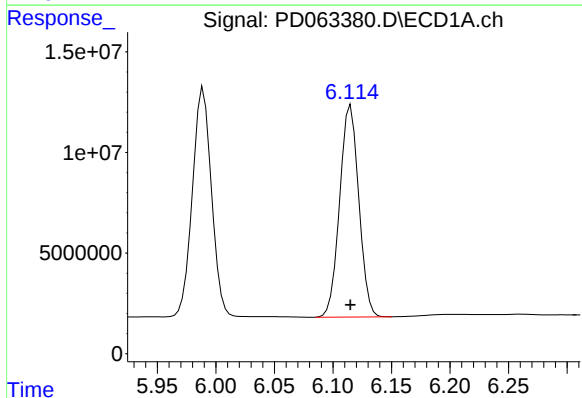


#16 4,4'-DDD

R.T.: 6.115 min
Delta R.T.: 0.000 min
Response: 119701309
Conc: 80.23 ng/ml

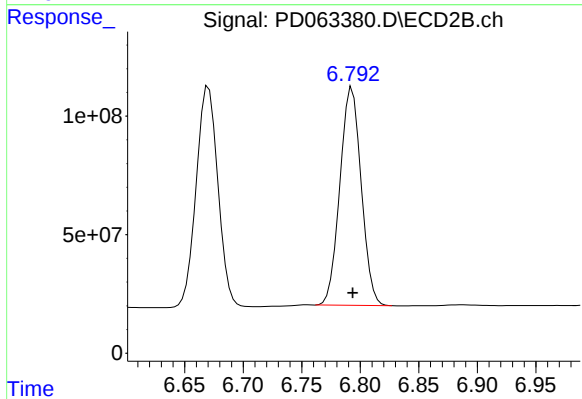

#16 4,4'-DDD


R.T.: 6.793 min
Delta R.T.: 0.000 min
Response: 1164377191
Conc: 75.78 ng/ml

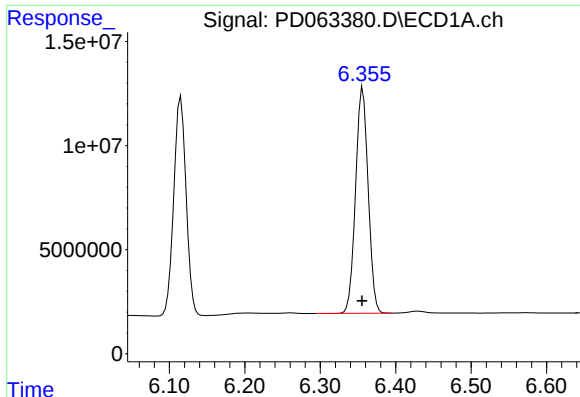

#17 4,4'-DDT


R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 125510410
Conc: 81.62 ng/ml

Instrument :
ECD_D
ClientSampleId :

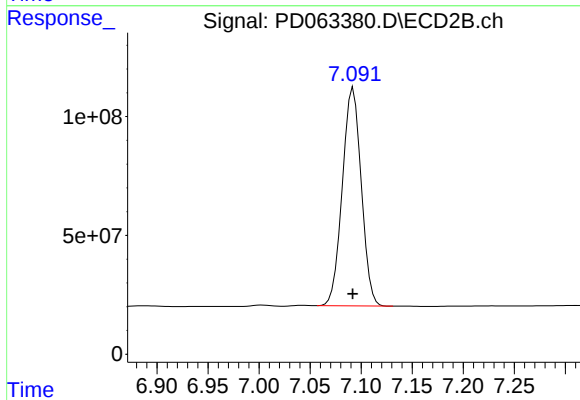


#17 4,4'-DDT

R.T.: 7.092 min
Delta R.T.: 0.000 min
Response: 1182825044
Conc: 76.34 ng/ml

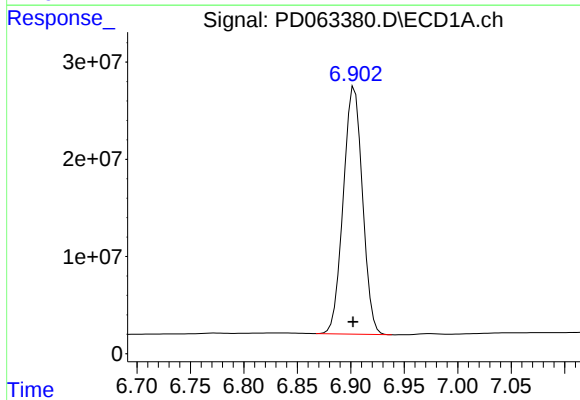


#20 Methoxychlor

R.T.: 6.904 min
Delta R.T.: 0.001 min
Response: 318781062
Conc: 376.85 ng/ml

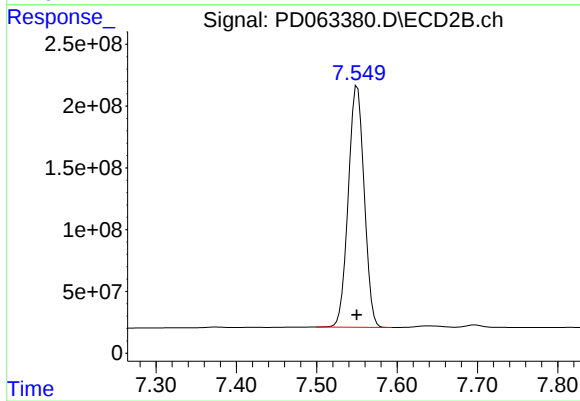

#20 Methoxychlor

R.T.: 7.551 min
Delta R.T.: 0.000 min
Response: 2686613068
Conc: 365.10 ng/ml

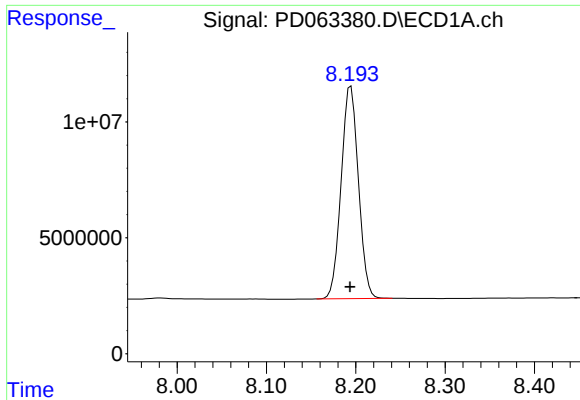

#27 Decachlorobiphenyl


R.T.: 8.194 min

Delta R.T.: 0.000 min

Response: 123035943

Conc: 75.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

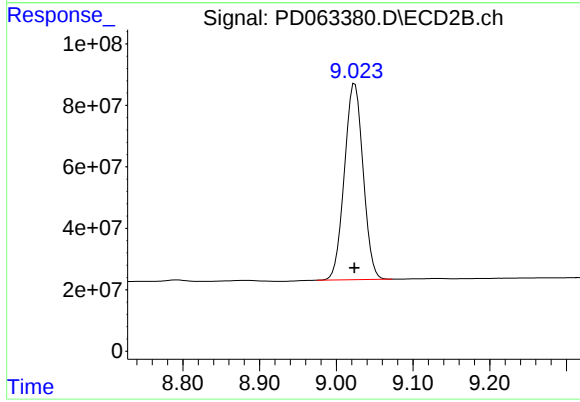

#27 Decachlorobiphenyl

R.T.: 9.024 min

Delta R.T.: 0.000 min

Response: 1088688640

Conc: 74.42 ng/ml