

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060321\
 Data File : PD063382.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 19:08
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 05:50:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 05:48:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.971	109.9E6	1049.3E6	80.202	73.795
27)	SA Decachlor...	8.194	9.025	250.5E6	2159.5E6	153.442	147.625
Target Compounds							
2)	A alpha-BHC	3.875	4.358	178.8E6	1696.4E6	87.841	76.280
3)	MA gamma-BHC...	4.158	4.642	166.2E6	1564.3E6	84.040	75.917
4)	MA Heptachlor	4.459	5.150	163.2E6	1558.8E6	84.117	74.249
9)	A Endosulfan I	5.489	6.196	136.5E6	1335.0E6	83.463	74.116
13)	MA Dieldrin	5.732	6.452	320.2E6	2875.9E6	169.984	149.046
14)	MA Endrin	5.989	6.670	268.2E6	2361.0E6	165.237	147.303
16)	A 4,4'-DDD	6.115	6.793	255.5E6	2332.5E6	171.238	151.812
17)	MA 4,4'-DDT	6.356	7.091	271.4E6	2387.7E6	176.456	154.111
20)	A Methoxychlor	6.903	7.550	620.3E6	5050.1E6	733.323	686.291


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060321\
Data File : PD063382.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 19:08
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 05:50:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 05:48:53 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

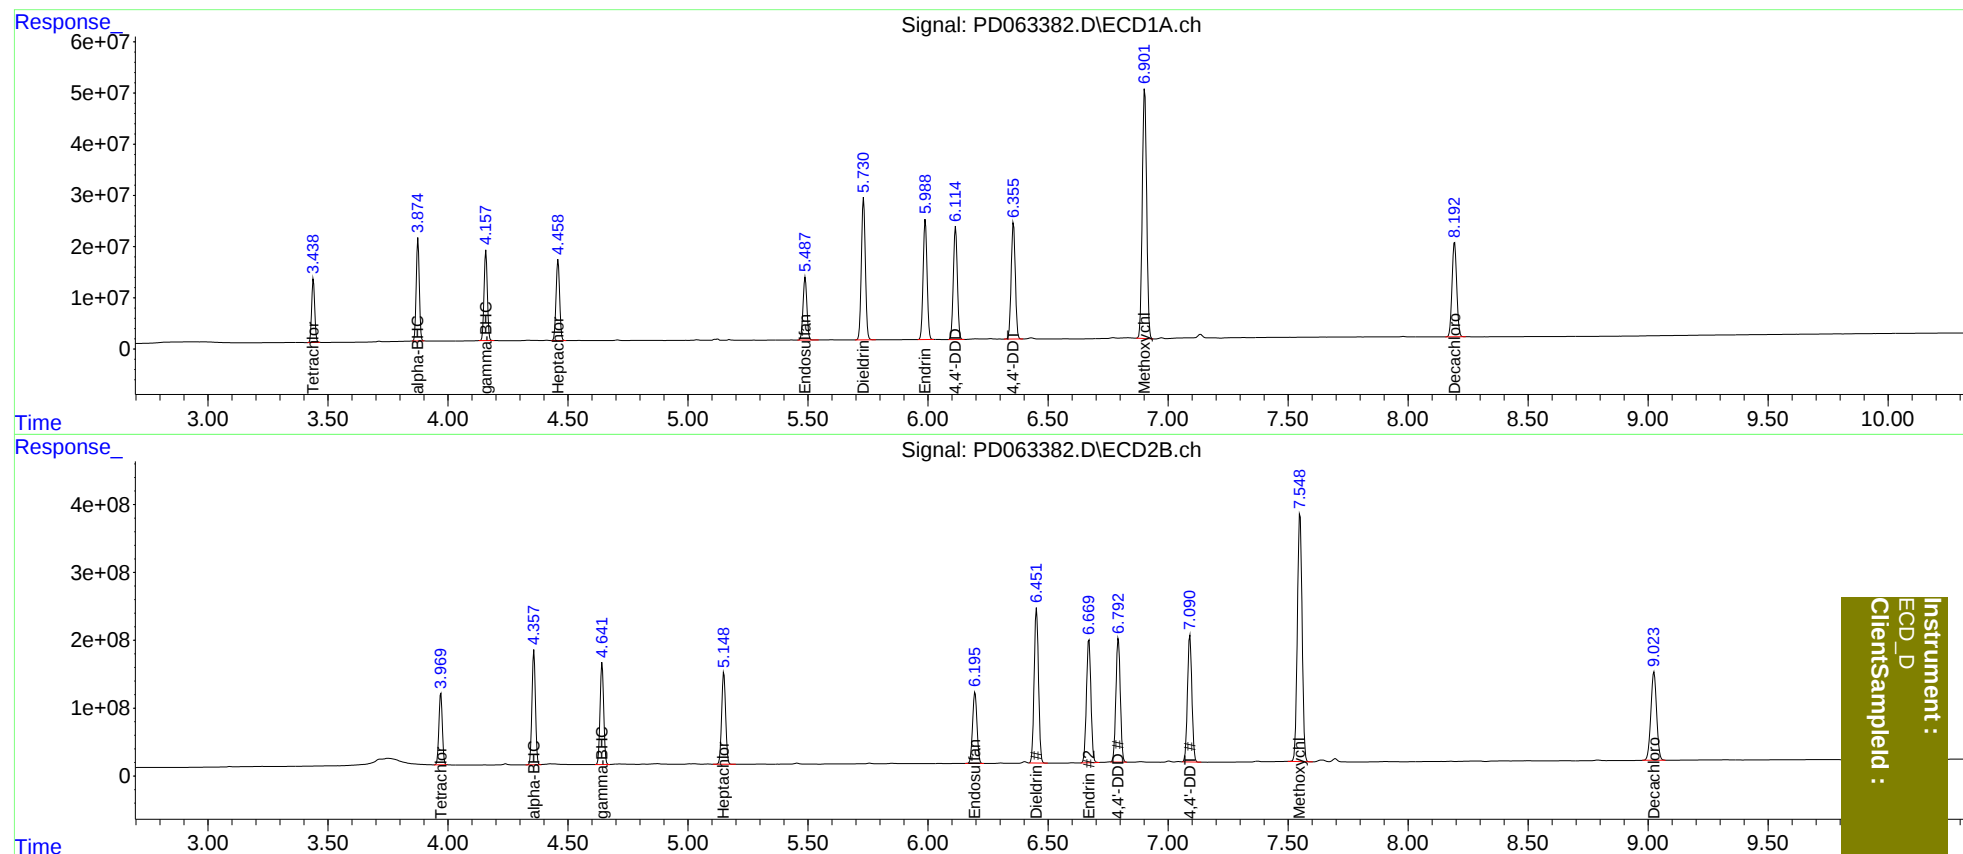


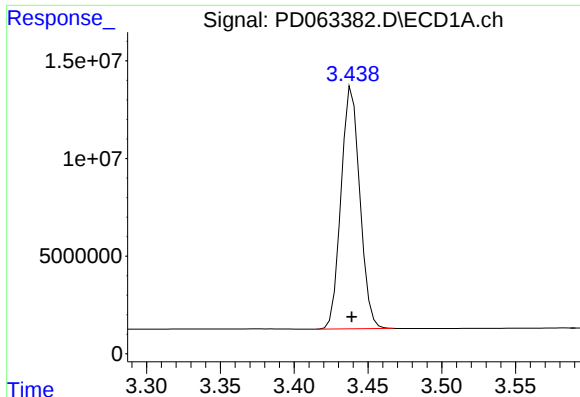

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 109910173
Conc: 80.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

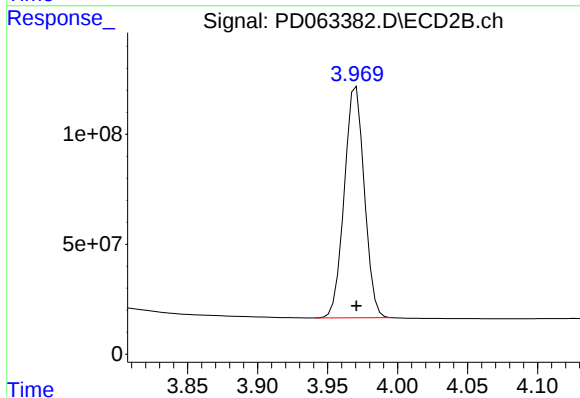


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 1049348386
Conc: 73.79 ng/ml

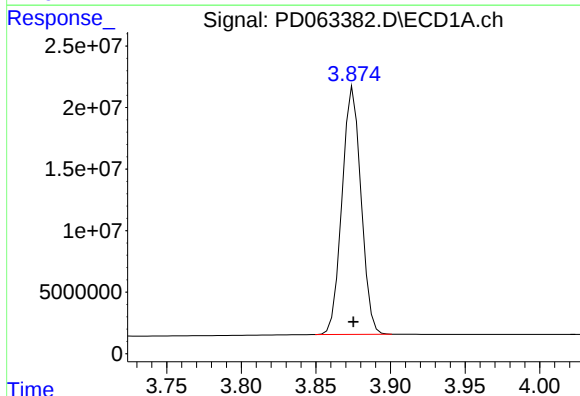


#2 alpha-BHC

R.T.: 3.875 min
Delta R.T.: 0.000 min
Response: 178756700
Conc: 87.84 ng/ml

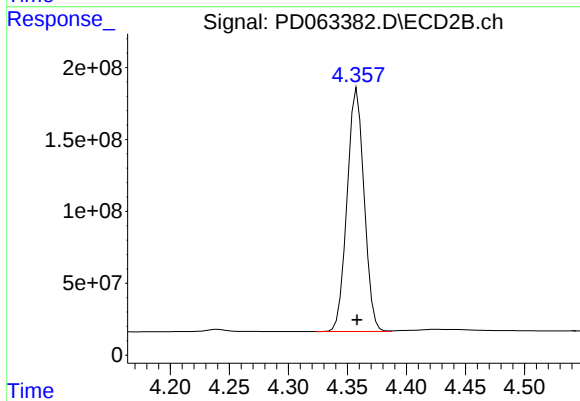

#2 alpha-BHC


R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 1696410784
Conc: 76.28 ng/ml

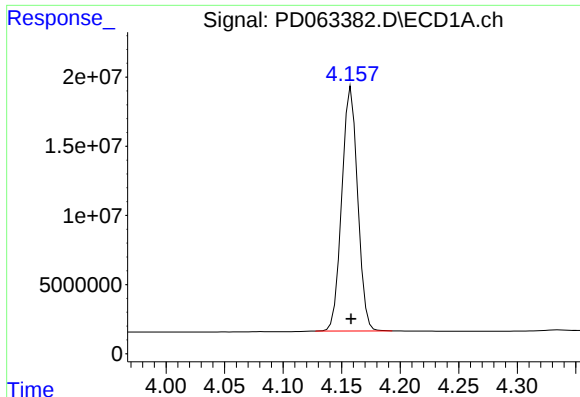

#3 gamma-BHC (Lindane)


R.T.: 4.158 min
Delta R.T.: 0.000 min
Response: 166207920
Conc: 84.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

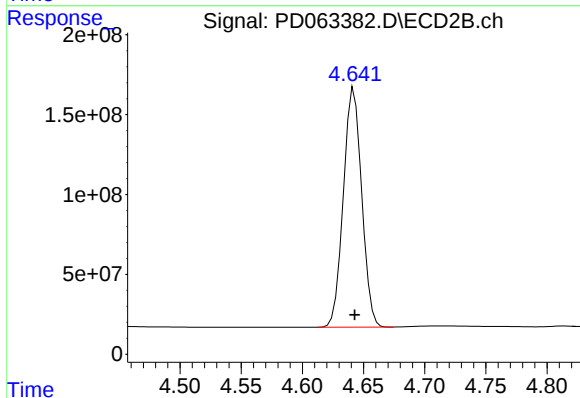


#3 gamma-BHC (Lindane)

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 1564346396
Conc: 75.92 ng/ml

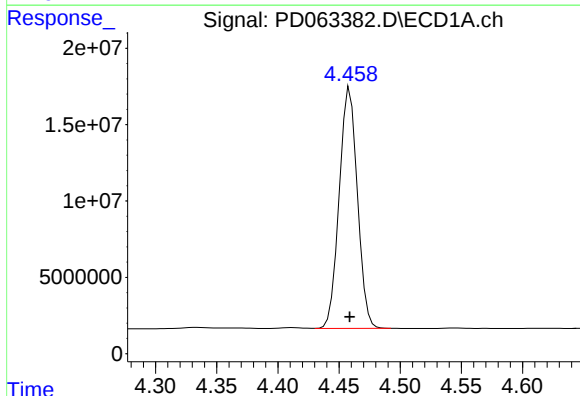


#4 Heptachlor

R.T.: 4.459 min
Delta R.T.: 0.000 min
Response: 163239825
Conc: 84.12 ng/ml

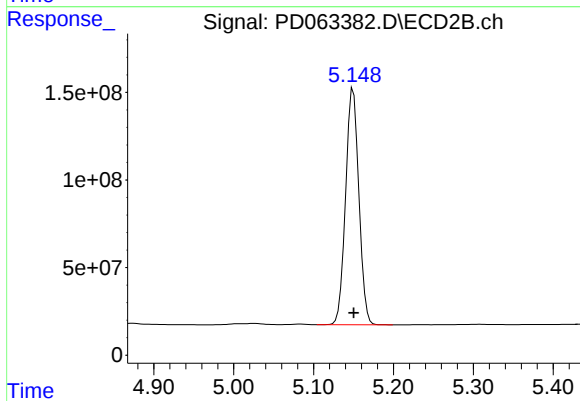

#4 Heptachlor


R.T.: 5.150 min
Delta R.T.: 0.000 min
Response: 1558825559
Conc: 74.25 ng/ml

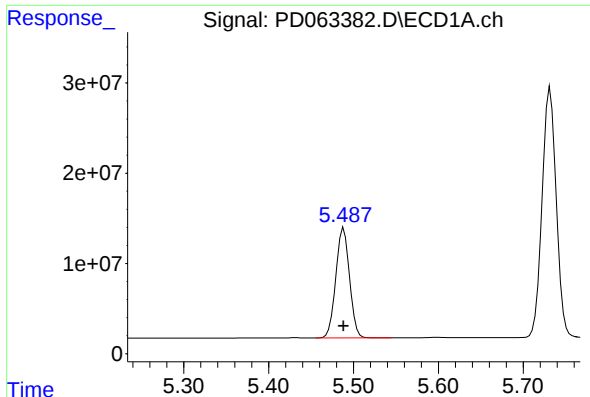

#9 Endosulfan I


R.T.: 5.489 min
Delta R.T.: 0.000 min
Response: 136467451
Conc: 83.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

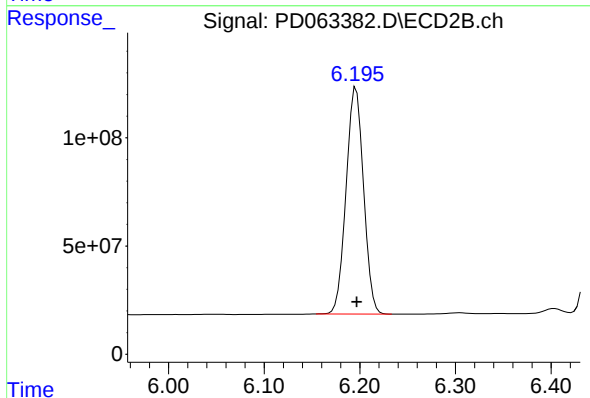


#9 Endosulfan I

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 1334962920
Conc: 74.12 ng/ml

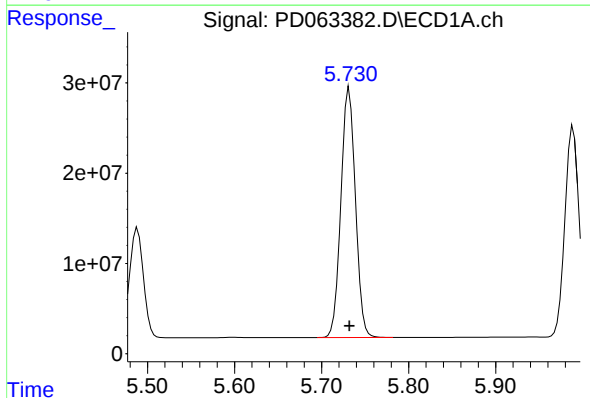


#13 Dieldrin

R.T.: 5.732 min
Delta R.T.: 0.000 min
Response: 320185890
Conc: 169.98 ng/ml

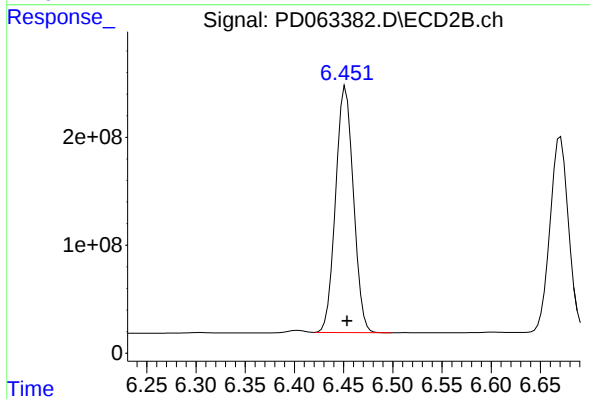

#13 Dieldrin


R.T.: 6.452 min
Delta R.T.: -0.001 min
Response: 2875898695
Conc: 149.05 ng/ml

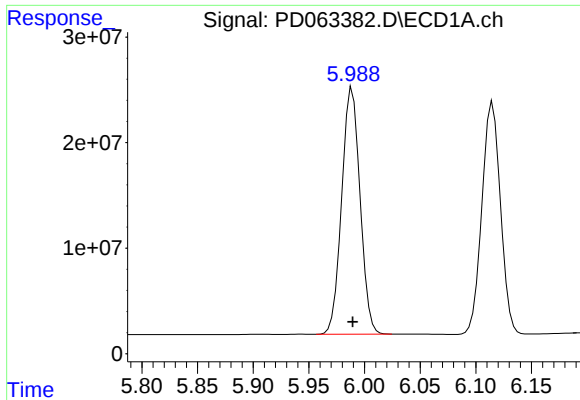

#14 Endrin


R.T.: 5.989 min
Delta R.T.: 0.000 min
Response: 268178433
Conc: 165.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

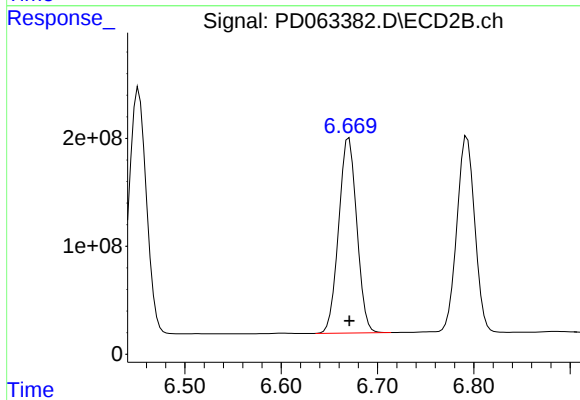


#14 Endrin

R.T.: 6.670 min
Delta R.T.: 0.000 min
Response: 2360954197
Conc: 147.30 ng/ml

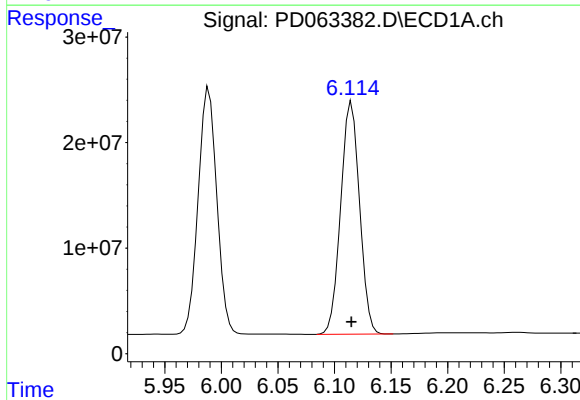


#16 4,4'-DDD

R.T.: 6.115 min
Delta R.T.: 0.000 min
Response: 255473347
Conc: 171.24 ng/ml

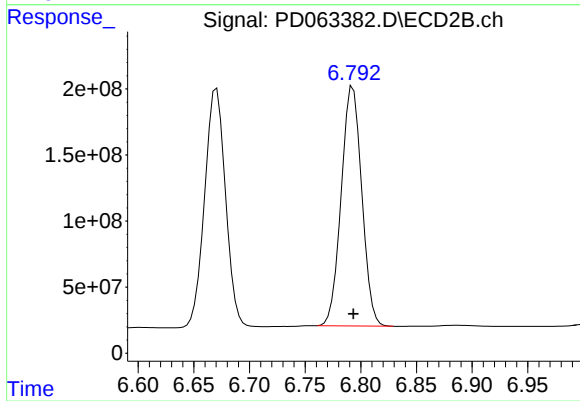

#16 4,4'-DDD


R.T.: 6.793 min
Delta R.T.: 0.000 min
Response: 2332477041
Conc: 151.81 ng/ml

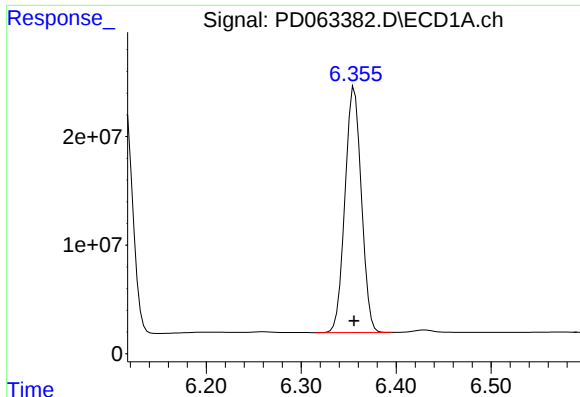

#17 4,4'-DDT


R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 271355693
Conc: 176.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

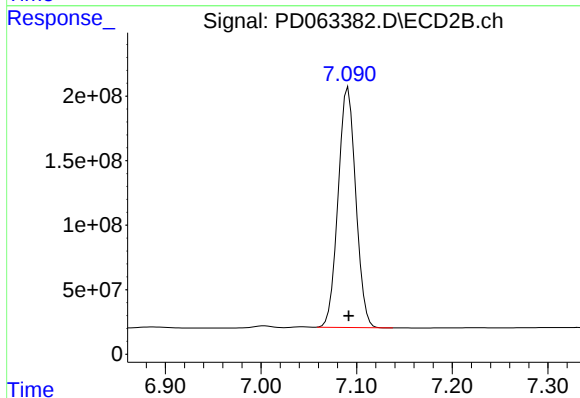


#17 4,4'-DDT

R.T.: 7.091 min
Delta R.T.: 0.000 min
Response: 2387679558
Conc: 154.11 ng/ml

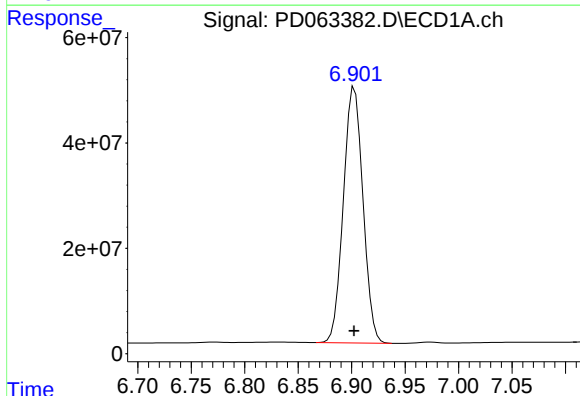


#20 Methoxychlor

R.T.: 6.903 min
Delta R.T.: 0.000 min
Response: 620329752
Conc: 733.32 ng/ml

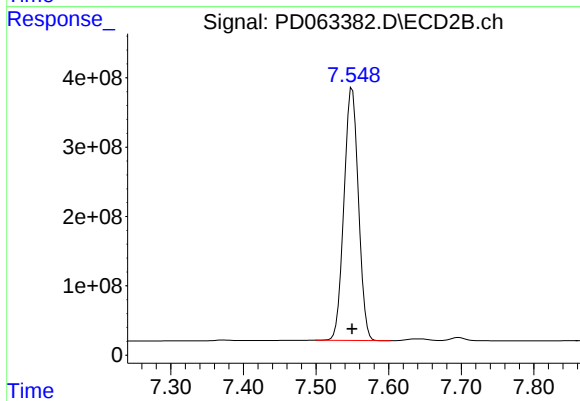

#20 Methoxychlor


R.T.: 7.550 min
Delta R.T.: 0.000 min
Response: 5050099752
Conc: 686.29 ng/ml

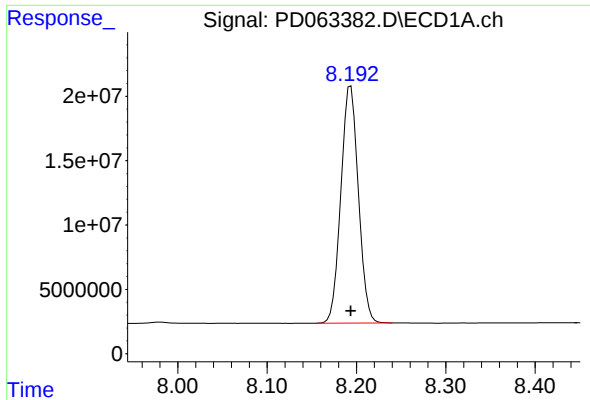

#27 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 250456497
Conc: 153.44 ng/ml

Instrument :
ECD_D
ClientSampleId :

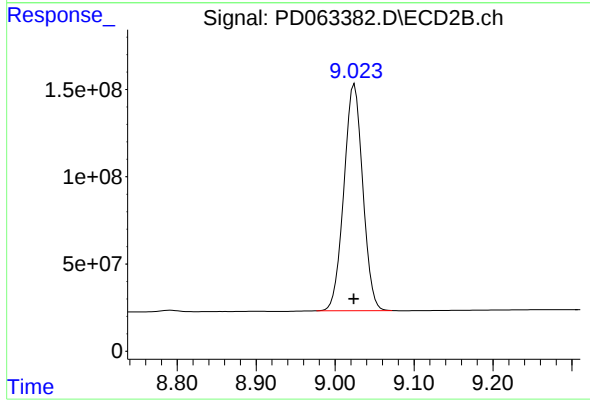

#27 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.000 min
Response: 2159526059
Conc: 147.62 ng/ml