

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060321\
 Data File : PD063393.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 21:41
 Operator : AR\AJ
 Sample : M2491-04MSD
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JLX81MSD

Manual Integrations
 APPROVED

Ankita
 6/3/2021 12:13:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 06:30:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	16344526	166.4E6	11.908	11.817
2)	SA Decachlor...	8.194	9.024	38737889	355.3E6	23.843	24.218
Target Compounds							
2)	A alpha-BHC	3.876	4.358	60323220	625.6E6	29.545	28.309
3)	MA gamma-BHC...	4.159	4.642	58307406	593.3E6	28.962	29.041
4)	MA Heptachlor	4.460	5.149	57955344	598.7E6	29.783	28.814
5)	MB Aldrin	4.707	5.454	56100937	588.4E6	29.866	28.592
6)	B beta-BHC	4.410	4.812	25360008	214.3E6	27.262	23.951m
7)	B delta-BHC	4.614	5.029	57652461	565.4E6	29.541	25.631
8)	B Heptachlo...	5.150	5.839	51874544	530.2E6	29.489	26.641m
9)	A Endosulfan I	5.490	6.196	45541414	500.3E6	27.699	28.016
10)	B trans-Chl...	5.377	6.072	54159468	537.2E6	29.627	26.955m
11)	B cis-Chlor...	5.436	6.146	51045101	524.4E6	28.780	27.745
12)	B 4,4'-DDE	5.599	6.303	107.2E6	1005.7E6	59.355	53.149
13)	MA Dieldrin	5.732	6.453	112.4E6	1092.9E6	59.993	57.120
14)	MA Endrin	5.990	6.670	99237614	923.1E6	61.403	58.296
15)	B Endosulfa...	6.263	6.880	94065093	924.4E6	62.633	61.069
16)	A 4,4'-DDD	6.115	6.793	90746839	929.5E6	61.410	61.183
17)	MA 4,4'-DDT	6.356	7.091	93196359	900.9E6	61.385	58.614
18)	B Endrin al...	6.431	7.004	80021261	782.5E6	61.410	59.282
19)	B Endosulfa...	6.645	7.227	87738051	901.3E6	61.099	57.837
20)	A Methoxychlor	6.903	7.550	246.7E6	2106.2E6	298.895	291.920
21)	B Endrin ke...	7.137	7.697	108.1E6	928.9E6	61.284	60.283

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060321\
Data File : PD063393.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 21:41
Operator : AR\AJ
Sample : M2491-04MSD
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 06:30:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

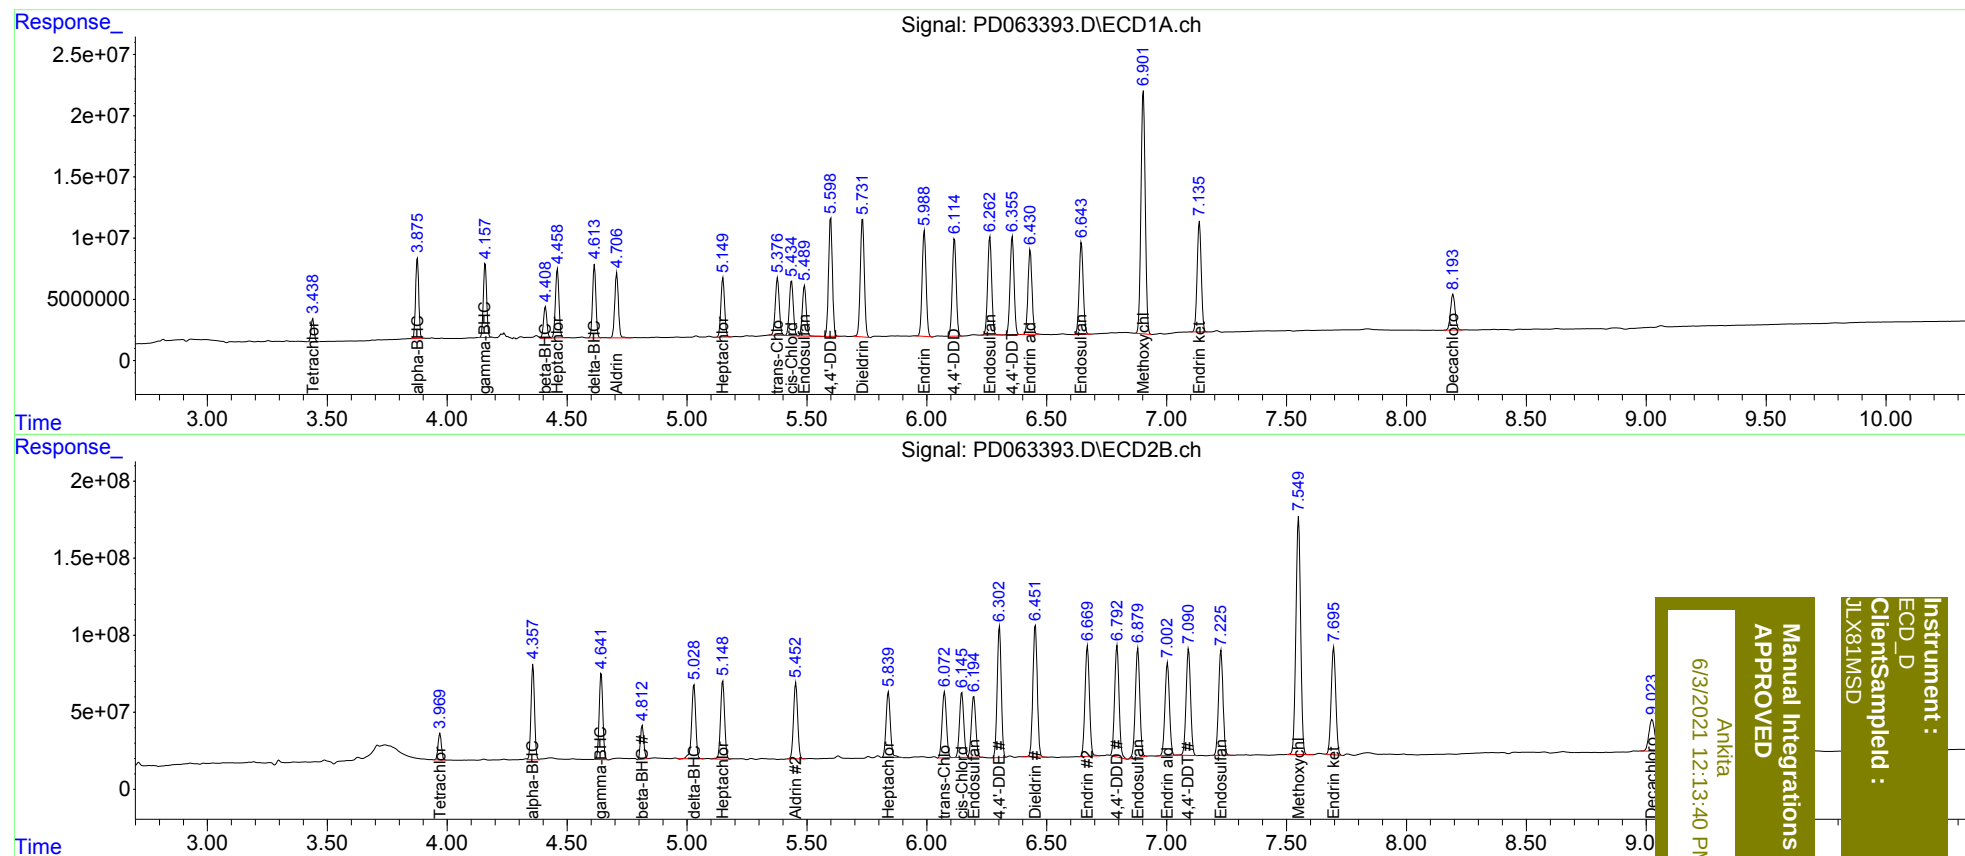

Manual Integrations
APPROVED

Ankita
6/3/2021 12:13:40 PM

Instrument :
ECD_D
Client Sampled :
JLX81MSD