

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060321\
Data File : PD063399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 23:05
Operator : AR\AJ
Sample : INDA344
Misc :
ALS Vial : 32 Sample Multiplier: 1


Instrument :
ECD_D
LabSampleId :
INDA344

Manual Integrations
APPROVED

Ankita
6/3/2021 12:13:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 06:15:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

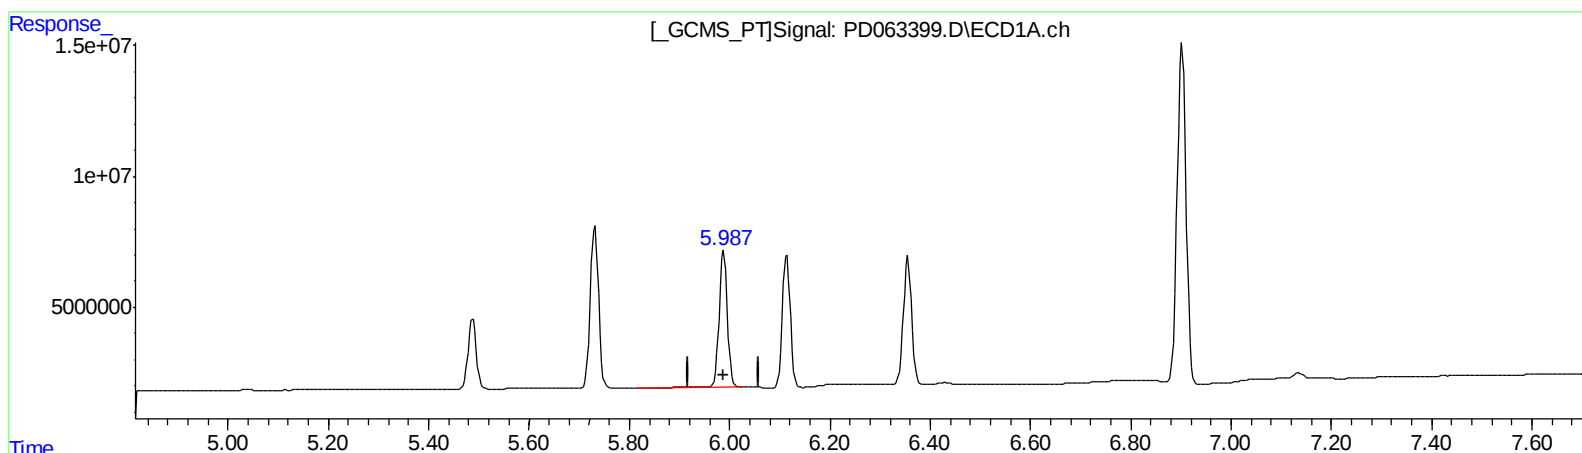

(14) Endrin (MA)

5.988min 37.134 ng/ml

response 60014628

(14) Endrin #2 (MA)

6.671min 36.987 ng/ml

response 585685453

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060321\
Data File : PD063399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 23:05
Operator : AR\AJ
Sample : INDA344
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_D
LabSampleId :
INDA344

Manual Integrations
APPROVED

Ankita
6/3/2021 12:13:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 06:15:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

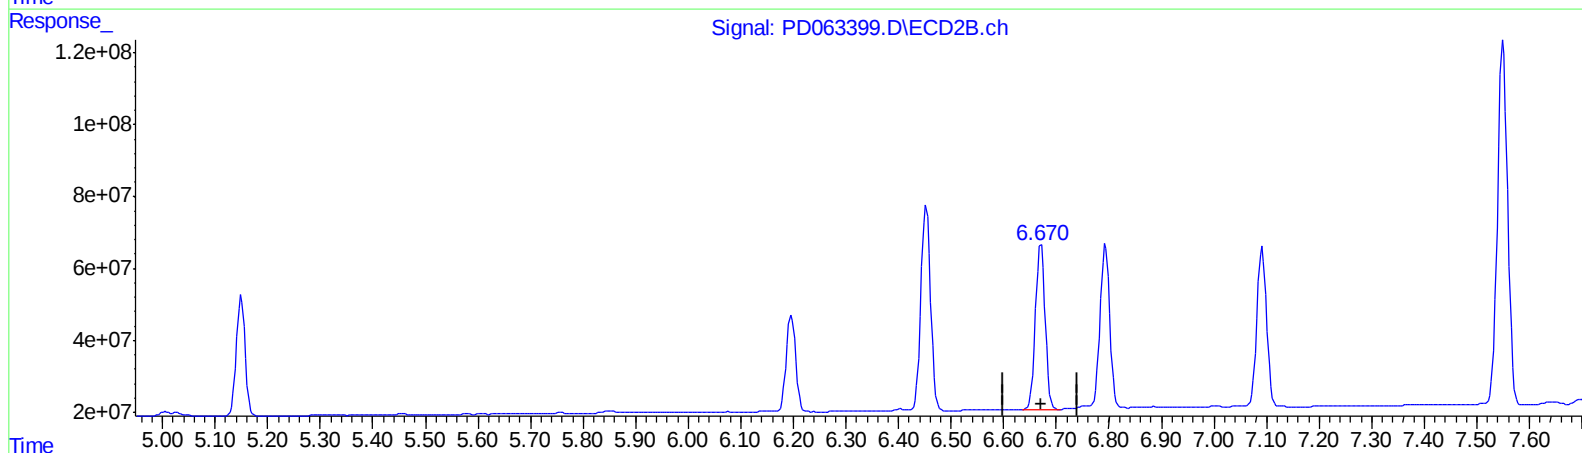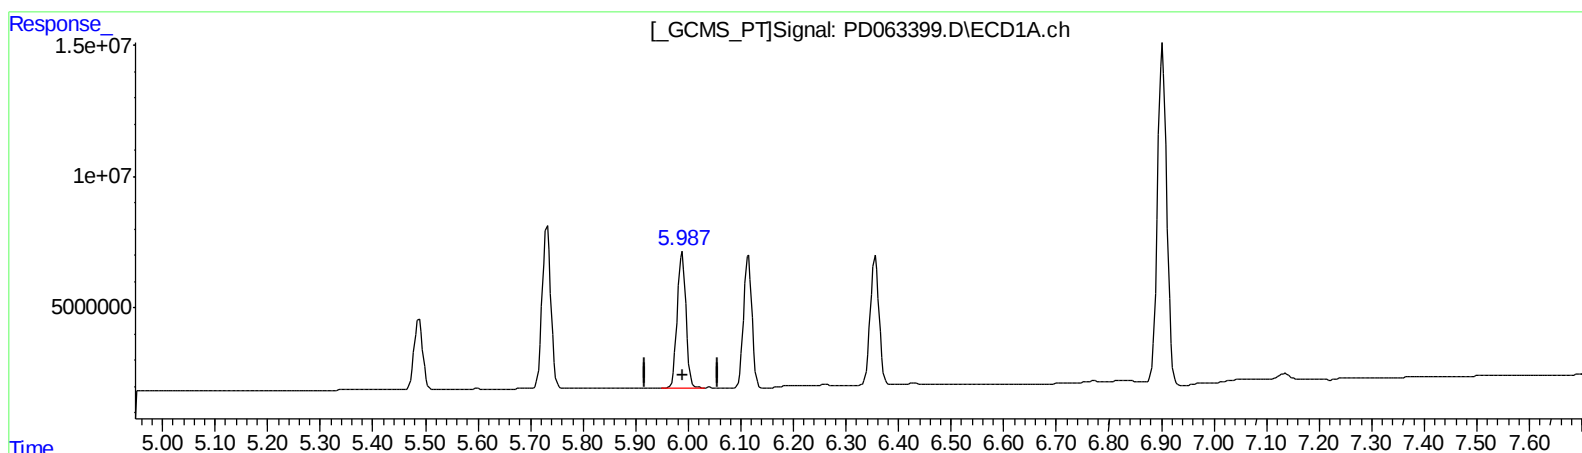

QEdit

(14) Endrin (MA)

5.987min 36.981 ng/ml m

response 59767436

(14) Endrin #2 (MA)

6.671min 36.987 ng/ml

response 585685453

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060321\
 Data File : PD063399.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 23:05
 Operator : AR\AJ
 Sample : INDA344
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 LabSampleId :
 INDA344

Manual Integrations
 APPROVED

Ankita
 6/3/2021 12:13:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 06:15:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.439	3.970	26085485	268.8E6	19.004	19.094
27) SA Decachlor...	8.193	9.025	61257045	548.7E6	37.704	37.397
Target Compounds						
2) A alpha-BHC	3.875	4.358	38434594	417.1E6	18.824	18.874
3) MA gamma-BHC...	4.158	4.642	37110683	384.3E6	18.433	18.808
4) MA Heptachlor	4.459	5.150	36319453	393.4E6	18.664	18.933
9) A Endosulfan I	5.488	6.196	30782635	336.0E6	18.723	18.815
13) MA Dieldrin	5.731	6.453	70795442	722.9E6	37.793	37.778
14) MA Endrin	5.987	6.671	59767436	585.7E6	36.981m	36.987
16) A 4,4'-DDD	6.114	6.793	56069502	574.9E6	37.943	37.843
17) MA 4,4'-DDT	6.356	7.092	57173711	572.5E6	37.658	37.250
20) A Methoxychlor	6.902	7.550	158.1E6	1368.7E6	191.554	189.708

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

AJ
 06/04/21