

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060321\
 Data File : PD063367.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 15:29
 Operator : AR\AJ
 Sample : RESC07
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC007

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 06:17:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.970	27082954	279.5E6	19.731	19.855
2)	SA Decachlor...	8.194	9.024	65067059	581.3E6	40.049	39.620
Target Compounds							
2)	A alpha-BHC	3.875	4.358	19873193	229.5E6	9.733	10.383
3)	MA gamma-BHC...	4.158	4.642	19734082	211.6E6	9.802	10.357
4)	MA Heptachlor	4.459	5.150	19206622	216.8E6	9.870	10.433
5)	MB Aldrin	4.707	5.454	18063263	208.8E6	9.616	10.147
6)	B beta-BHC	4.410	4.813	9283170	92082896	9.980	10.294
7)	B delta-BHC	4.613	5.029	18321552	217.8E6	9.388	9.875
8)	B Heptachlo...	5.150	5.840	17001686	200.7E6	9.665	10.085
9)	A Endosulfan I	5.489	6.196	16336719	187.5E6	9.936	10.501
10)	B trans-Chl...	5.377	6.074	17373374	201.5E6	9.504	10.112
11)	B cis-Chlor...	5.435	6.146	17058568	189.5E6	9.618	10.023
12)	B 4,4'-DDE	5.599	6.303	34287595	383.8E6	18.988	20.284
13)	MA Dieldrin	5.732	6.453	36936164	398.2E6	19.718	20.809
14)	MA Endrin	5.990	6.670	31933068	328.5E6	19.758	20.747
15)	B Endosulfa...	6.263	6.879	29314137	309.2E6	19.519	20.426
16)	A 4,4'-DDD	6.115	6.793	29138530	315.6E6	19.718	20.772
17)	MA 4,4'-DDT	6.357	7.091	29158940	314.6E6	19.206	20.469
18)	B Endrin al...	6.432	7.003	26225223	269.5E6	20.126	20.416
19)	B Endosulfa...	6.645	7.226	28119617	319.1E6	19.582	20.476
20)	A Methoxychlor	6.903	7.549	85653307	776.2E6	103.795	107.585
21)	B Endrin ke...	7.137	7.697	35964461	319.5E6	20.389	20.732

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060321\
Data File : PD063367.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 15:29
Operator : AR\AJ
Sample : RESC07
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 06:17:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

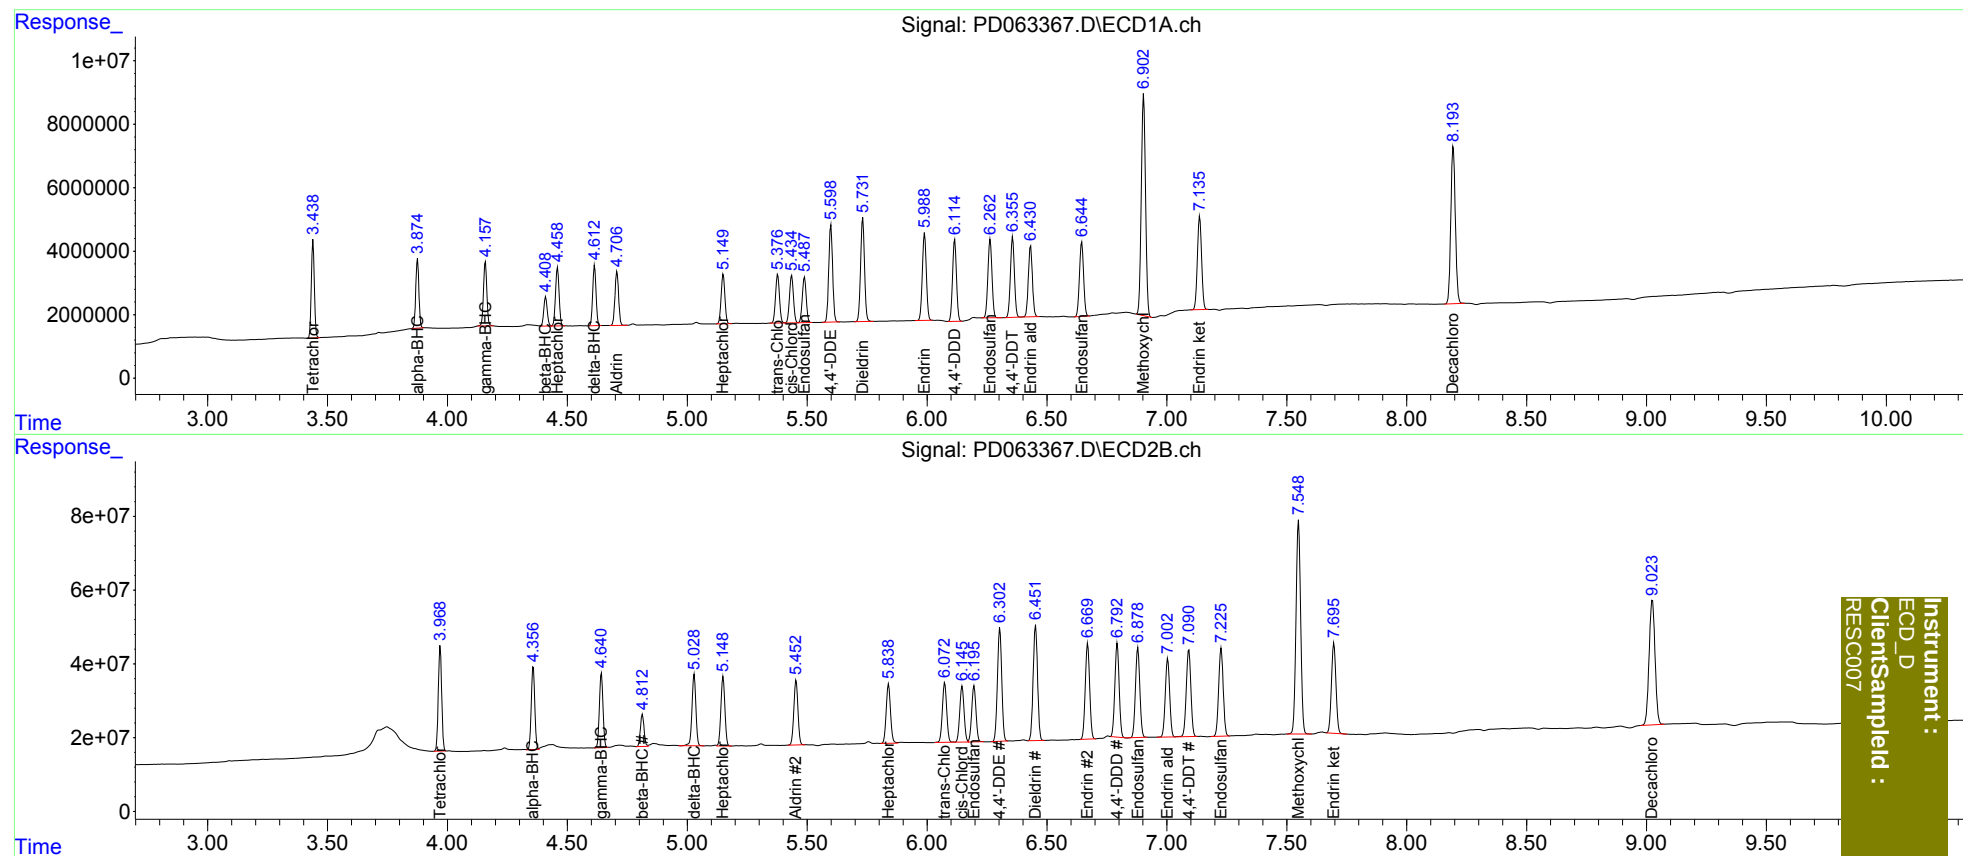

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060321\
Data File : PD063367.D
Acq On : 02 Jun 2021 15:29
Operator : AR\AJ
Sample : RESC07
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC007

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
Title : GC Extractables
Last Update : Thu Jun 03 06:08:10 2021
Integrator: ChemStation

RT#1	RT#2	Resolution
3.439	3.875	100.00%
3.875	4.158	100.00%
4.158	4.410	100.00%
4.410	4.459	100.00%
4.459	4.613	100.00%
4.613	4.707	100.00%
4.707	5.150	100.00%
5.150	5.377	100.00%
5.377	5.435	100.00%
5.435	5.489	100.00%
5.489	5.599	100.00%
5.599	5.732	100.00%
5.732	5.990	100.00%
5.990	6.115	100.00%
6.115	6.263	100.00%
6.263	6.357	100.00%
6.357	6.432	100.00%
6.432	6.645	100.00%
6.645	6.903	100.00%
6.903	7.137	100.00%
7.137	8.194	100.00%

Signal #2


3.970	4.358	100.00%
4.358	4.642	100.00%
4.642	4.813	100.00%
4.813	5.029	100.00%
5.029	5.150	100.00%
5.150	5.454	100.00%
5.454	5.840	100.00%
5.840	6.074	100.00%
6.074	6.146	100.00%
6.146	6.196	99.24%
6.196	6.303	100.00%
6.303	6.453	100.00%
6.453	6.670	100.00%
6.670	6.793	100.00%
6.793	6.879	100.00%
6.879	7.003	100.00%
7.003	7.091	100.00%
7.091	7.226	100.00%
7.226	7.549	100.00%
7.549	7.697	100.00%
7.697	9.024	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060321\
Data File : PD063367.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 15:29
Operator : AR\AJ
Sample : RESC07
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC007

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 06:17:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

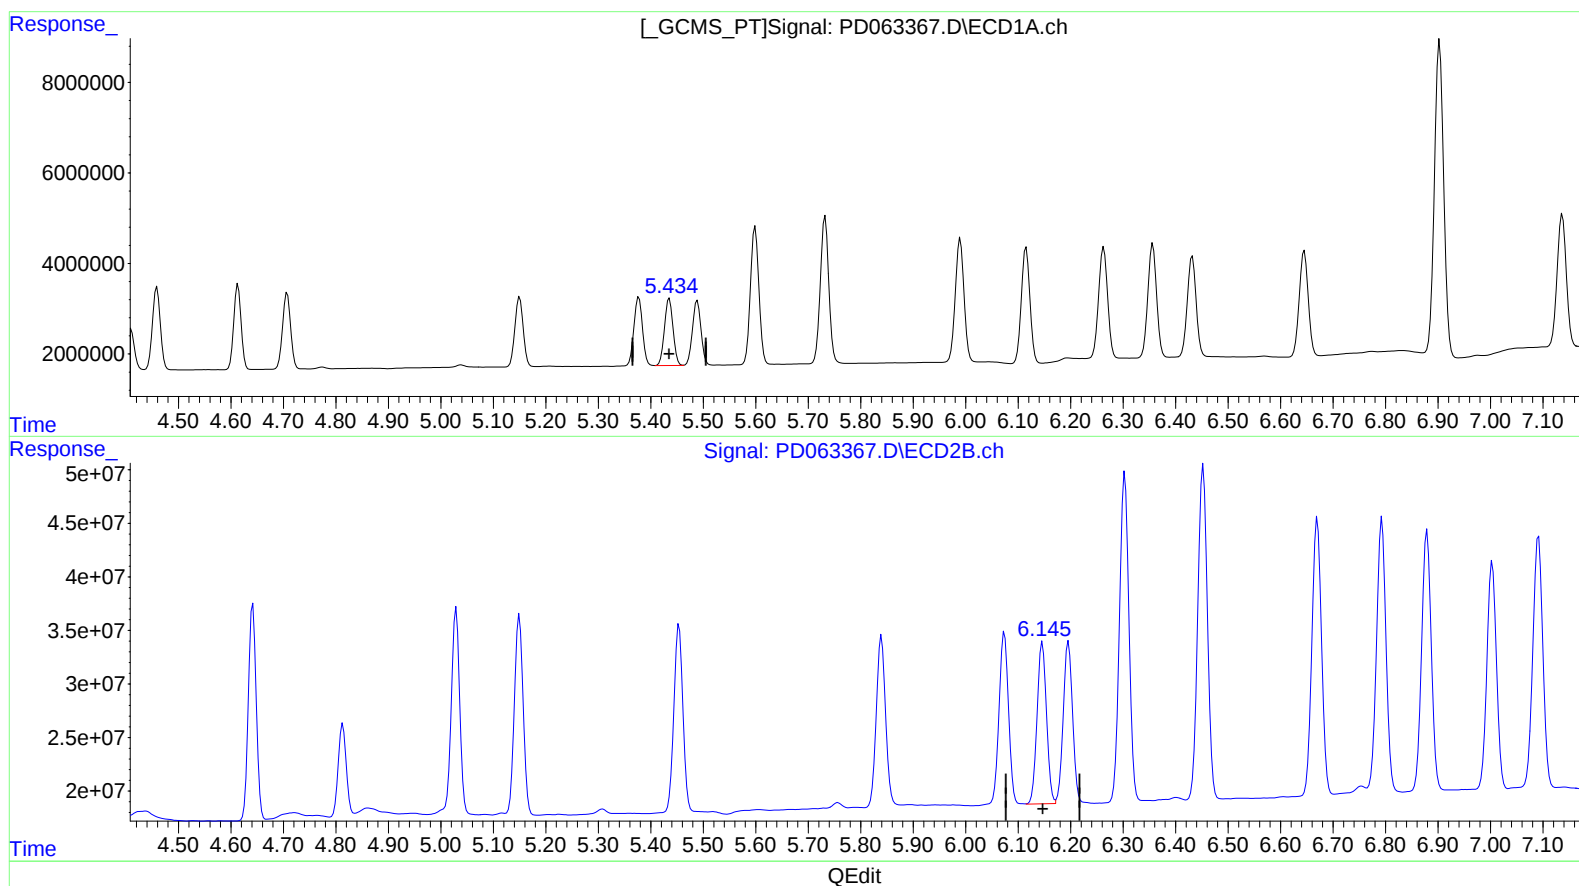

(11) cis-Chlordane (B)

5.435min 9.618 ng/ml

response 17058568

(11) cis-Chlordane #2 (B)

6.146min 10.023 ng/ml

response 189452266