

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060321\
 Data File : PD063392.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 21:27
 Operator : AR\AJ
 Sample : M2491-03MS
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JLX81MS

Manual Integrations
 APPROVED

Ankita
 6/3/2021 12:13:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 06:30:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.970	16280769	165.7E6	11.861	11.768
27)	SA Decachlor...	8.194	9.024	38663853	350.5E6	23.798	23.889
Target Compounds							
2)	A alpha-BHC	3.875	4.358	59689207	622.9E6	29.234	28.187
3)	MA gamma-BHC...	4.158	4.643	57339157	589.6E6	28.481	28.857
4)	MA Heptachlor	4.459	5.150	57479296	591.4E6	29.538	28.463
5)	MB Aldrin	4.707	5.454	55618571	585.6E6	29.609	28.453
6)	B beta-BHC	4.410	4.812	25620072	213.6E6	27.542	23.875m
7)	B delta-BHC	4.613	5.030	57105933	568.2E6	29.261	25.757
8)	B Heptachlo...	5.150	5.838	51421279	532.2E6	29.232	26.742m
9)	A Endosulfan I	5.489	6.196	45267945	499.0E6	27.533	27.941
10)	B trans-Chl...	5.376	6.073	53490481	534.0E6	29.261	26.797m
11)	B cis-Chlor...	5.435	6.146	50633969	521.0E6	28.549	27.562
12)	B 4,4'-DDE	5.599	6.303	106.3E6	1004.1E6	58.860	53.064
13)	MA Dieldrin	5.732	6.453	111.1E6	1083.3E6	59.329	56.614
14)	MA Endrin	5.989	6.671	98526723	918.5E6	60.963	58.002
15)	B Endosulfa...	6.263	6.880	93001452	919.2E6	61.924	60.725
16)	A 4,4'-DDD	6.116	6.793	90066383	924.2E6	60.949	60.837
17)	MA 4,4'-DDT	6.356	7.091	92442630	896.2E6	60.888	58.313
18)	B Endrin al...	6.431	7.004	79612413	778.3E6	61.097	58.964
19)	B Endosulfa...	6.644	7.227	86289497	896.9E6	60.090	57.554
20)	A Methoxychlor	6.903	7.550	245.1E6	2090.3E6	296.985	289.711
21)	B Endrin ke...	7.136	7.697	107.4E6	921.9E6	60.904	59.822

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060321\
Data File : PD063392.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 21:27
Operator : AR\AJ
Sample : M2491-03MS
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 06:30:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

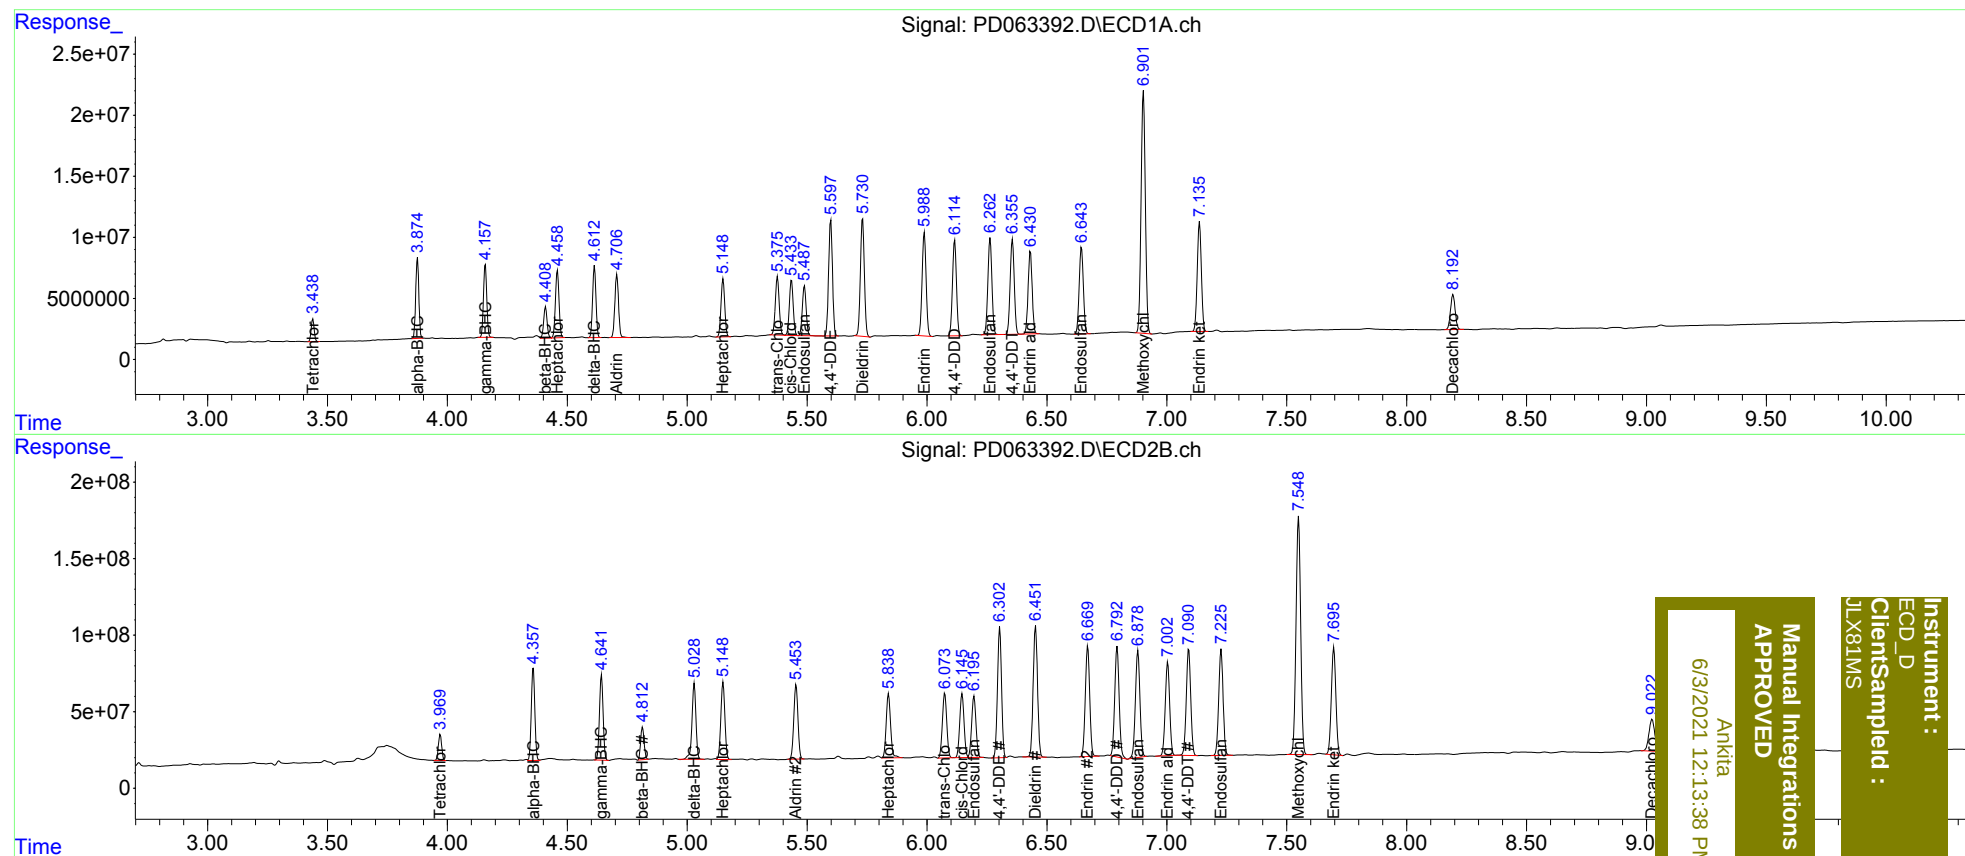

Manual Integrations
APPROVED

Ankita
6/3/2021 12:13:38 PM

Instrument :
ECD_D
Client Sample :
JLX81MS