

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
 Data File : PD069960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2022 11:46
 Operator : AR\AJ
 Sample : PB145038BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 04:04:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	4.168	21416684	187.3E6	20.124	21.253
28)	SA Decachlor...	8.194	9.361	22412937	117.4E6	20.548	21.709
Target Compounds							
3)	MA gamma-BHC...	4.166	0.000	2811157	0	1.629	N.D. #
22)	Mirex	0.000	8.395f	0	115.8E6	N.D.	21.673 #
23)	Chlordane-1	4.339f	0.000	2902187	0	74.099	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
Data File : PD069960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2022 11:46
Operator : AR\AJ
Sample : PB145038BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 04:04:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

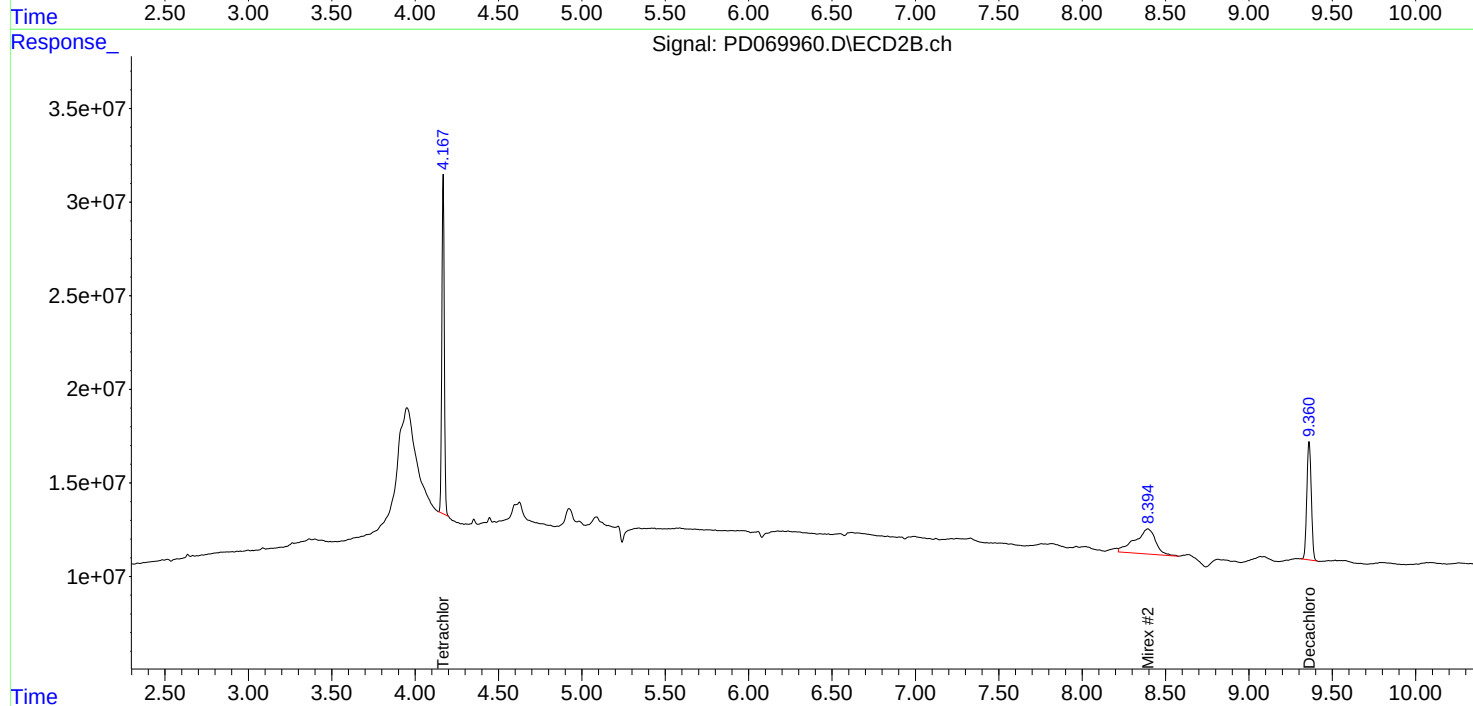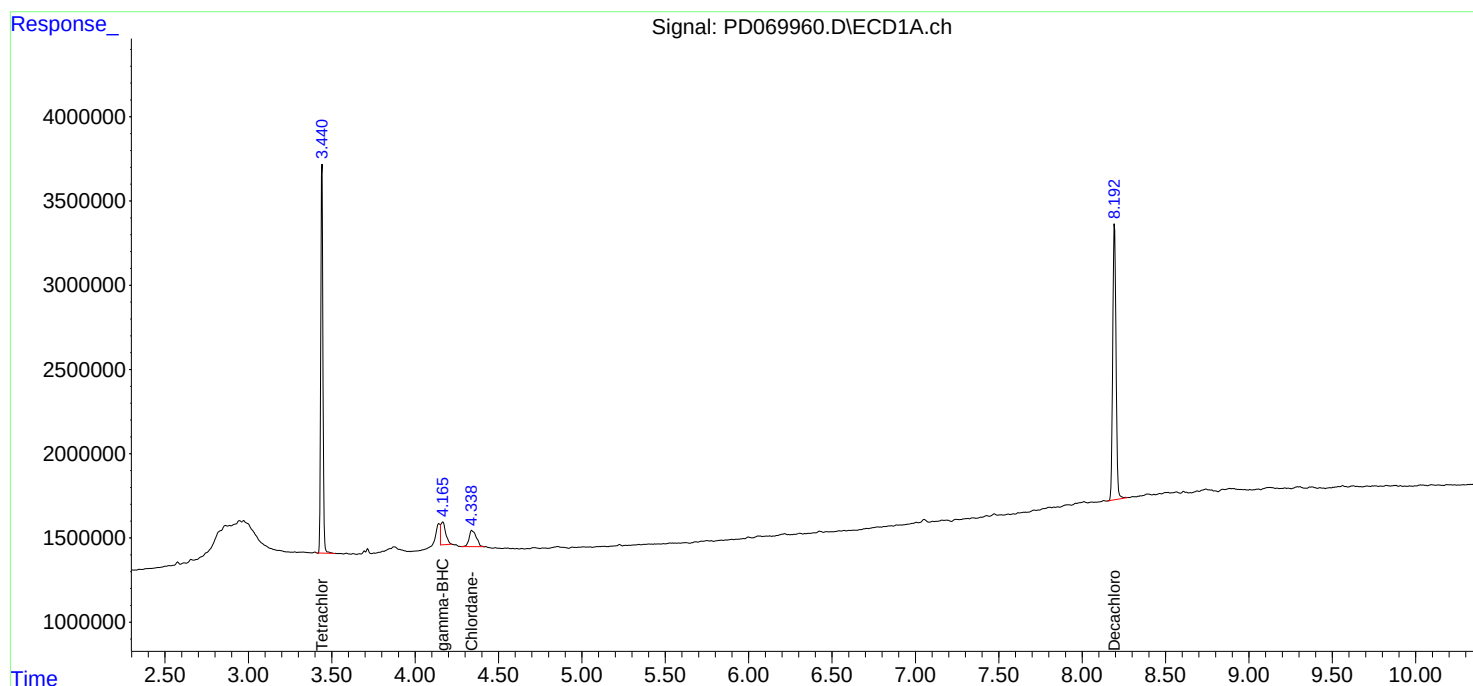


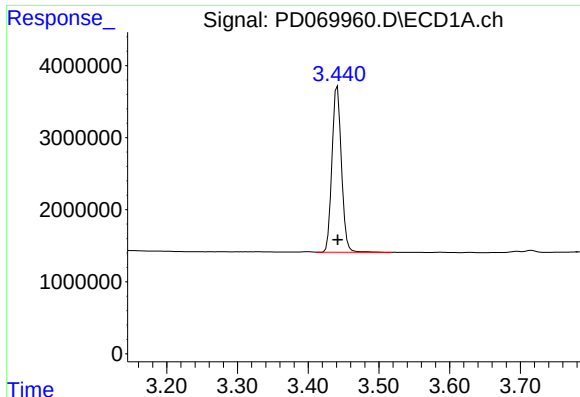

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 21416684
Conc: 20.12 ng/ml

Instrument :
ECD_D
ClientSampleId :

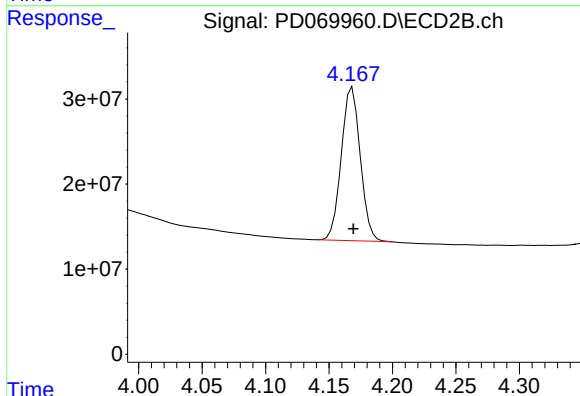


#1 Tetrachloro-m-xylene

R.T.: 4.168 min
Delta R.T.: 0.000 min
Response: 187276271
Conc: 21.25 ng/ml

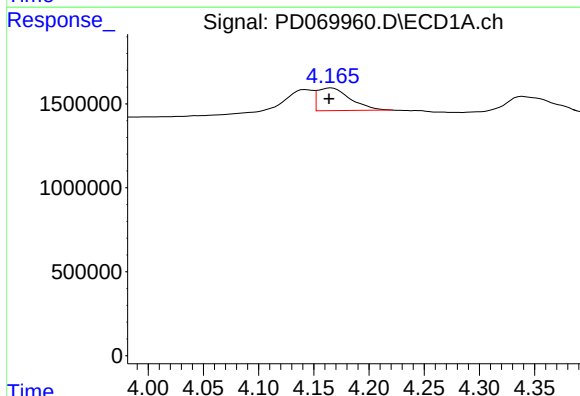


#3 gamma-BHC (Lindane)

R.T.: 4.166 min
Delta R.T.: 0.002 min
Response: 2811157
Conc: 1.63 ng/ml

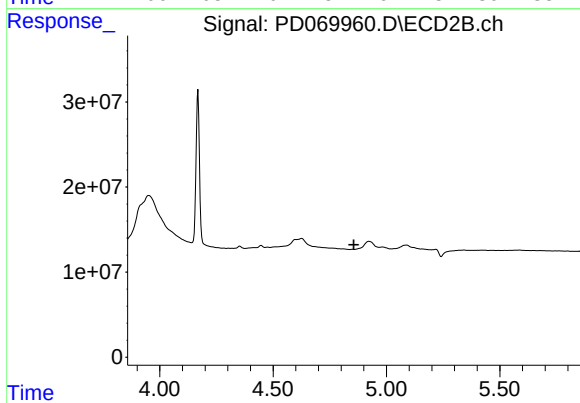

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.856 min
Response: 0
Conc: N.D.

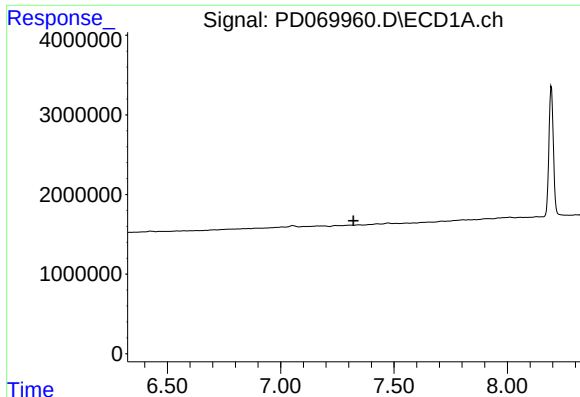

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.321 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

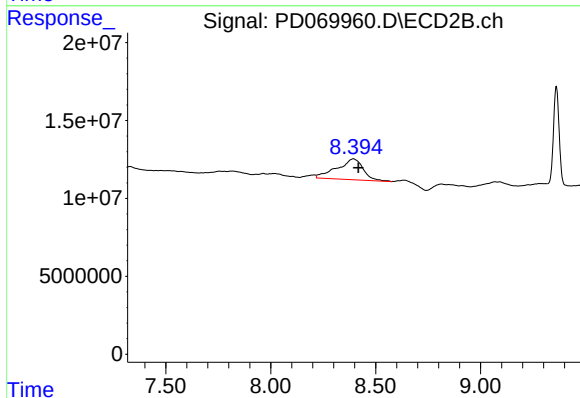


#22 Mirex

R.T.: 8.395 min
Delta R.T.: -0.023 min
Response: 115783592
Conc: 21.67 ng/ml

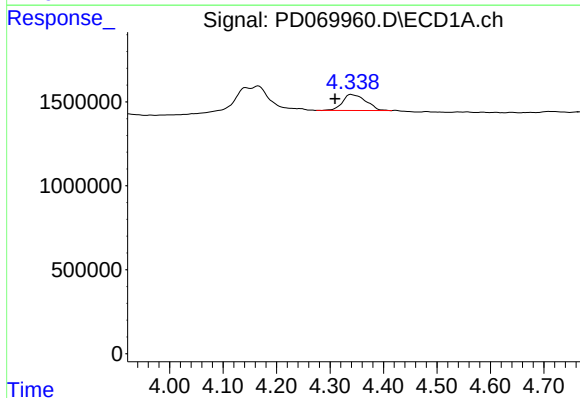


#23 Chlordane-1

R.T.: 4.339 min
Delta R.T.: 0.029 min
Response: 2902187
Conc: 74.10 ng/ml

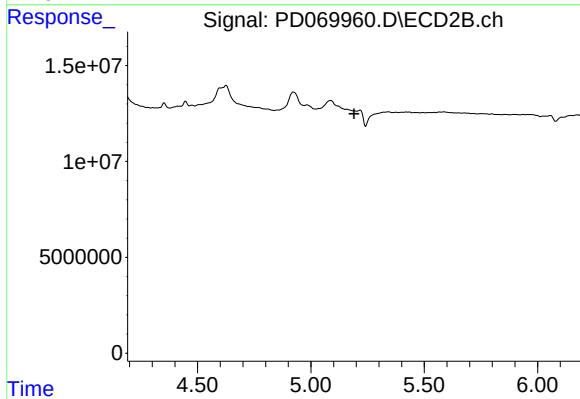

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.190 min
Response: 0
Conc: N.D.

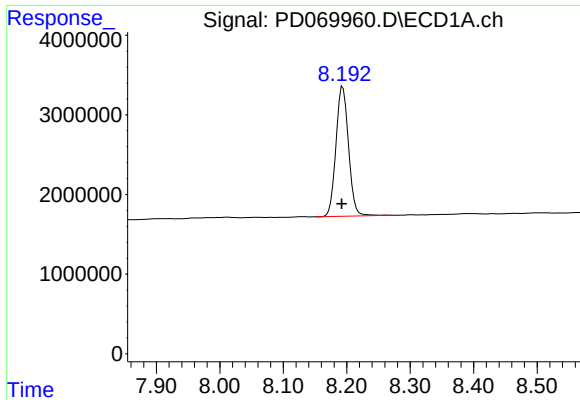

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.002 min
Response: 22412937
Conc: 20.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

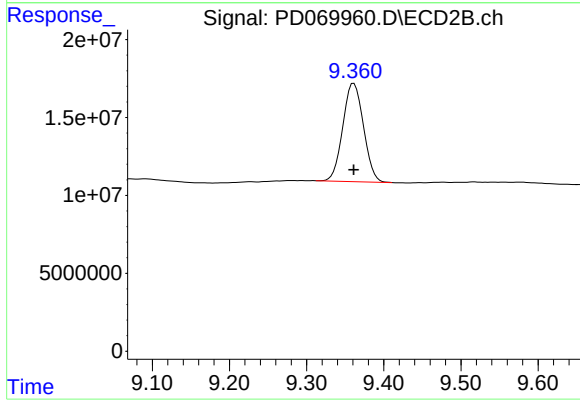

#28 Decachlorobiphenyl

R.T.: 9.361 min
Delta R.T.: 0.000 min
Response: 117404180
Conc: 21.71 ng/ml