

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
 Data File : PD069967.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2022 15:14
 Operator : AR\AJ
 Sample : N2895-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 04:06:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	4.189f	9746604	59343793	9.159	6.735 #
28)	SA Decachlor...	8.195	9.384f	12132477	59457287	11.123	10.994
Target Compounds							
3)	MA gamma-BHC...	4.171	0.000	3475144	0	2.013	N.D. #
13)	MA Dieldrin	5.747	6.710	1084256	10349914	0.824	1.097 #
14)	MA Endrin	5.987	0.000	1988688	0	1.722	N.D. #
15)	B Endosulfa...	0.000	7.138	0	4312251	N.D.	0.581 #
17)	MA 4,4'-DDT	6.354	7.334	9012896	72124095	9.094	9.856
18)	B Endrin al...	6.448	0.000	3119649	0	3.631	N.D. #
19)	B Endosulfa...	6.642	7.471	5725116	19815578	4.967	2.688 #
20)	A Methoxychlor	6.887f	0.000	14558374	0	25.662	N.D. #
21)	B Endrin ke...	7.164f	7.934f	5685725	107.3E6	4.267	13.483 #
27)	Chlordane-5	0.000	7.187f	0	5993028	N.D.	21.181 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
Data File : PD069967.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2022 15:14
Operator : AR\AJ
Sample : N2895-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 04:06:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

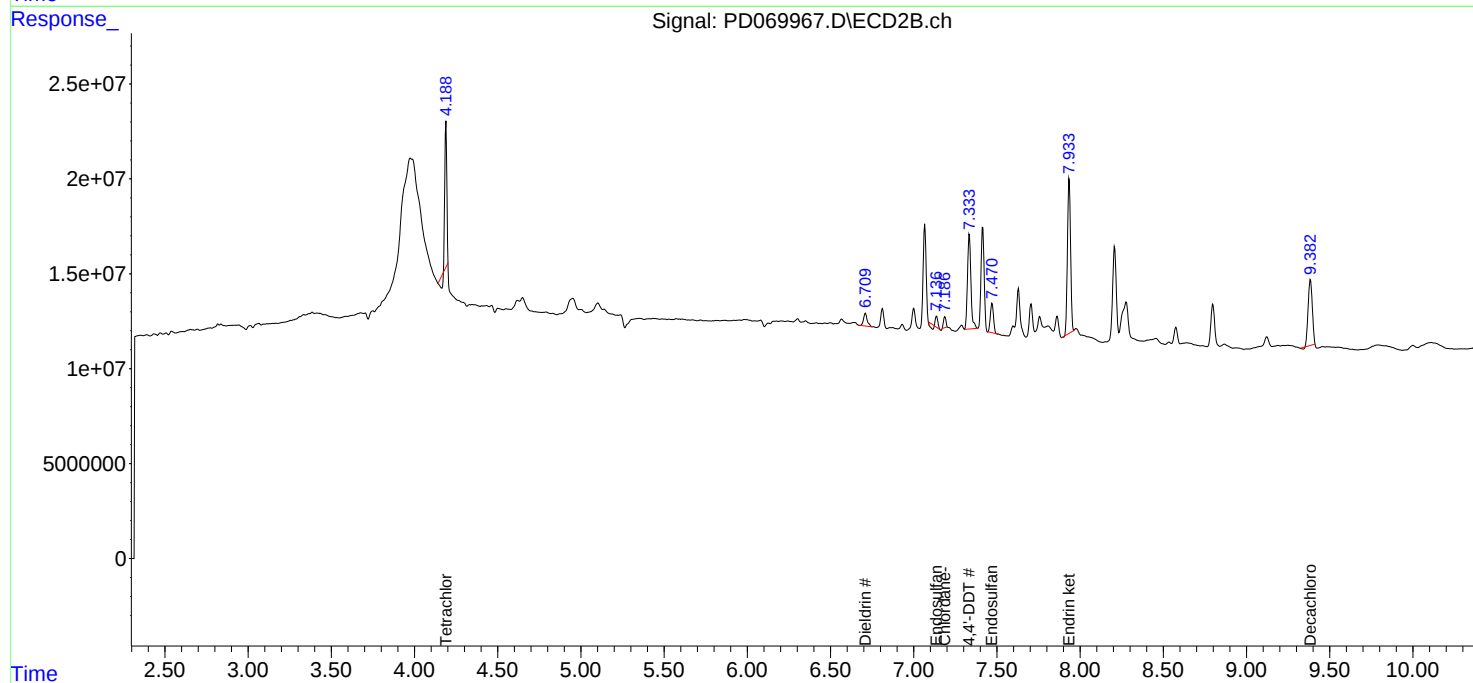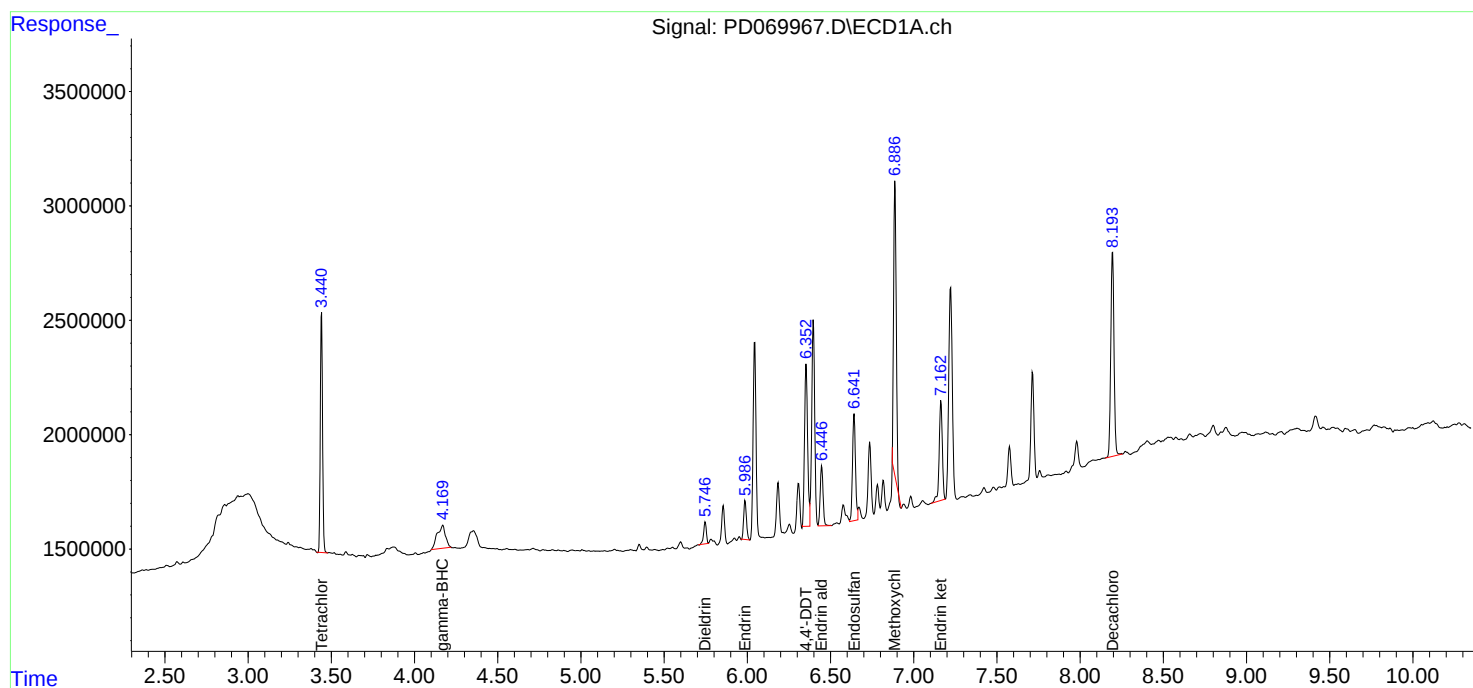


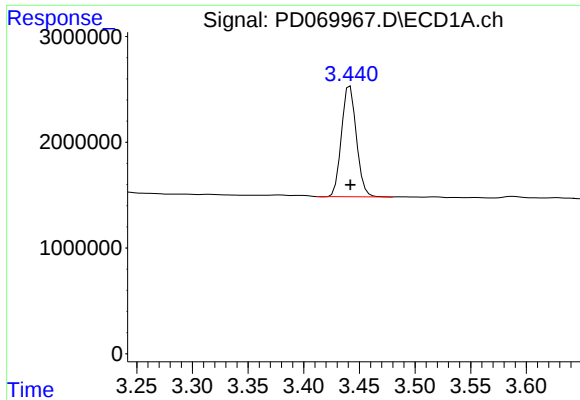

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 9746604
Conc: 9.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

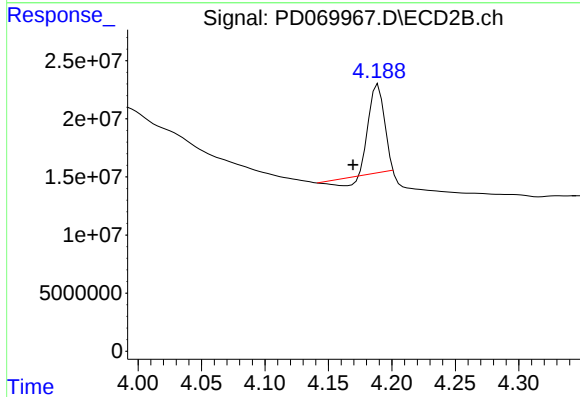


#1 Tetrachloro-m-xylene

R.T.: 4.189 min
Delta R.T.: 0.020 min
Response: 59343793
Conc: 6.73 ng/ml

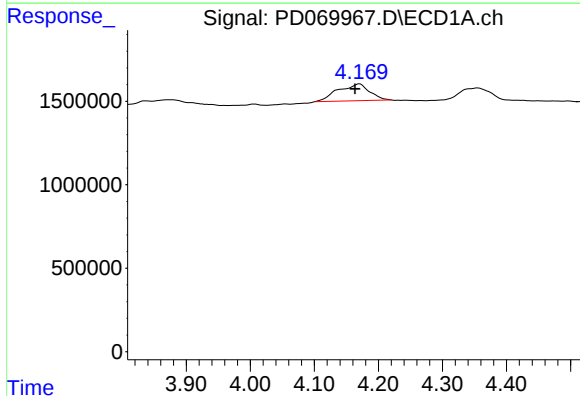


#3 gamma-BHC (Lindane)

R.T.: 4.171 min
Delta R.T.: 0.007 min
Response: 3475144
Conc: 2.01 ng/ml

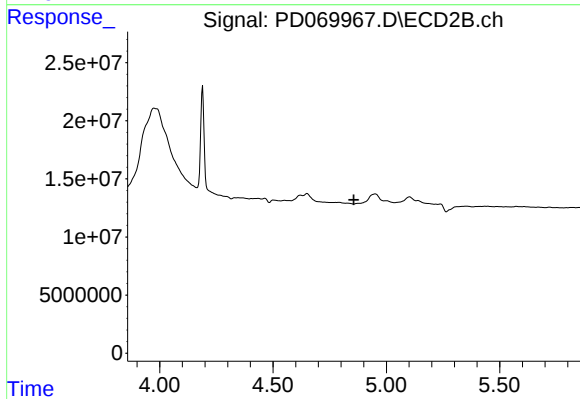

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.856 min
Response: 0
Conc: N.D.

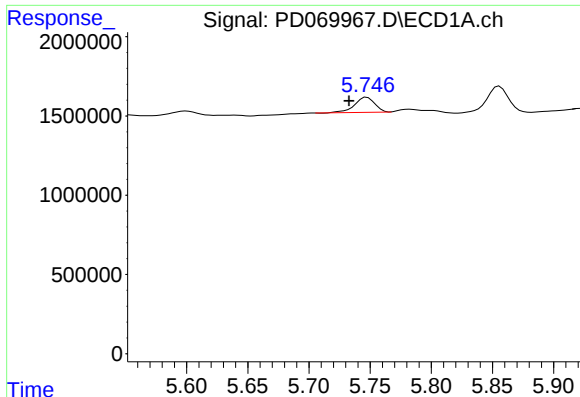

#13 Dieldrin


R.T.: 5.747 min
Delta R.T.: 0.015 min
Response: 1084256
Conc: 0.82 ng/ml

Instrument :
ECD_D
ClientSampleId :

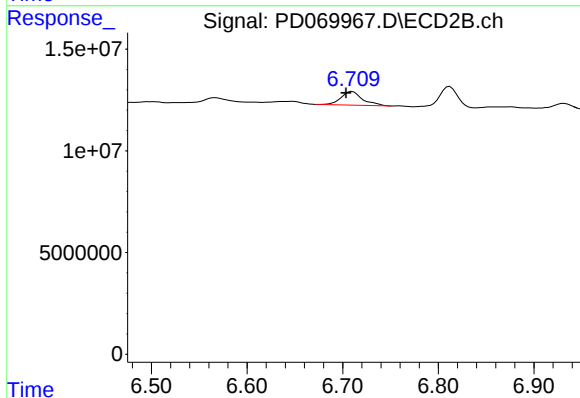


#13 Dieldrin

R.T.: 6.710 min
Delta R.T.: 0.006 min
Response: 10349914
Conc: 1.10 ng/ml

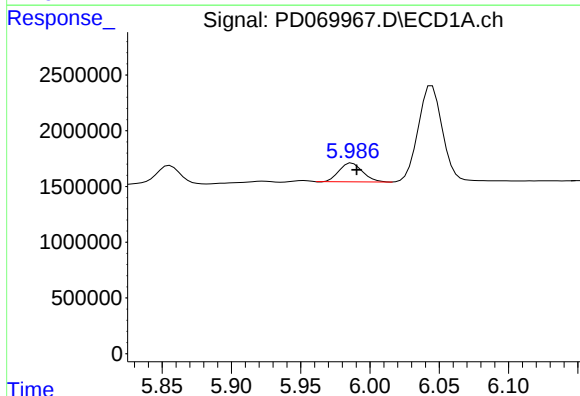


#14 Endrin

R.T.: 5.987 min
Delta R.T.: -0.003 min
Response: 1988688
Conc: 1.72 ng/ml

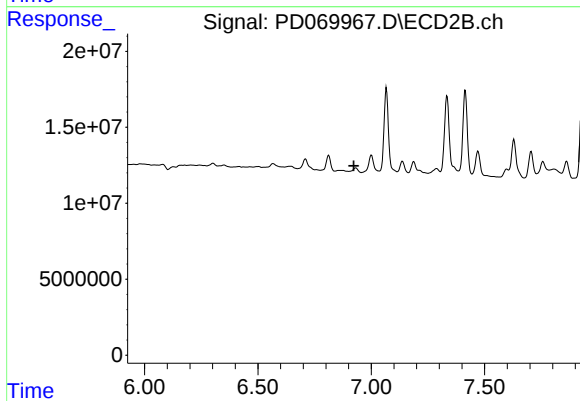

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.924 min
Response: 0
Conc: N.D.

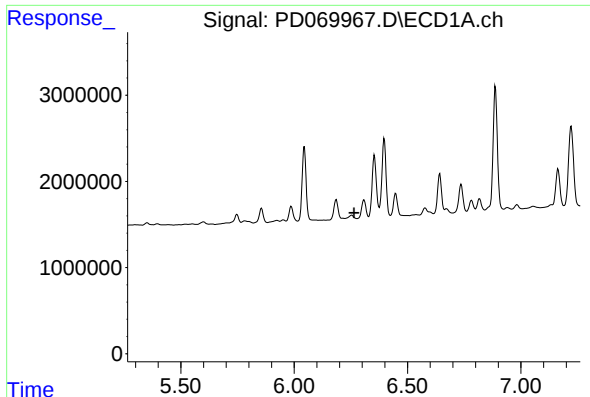

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.264 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

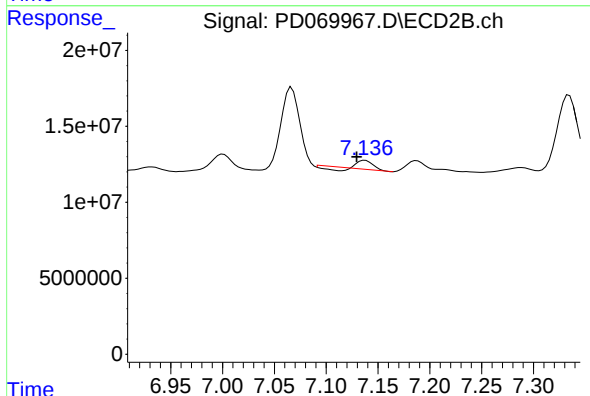


#15 Endosulfan II

R.T.: 7.138 min
Delta R.T.: 0.008 min
Response: 4312251
Conc: 0.58 ng/ml

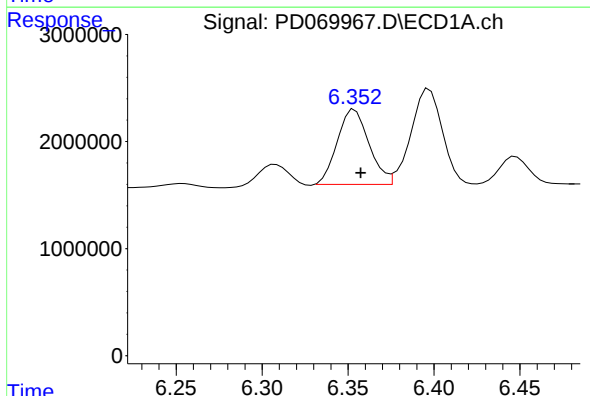


#17 4,4'-DDT

R.T.: 6.354 min
Delta R.T.: -0.003 min
Response: 9012896
Conc: 9.09 ng/ml

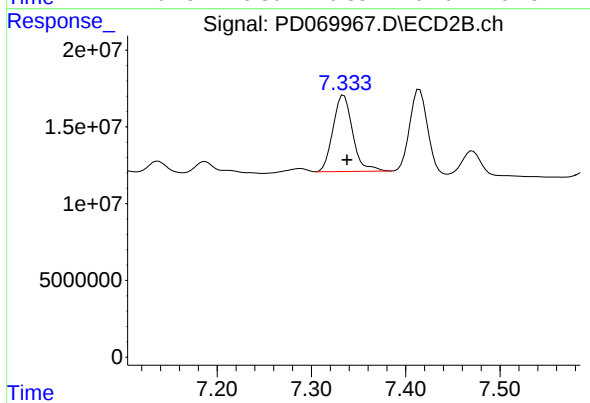

#17 4,4'-DDT


R.T.: 7.334 min
Delta R.T.: -0.003 min
Response: 72124095
Conc: 9.86 ng/ml

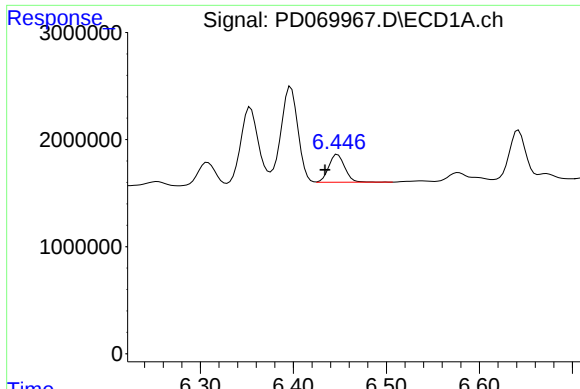

#18 Endrin aldehyde


R.T.: 6.448 min
Delta R.T.: 0.013 min
Response: 3119649
Conc: 3.63 ng/ml

Instrument :
ECD_D
ClientSampleId :

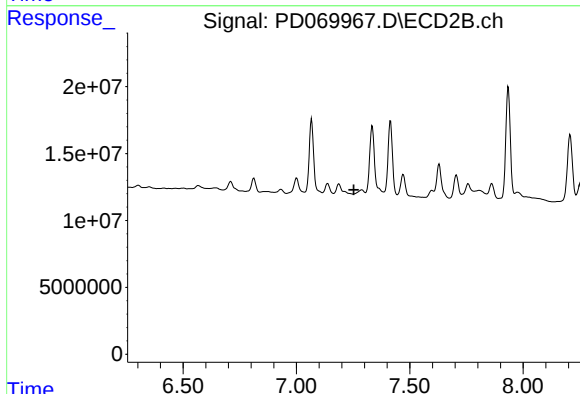


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

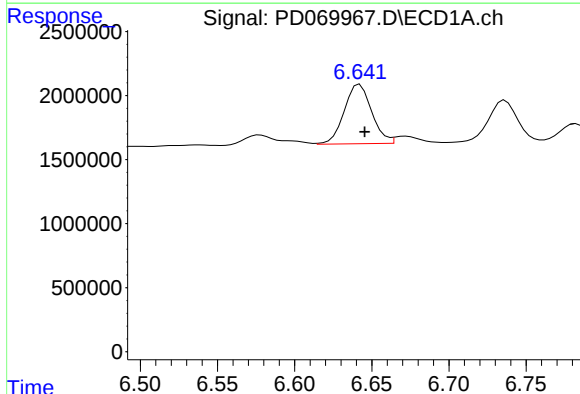


#19 Endosulfan Sulfate

R.T.: 6.642 min
Delta R.T.: -0.003 min
Response: 5725116
Conc: 4.97 ng/ml

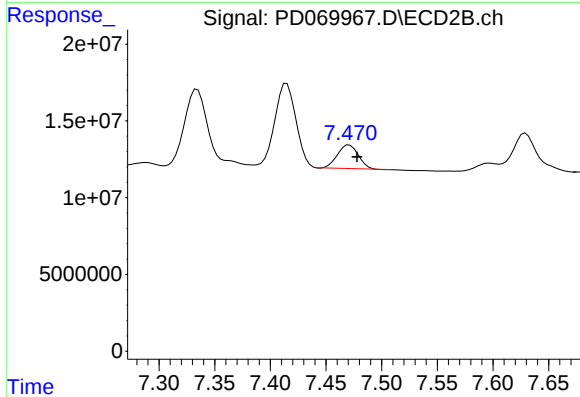

#19 Endosulfan Sulfate


R.T.: 7.471 min
Delta R.T.: -0.007 min
Response: 19815578
Conc: 2.69 ng/ml

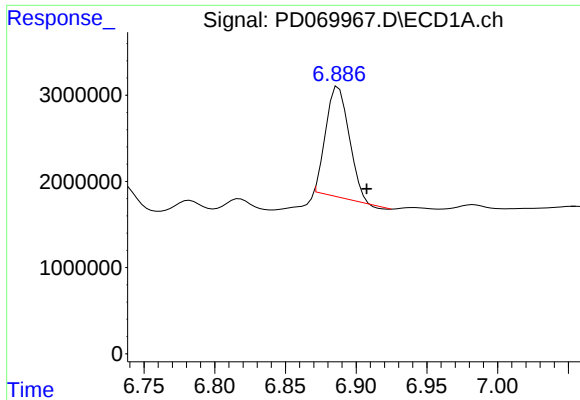

#20 Methoxychlor


R.T.: 6.887 min
Delta R.T.: -0.020 min
Response: 14558374
Conc: 25.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

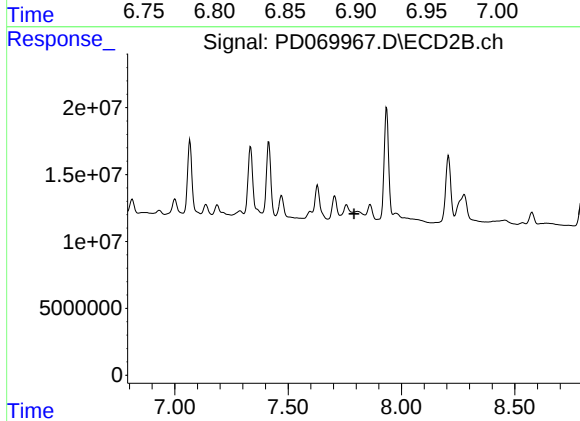


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.792 min
Response: 0
Conc: N.D.

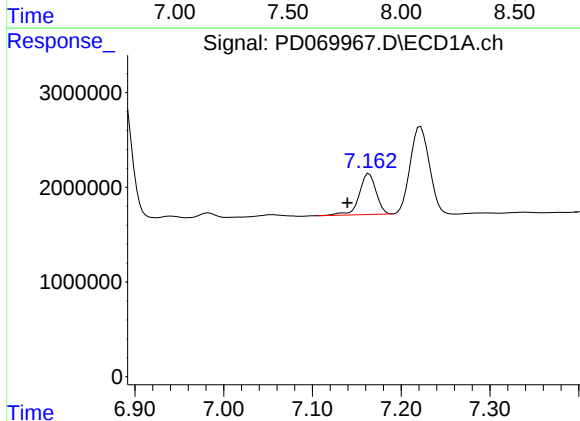


#21 Endrin ketone

R.T.: 7.164 min
Delta R.T.: 0.025 min
Response: 5685725
Conc: 4.27 ng/ml

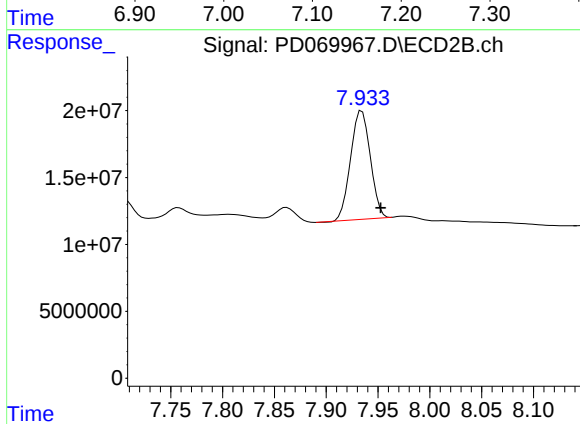

#21 Endrin ketone


R.T.: 7.934 min
Delta R.T.: -0.018 min
Response: 107340108
Conc: 13.48 ng/ml

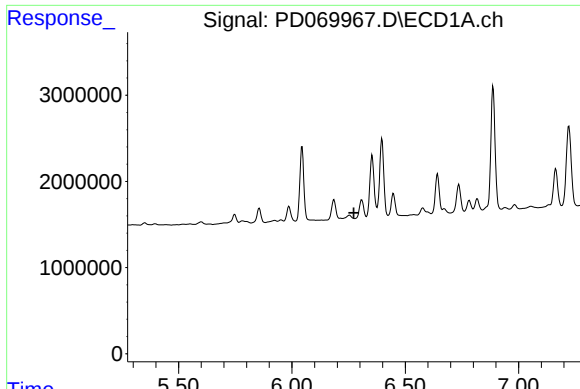

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.273 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

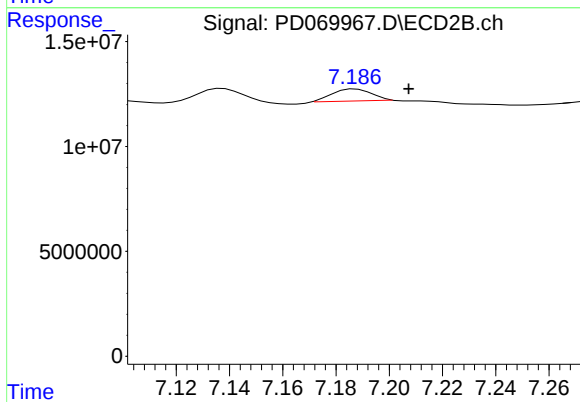


#27 Chlordane-5

R.T.: 7.187 min
Delta R.T.: -0.020 min
Response: 5993028
Conc: 21.18 ng/ml

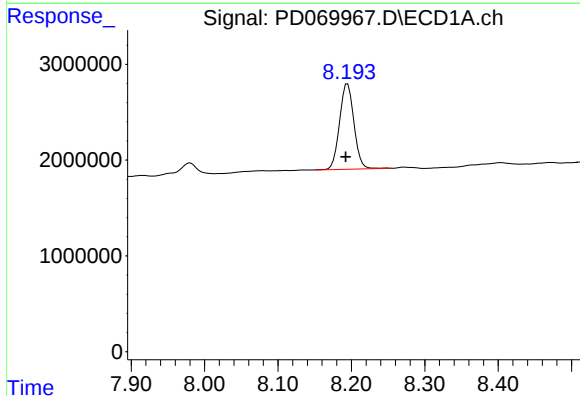

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.003 min
Response: 12132477
Conc: 11.12 ng/ml

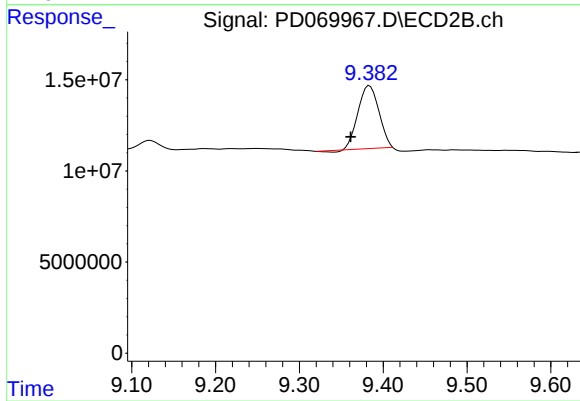

#28 Decachlorobiphenyl

R.T.: 9.384 min
Delta R.T.: 0.022 min
Response: 59457287
Conc: 10.99 ng/ml