

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
 Data File : PD069968.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2022 15:28
 Operator : AR\AJ
 Sample : N2895-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 04:07:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	4.169	10342102	96779444	9.718	10.983
28)	SA Decachlor...	8.194	9.364	10261147	56492128	9.408	10.446
Target Compounds							
3)	MA gamma-BHC...	4.171	0.000	3087834	0	1.789	N.D. #
12)	B 4,4'-DDE	5.601	6.546	770044	8430495	0.608	0.932 #
13)	MA Dieldrin	5.747	6.690	3209811	25420364	2.438	2.694
14)	MA Endrin	5.986	0.000	2881659	0	2.496	N.D. #
15)	B Endosulfa...	6.255	7.117	1084344	12022191	0.975	1.619 #
16)	A 4,4'-DDD	0.000	7.047	0	77489145	N.D.	10.464 #
17)	MA 4,4'-DDT	6.354	7.314f	12663890	99742794	12.778	13.630
18)	B Endrin al...	6.447	0.000	6011769	0	6.997	N.D. #
19)	B Endosulfa...	6.642	7.450f	11084671	-9504670	9.616	N.D. #
20)	A Methoxychlor	6.887f	0.000	21881235	0	38.571	N.D. #
21)	B Endrin ke...	7.163f	7.953	8258154	10857161	6.197	1.364 #
27)	Chlordane-5	6.255f	0.000	1084344	0	25.783	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
Data File : PD069968.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2022 15:28
Operator : AR\AJ
Sample : N2895-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 04:07:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

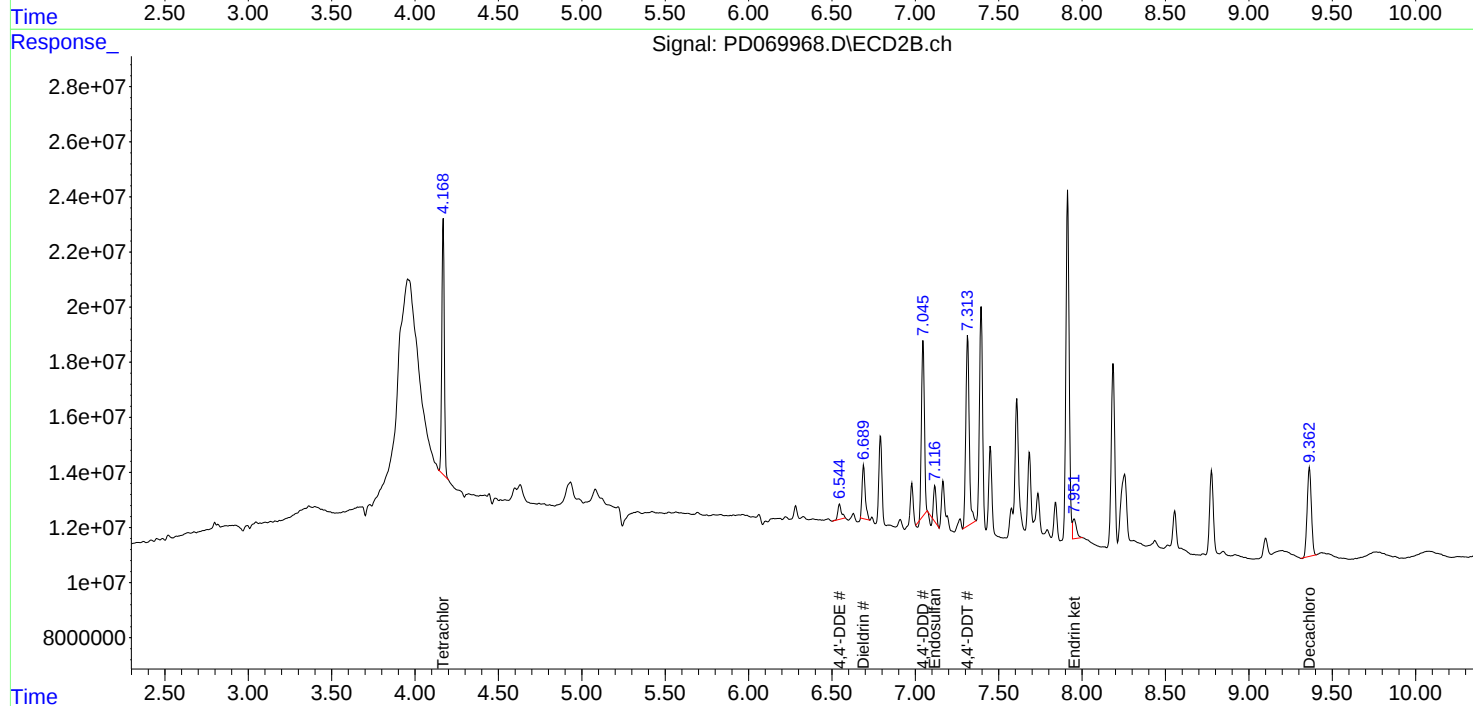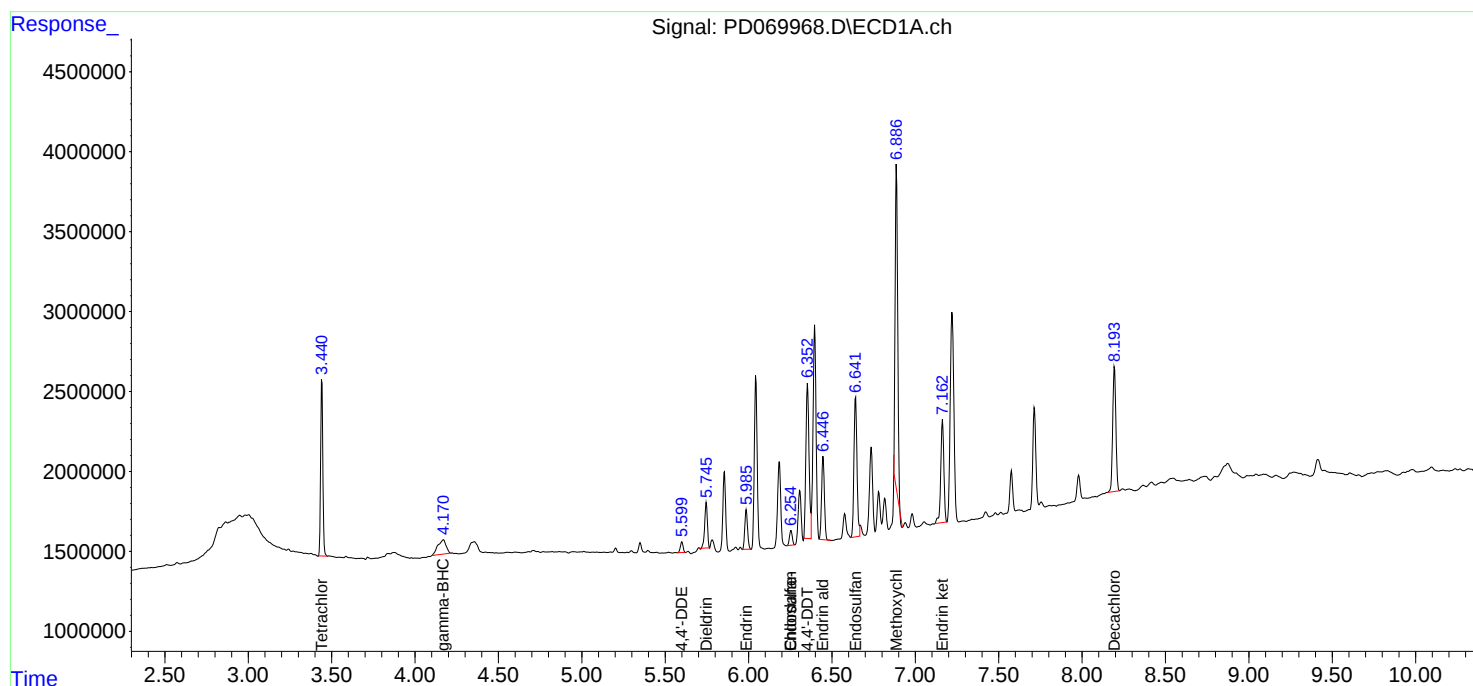


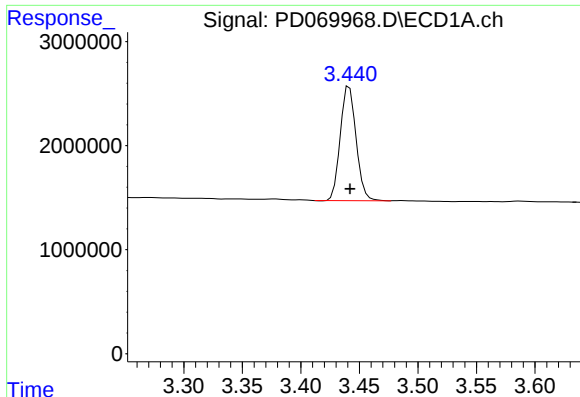

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 10342102
Conc: 9.72 ng/ml

Instrument :
ECD_D
ClientSampleId :

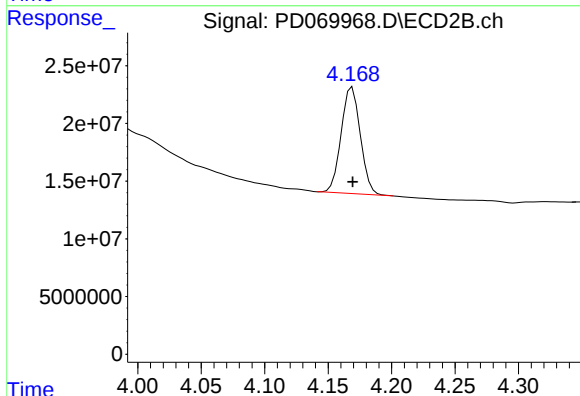


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 96779444
Conc: 10.98 ng/ml

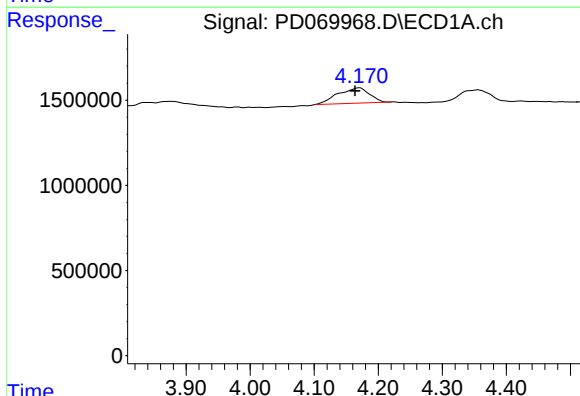


#3 gamma-BHC (Lindane)

R.T.: 4.171 min
Delta R.T.: 0.007 min
Response: 3087834
Conc: 1.79 ng/ml

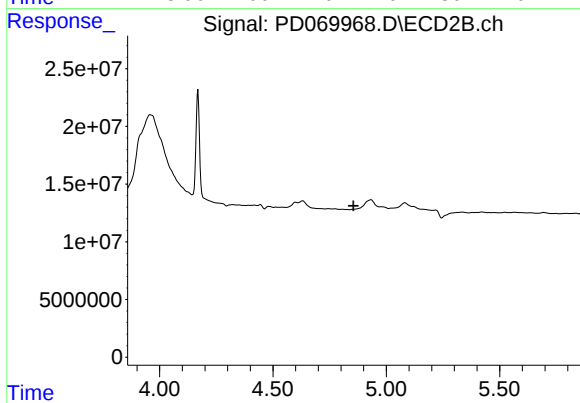

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.856 min
Response: 0
Conc: N.D.

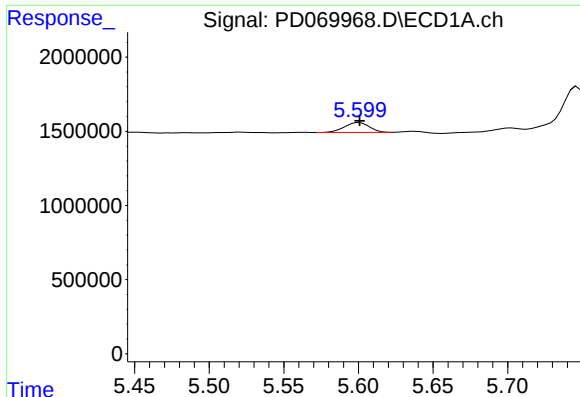

#12 4,4'-DDE


R.T.: 5.601 min
Delta R.T.: 0.000 min
Response: 770044
Conc: 0.61 ng/ml

Instrument :
ECD_D
ClientSampleId :

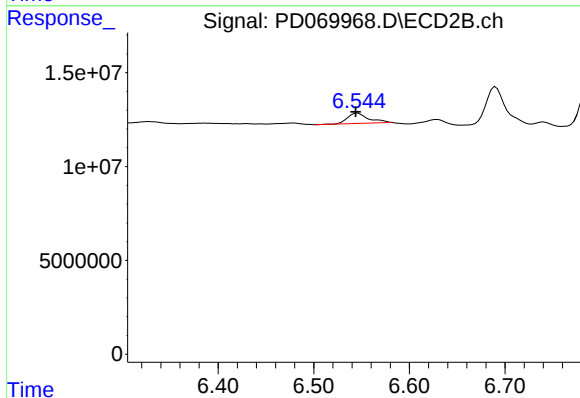


#12 4,4'-DDE

R.T.: 6.546 min
Delta R.T.: 0.002 min
Response: 8430495
Conc: 0.93 ng/ml

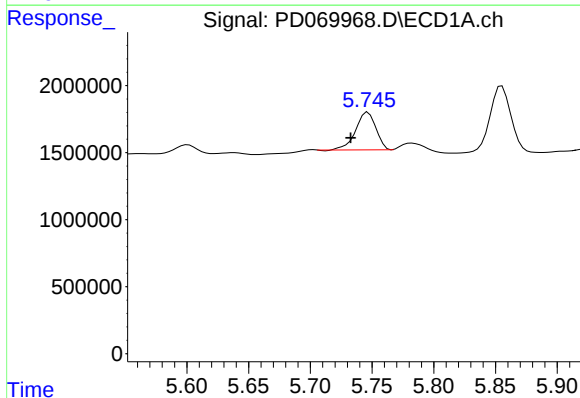


#13 Dieldrin

R.T.: 5.747 min
Delta R.T.: 0.014 min
Response: 3209811
Conc: 2.44 ng/ml

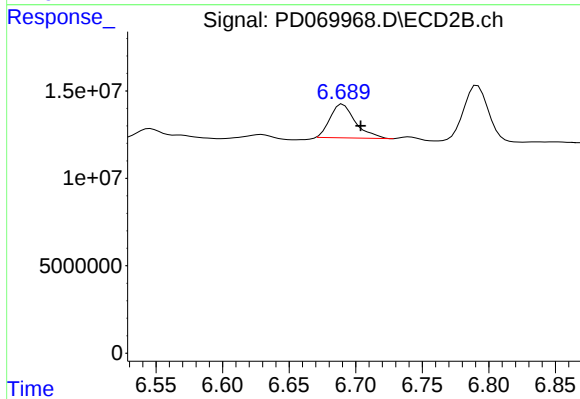

#13 Dieldrin


R.T.: 6.690 min
Delta R.T.: -0.013 min
Response: 25420364
Conc: 2.69 ng/ml

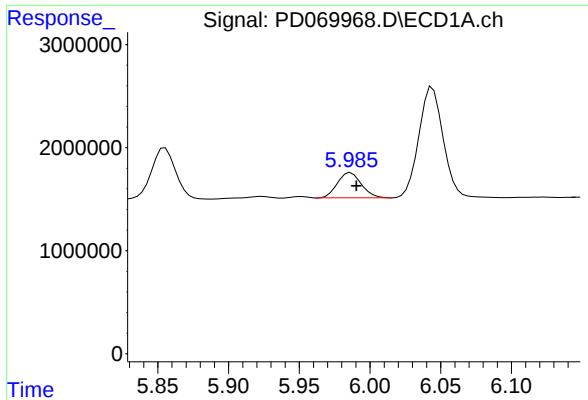

#14 Endrin


R.T.: 5.986 min
Delta R.T.: -0.004 min
Response: 2881659
Conc: 2.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

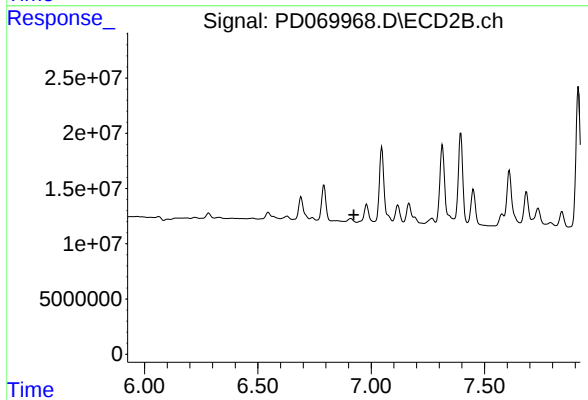


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.924 min
Response: 0
Conc: N.D.

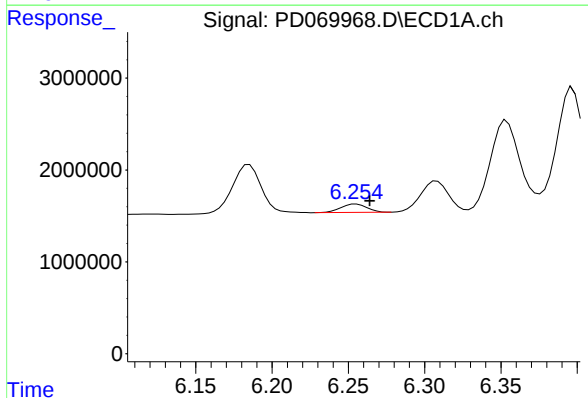


#15 Endosulfan II

R.T.: 6.255 min
Delta R.T.: -0.009 min
Response: 1084344
Conc: 0.97 ng/ml

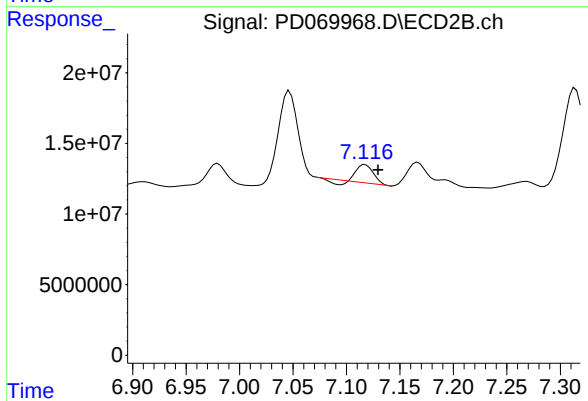

#15 Endosulfan II


R.T.: 7.117 min
Delta R.T.: -0.012 min
Response: 12022191
Conc: 1.62 ng/ml

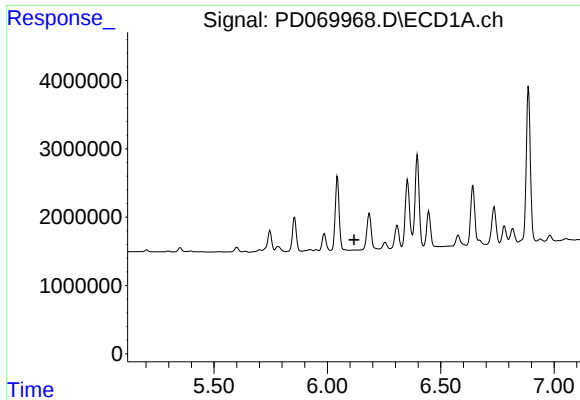

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

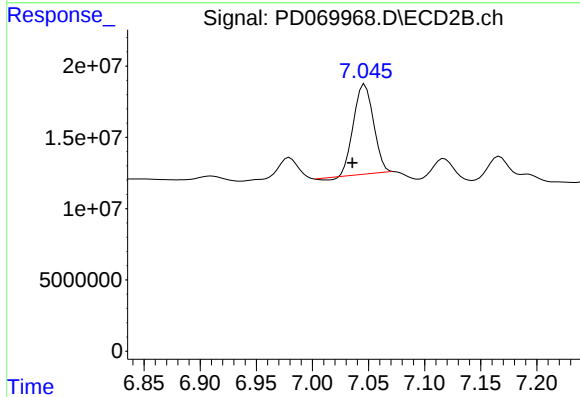


#16 4,4'-DDD

R.T.: 7.047 min
Delta R.T.: 0.011 min
Response: 77489145
Conc: 10.46 ng/ml

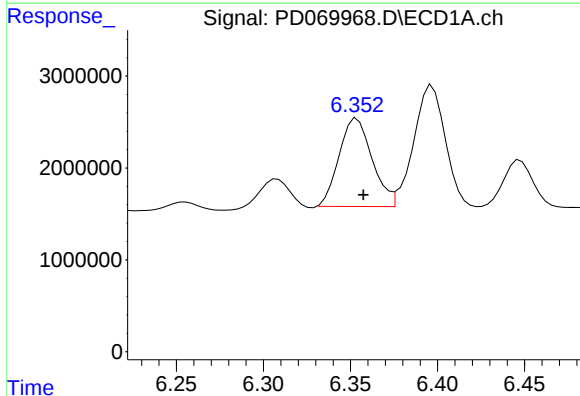


#17 4,4'-DDT

R.T.: 6.354 min
Delta R.T.: -0.004 min
Response: 12663890
Conc: 12.78 ng/ml

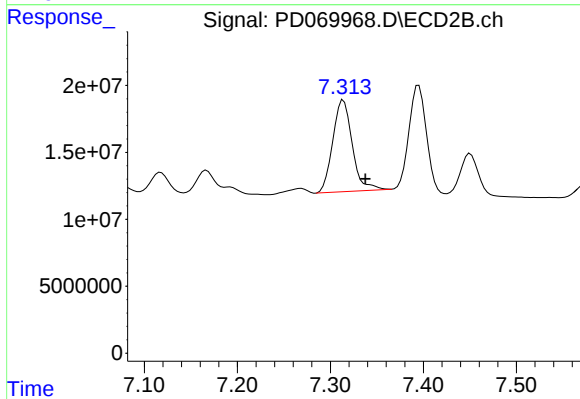

#17 4,4'-DDT


R.T.: 7.314 min
Delta R.T.: -0.024 min
Response: 99742794
Conc: 13.63 ng/ml

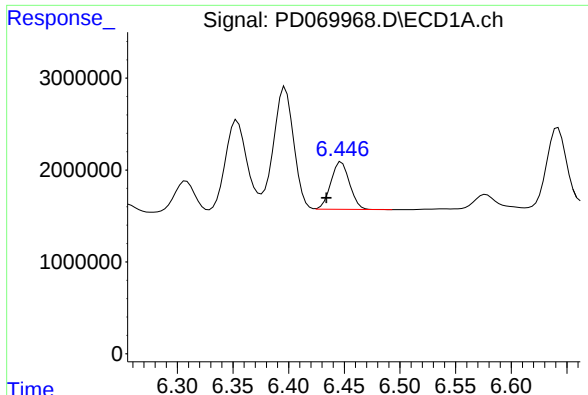

#18 Endrin aldehyde


R.T.: 6.447 min
Delta R.T.: 0.013 min
Response: 6011769
Conc: 7.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

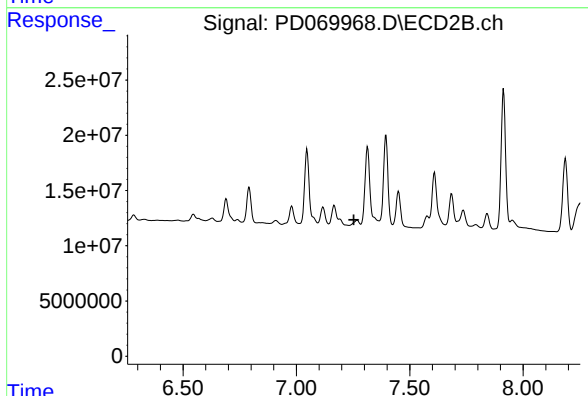


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

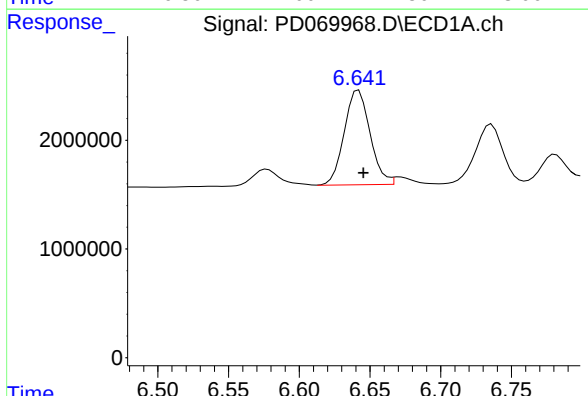


#19 Endosulfan Sulfate

R.T.: 6.642 min
Delta R.T.: -0.003 min
Response: 11084671
Conc: 9.62 ng/ml

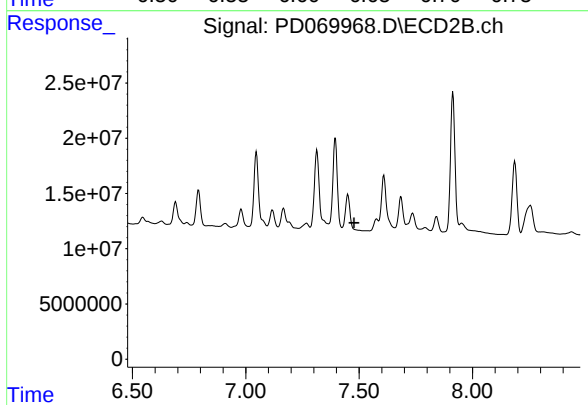

#19 Endosulfan Sulfate


R.T.: 7.450 min
Delta R.T.: -0.027 min
Response: -9504670
Conc: N.D.

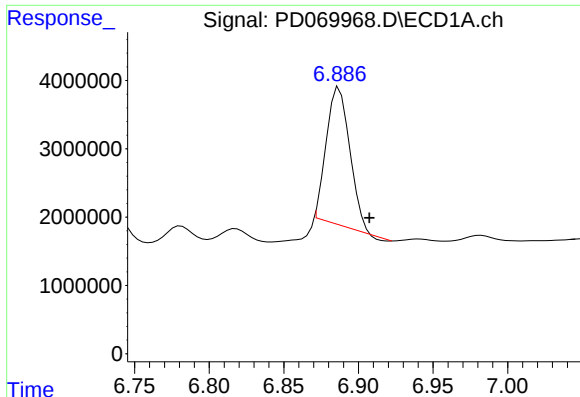

#20 Methoxychlor


R.T.: 6.887 min
Delta R.T.: -0.020 min
Response: 21881235
Conc: 38.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

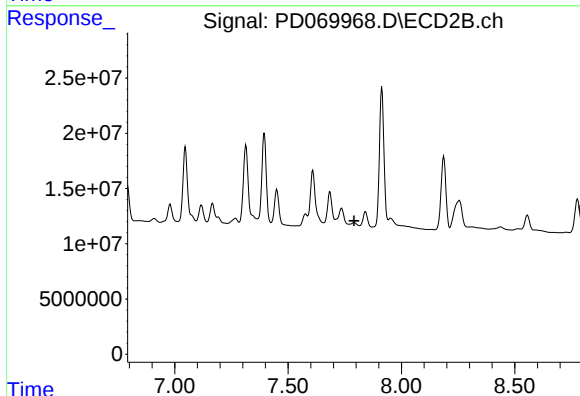


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.792 min
Response: 0
Conc: N.D.

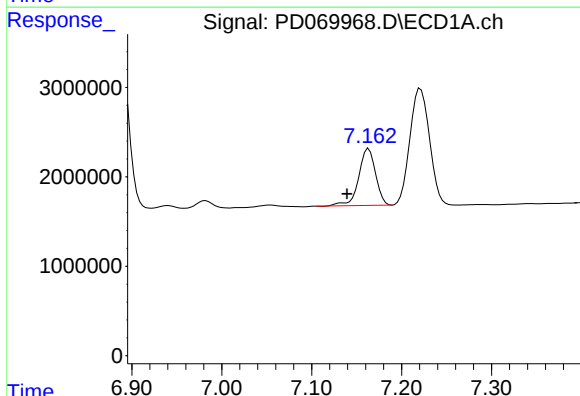


#21 Endrin ketone

R.T.: 7.163 min
Delta R.T.: 0.024 min
Response: 8258154
Conc: 6.20 ng/ml

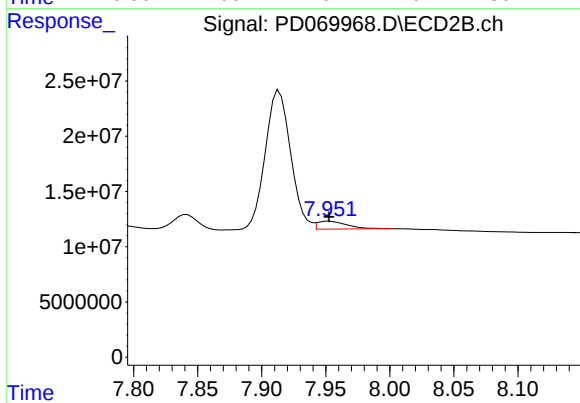

#21 Endrin ketone


R.T.: 7.953 min
Delta R.T.: 0.000 min
Response: 10857161
Conc: 1.36 ng/ml

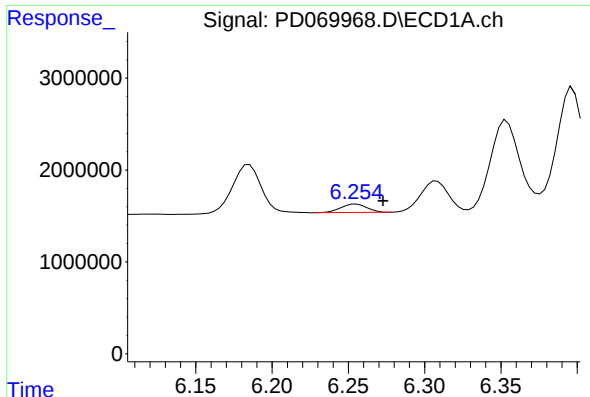

#27 Chlordane-5


R.T.: 6.255 min
Delta R.T.: -0.018 min
Response: 1084344
Conc: 25.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

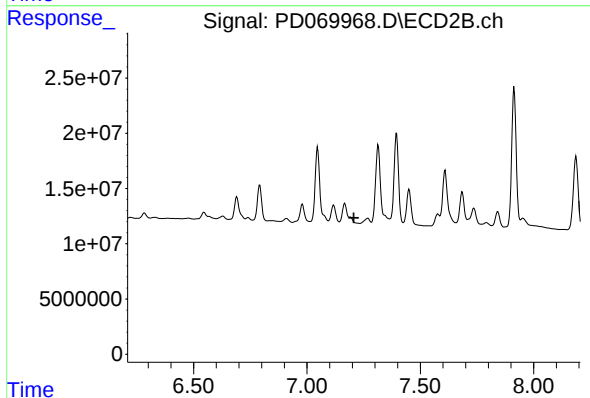


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.207 min
Response: 0
Conc: N.D.

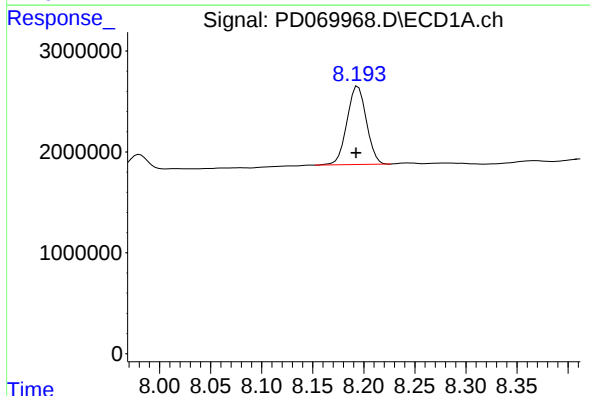

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.002 min
Response: 10261147
Conc: 9.41 ng/ml

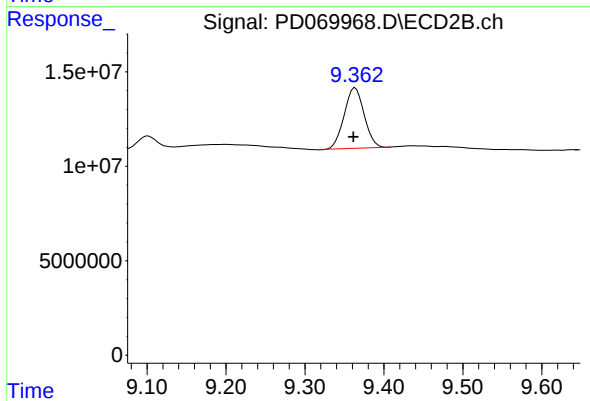

#28 Decachlorobiphenyl

R.T.: 9.364 min
Delta R.T.: 0.002 min
Response: 56492128
Conc: 10.45 ng/ml