

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
 Data File : PD069972.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2022 16:24
 Operator : AR\AJ
 Sample : N2894-17
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 04:08:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	4.169	21224030	196.7E6	19.943	22.328
28)	SA Decachlor...	8.194	9.364	14816151	95420119	13.584	17.644 #
Target Compounds							
3)	MA gamma-BHC...	4.172	0.000	2391391	0	1.386	N.D. #
14)	MA Endrin	5.986	0.000	3074322	0	2.663	N.D. #
16)	A 4,4'-DDD	0.000	7.047	0	6866837	N.D.	0.927 #
17)	MA 4,4'-DDT	6.353	7.313f	1987312	13149962	2.005	1.797
19)	B Endosulfa...	6.642	0.000	815794	0	0.708	N.D. #
20)	A Methoxychlor	6.887f	0.000	2949123	0	5.199	N.D. #
21)	B Endrin ke...	7.163f	0.000	777093	0	0.583	N.D. #
23)	Chlordane-1	4.316	0.000	682871	0	17.435	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
Data File : PD069972.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2022 16:24
Operator : AR\AJ
Sample : N2894-17
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 04:08:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

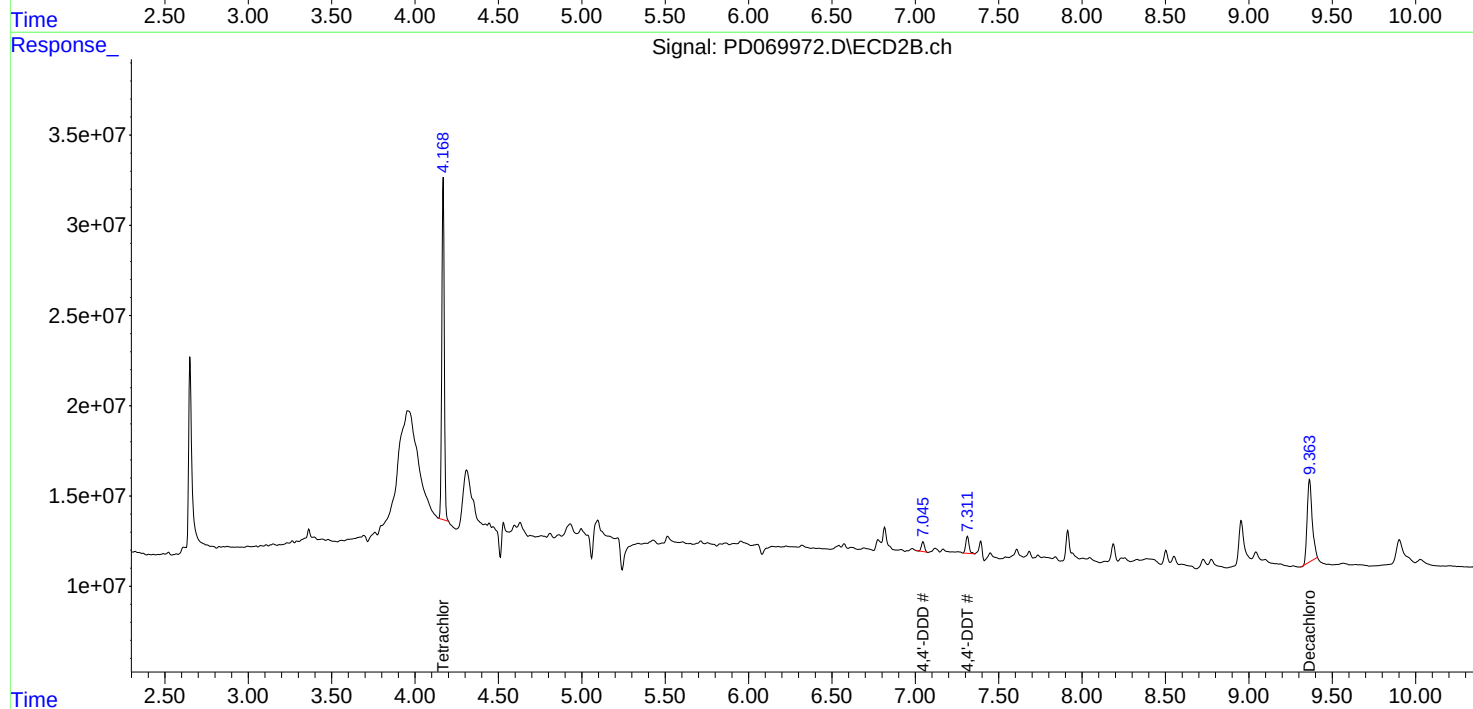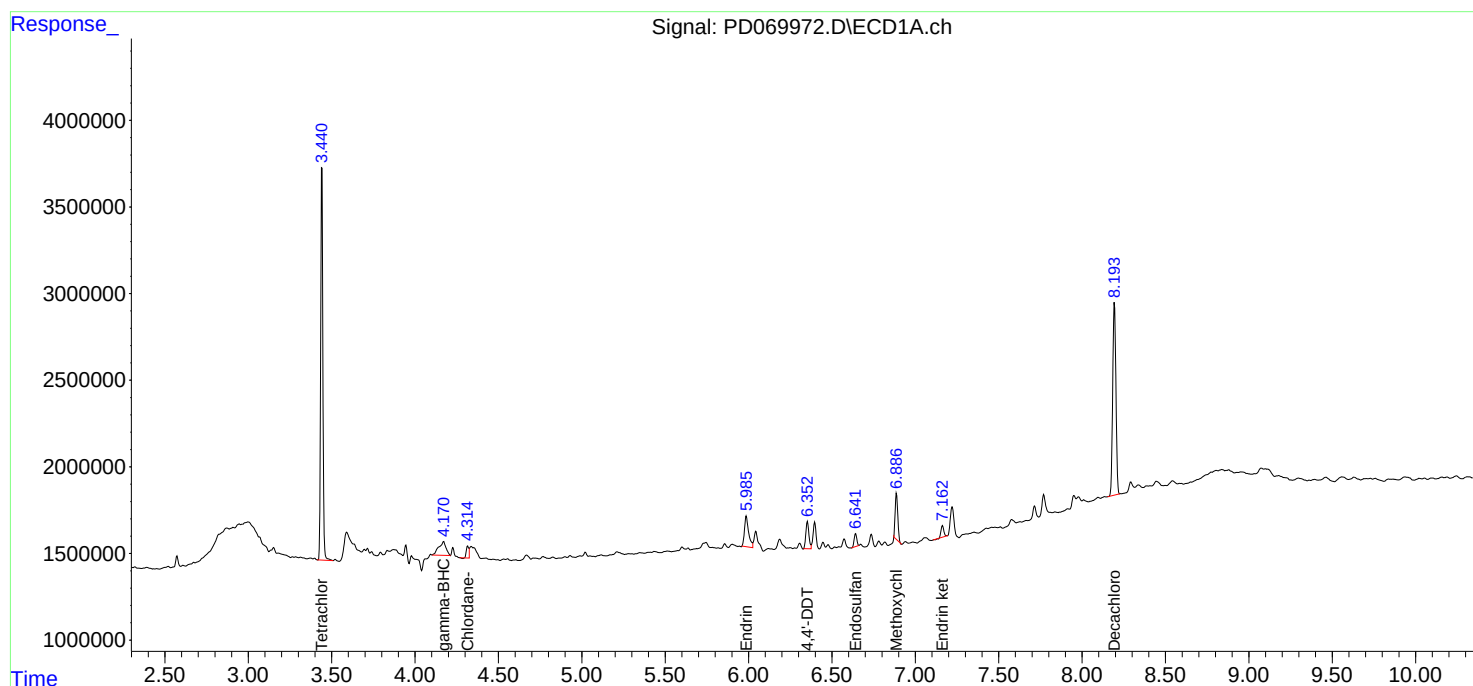


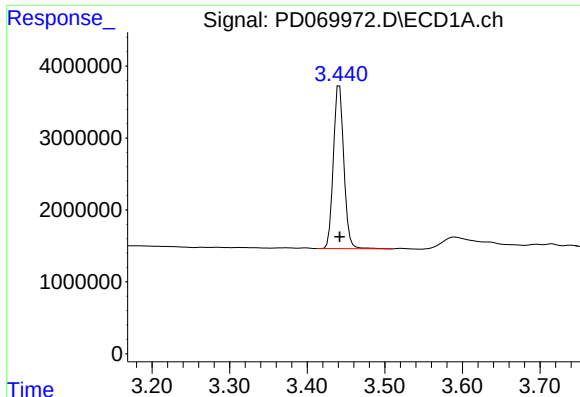

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 21224030
Conc: 19.94 ng/ml

Instrument :
ECD_D
ClientSampleId :

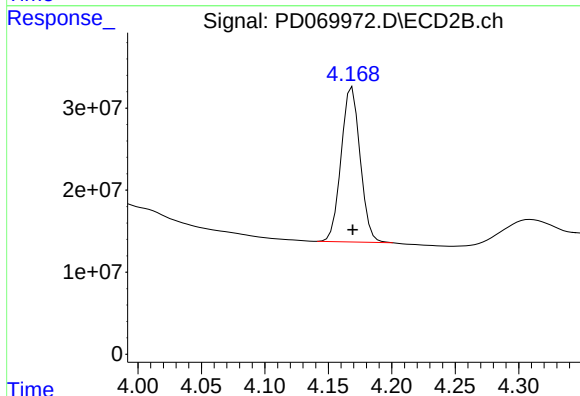


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 196744382
Conc: 22.33 ng/ml

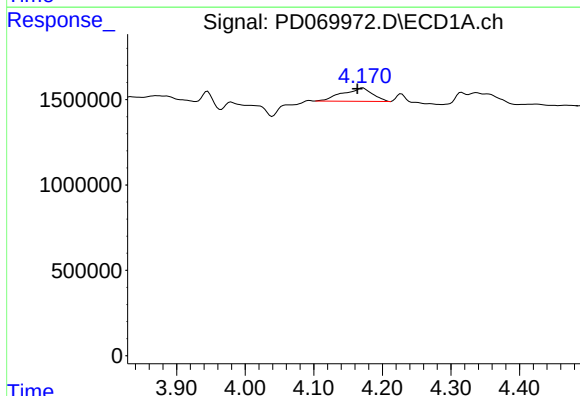


#3 gamma-BHC (Lindane)

R.T.: 4.172 min
Delta R.T.: 0.008 min
Response: 2391391
Conc: 1.39 ng/ml

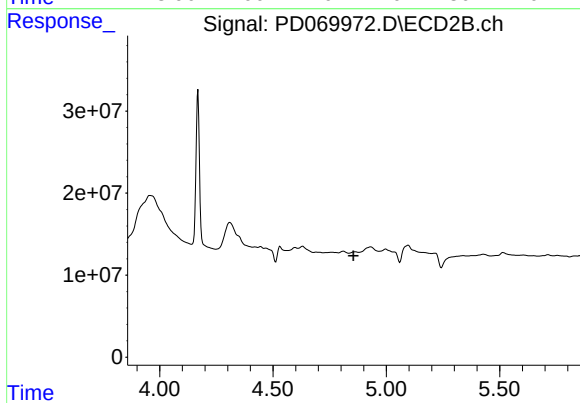

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.856 min
Response: 0
Conc: N.D.

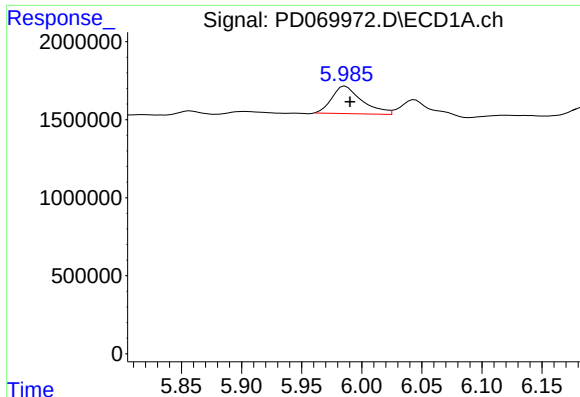

#14 Endrin


R.T.: 5.986 min
Delta R.T.: -0.004 min
Response: 3074322
Conc: 2.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

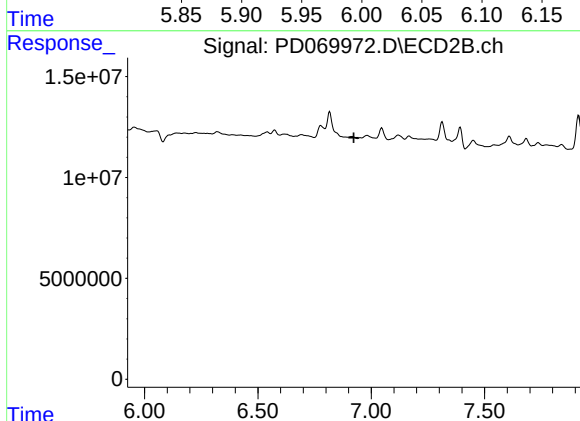


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.924 min
Response: 0
Conc: N.D.

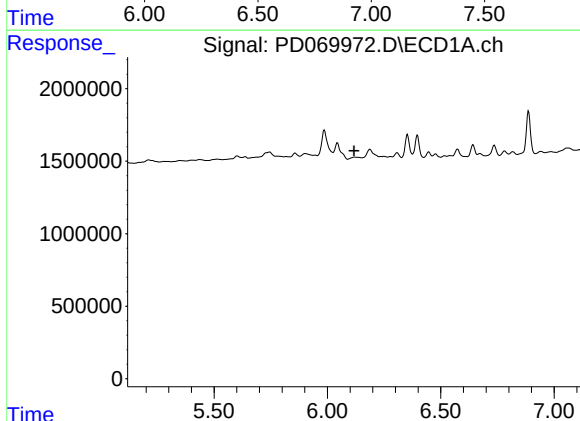


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.118 min
Response: 0
Conc: N.D.

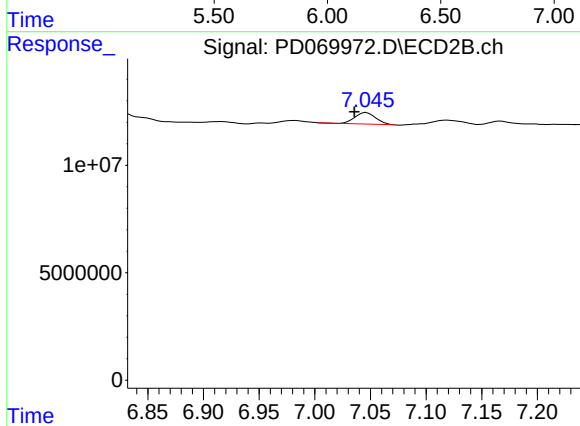

#16 4,4'-DDD


R.T.: 7.047 min
Delta R.T.: 0.011 min
Response: 6866837
Conc: 0.93 ng/ml

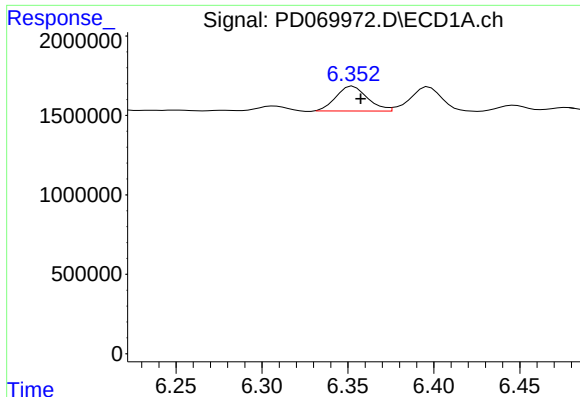

#17 4,4'-DDT


R.T.: 6.353 min
Delta R.T.: -0.004 min
Response: 1987312
Conc: 2.01 ng/ml

Instrument :
ECD_D
ClientSampleId :

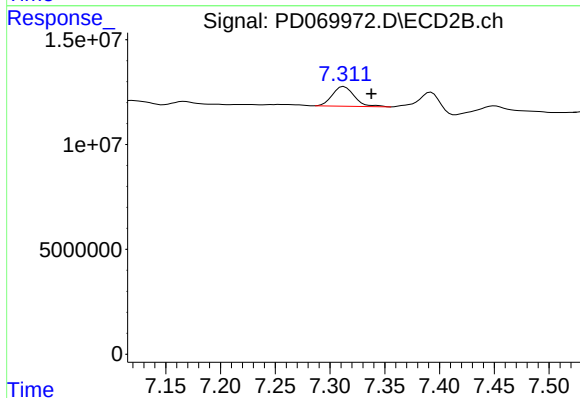


#17 4,4'-DDT

R.T.: 7.313 min
Delta R.T.: -0.025 min
Response: 13149962
Conc: 1.80 ng/ml

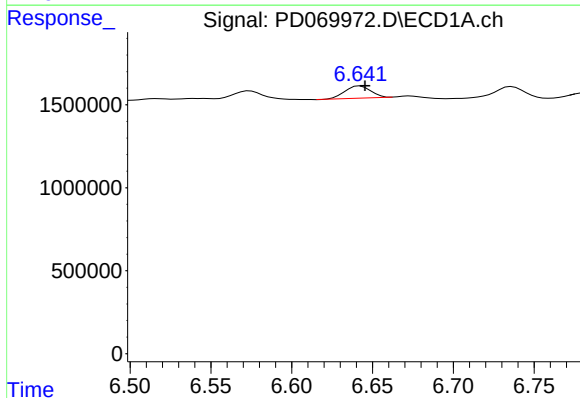


#19 Endosulfan Sulfate

R.T.: 6.642 min
Delta R.T.: -0.003 min
Response: 815794
Conc: 0.71 ng/ml

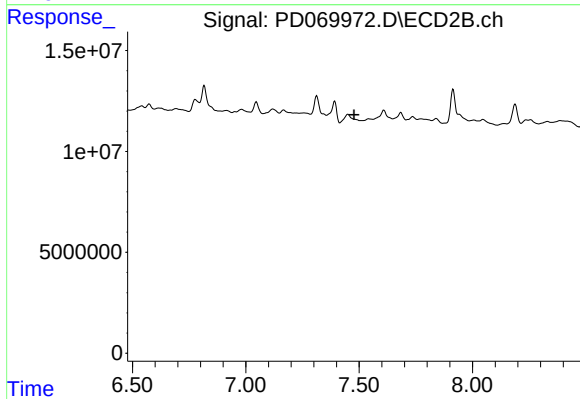

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.478 min
Response: 0
Conc: N.D.

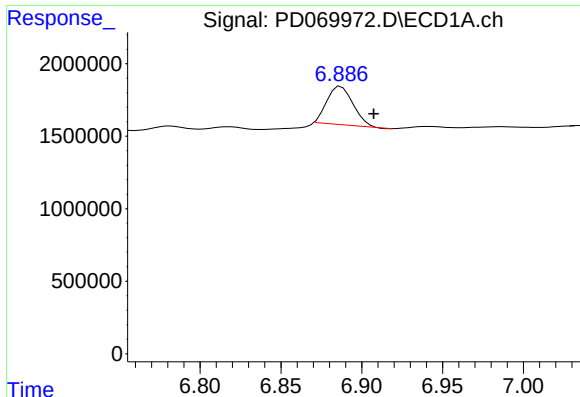

#20 Methoxychlor


R.T.: 6.887 min
Delta R.T.: -0.020 min
Response: 2949123
Conc: 5.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

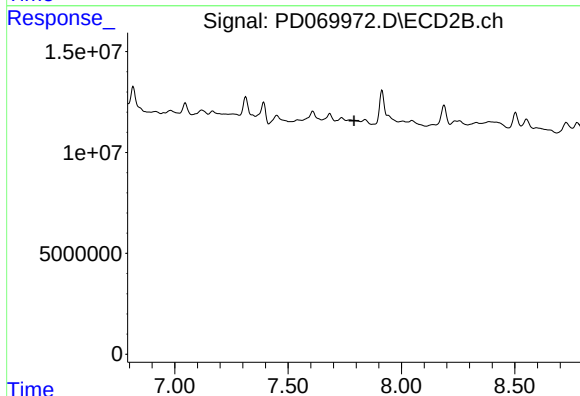


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.792 min
Response: 0
Conc: N.D.

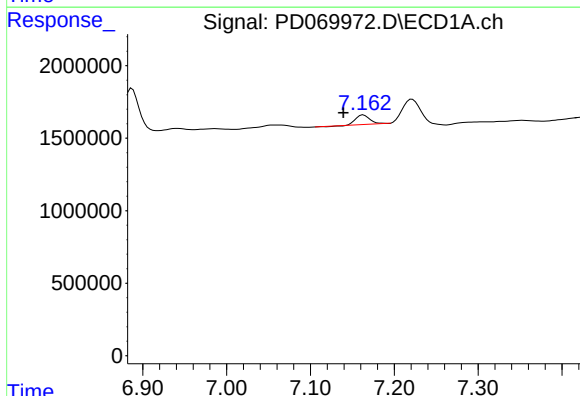


#21 Endrin ketone

R.T.: 7.163 min
Delta R.T.: 0.024 min
Response: 777093
Conc: 0.58 ng/ml

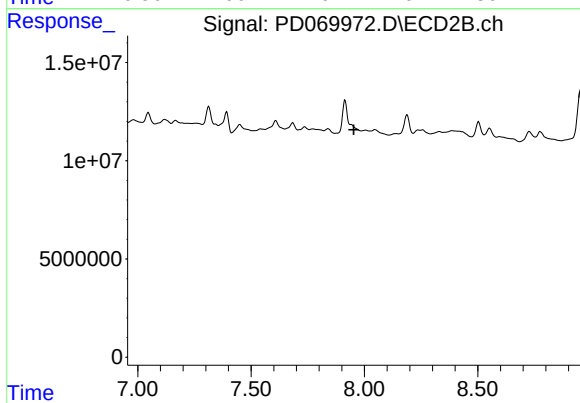

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.953 min
Response: 0
Conc: N.D.

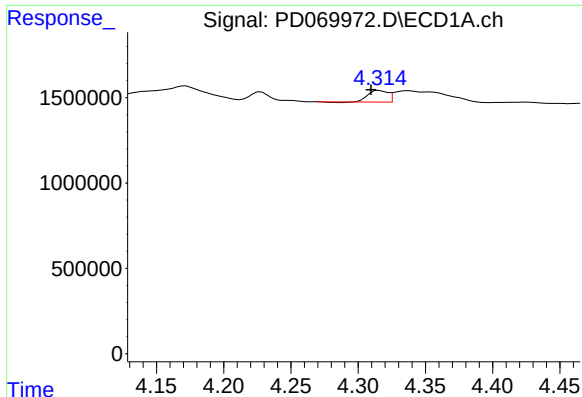

#23 Chlordane-1


R.T.: 4.316 min
Delta R.T.: 0.006 min
Response: 682871
Conc: 17.44 ng/ml

Instrument :
ECD_D
ClientSampleId :

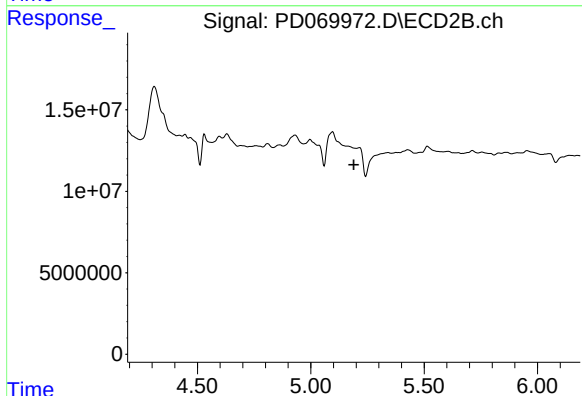


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.190 min
Response: 0
Conc: N.D.

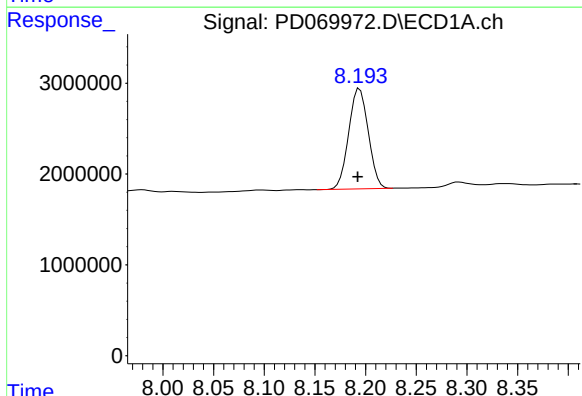

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.002 min
Response: 14816151
Conc: 13.58 ng/ml

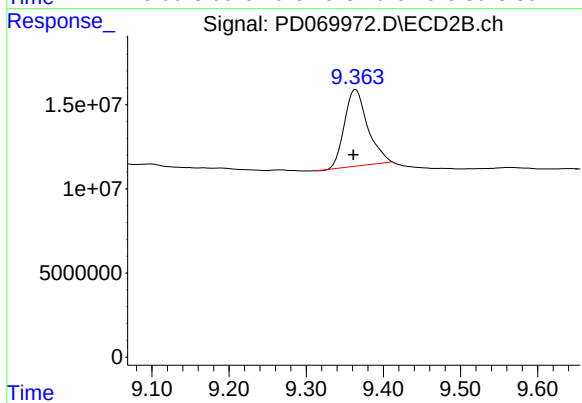

#28 Decachlorobiphenyl

R.T.: 9.364 min
Delta R.T.: 0.003 min
Response: 95420119
Conc: 17.64 ng/ml