

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
 Data File : PD069981.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2022 18:46
 Operator : AR\AJ
 Sample : N2984-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 04:10:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	4.169	22963027	207.4E6	21.578	23.537
28)	SA Decachlor...	8.194	9.363	21306835	116.8E6	19.534	21.604
Target Compounds							
3)	MA gamma-BHC...	4.170	0.000	2512959	0	1.456	N.D. #
12)	B 4,4'-DDE	5.601	0.000	941101	0	0.743	N.D. #
14)	MA Endrin	5.987	6.917	890307	4933173	0.771	0.731
16)	A 4,4'-DDD	0.000	7.046	0	23488916	N.D.	3.172 #
17)	MA 4,4'-DDT	6.354	7.314f	5552047	41026011	5.602	5.606
18)	B Endrin al...	6.447	0.000	1931584	0	2.248	N.D. #
19)	B Endosulfa...	6.642	0.000	2585863	0	2.243	N.D. #
20)	A Methoxychlor	6.888f	0.000	8237442	0	14.520	N.D. #
21)	B Endrin ke...	7.162f	0.000	2464980	0	1.850	N.D. #
23)	Chlordane-1	4.338f	0.000	19891	0	0.508	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
Data File : PD069981.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2022 18:46
Operator : AR\AJ
Sample : N2984-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 04:10:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

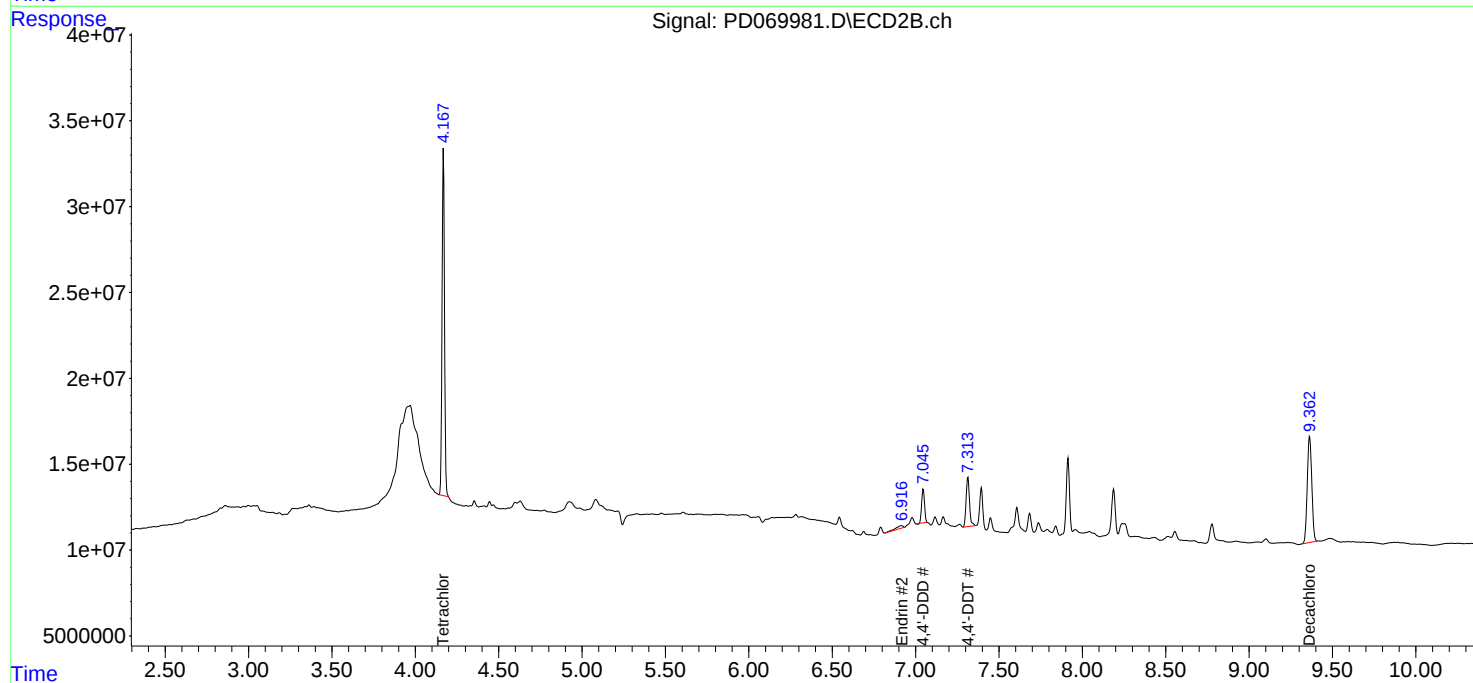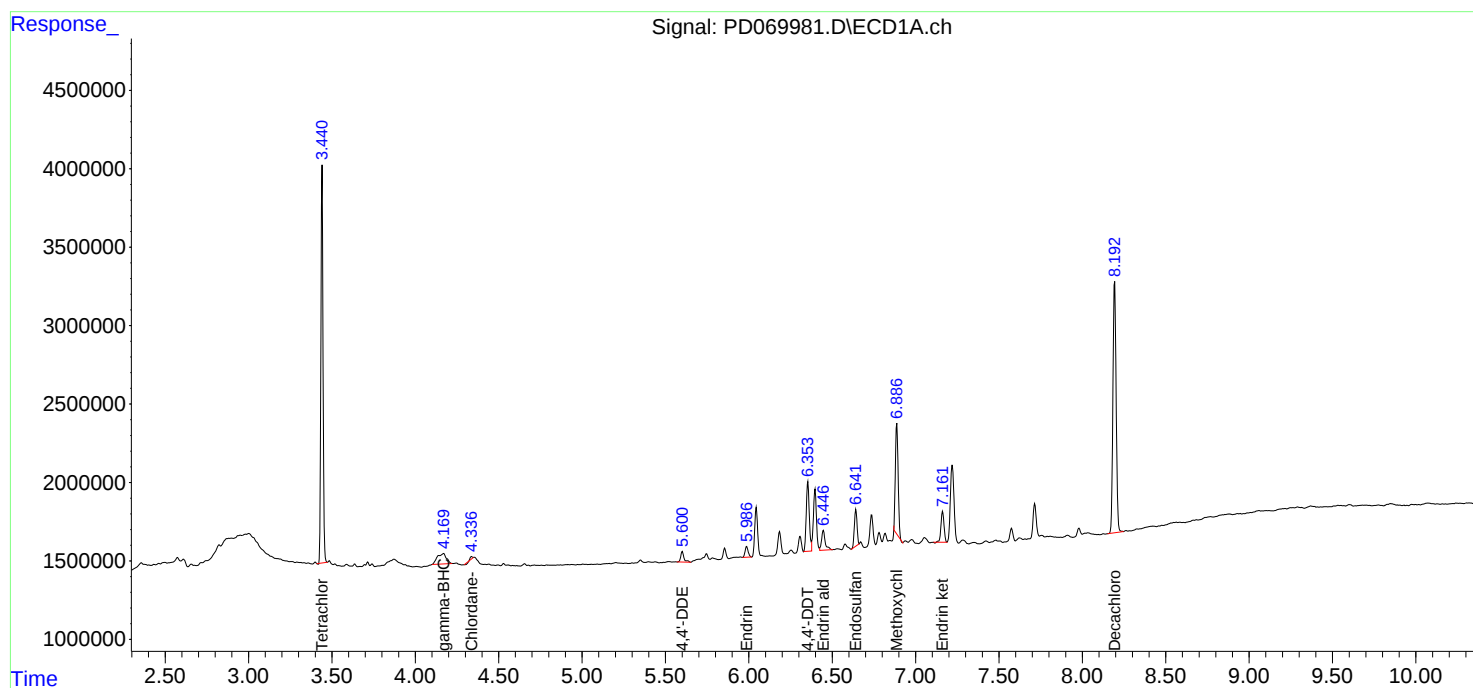


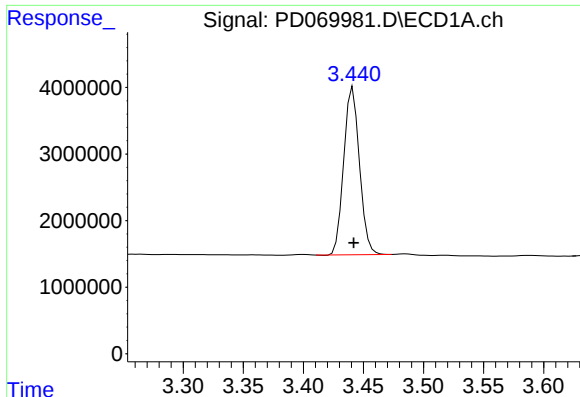

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 22963027
Conc: 21.58 ng/ml

Instrument :
ECD_D
ClientSampleId :

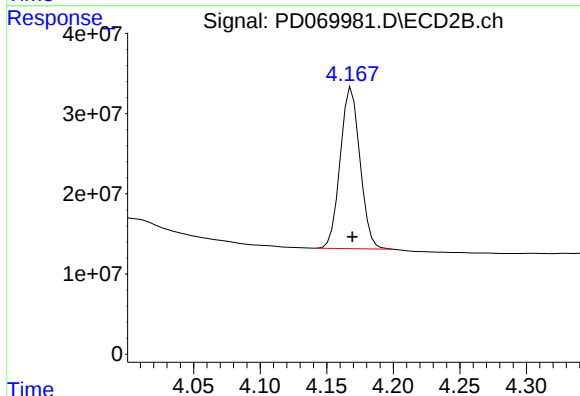


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 207399534
Conc: 23.54 ng/ml

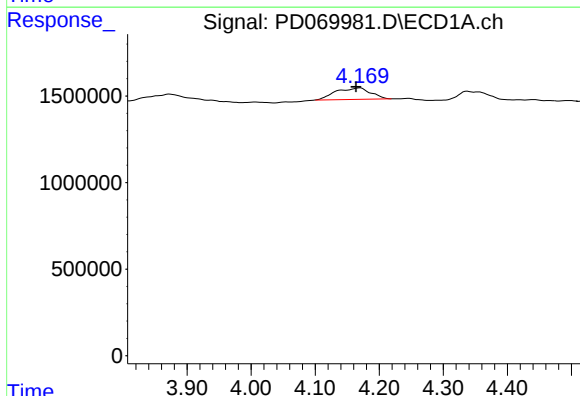


#3 gamma-BHC (Lindane)

R.T.: 4.170 min
Delta R.T.: 0.007 min
Response: 2512959
Conc: 1.46 ng/ml

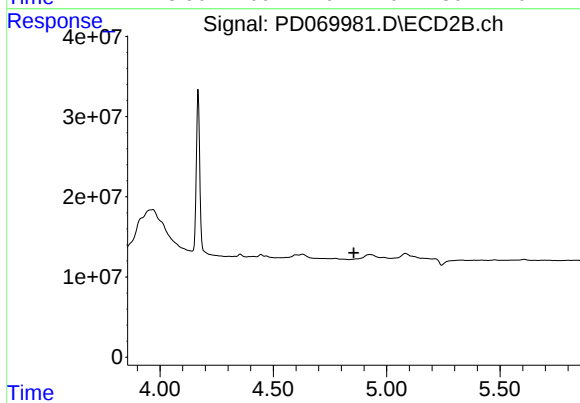

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.856 min
Response: 0
Conc: N.D.

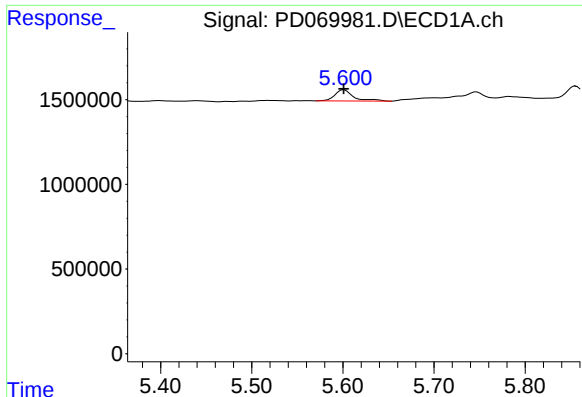

#12 4,4'-DDE


R.T.: 5.601 min
Delta R.T.: 0.000 min
Response: 941101
Conc: 0.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

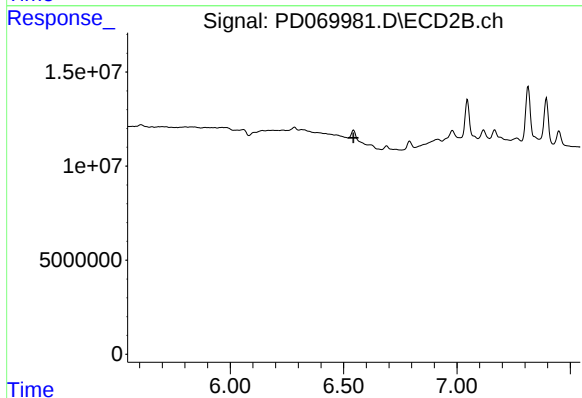


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.544 min
Response: 0
Conc: N.D.

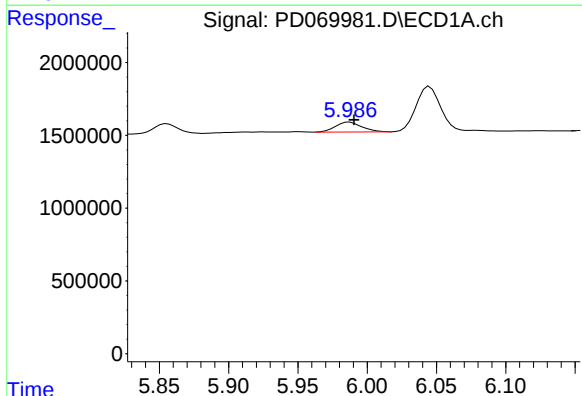


#14 Endrin

R.T.: 5.987 min
Delta R.T.: -0.003 min
Response: 890307
Conc: 0.77 ng/ml

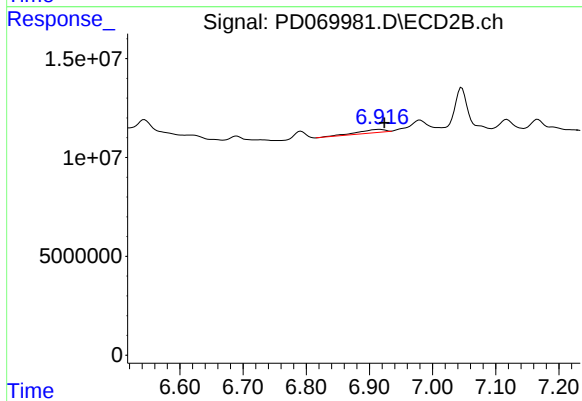

#14 Endrin


R.T.: 6.917 min
Delta R.T.: -0.007 min
Response: 4933173
Conc: 0.73 ng/ml

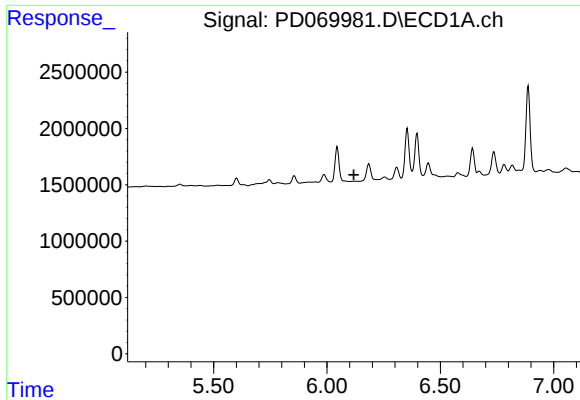

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

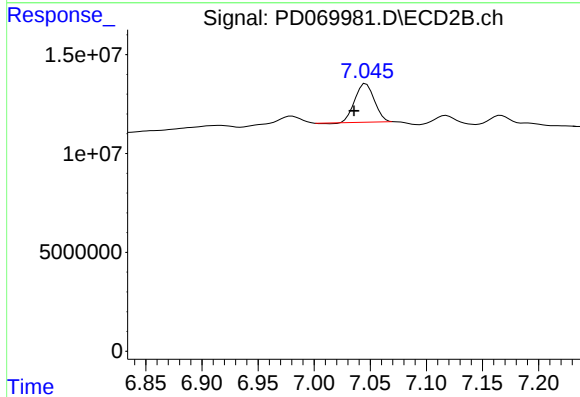


#16 4,4'-DDD

R.T.: 7.046 min
Delta R.T.: 0.011 min
Response: 23488916
Conc: 3.17 ng/ml

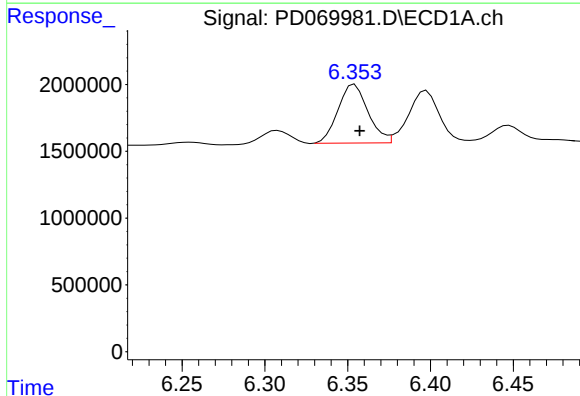


#17 4,4'-DDT

R.T.: 6.354 min
Delta R.T.: -0.003 min
Response: 5552047
Conc: 5.60 ng/ml

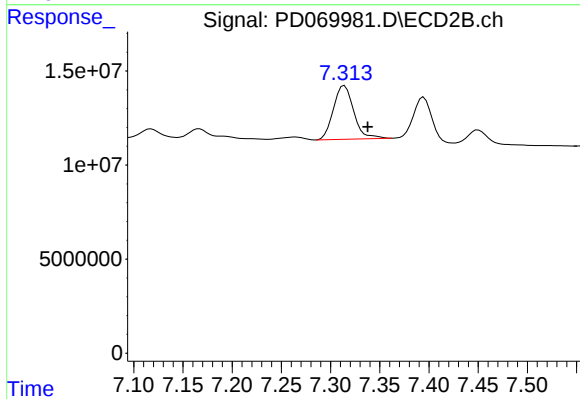

#17 4,4'-DDT


R.T.: 7.314 min
Delta R.T.: -0.024 min
Response: 41026011
Conc: 5.61 ng/ml

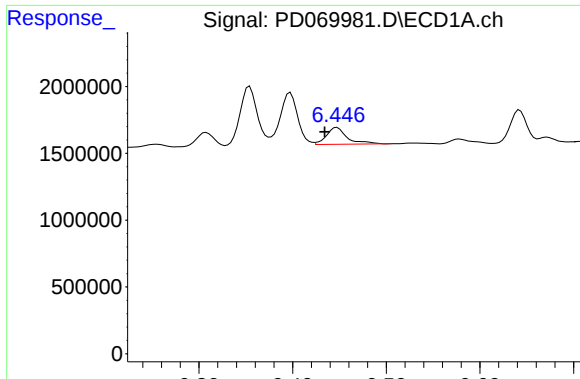

#18 Endrin aldehyde


R.T.: 6.447 min
Delta R.T.: 0.013 min
Response: 1931584
Conc: 2.25 ng/ml

Instrument :
ECD_D
ClientSampleId :

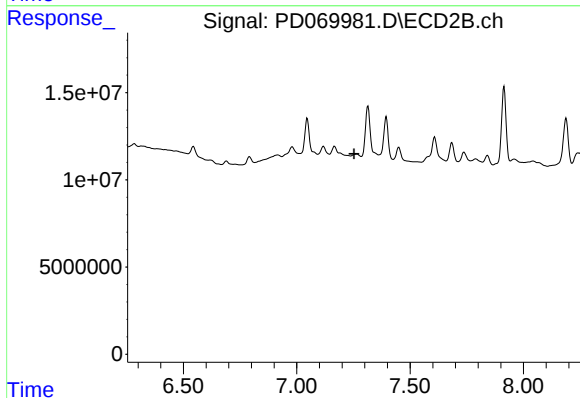


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

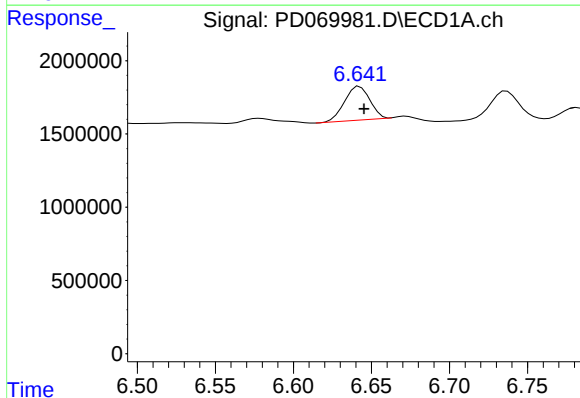


#19 Endosulfan Sulfate

R.T.: 6.642 min
Delta R.T.: -0.003 min
Response: 2585863
Conc: 2.24 ng/ml

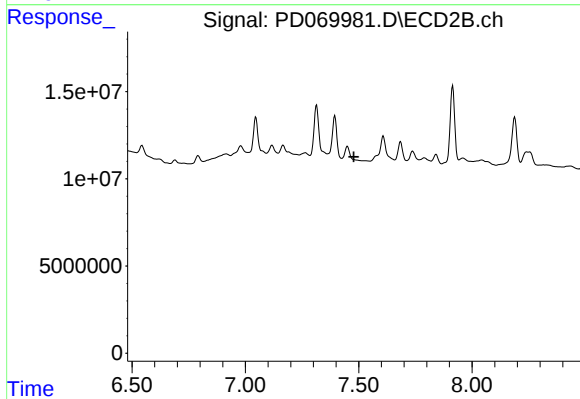

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.478 min
Response: 0
Conc: N.D.

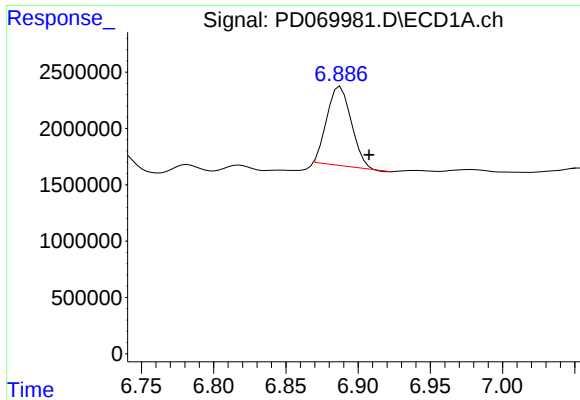

#20 Methoxychlor


R.T.: 6.888 min
Delta R.T.: -0.020 min
Response: 8237442
Conc: 14.52 ng/ml

Instrument :
ECD_D
ClientSampleId :

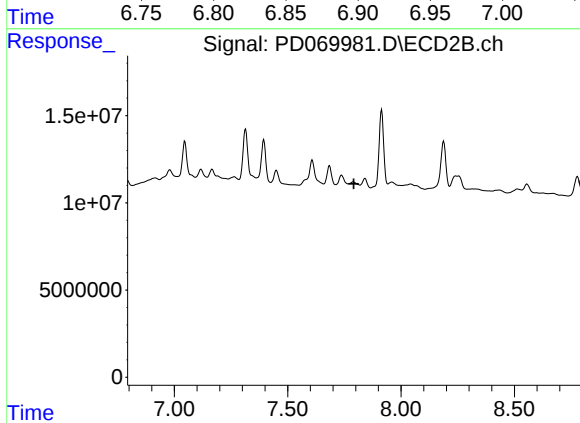


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.792 min
Response: 0
Conc: N.D.

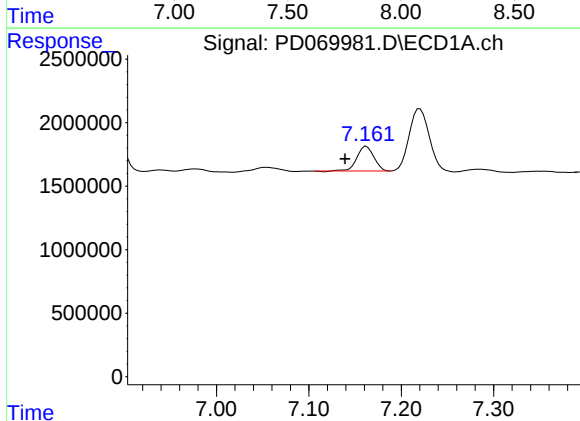


#21 Endrin ketone

R.T.: 7.162 min
Delta R.T.: 0.023 min
Response: 2464980
Conc: 1.85 ng/ml

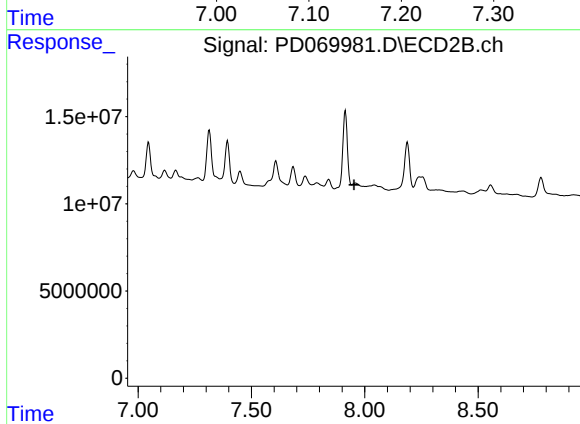

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.953 min
Response: 0
Conc: N.D.

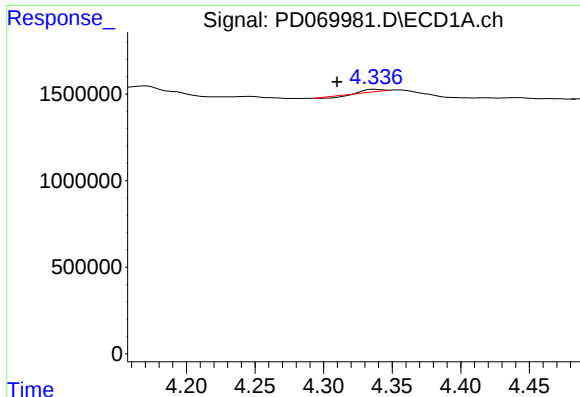

#23 Chlordane-1


R.T.: 4.338 min
Delta R.T.: 0.028 min
Response: 19891
Conc: 0.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

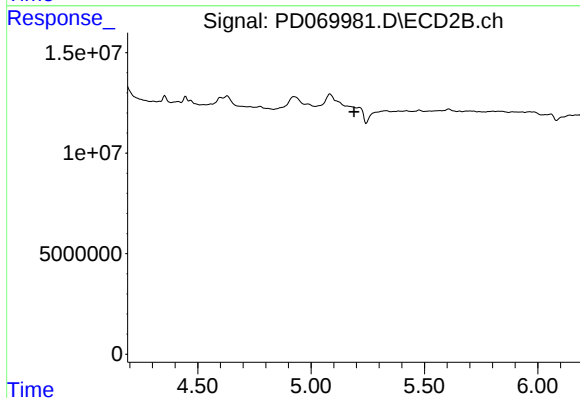


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.190 min
Response: 0
Conc: N.D.

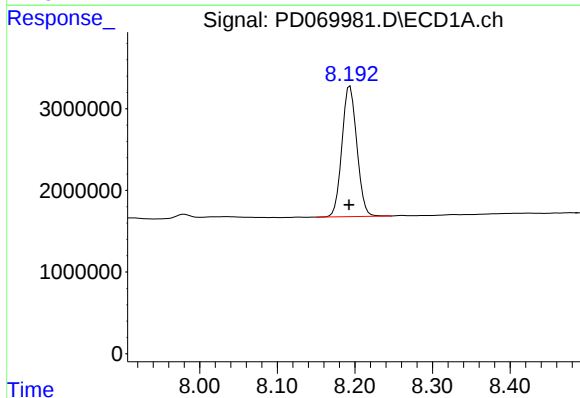

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.002 min
Response: 21306835
Conc: 19.53 ng/ml

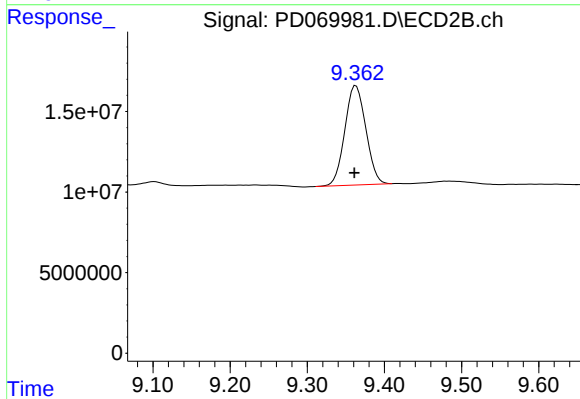

#28 Decachlorobiphenyl

R.T.: 9.363 min
Delta R.T.: 0.002 min
Response: 116839118
Conc: 21.60 ng/ml