

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
 Data File : PD069994.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2022 23:16
 Operator : AR\AJ
 Sample : N2984-12
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 04:12:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	4.168	19983975	183.7E6	18.778	20.847
28)	SA Decachlor...	8.194	9.363	15082803	86227833	13.828	15.944
Target Compounds							
3)	MA gamma-BHC...	4.168	0.000	3522002	0	2.041	N.D. #
15)	B Endosulfa...	6.280f	0.000	952335	0	0.856	N.D. #
16)	A 4,4'-DDD	0.000	7.046	0	19943463	N.D.	2.693 #
17)	MA 4,4'-DDT	6.353	7.314f	3931562	30757552	3.967	4.203
18)	B Endrin al...	6.447	0.000	565005	0	0.658	N.D. #
19)	B Endosulfa...	6.642	0.000	1199936	0	1.041	N.D. #
20)	A Methoxychlor	6.887f	0.000	5890047	0	10.383	N.D. #
21)	B Endrin ke...	7.163f	0.000	1791903	0	1.345	N.D. #
23)	Chlordane-1	4.338f	0.000	1816635	0	46.382	N.D. #
27)	Chlordane-5	6.280	0.000	952335	0	22.645	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
Data File : PD069994.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2022 23:16
Operator : AR\AJ
Sample : N2984-12
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 04:12:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

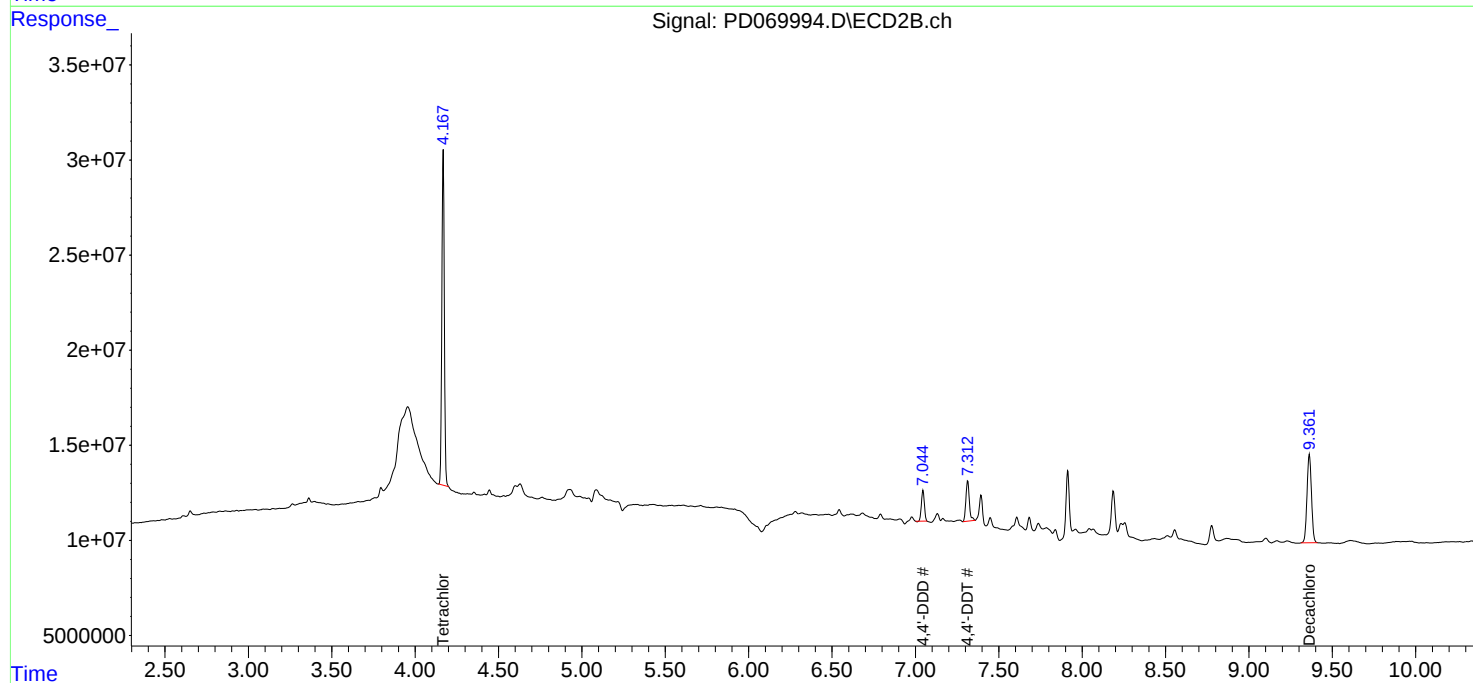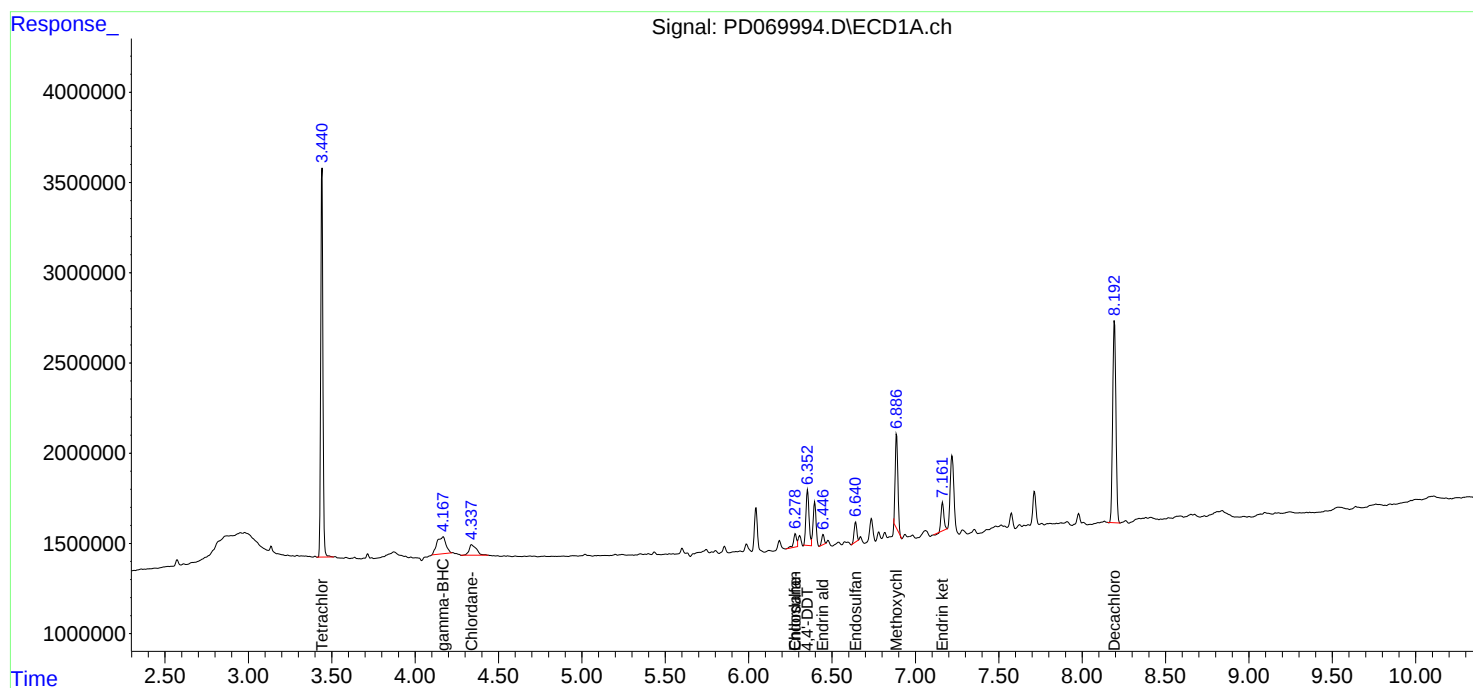


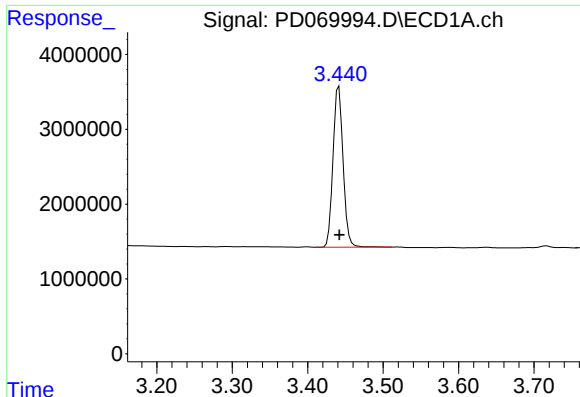

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 19983975
Conc: 18.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

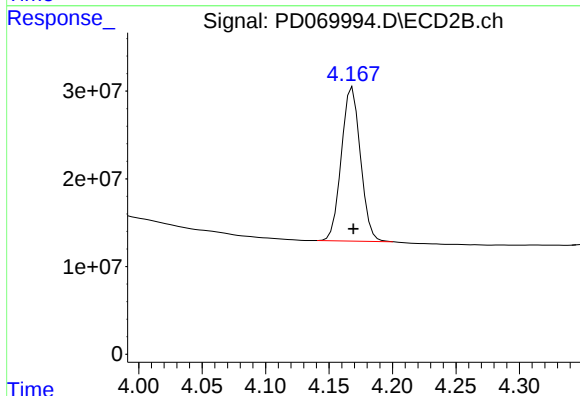


#1 Tetrachloro-m-xylene

R.T.: 4.168 min
Delta R.T.: 0.000 min
Response: 183696654
Conc: 20.85 ng/ml

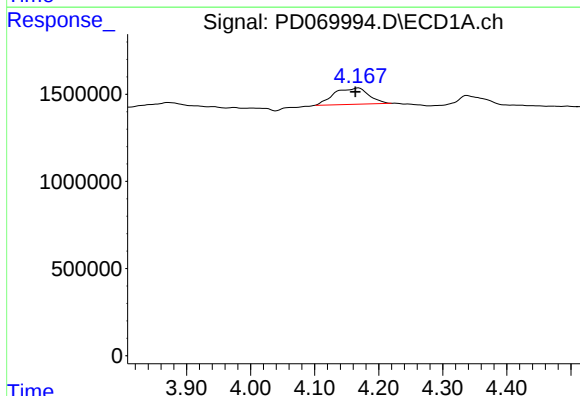


#3 gamma-BHC (Lindane)

R.T.: 4.168 min
Delta R.T.: 0.005 min
Response: 3522002
Conc: 2.04 ng/ml

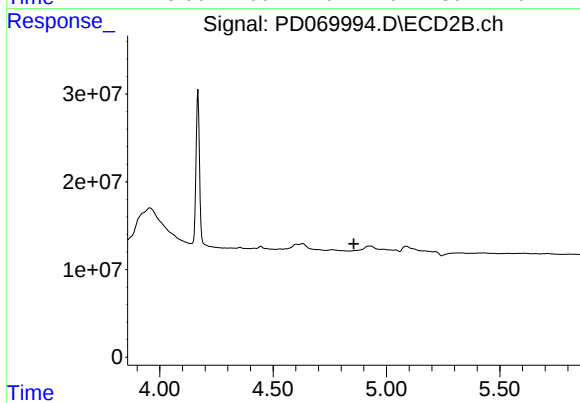

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.856 min
Response: 0
Conc: N.D.

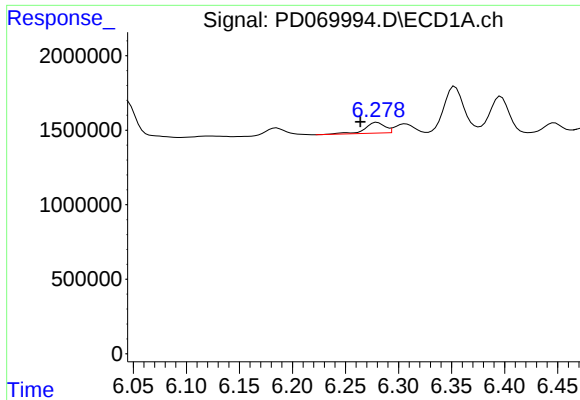

#15 Endosulfan II


R.T.: 6.280 min
Delta R.T.: 0.016 min
Response: 952335
Conc: 0.86 ng/ml

Instrument :
ECD_D
ClientSampleId :

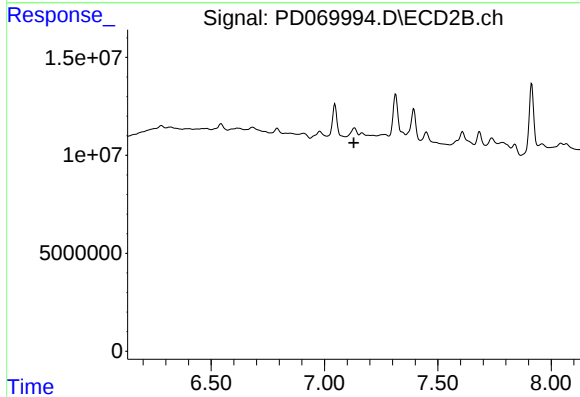


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.130 min
Response: 0
Conc: N.D.

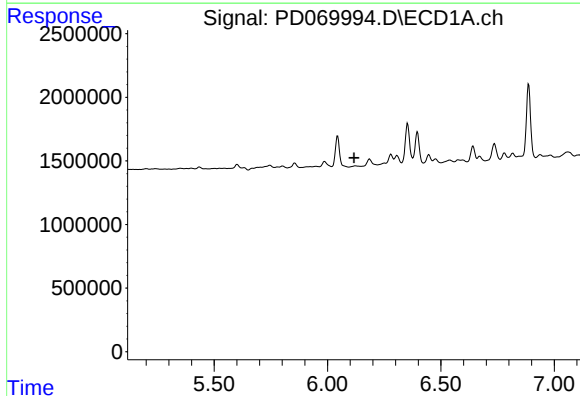


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.118 min
Response: 0
Conc: N.D.

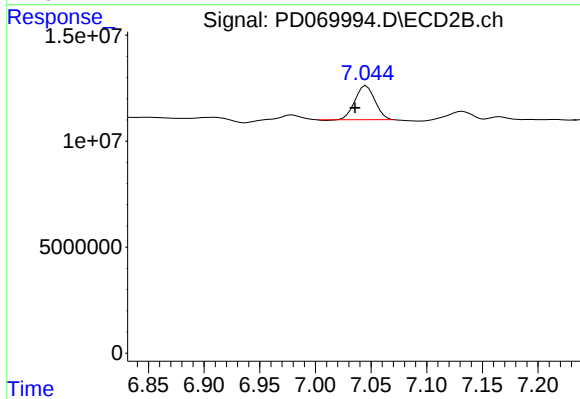

#16 4,4'-DDD


R.T.: 7.046 min
Delta R.T.: 0.010 min
Response: 19943463
Conc: 2.69 ng/ml

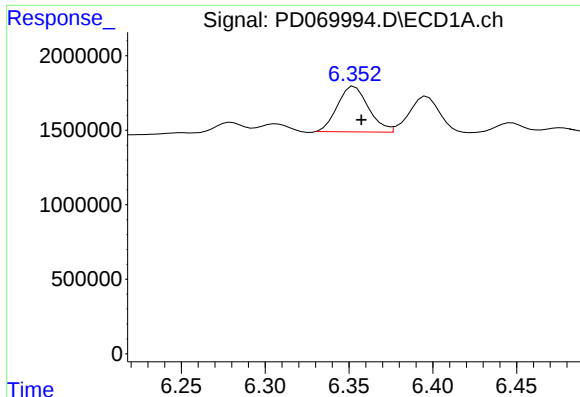

#17 4,4'-DDT


R.T.: 6.353 min
Delta R.T.: -0.004 min
Response: 3931562
Conc: 3.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

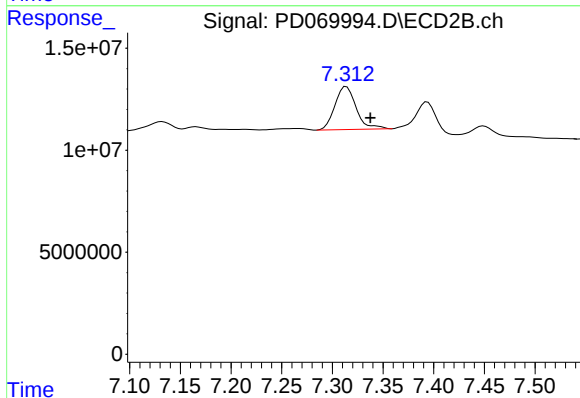


#17 4,4'-DDT

R.T.: 7.314 min
Delta R.T.: -0.024 min
Response: 30757552
Conc: 4.20 ng/ml

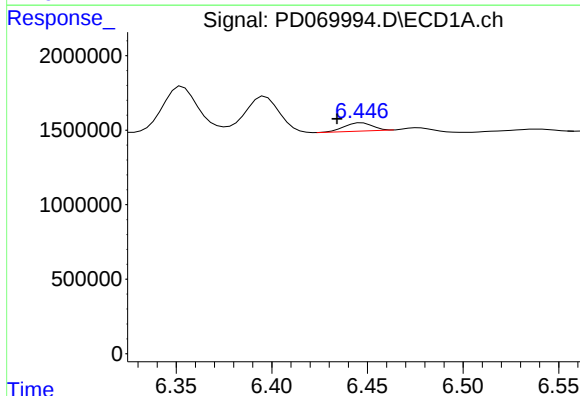


#18 Endrin aldehyde

R.T.: 6.447 min
Delta R.T.: 0.013 min
Response: 565005
Conc: 0.66 ng/ml

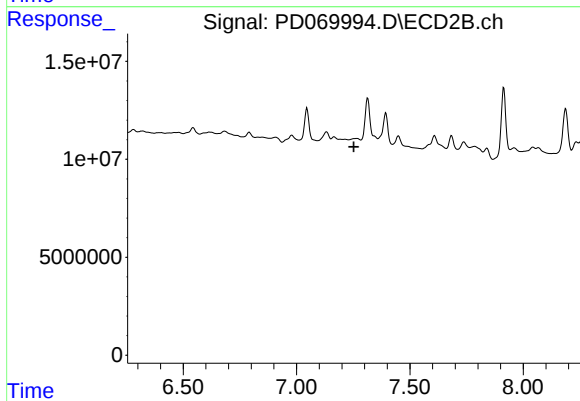

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

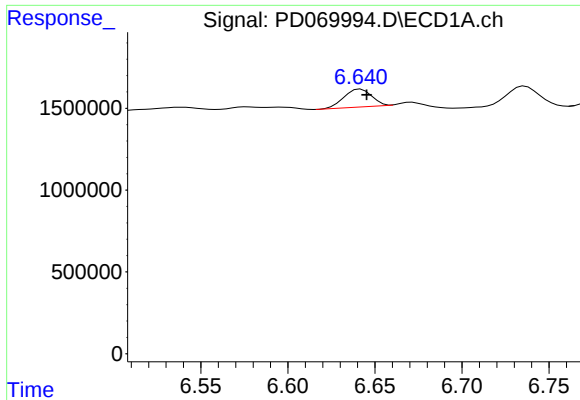

#19 Endosulfan Sulfate


R.T.: 6.642 min
Delta R.T.: -0.004 min
Response: 1199936
Conc: 1.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

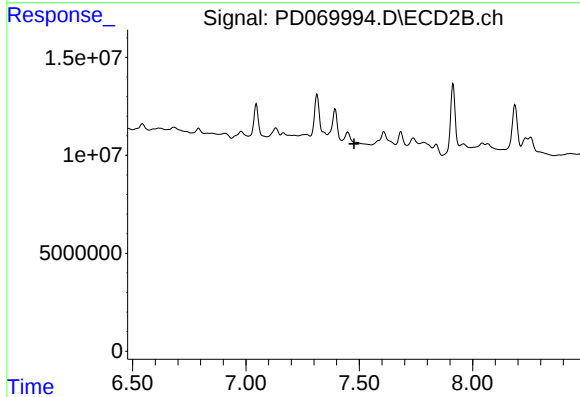


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.478 min
Response: 0
Conc: N.D.

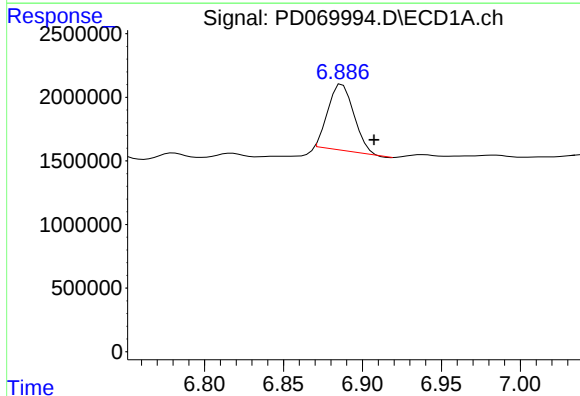


#20 Methoxychlor

R.T.: 6.887 min
Delta R.T.: -0.020 min
Response: 5890047
Conc: 10.38 ng/ml

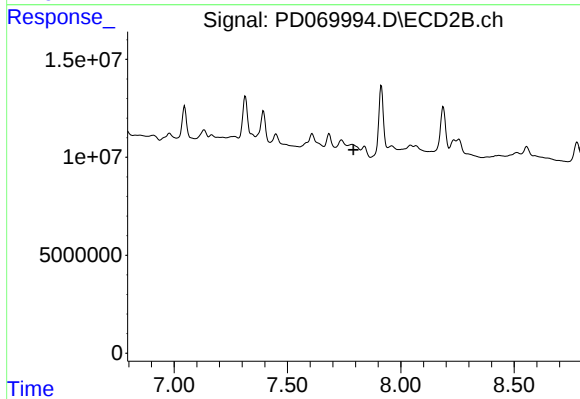

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.792 min
Response: 0
Conc: N.D.

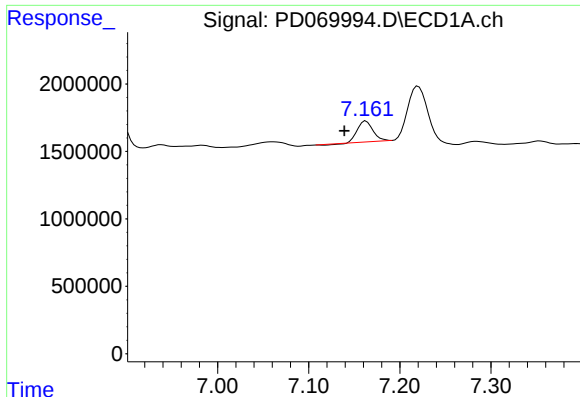

#21 Endrin ketone


R.T.: 7.163 min
Delta R.T.: 0.024 min
Response: 1791903
Conc: 1.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

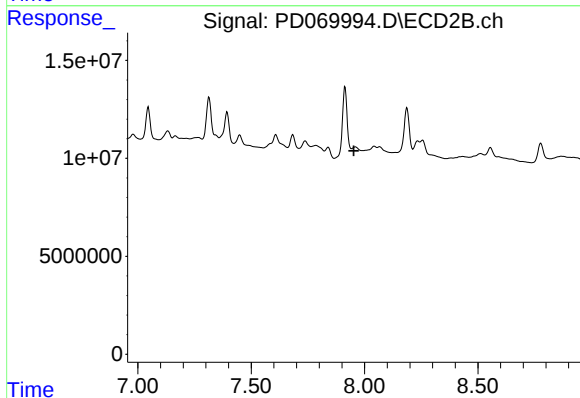


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.953 min
Response: 0
Conc: N.D.

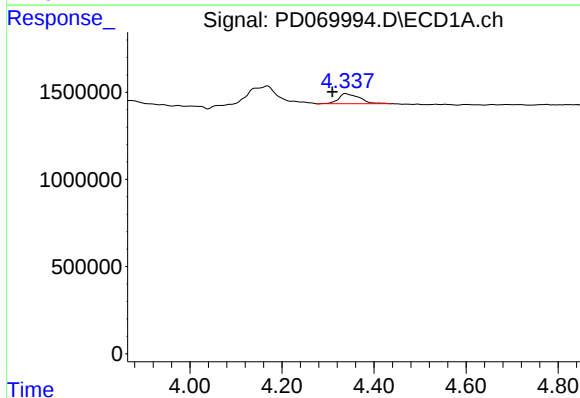


#23 Chlordane-1

R.T.: 4.338 min
Delta R.T.: 0.029 min
Response: 1816635
Conc: 46.38 ng/ml

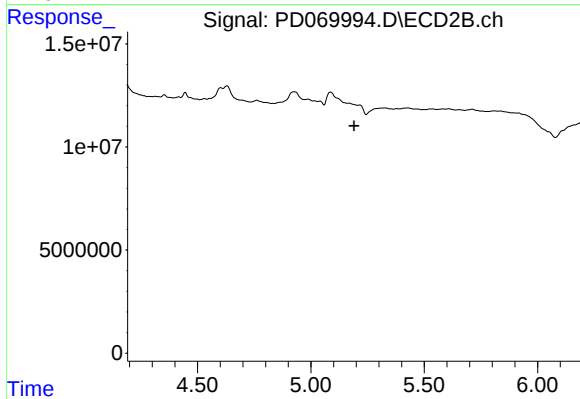

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.190 min
Response: 0
Conc: N.D.

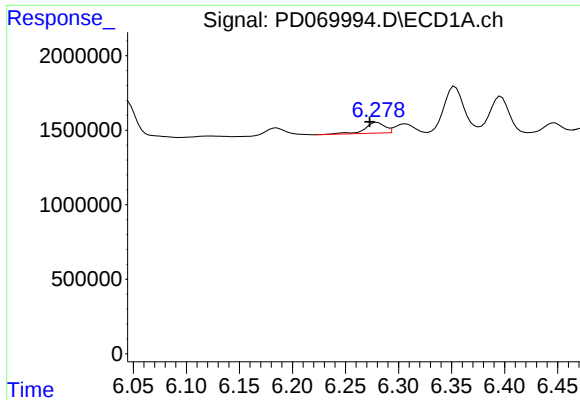

#27 Chlordane-5


R.T.: 6.280 min
Delta R.T.: 0.007 min
Response: 952335
Conc: 22.64 ng/ml

Instrument :
ECD_D
ClientSampleId :

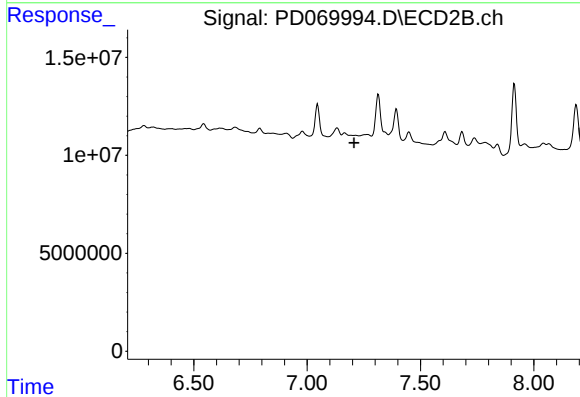


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.207 min
Response: 0
Conc: N.D.

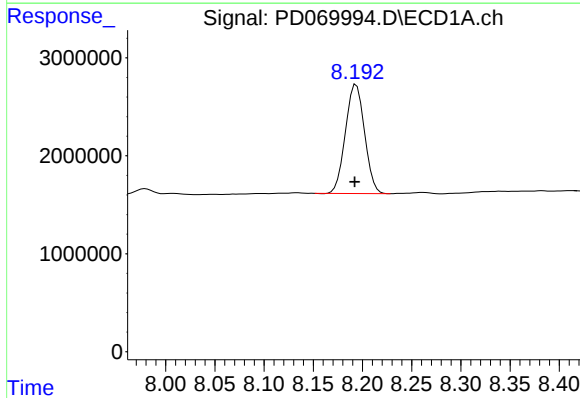

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.001 min
Response: 15082803
Conc: 13.83 ng/ml

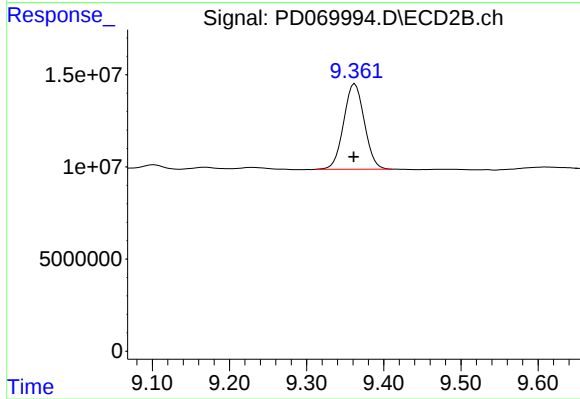

#28 Decachlorobiphenyl

R.T.: 9.363 min
Delta R.T.: 0.001 min
Response: 86227833
Conc: 15.94 ng/ml