

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
 Data File : PD069997.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2022 23:58
 Operator : AR\AJ
 Sample : N2984-15
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 04:13:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
 Quant Title : GC Extractables
 QLast Update : Thu May 26 05:06:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	4.168	22247182	205.1E6	20.905	23.274
28)	SA Decachlor...	8.194	9.363	20386713	115.9E6	18.691	21.436
Target Compounds							
3)	MA gamma-BHC...	4.168	0.000	3159275	0	1.830	N.D. #
24)	Chlordane-2	4.823	0.000	2644962	0	60.212	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060322\
Data File : PD069997.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2022 23:58
Operator : AR\AJ
Sample : N2984-15
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 04:13:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052622.M
Quant Title : GC Extractables
QLast Update : Thu May 26 05:06:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

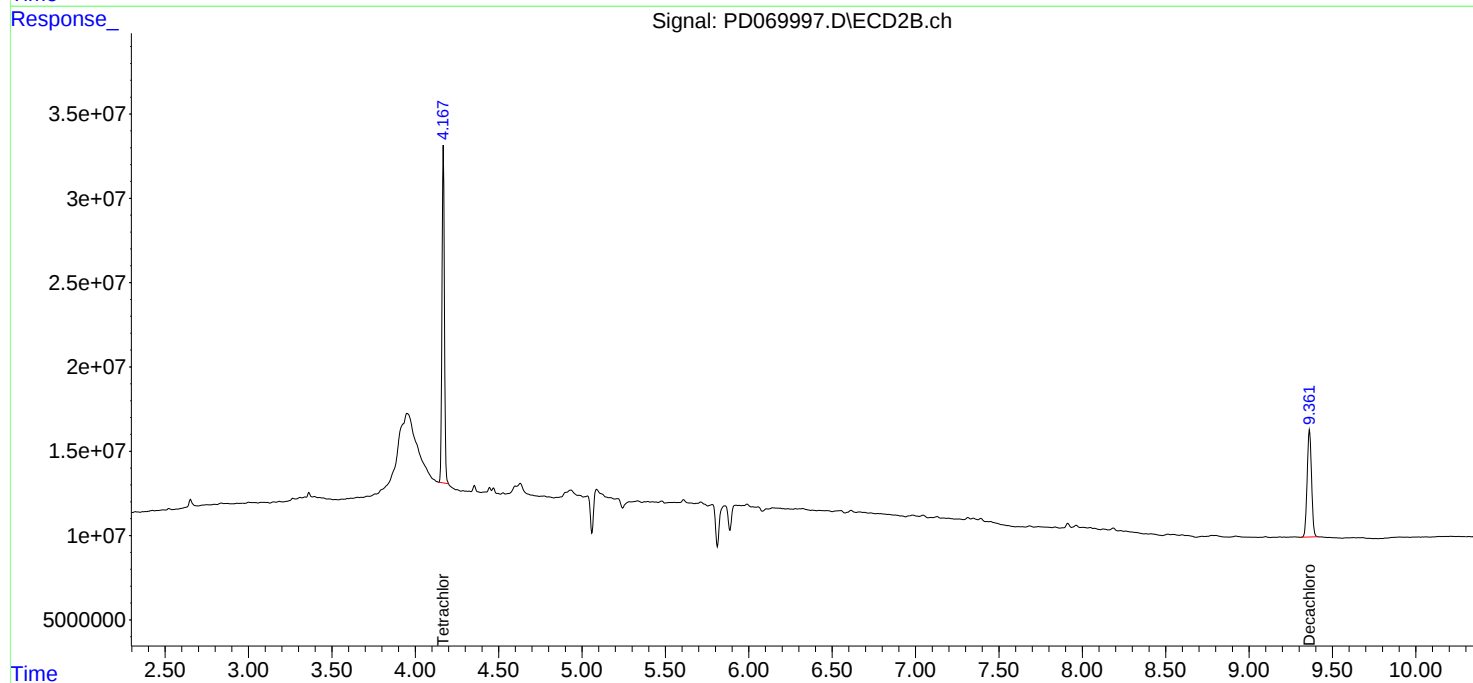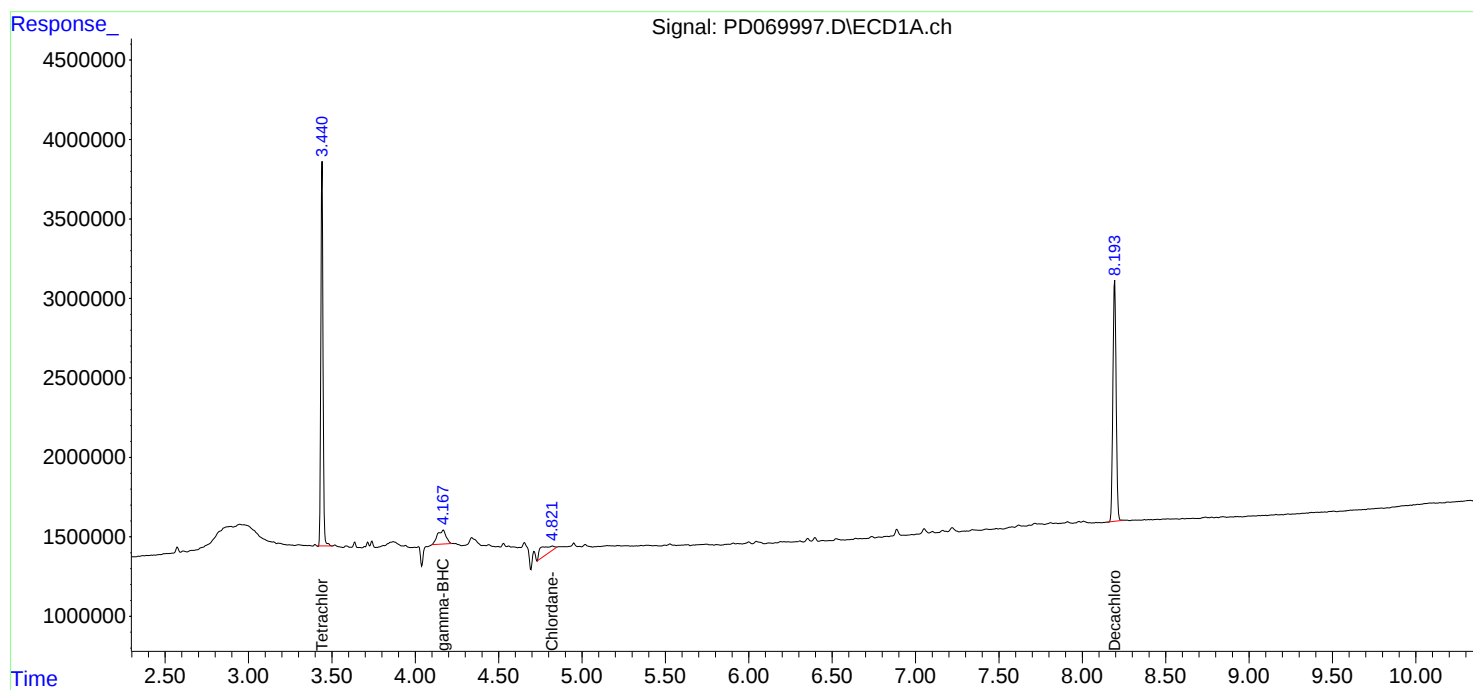


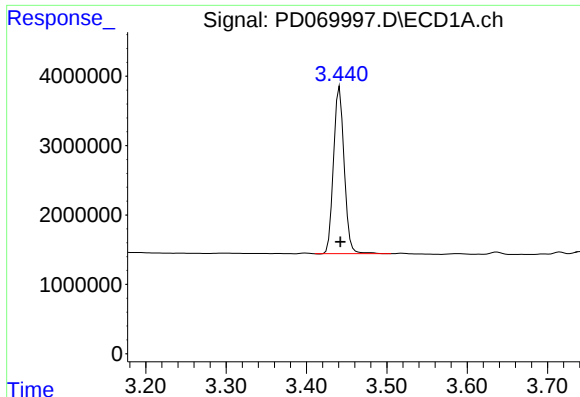

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 22247182
Conc: 20.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

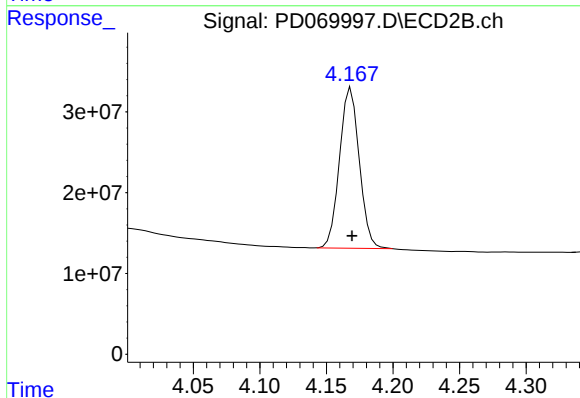


#1 Tetrachloro-m-xylene

R.T.: 4.168 min
Delta R.T.: 0.000 min
Response: 205088256
Conc: 23.27 ng/ml

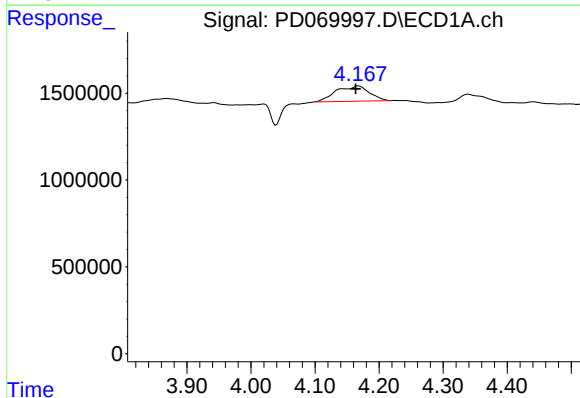


#3 gamma-BHC (Lindane)

R.T.: 4.168 min
Delta R.T.: 0.004 min
Response: 3159275
Conc: 1.83 ng/ml

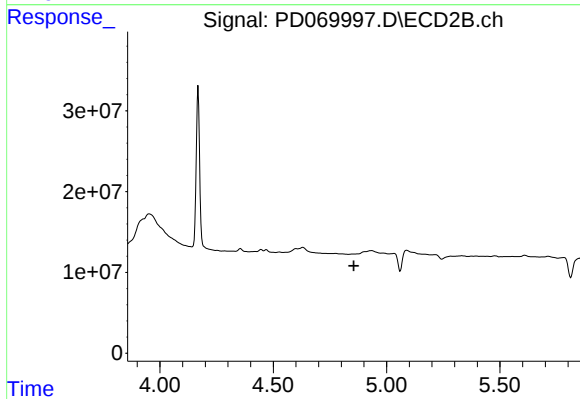

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.856 min
Response: 0
Conc: N.D.

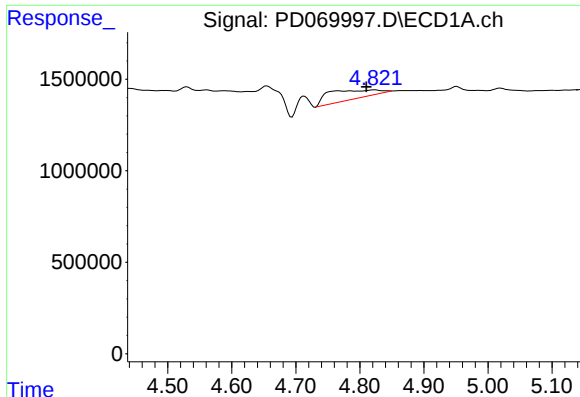

#24 Chlordane-2


R.T.: 4.823 min
Delta R.T.: 0.012 min
Response: 2644962
Conc: 60.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

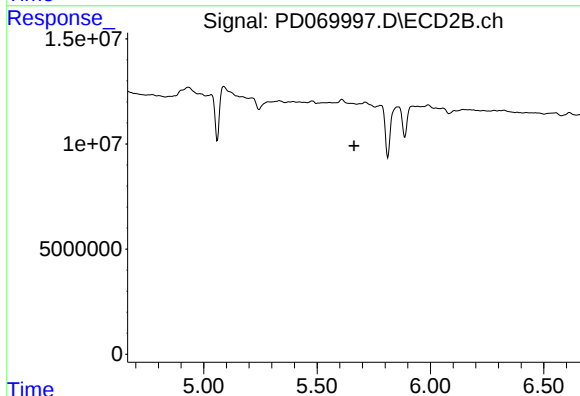


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.664 min
Response: 0
Conc: N.D.

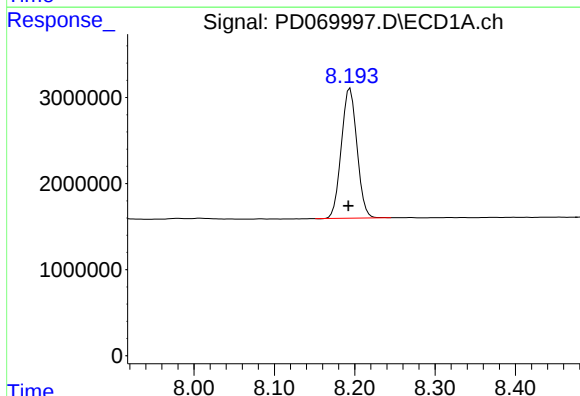

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.002 min
Response: 20386713
Conc: 18.69 ng/ml

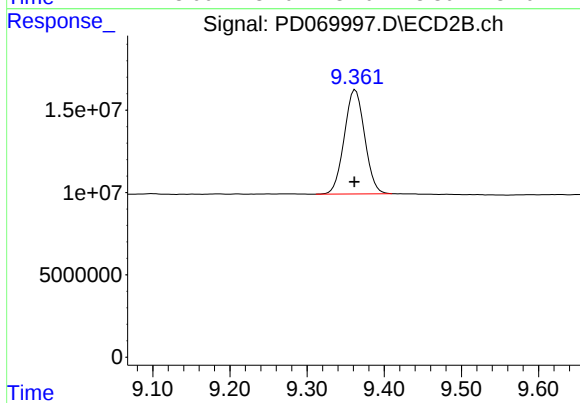

#28 Decachlorobiphenyl

R.T.: 9.363 min
Delta R.T.: 0.001 min
Response: 115929776
Conc: 21.44 ng/ml